

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062124\
 Data File : BN032148.D
 Acq On : 22 Jun 2024 01:57
 Operator : MA/JU
 Sample : PB161510BS
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB161510BS

Quant Time: Jun 22 03:21:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN061024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 19 11:30:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	0.000	152	0	0.000	ng	-7.65
7) Naphthalene-d8	0.000	136	0	0.000	ng	-10.42
13) Acenaphthene-d10	0.000	164	0	0.000	ng	-14.28
19) Phenanthrene-d10	0.000	188	0	0.000	ng	-17.03
29) Chrysene-d12	0.000	240	0	0.000	ng	-21.23
35) Perylene-d12	0.000	264	0	0.000	ng	-23.45
System Monitoring Compounds						
4) 2-Fluorophenol	0.000	112	0	0.000	ng	
5) Phenol-d6	0.000	99	0	0.000	ng	
8) Nitrobenzene-d5	0.000	82	0	0.000	ng	
11) 2-Methylnaphthalene-d10	0.000	152	0	0.000	ng	
14) 2,4,6-Tribromophenol	0.000	330	0	0.000	ng	
15) 2-Fluorobiphenyl	0.000	172	0	0.000	ng	
27) Fluoranthene-d10	0.000	212	0	0.000	ng	
31) Terphenyl-d14	0.000	244	0	0.000	ng	


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062124\
Data File : BN032148.D
Acq On : 22 Jun 2024 01:57
Operator : MA/JU
Sample : PB161510BS
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB161510BS

Quant Time: Jun 22 03:21:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN061024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 19 11:30:34 2024
Response via : Initial Calibration

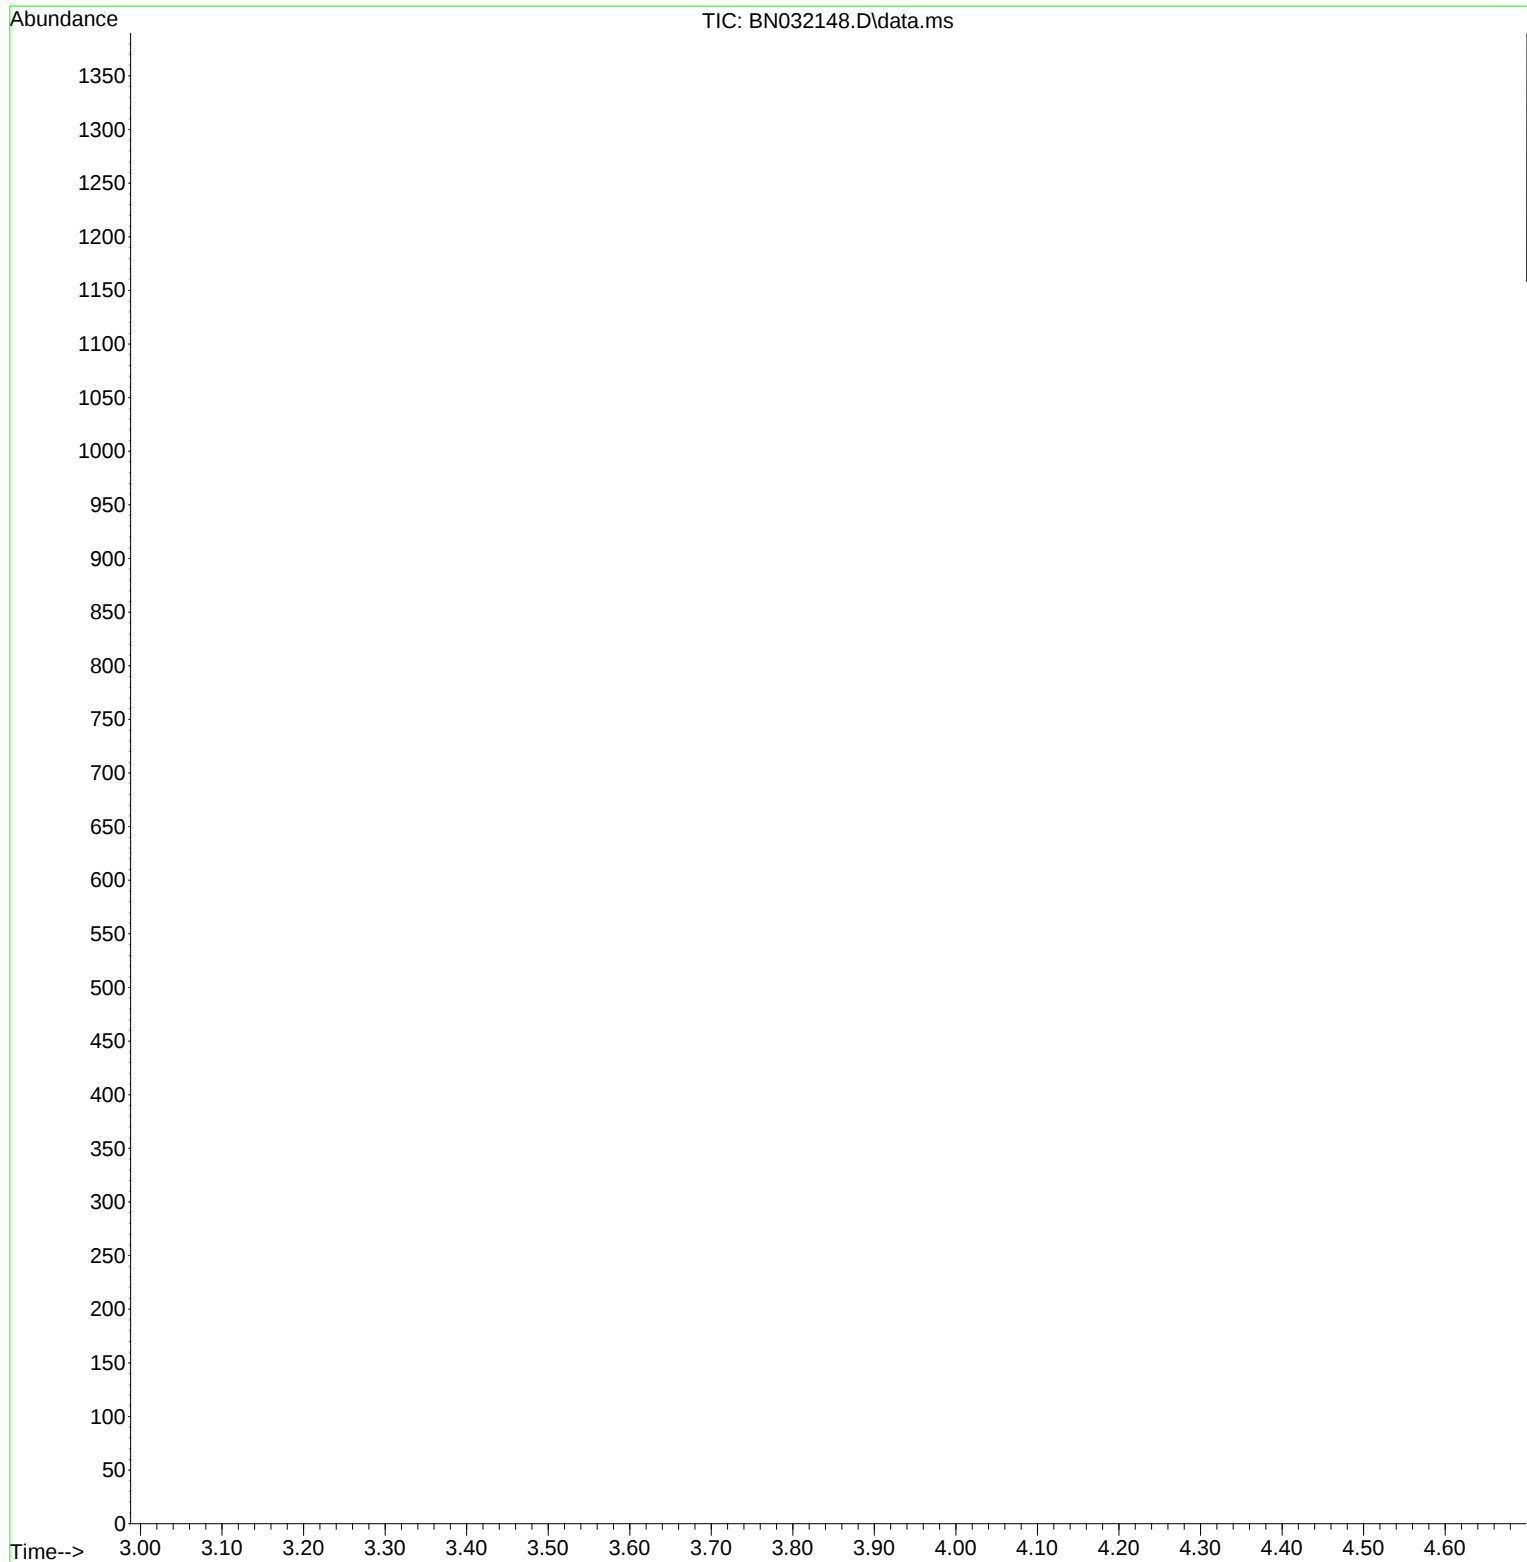


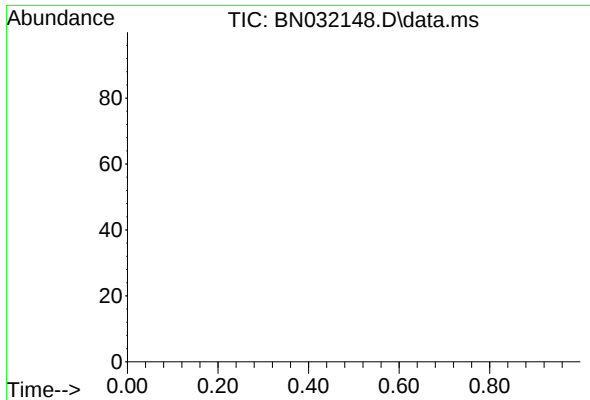


#1
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ng
 Expected RT: 7.65 min
 Lab File: BN032148.D
 Acq: 22 Jun 2024 01:57

Instrument :
 BNA_N
 ClientSampleId :
 PB161510BS

Tgt Ion: 152


Sig	Exp Ratio
152	100
150	151.2
115	61.7

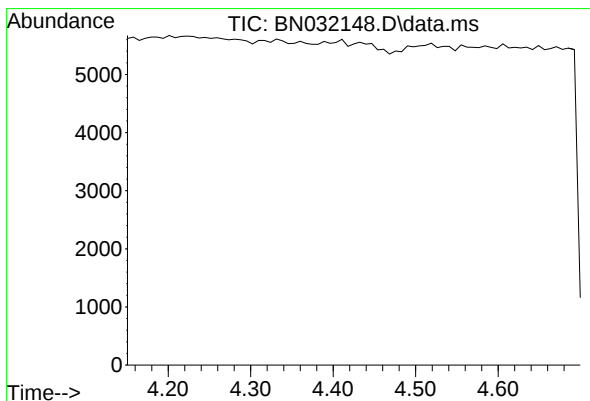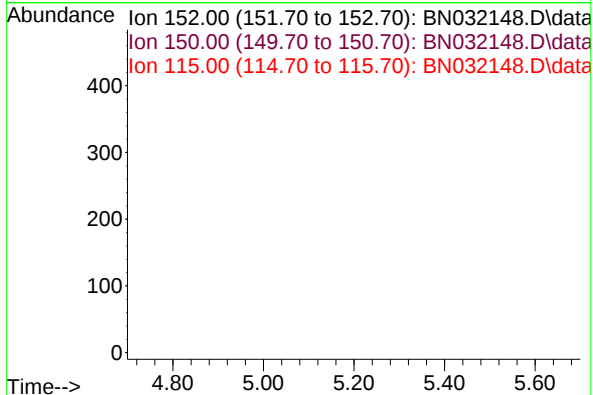


#4
 2-Fluorophenol
 Concen: 0.000 ng
 Expected RT: 5.25 min
 Lab File: BN032148.D
 Acq: 22 Jun 2024 01:57

Tgt Ion: 112

Sig	Exp Ratio
112	100
64	53.0
63	27.6

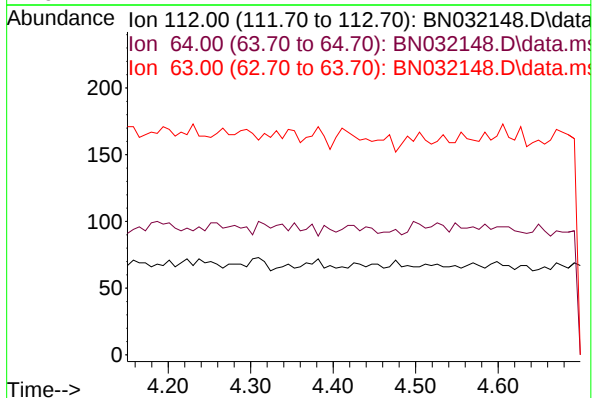


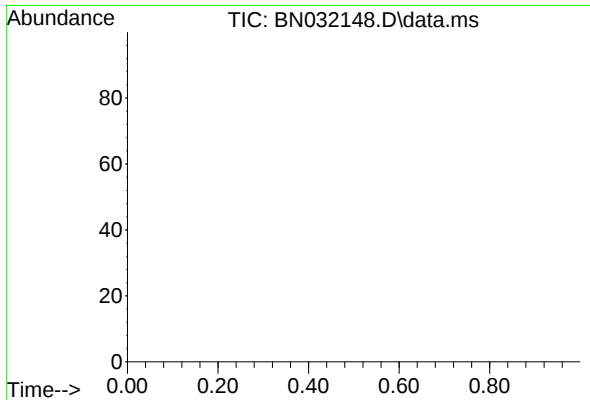


#5
 Phenol-d6
 Concen: 0.000 ng
 Expected RT: 6.83 min
 Lab File: BN032148.D
 Acq: 22 Jun 2024 01:57

Instrument :
 BNA_N
 ClientSampleId :
 PB161510BS

Tgt Ion: 99


Sig	Exp Ratio
99	100
42	16.0
71	31.8

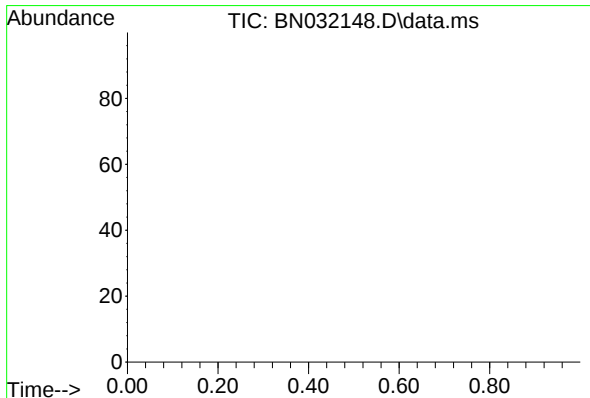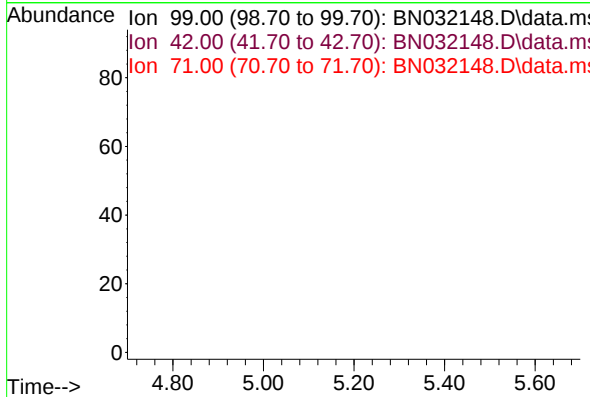


#7
 Naphthalene-d8
 Concen: 0.000 ng
 Expected RT: 10.42 min
 Lab File: BN032148.D
 Acq: 22 Jun 2024 01:57

Tgt Ion: 136

Sig	Exp Ratio
136	100
137	11.1
54	7.0
68	6.2

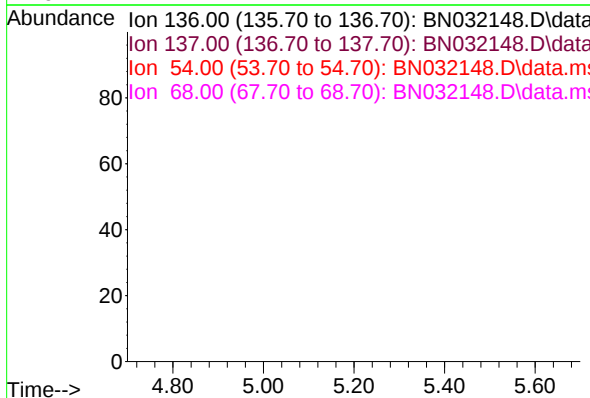


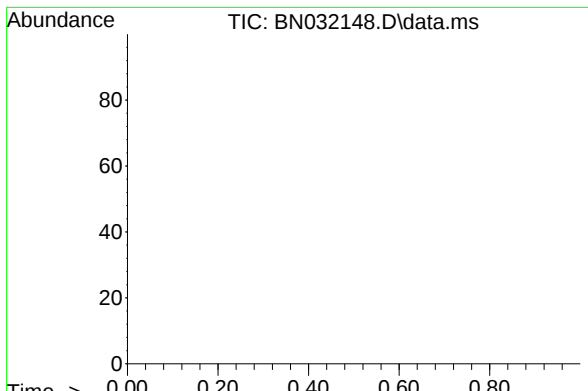


#8
 Nitrobenzene-d5
 Concen: 0.000 ng
 Expected RT: 8.80 min
 Lab File: BN032148.D
 Acq: 22 Jun 2024 01:57

Instrument :
 BNA_N
 ClientSampleId :
 PB161510BS

Tgt Ion: 82


Sig	Exp Ratio
82	100
128	40.1
54	49.6

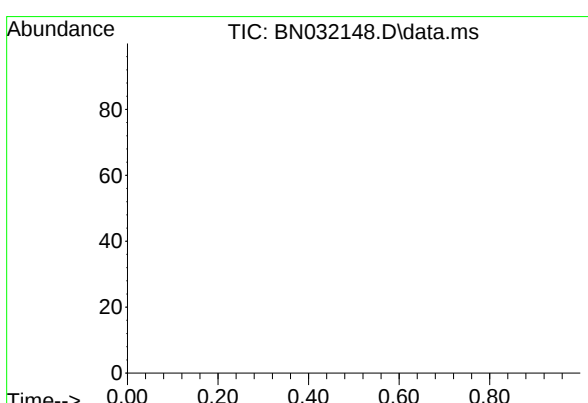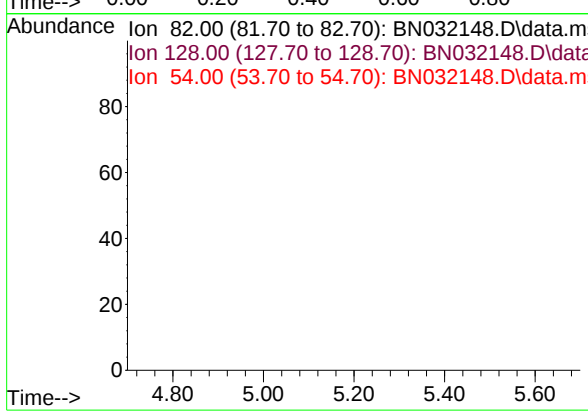


#11
 2-Methylnaphthalene-d10
 Concen: 0.000 ng
 Expected RT: 12.02 min
 Lab File: BN032148.D
 Acq: 22 Jun 2024 01:57

Tgt Ion: 152

Sig	Exp Ratio
152	100
151	20.4


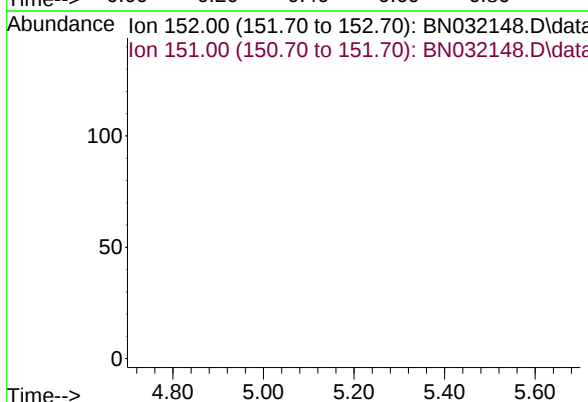


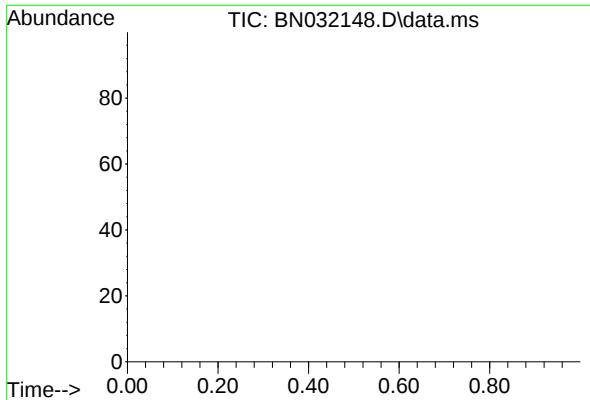

#13
 Acenaphthene-d10
 Concen: 0.000 ng
 Expected RT: 14.28 min
 Lab File: BN032148.D
 Acq: 22 Jun 2024 01:57


Instrument :
 BNA_N
 ClientSampleId :
 PB161510BS


Tgt Ion: 164
 Sig Exp Ratio
 164 100
 162 100.9
 160 45.3

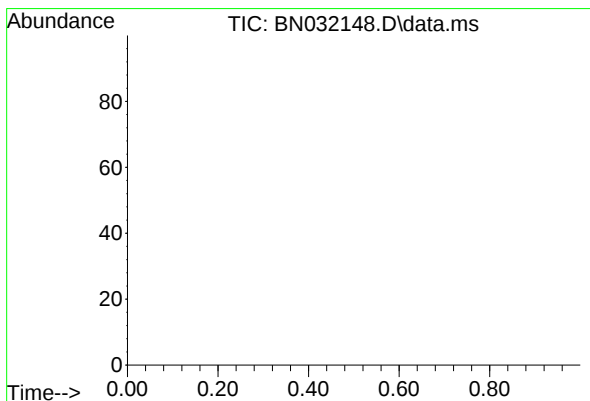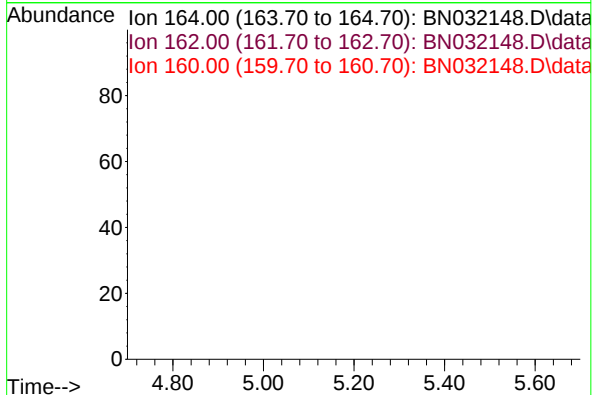

#14
 2,4,6-Tribromophenol
 Concen: 0.000 ng
 Expected RT: 15.79 min
 Lab File: BN032148.D
 Acq: 22 Jun 2024 01:57

Tgt Ion: 330
 Sig Exp Ratio
 330 100
 332 96.9
 141 43.4

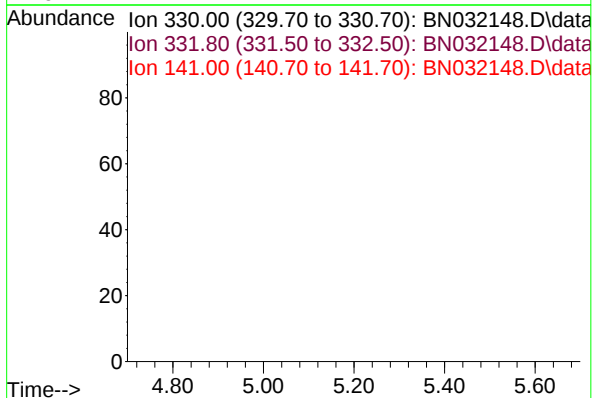


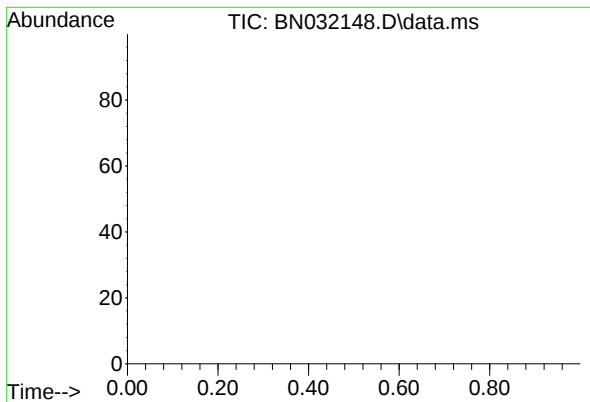


#15
2-Fluorobiphenyl
Concen: 0.000 ng
Expected RT: 12.91 min

Lab File: BN032148.D
Acq: 22 Jun 2024 01:57

Instrument :
BNA_N
ClientSampleId :
PB161510BS


Tgt Ion: 172
Sig Exp Ratio
172 100
171 35.7
170 24.0

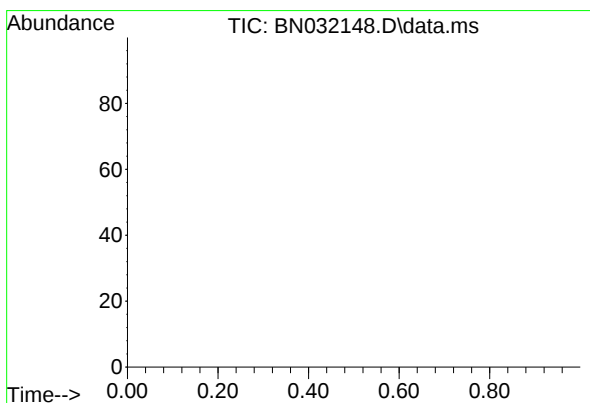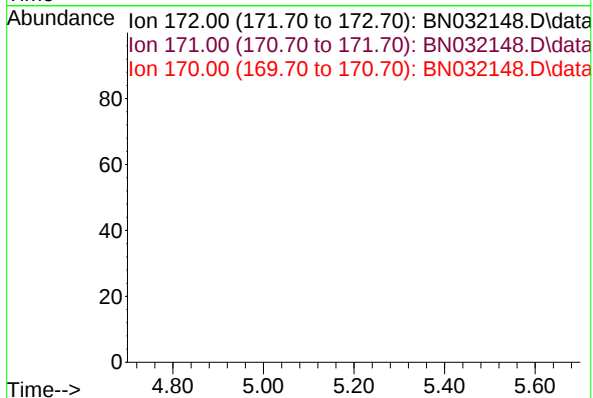


#19
Phenanthrene-d10
Concen: 0.000 ng
Expected RT: 17.03 min

Lab File: BN032148.D
Acq: 22 Jun 2024 01:57

Tgt Ion: 188
Sig Exp Ratio
188 100
94 0.0
80 8.0


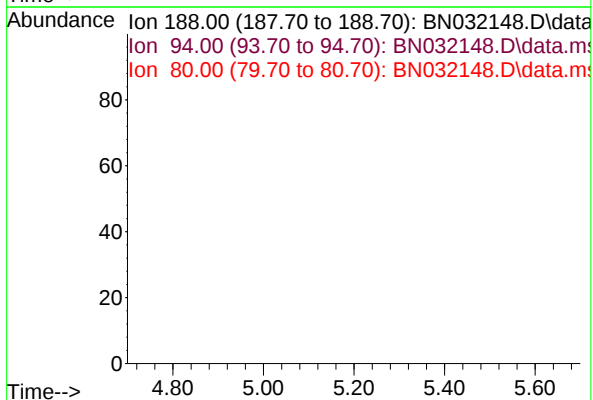


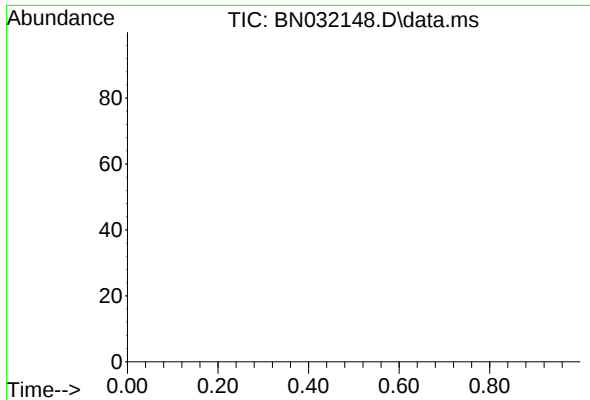

#27
 Fluoranthene-d10
 Concen: 0.000 ng
 Expected RT: 19.07 min
 Lab File: BN032148.D
 Acq: 22 Jun 2024 01:57


Instrument :
 BNA_N
 ClientSampleId :
 PB161510BS


Tgt Ion: 212
 Sig Exp Ratio
 212 100
 106 14.8
 104 8.3

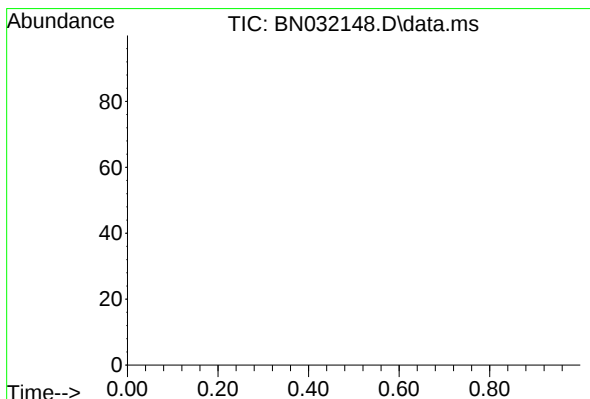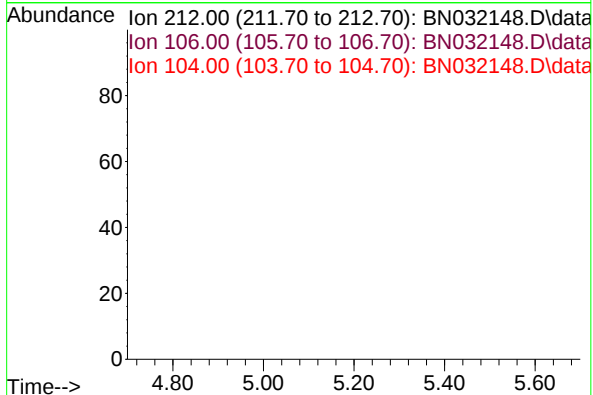

#29
 Chrysene-d12
 Concen: 0.000 ng
 Expected RT: 21.23 min
 Lab File: BN032148.D
 Acq: 22 Jun 2024 01:57

Tgt Ion: 240
 Sig Exp Ratio
 240 100
 120 10.3
 236 27.3

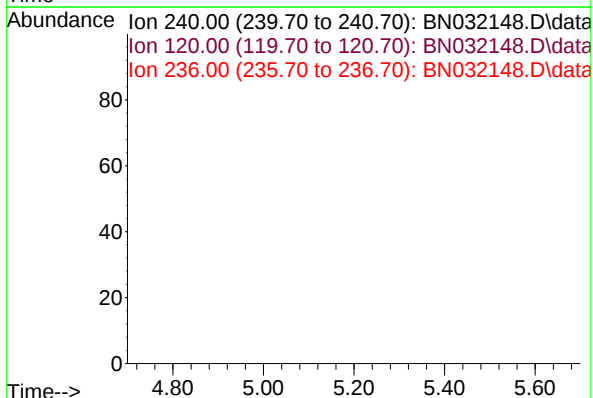


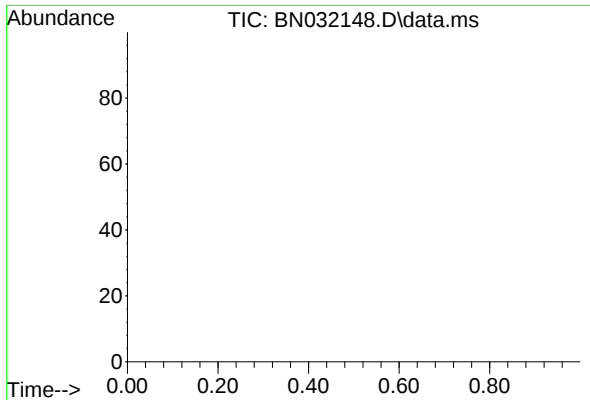


#31
Terphenyl-d14
Concen: 0.000 ng
Expected RT: 19.67 min

Lab File: BN032148.D
Acq: 22 Jun 2024 01:57

Instrument :
BNA_N
ClientSampleId :
PB161510BS

Tgt Ion: 244
Sig Exp Ratio
244 100
212 8.1
122 14.2

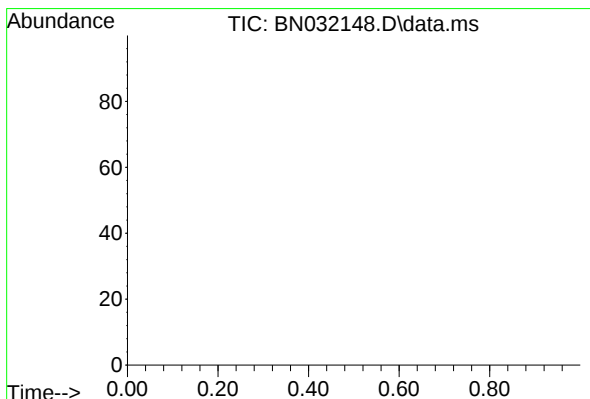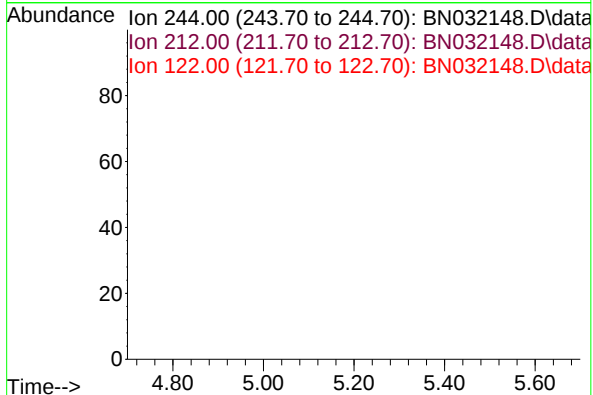

#35
Perylene-d12
Concen: 0.000 ng
Expected RT: 23.45 min

Lab File: BN032148.D
Acq: 22 Jun 2024 01:57

Tgt Ion: 264
Sig Exp Ratio
264 100
260 25.6
265 49.5

