
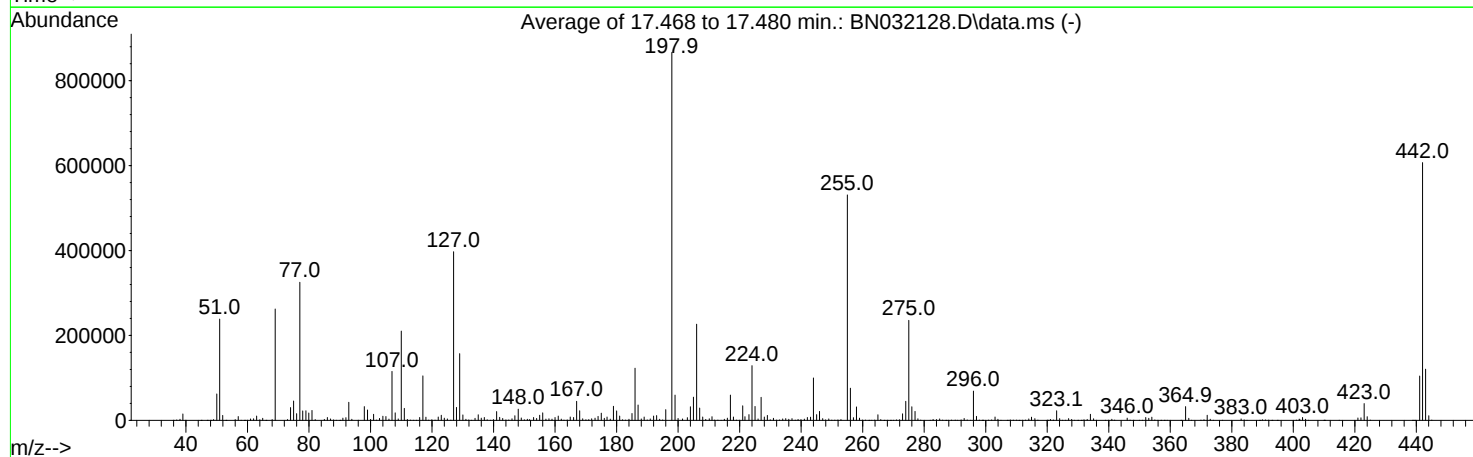


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062124\
Data File : BN032128.D
Acq On : 21 Jun 2024 12:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN061024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 19 11:30:34 2024

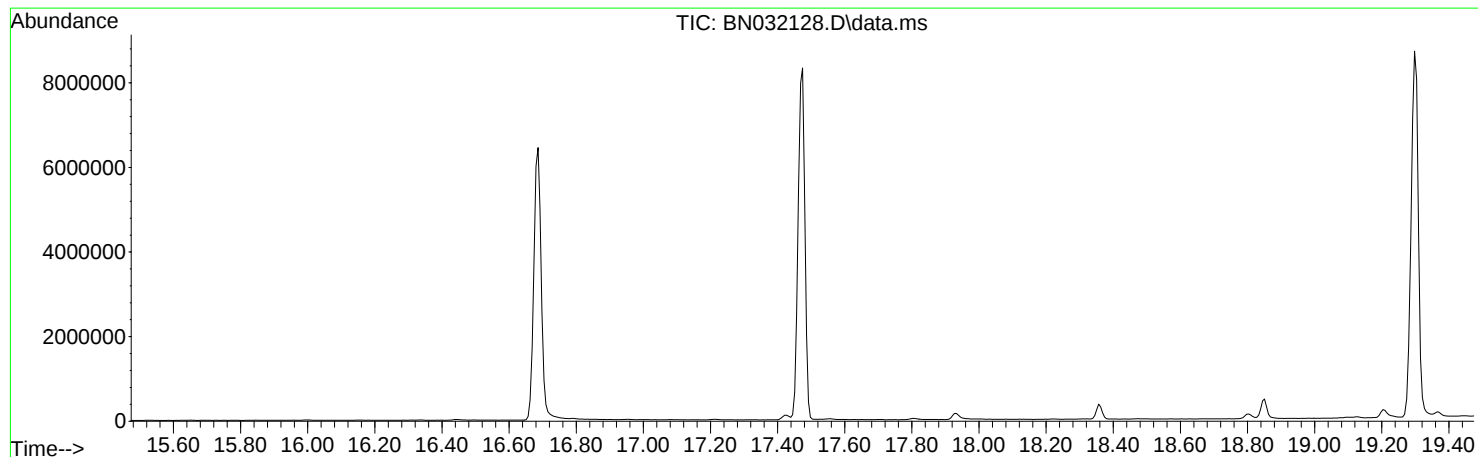

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.5	238385	PASS
68	69	0.00	2	0.7	1737	PASS
69	198	0.00	100	30.3	262338	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.9	397355	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	866368	PASS
199	198	5	9	6.9	59416	PASS
275	198	10	60	27.2	235605	PASS
365	198	1	100	3.7	32365	PASS
441	198	0.01	100	12.0	104245	PASS
442	442	50	100	100.0	606997	PASS
443	442	15	24	19.9	120592	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/21/2024	BNA_N	<u>BN032128.D</u>
Compound Name	Response	Retention Time
DDT	2259917	20.527
DDD	469287	20.086
DDE	3700	19.574
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
472987	2732904	17.31

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062124\
Data File : BN032128.D
Acq On : 21 Jun 2024 12:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 21 13:37:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

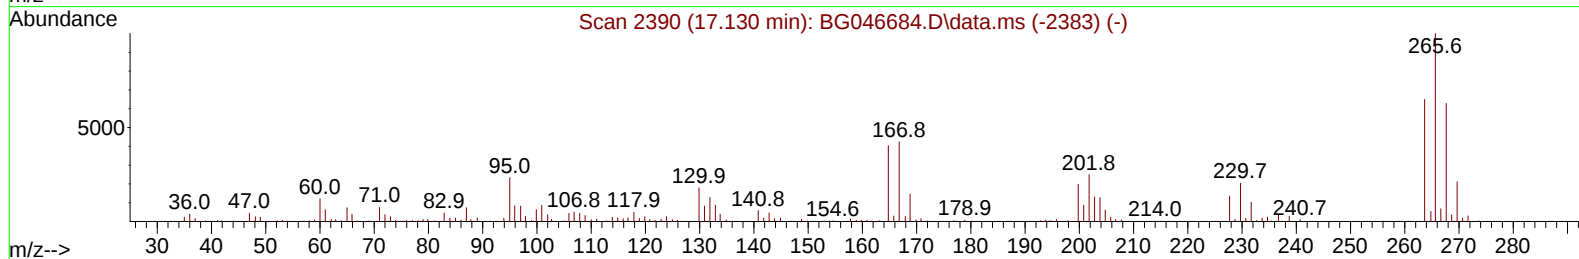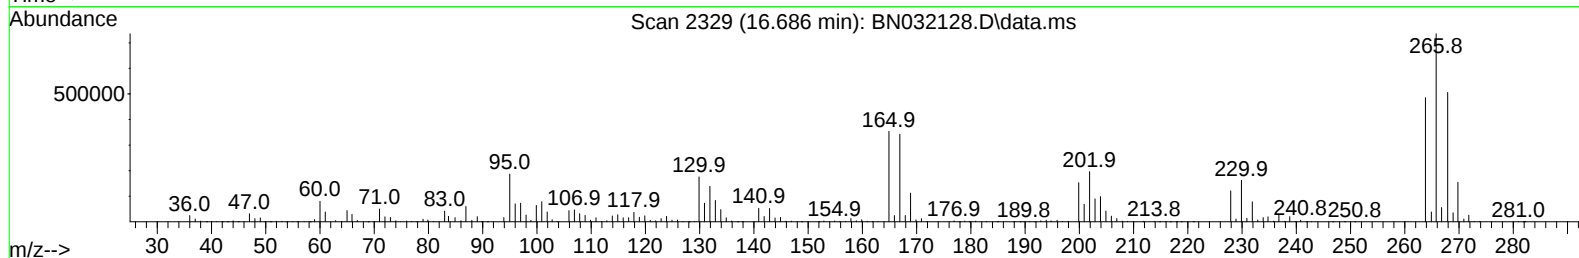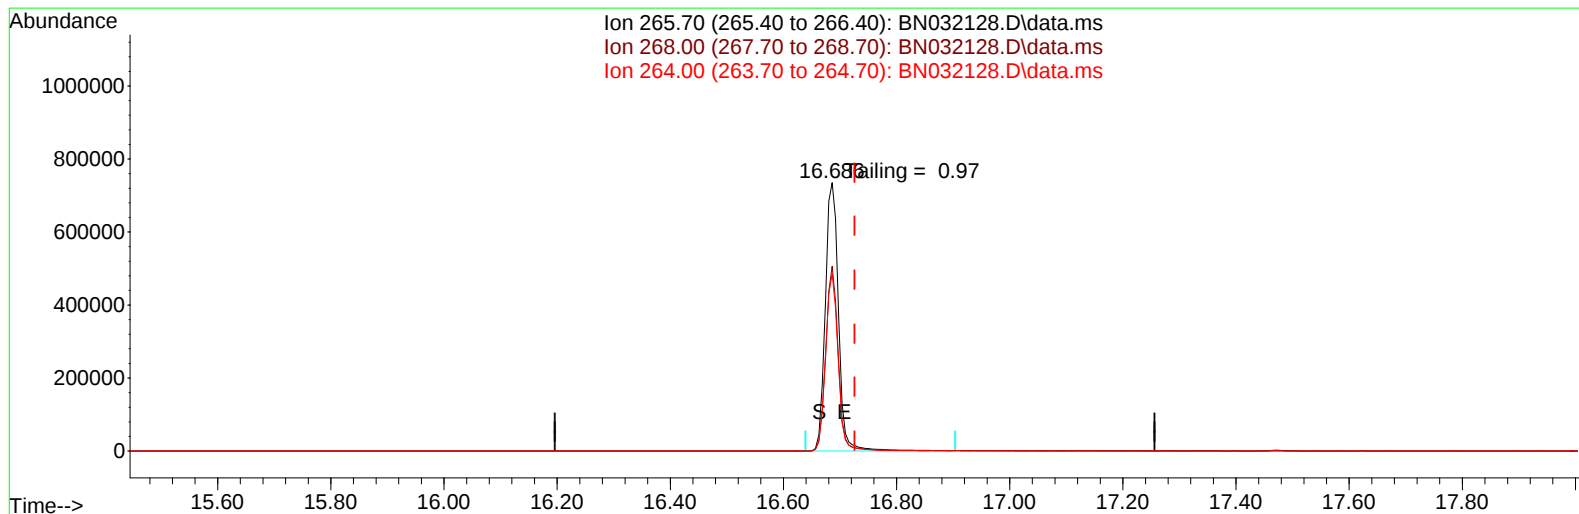

TIC: BN032128.D\data.ms

(70) Pentachlorophenol (C)

16.686min (-0.040) 25982.85 ng




response 1195506

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.82
264.00	61.60	66.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062124\
Data File : BN032128.D
Acq On : 21 Jun 2024 12:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 21 13:37:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

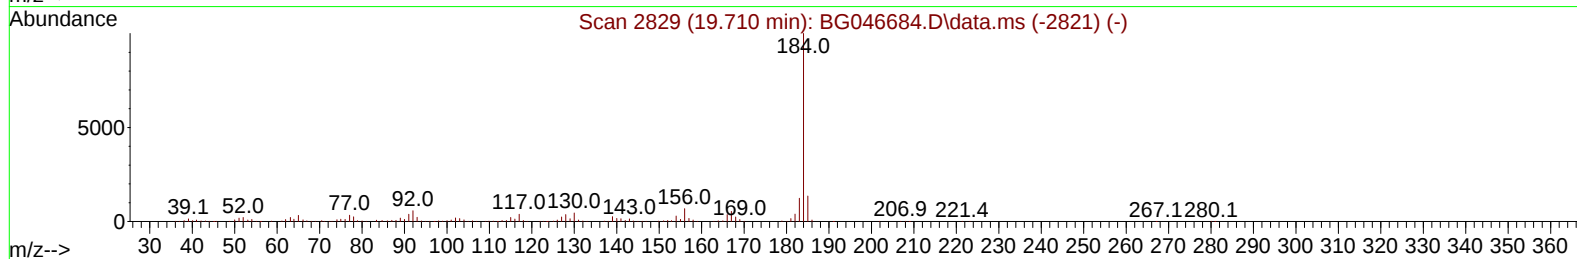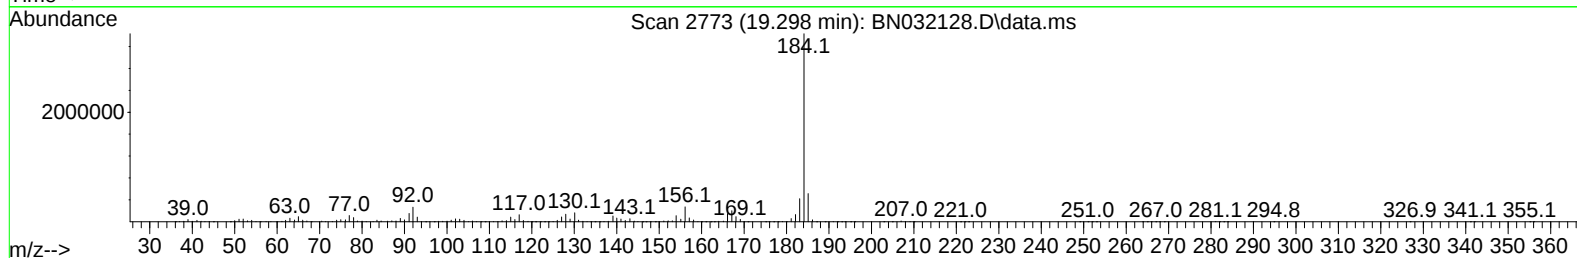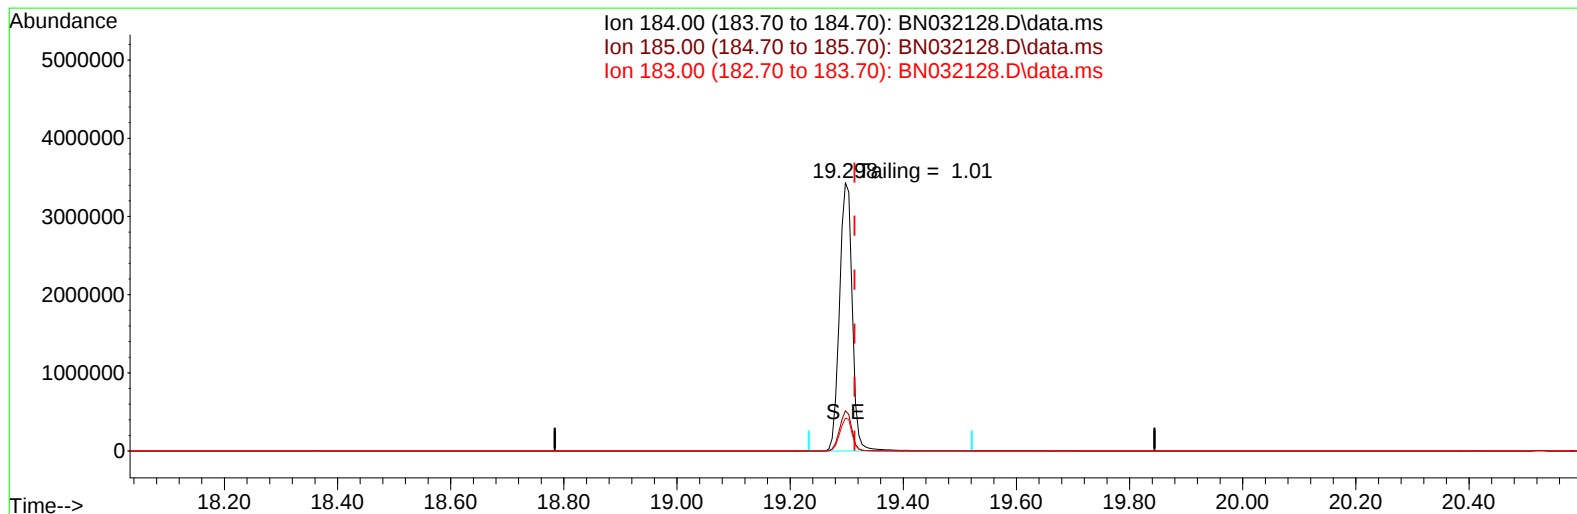

TIC: BN032128.D\data.ms

(77) Benzidine**19.298min (-0.016) 1367725.80 ng****response 5396564**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.01
183.00	13.20	12.28
0.00	0.00	0.00