


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062124\
Data File : BN032145.D
Acq On : 22 Jun 2024 00:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN061024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 19 11:30:34 2024

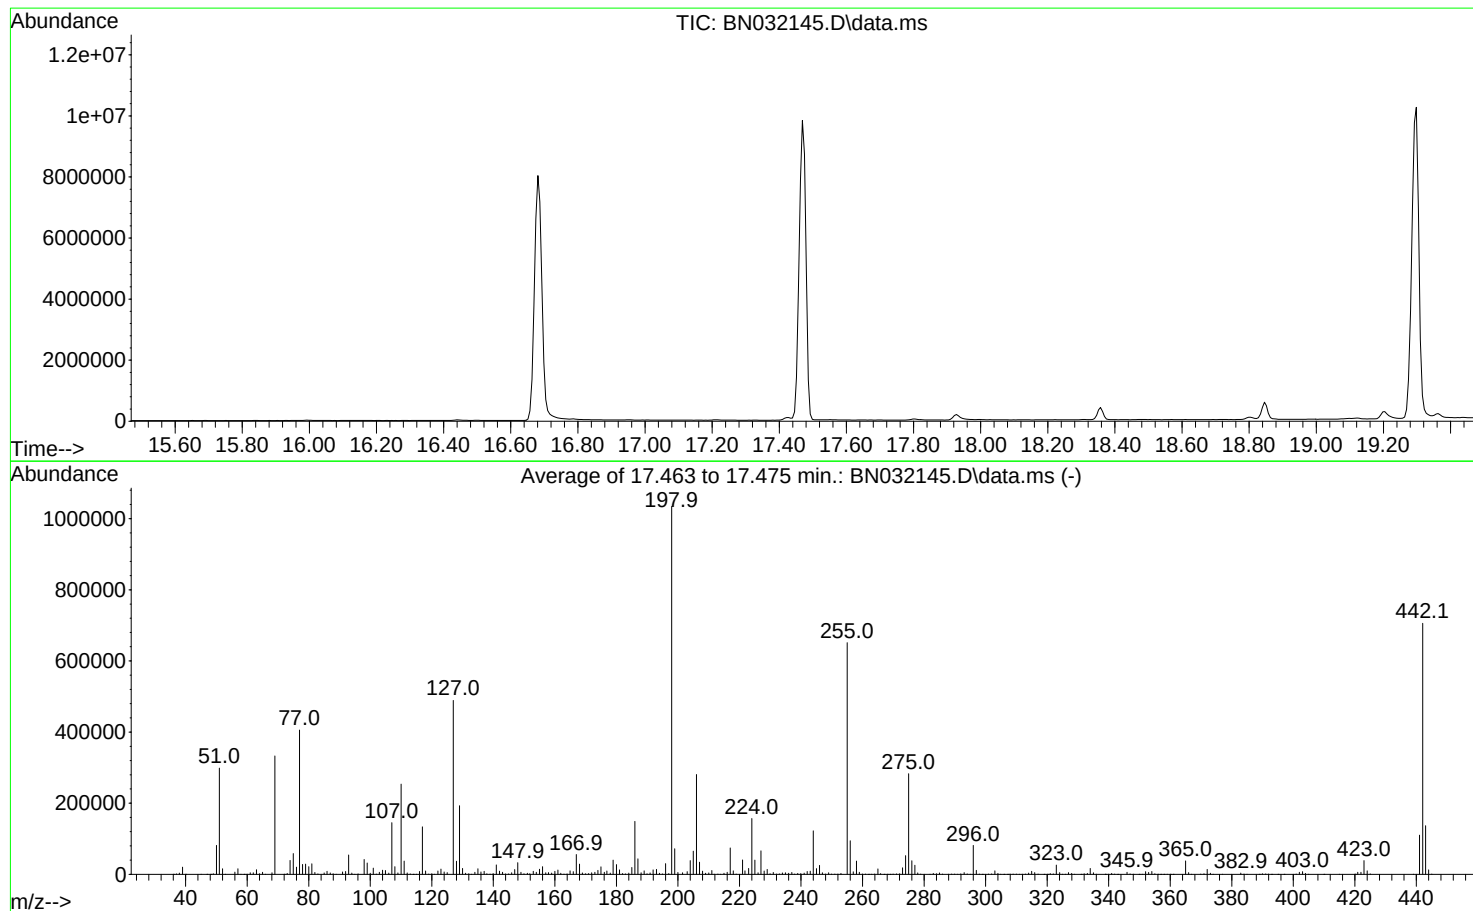

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.9	298628	PASS
68	69	0.00	2	1.4	4645	PASS
69	198	0.00	100	32.2	332672	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.3	489152	PASS
197	198	0.00	2	0.2	2280	PASS
198	198	100	100	100.0	1034197	PASS
199	198	5	9	7.0	71939	PASS
275	198	10	60	27.4	283072	PASS
365	198	1	100	3.7	38075	PASS
441	198	0.01	100	10.7	110197	PASS
442	442	50	100	100.0	705835	PASS
443	442	15	24	19.4	136891	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/21/2024	BNA_N	<u>BN032145.D</u>
Compound Name	Response	Retention Time
DDT	3190825	20.522
DDD	241816	20.081
DDE	5758	19.569
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
247574	3438399	7.20

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062124\
Data File : BN032145.D
Acq On : 22 Jun 2024 00:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 22 01:23:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

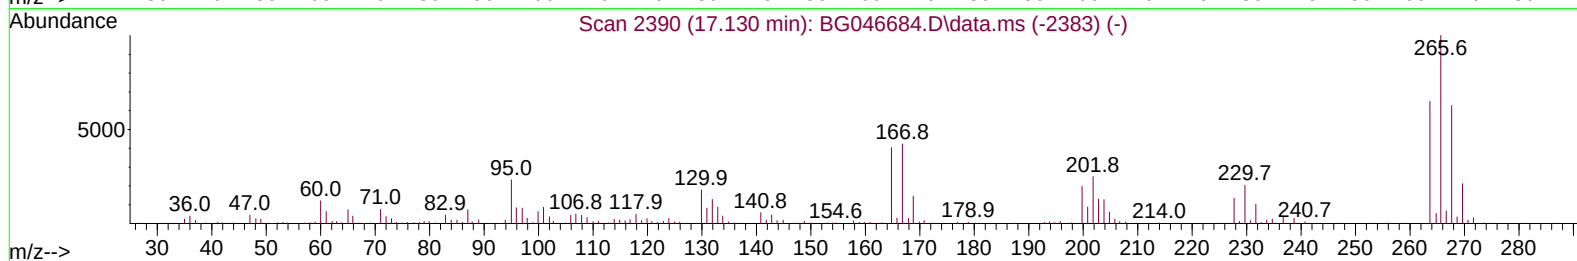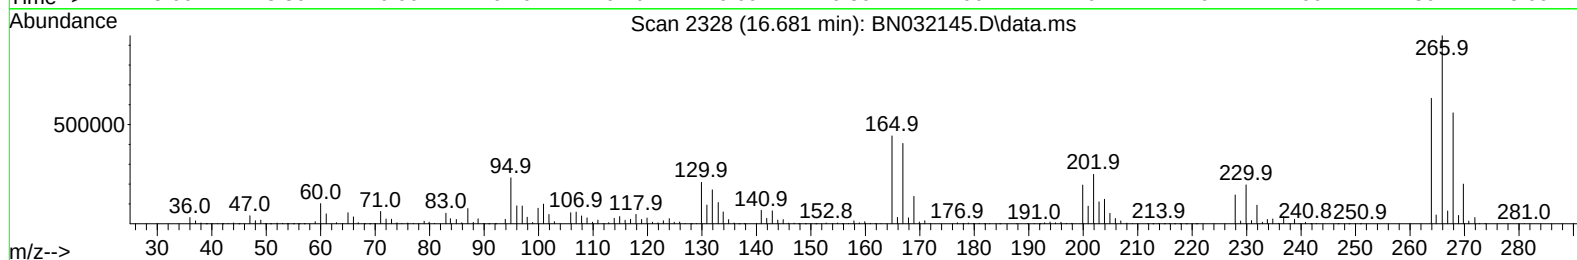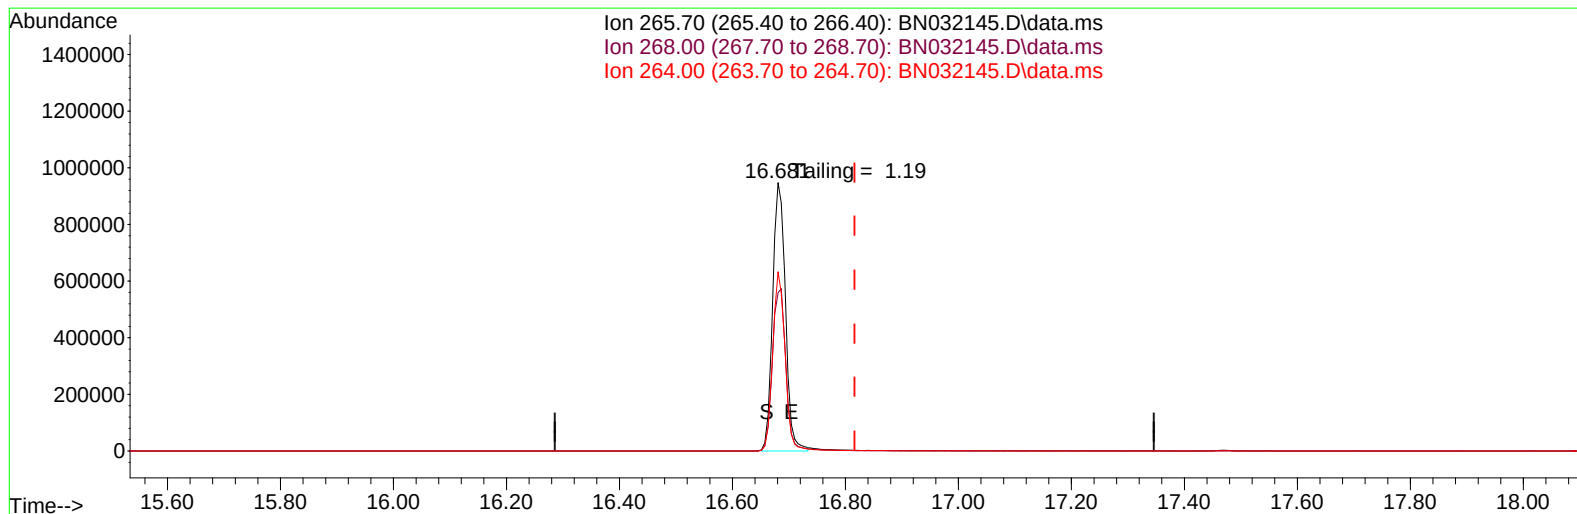

TIC: BN032145.D\data.ms

(70) Pentachlorophenol (C)

16.681min (-0.135) 27633.01 ng




response 1521902

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.98
264.00	61.60	66.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062124\
Data File : BN032145.D
Acq On : 22 Jun 2024 00:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 22 01:23:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 01:44:29 2024
Response via : Initial Calibration

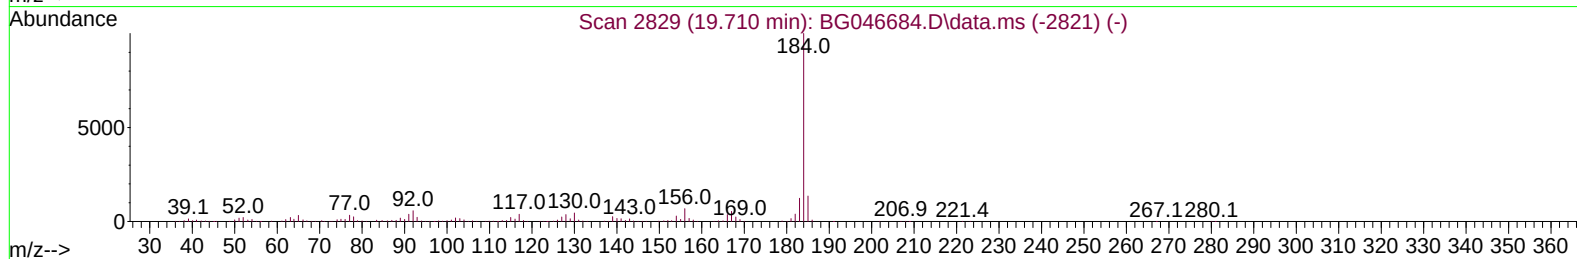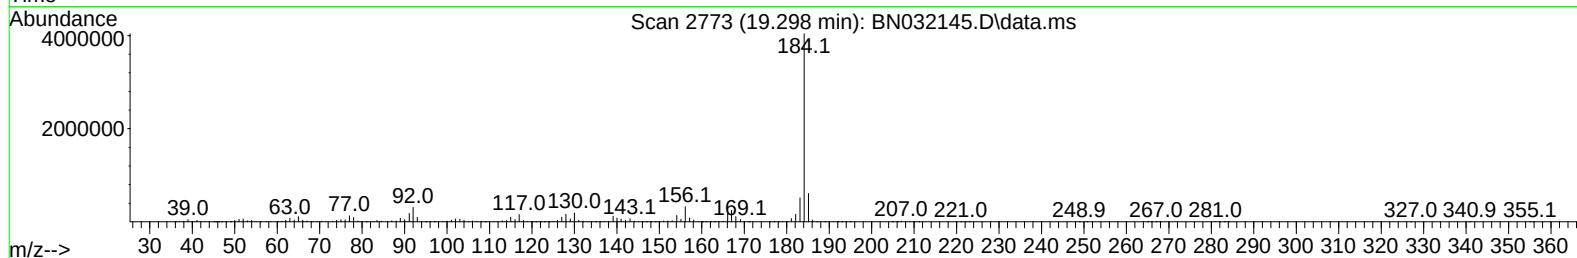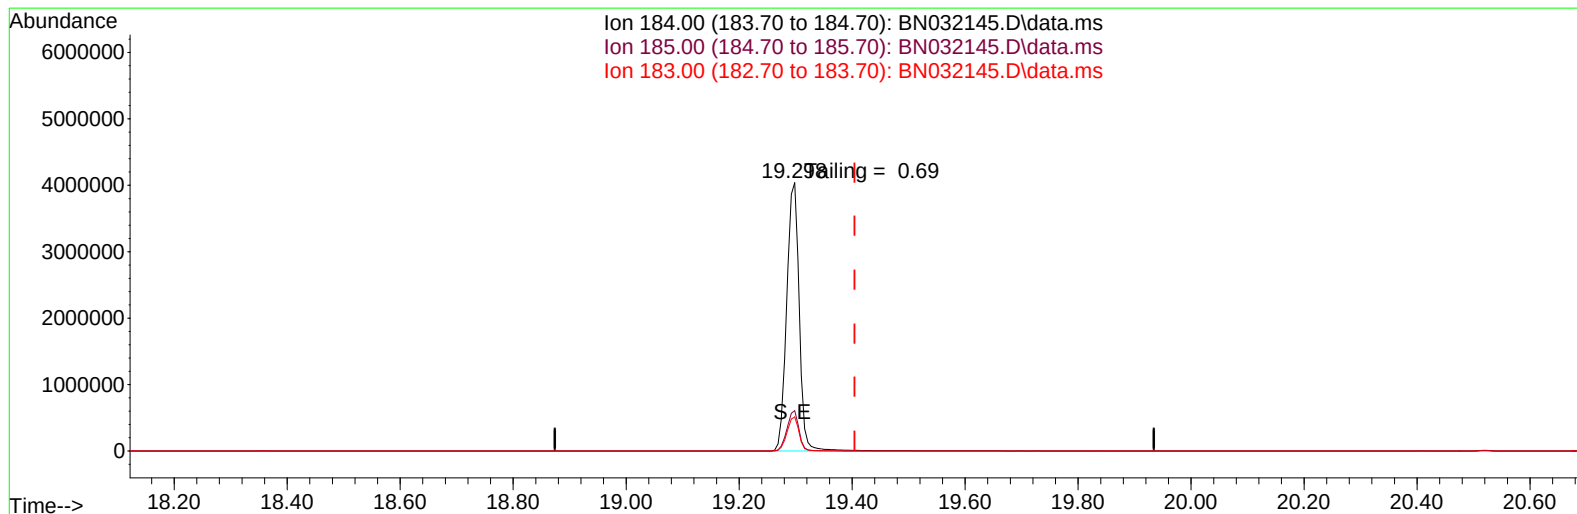

TIC: BN032145.D\data.ms

(77) Benzidine

19.298min (-0.106) 0.00 ng

response 6231428

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.04
183.00	13.20	12.72
0.00	0.00	0.00