
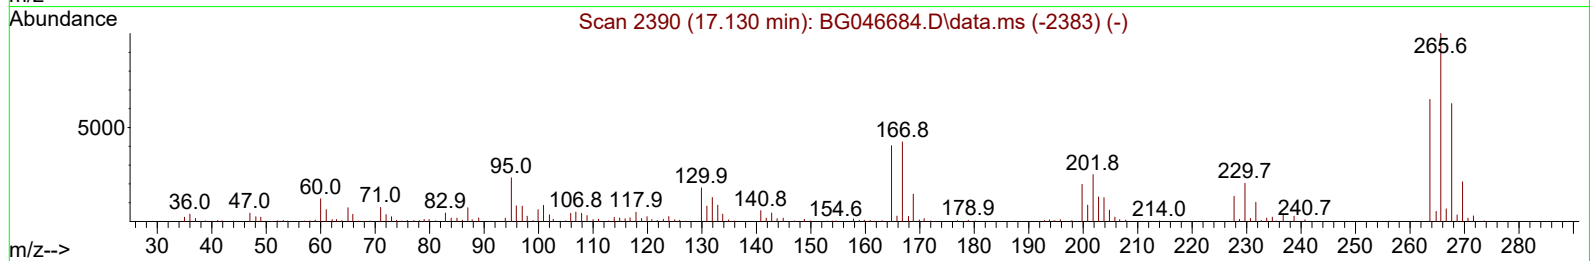
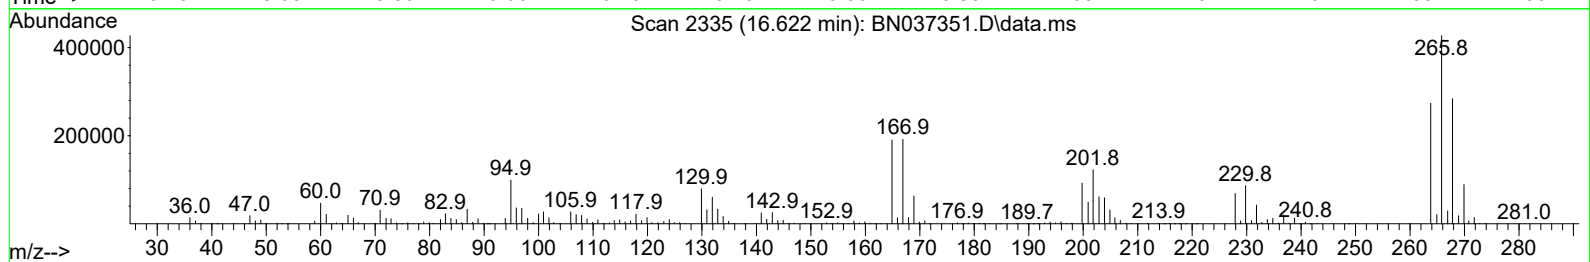


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062125\
Data File : BN037351.D
Acq On : 20 Jun 2025 15:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 21 02:21:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 21 02:21:08 2025
Response via : Initial Calibration

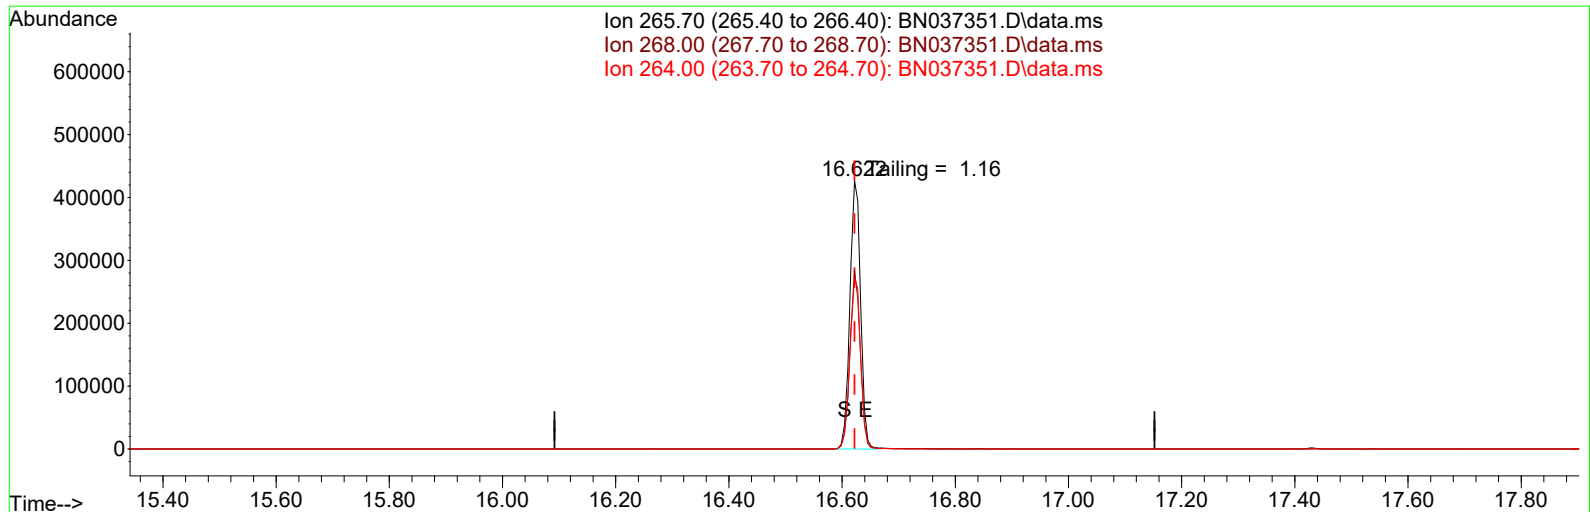

TIC: BN037351.D\data.ms

(70) Pentachlorophenol (C)




16.622min (0.000) 21508.69 ng

response 561749

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.53
264.00	61.60	64.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062125\
Data File : BN037351.D
Acq On : 20 Jun 2025 15:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 21 02:21:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 21 02:21:08 2025
Response via : Initial Calibration

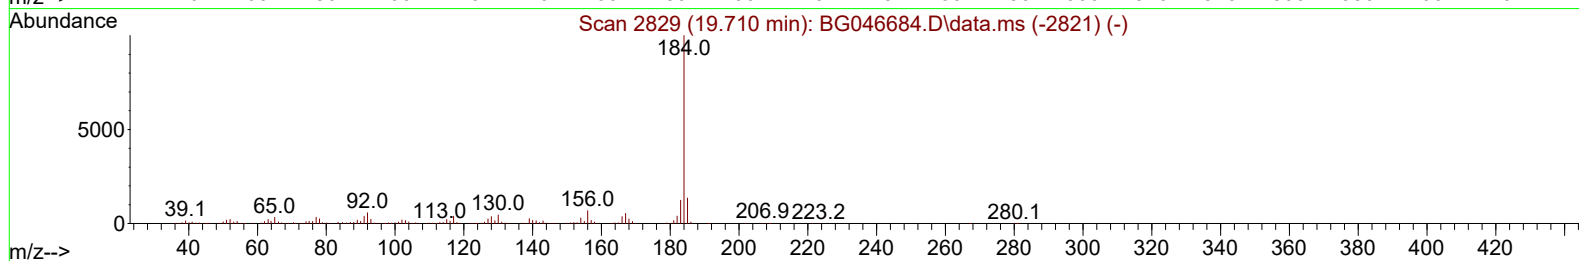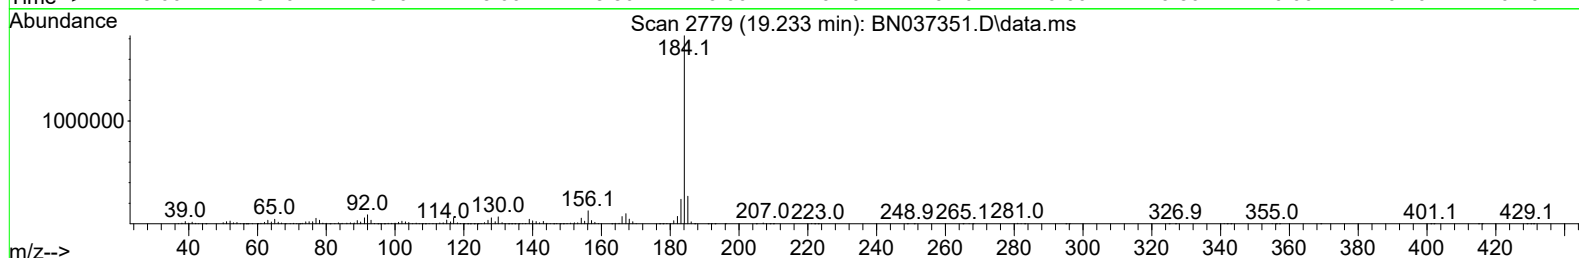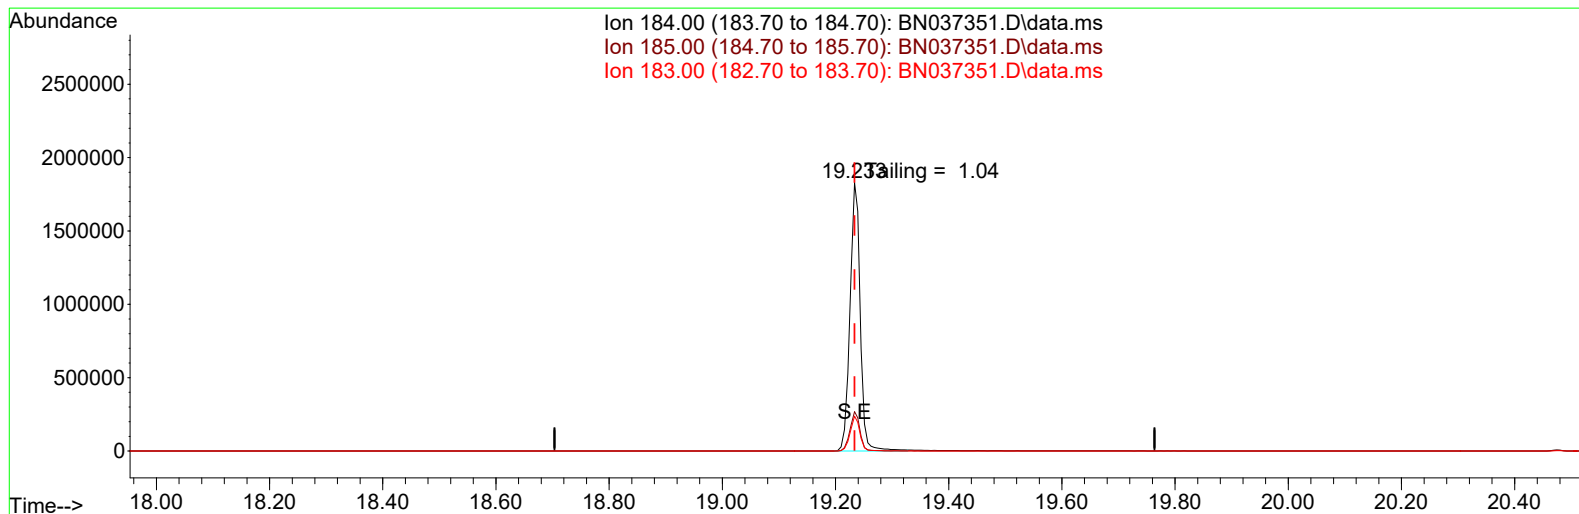

TIC: BN037351.D\data.ms

(77) Benzidine

19.233min (0.000) 0.00 ng

response 2309913

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.66
183.00	13.20	13.00
0.00	0.00	0.00