
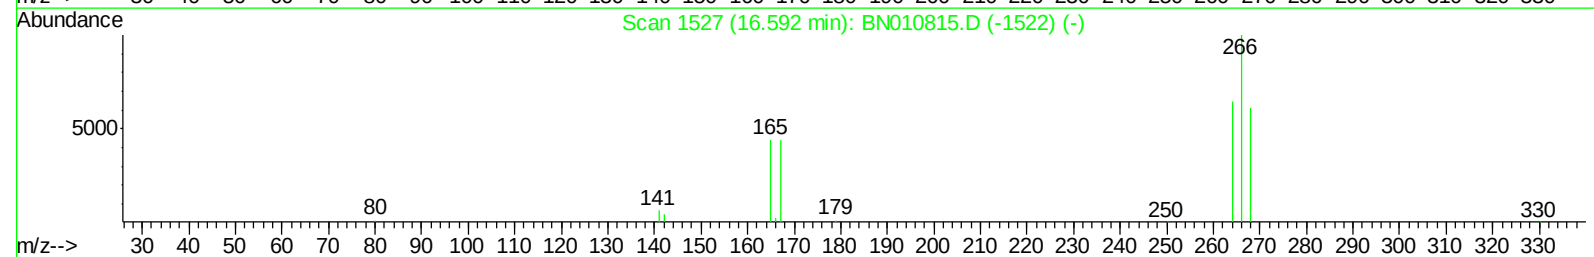
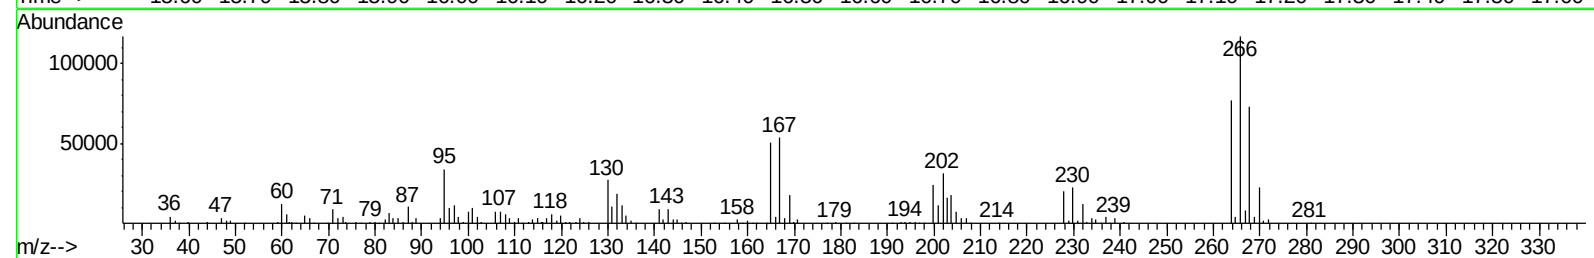


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN062220\  
 Data File : BN011019.D  
 Acq On : 23 Jun 2020 02:09  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 06:42:51 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN061020.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Jun 22 12:02:11 2020  
 Response via : Initial Calibration

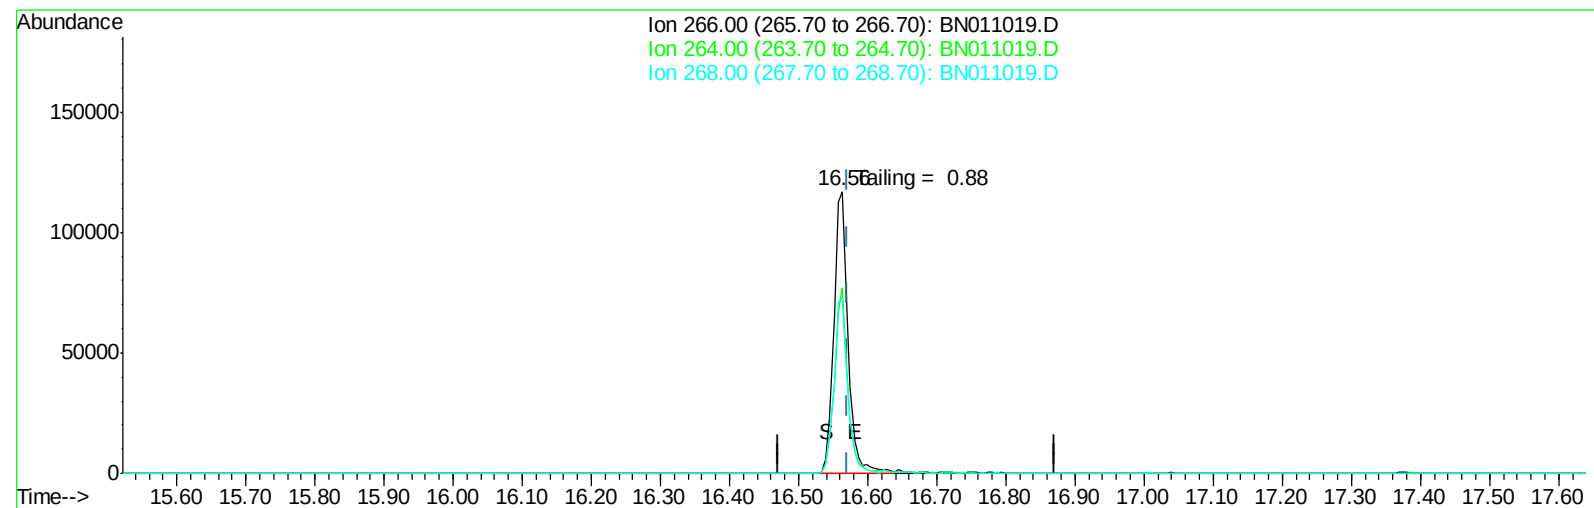

TIC: BN011019.D

(22) Pentachlorophenol

16.563min (-0.008) 0.00ng

response 167593

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 266.00 | 100   | 100   |
| 264.00 | 68.50 | 65.73 |
| 268.00 | 69.90 | 62.21 |
| 0.00   | 0.00  | 0.00  |