


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062220\
 Data File : BN011001.D
 Acq On : 22 Jun 2020 10:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN061020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 22 12:02:11 2020

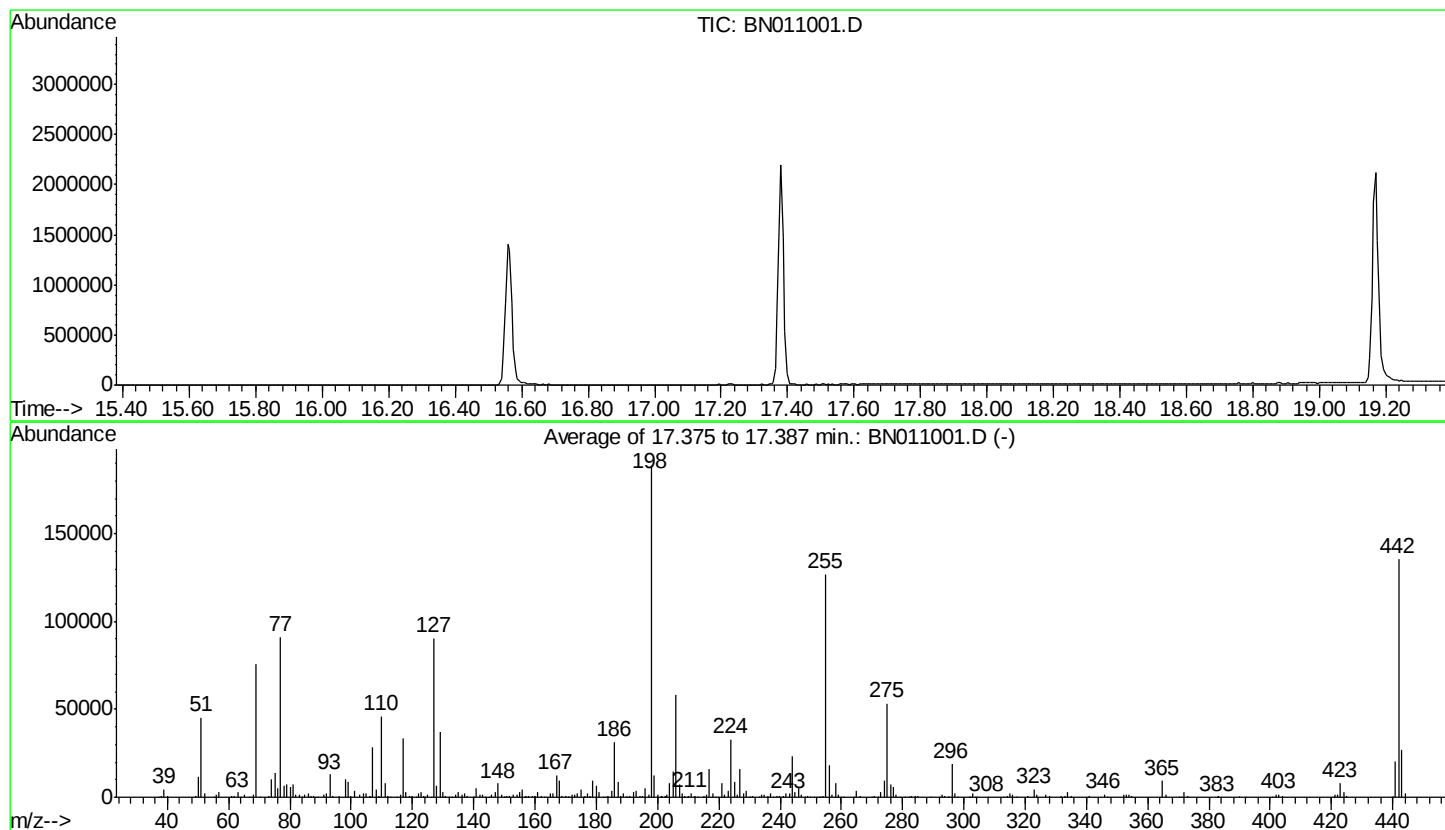

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.0	45304	PASS
68	69	0.00	2	2.0	1553	PASS
69	198	0.00	100	40.2	75888	PASS
70	69	0.00	2	0.4	338	PASS
127	198	10	80	48.0	90528	PASS
197	198	0.00	2	0.9	1720	PASS
198	198	100	100	100.0	188650	PASS
199	198	5	9	6.8	12745	PASS
275	198	10	60	28.3	53400	PASS
365	198	1	100	4.9	9306	PASS
441	198	0.01	100	10.7	20225	PASS
442	198	50	100	72.0	135800	PASS
443	442	15	24	19.9	27061	PASS