


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_N\DATA\BN062220\  
 Data File : BN011019.D  
 Acq On : 23 Jun 2020 02:09  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-SIM-BN061020.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Jun 22 12:02:11 2020

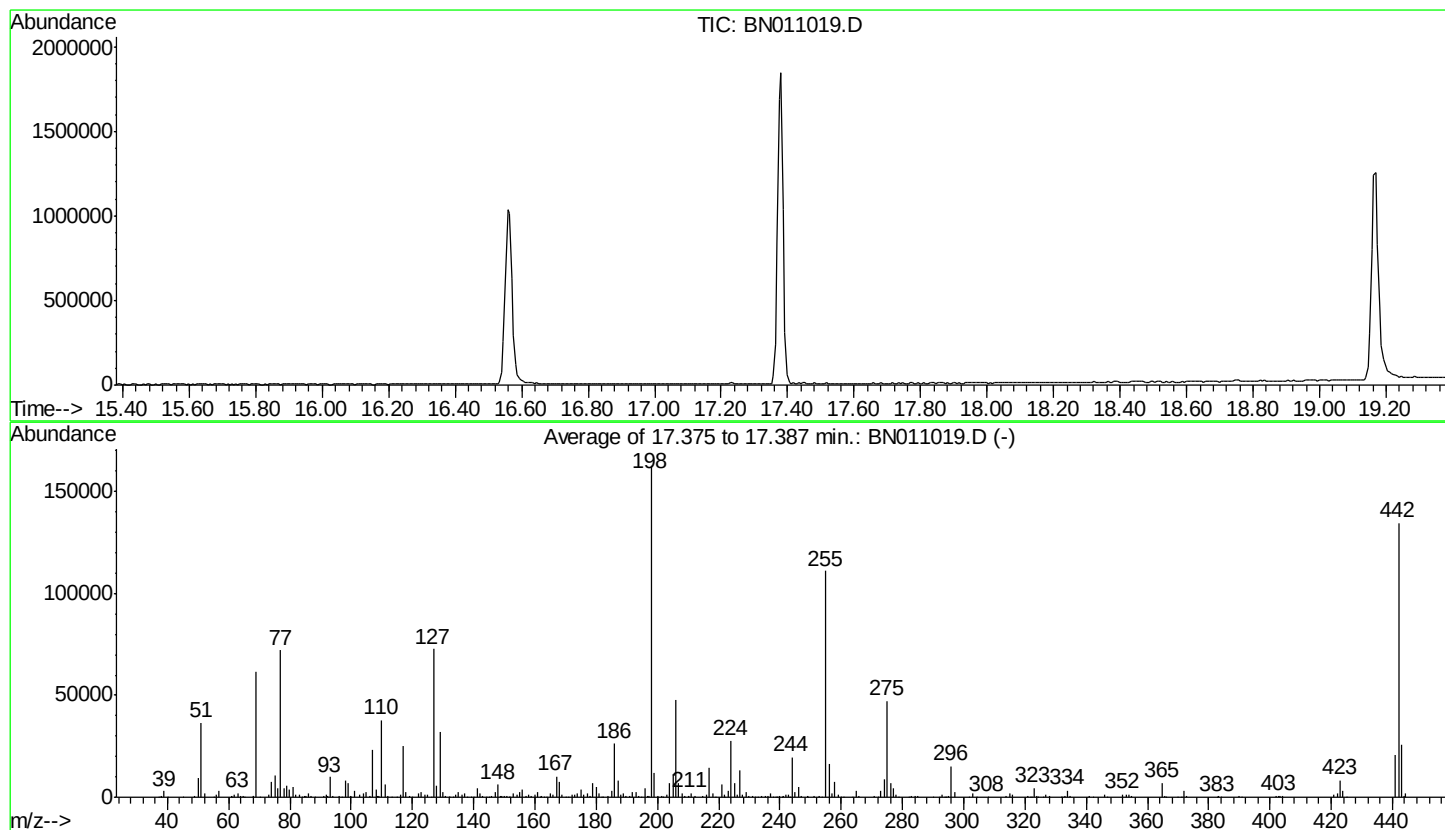

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 22.5      | 36656   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.2       | 765     | PASS             |
| 69          | 198          | 0.00         | 100          | 38.0      | 61797   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.5       | 303     | PASS             |
| 127         | 198          | 10           | 80           | 44.7      | 72776   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.5       | 847     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 162746  | PASS             |
| 199         | 198          | 5            | 9            | 7.2       | 11687   | PASS             |
| 275         | 198          | 10           | 60           | 29.0      | 47202   | PASS             |
| 365         | 198          | 1            | 100          | 4.4       | 7093    | PASS             |
| 441         | 198          | 0.01         | 100          | 12.9      | 20914   | PASS             |
| 442         | 198          | 50           | 100          | 82.8      | 134762  | PASS             |
| 443         | 442          | 15           | 24           | 19.0      | 25642   | PASS             |