

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BN032170.D
 Acq On : 22 Jun 2024 17:14
 Operator : MA/JU
 Sample : P2899-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA7

Quant Time: Jun 22 23:42:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 10:49:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	372899	20.000	ng/ul	0.00
20) Naphthalene-d8	10.410	136	1553237	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.275	164	938415	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.027	188	1669633	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.262	240	1208950	20.000	ng/ul	0.00
88) Perylene-d12	24.174	264	1395964	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.163	96	25308	2.808	ng/uL	0.00
4) Pyridine-d5	3.581	84	24716	0.974	ng/ul	0.01
7) Phenol-d5	6.810	99	527231	16.492	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	293340	15.688	ng/ul	0.00
11) 2-Chlorophenol-d4	7.163	132	464530	19.044	ng/ul	0.00
15) 4-Methylphenol-d8	8.340	113	417374	16.017	ng/ul	0.00
21) Nitrobenzene-d5	8.787	128	225216	18.964	ng/ul	0.00
24) 2-Nitrophenol-d4	9.504	143	241928	19.721	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.040	165	443045	19.345	ng/ul	0.00
31) 4-Chloroaniline-d4	10.563	131	53106	1.562	ng/ul	0.00
46) Dimethylphthalate-d6	13.692	166	1346806	20.601	ng/ul	0.00
49) Acenaphthylene-d8	13.969	160	1505491	20.027	ng/ul	0.00
54) 4-Nitrophenol-d4	14.504	143	183934	14.052	ng/ul	0.00
60) Fluorene-d10	15.275	176	1110006	20.067	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.410	200	146224	17.423	ng/ul	0.00
73) Anthracene-d10	17.121	188	1519772	21.261	ng/ul	0.00
81) Pyrene-d10	19.427	212	1377727	21.296	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.968	264	964758	14.473	ng/ul	-0.01
Target Compounds						
					Qvalue	
10) Bis(2-Chloroethyl)ether	7.063	93	48289	1.795	ng/ul#	26
16) Acetophenone	8.451	105	60287	1.527	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032170.D
Acq On : 22 Jun 2024 17:14
Operator : MA/JU
Sample : P2899-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AA7

Quant Time: Jun 22 23:42:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 10:49:40 2024
Response via : Initial Calibration

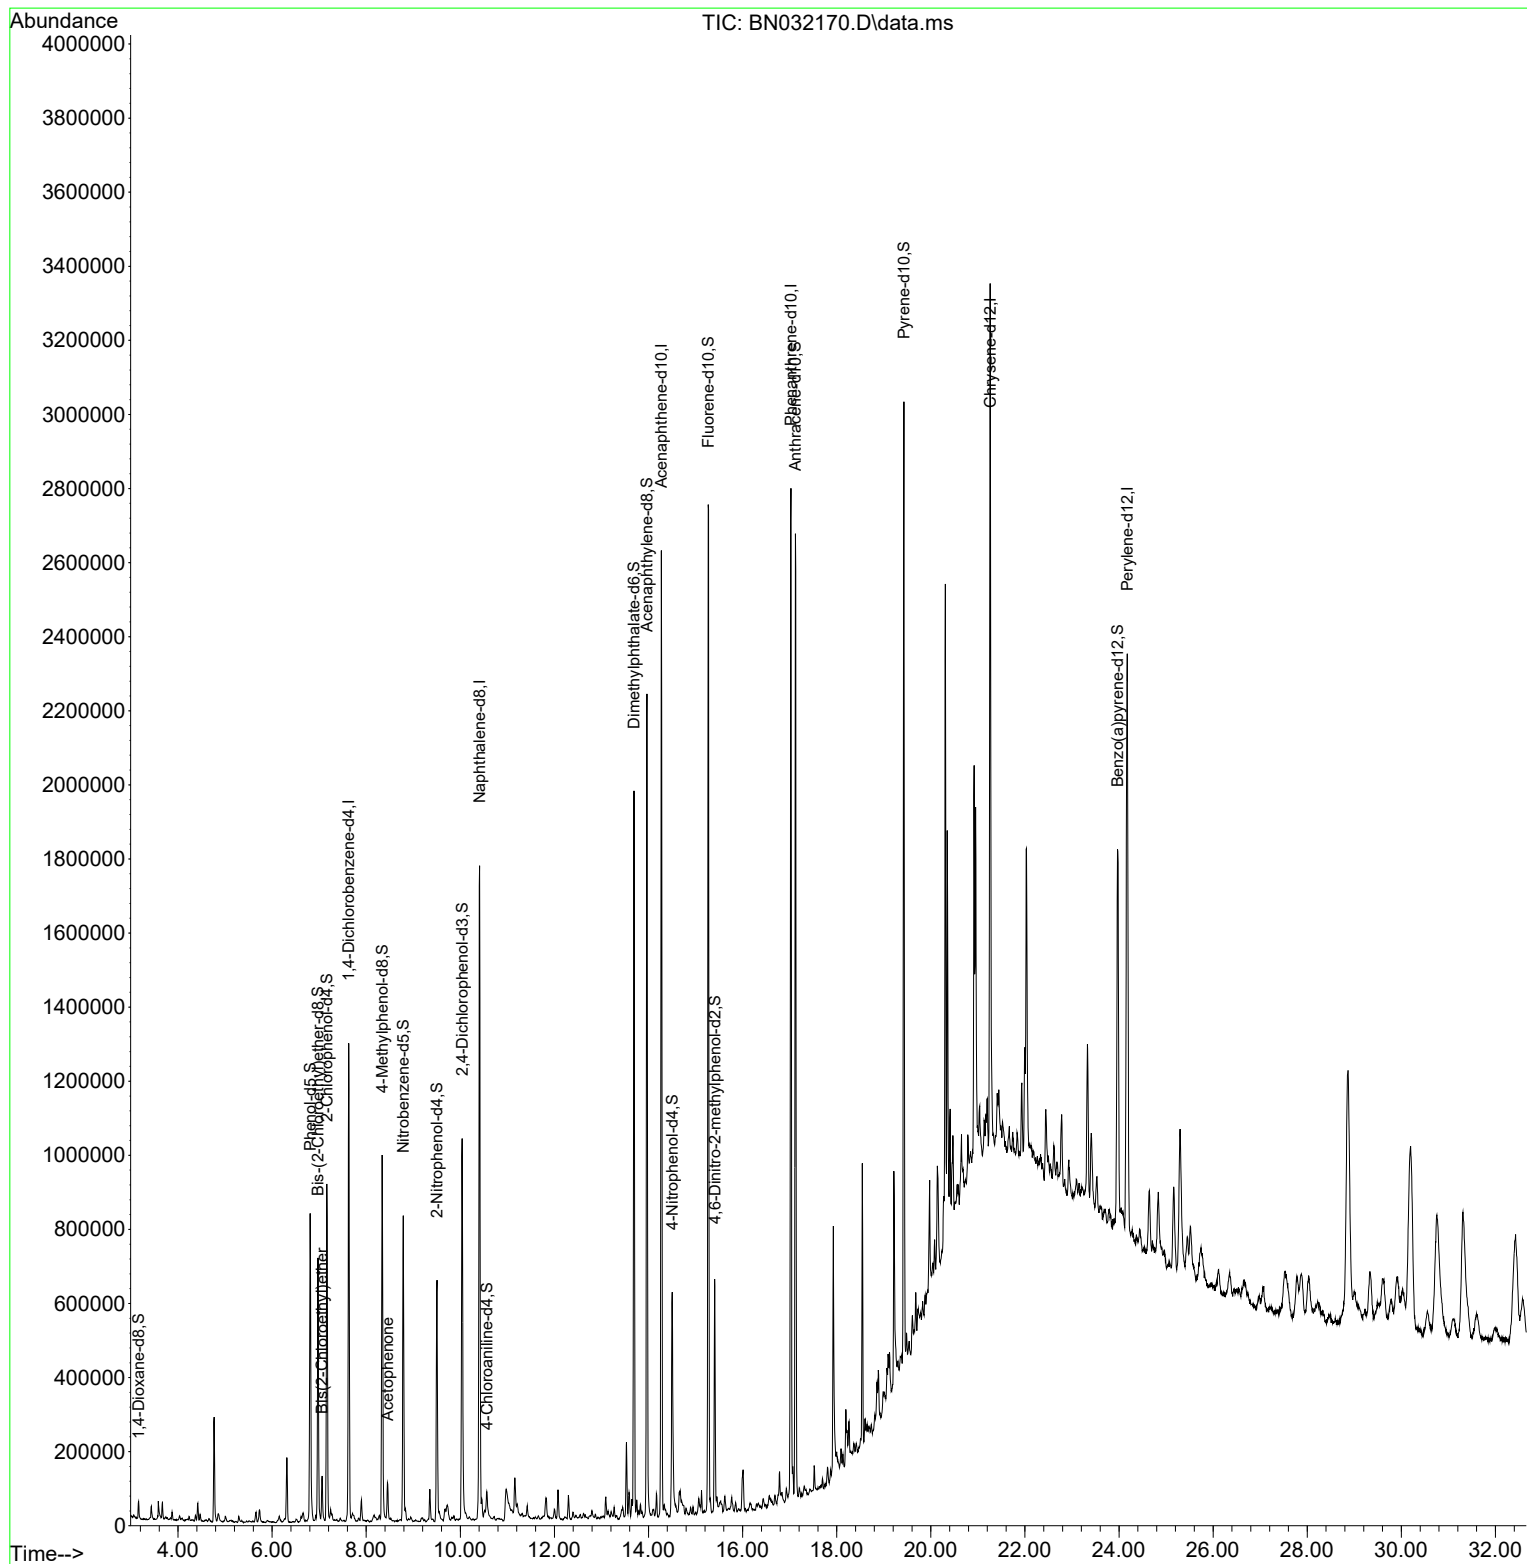

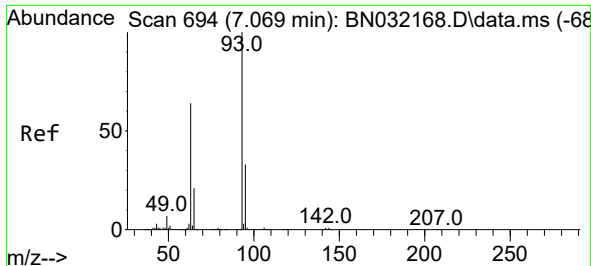

#10

Bis(2-Chloroethyl)ether

Concen: 1.795 ng/ul

RT: 7.063 min Scan# 694

Delta R.T. -0.012 min

Lab File: BN032170.D

Acq: 22 Jun 2024 17:14

Instrument :

BNA_N

ClientSampleId :

C0AA7





Tgt Ion: 93 Resp: 48289

Ion Ratio Lower Upper

93 100

63 2.0 56.8 85.2#

95 2.4 26.0 39.0#

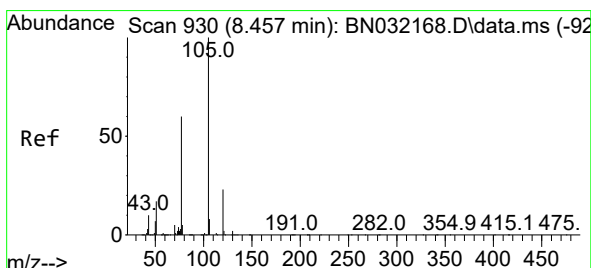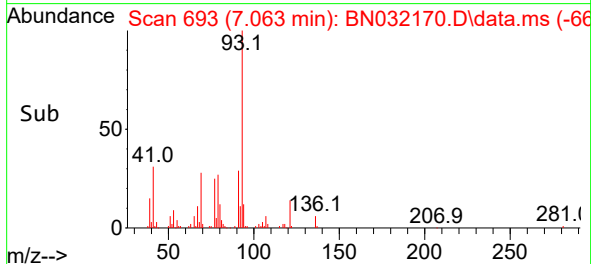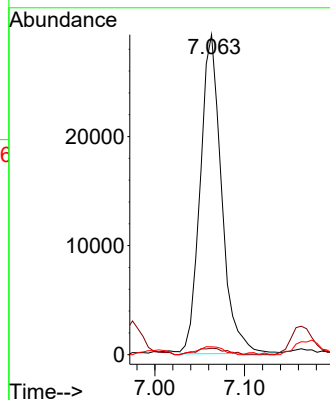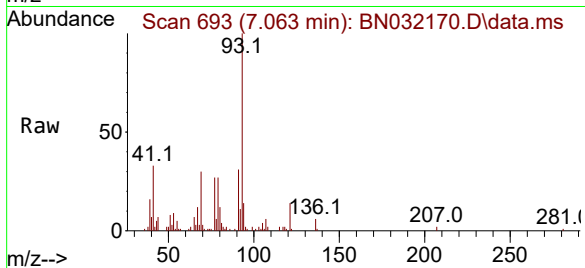

#16

Acetophenone

Concen: 1.527 ng/ul

RT: 8.451 min Scan# 929

Delta R.T. -0.012 min

Lab File: BN032170.D

Acq: 22 Jun 2024 17:14

Tgt Ion:105 Resp: 60287

Ion Ratio Lower Upper

105 100

77 71.0 58.6 87.8

51 22.1 17.2 25.8

