

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BN032177.D
 Acq On : 22 Jun 2024 21:50
 Operator : MA/JU
 Sample : P2899-18
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB9

Quant Time: Jun 22 23:43:43 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 10:49:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	322482	20.000	ng/ul	0.00
20) Naphthalene-d8	10.416	136	1254534	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.280	164	759397	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.027	188	1459159	20.000	ng/ul	0.00
79) Chrysene-d12	21.268	240	1264643	20.000	ng/ul	0.00
88) Perylene-d12	24.186	264	1488257	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.163	96	33960	4.357	ng/uL	0.00
4) Pyridine-d5	3.581	84	56310	2.566	ng/ul	0.01
7) Phenol-d5	6.816	99	657661	23.789	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	365096	22.578	ng/ul	0.00
11) 2-Chlorophenol-d4	7.169	132	596545	28.280	ng/ul	0.00
15) 4-Methylphenol-d8	8.345	113	461638	20.485	ng/ul	0.00
21) Nitrobenzene-d5	8.792	128	295852	30.843	ng/ul	0.00
24) 2-Nitrophenol-d4	9.504	143	325475	32.848	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.045	165	548579	29.656	ng/ul	0.00
31) 4-Chloroaniline-d4	10.563	131	132988	4.842	ng/ul	0.00
46) Dimethylphthalate-d6	13.698	166	1569697	29.671	ng/ul	0.00
49) Acenaphthylene-d8	13.969	160	1843510	30.305	ng/ul	0.00
54) 4-Nitrophenol-d4	14.516	143	269851	25.475	ng/ul	0.01
60) Fluorene-d10	15.274	176	1341497	29.969	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.416	200	192364	26.228	ng/ul	0.00
73) Anthracene-d10	17.127	188	1985640	31.785	ng/ul	0.00
81) Pyrene-d10	19.427	212	1877728	27.747	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.992	264	1511154	21.265	ng/ul	0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.457	105	119466	3.498	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.174	149	100172	1.753	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032177.D
Acq On : 22 Jun 2024 21:50
Operator : MA/JU
Sample : P2899-18
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB9

Quant Time: Jun 22 23:43:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 10:49:40 2024
Response via : Initial Calibration




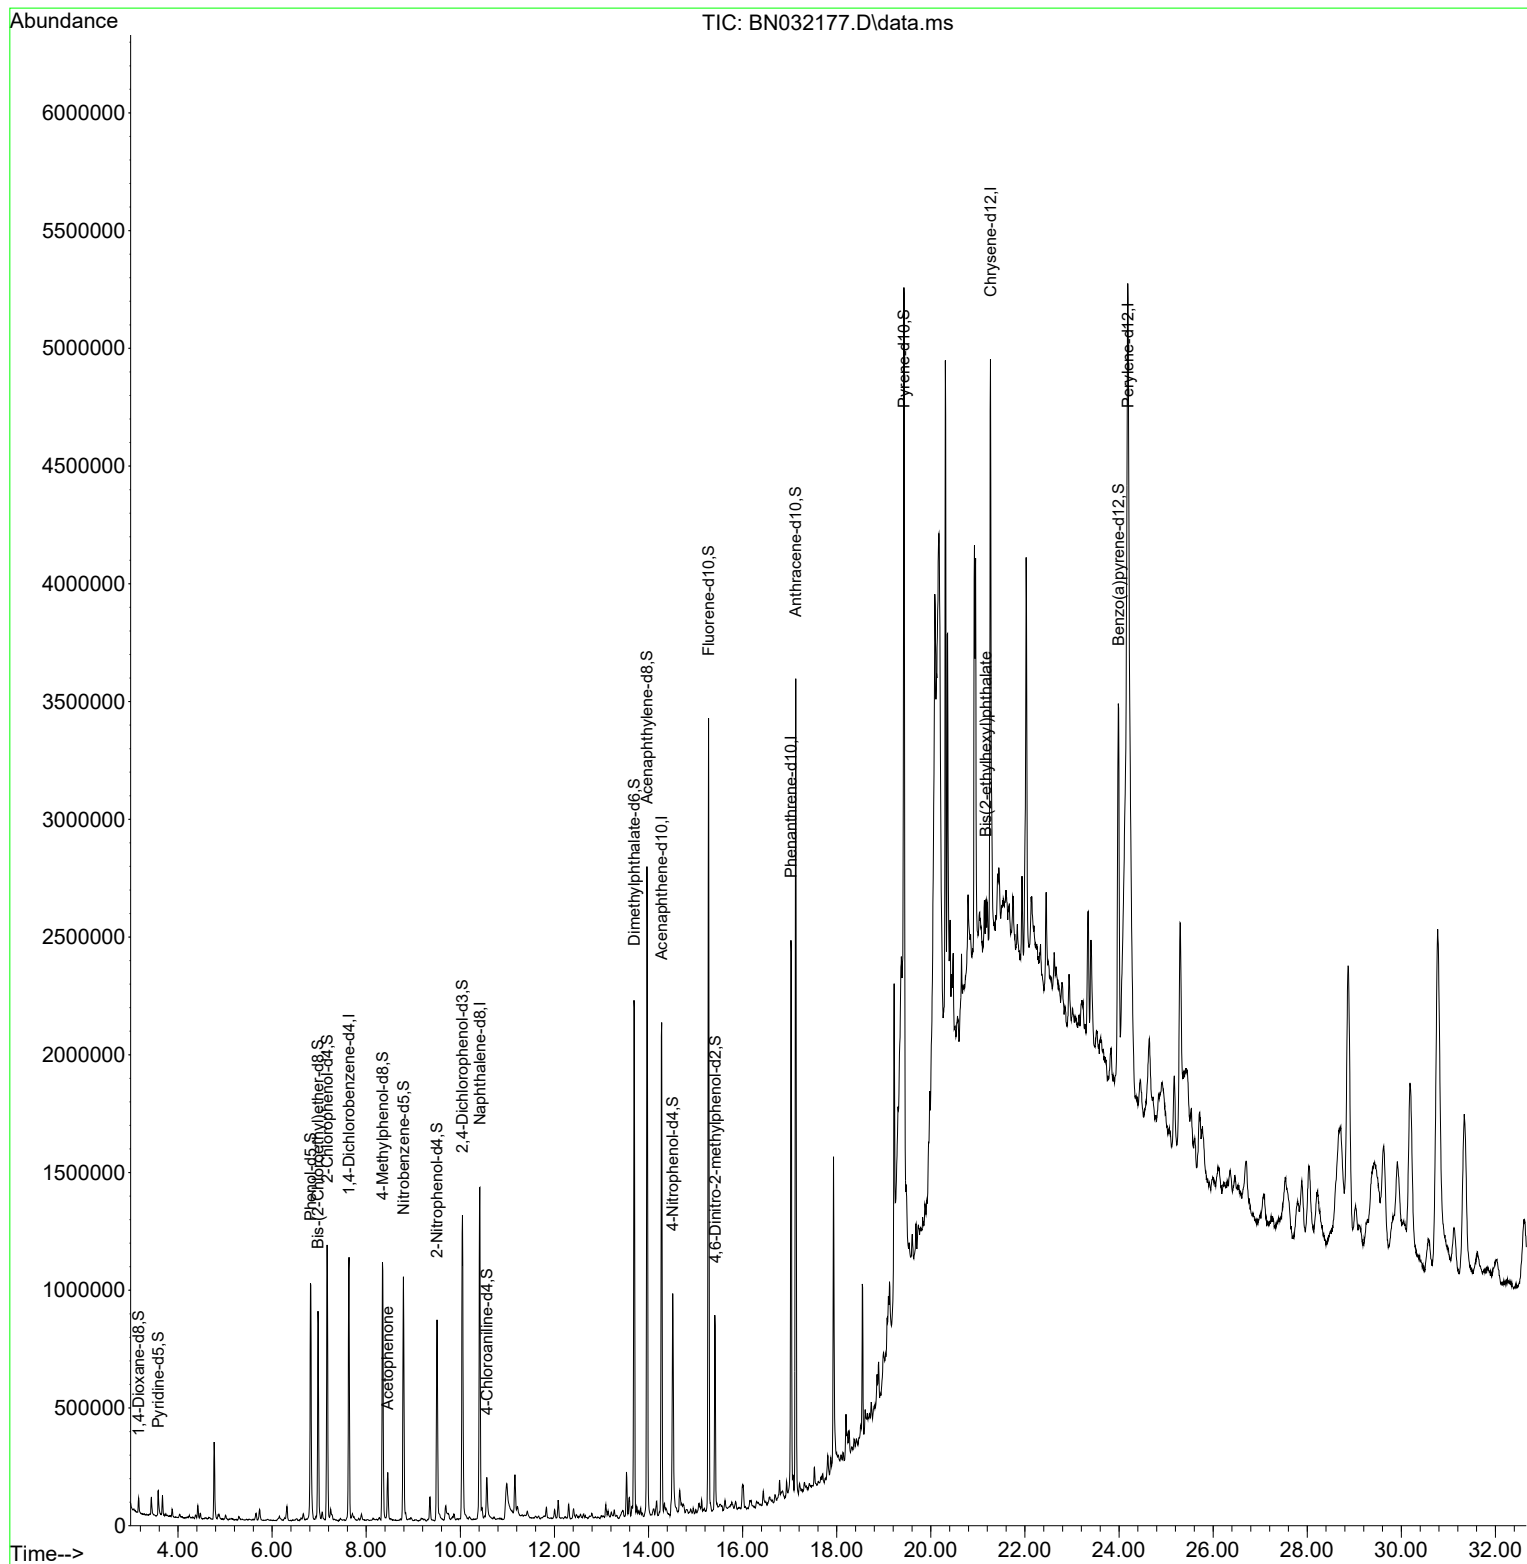


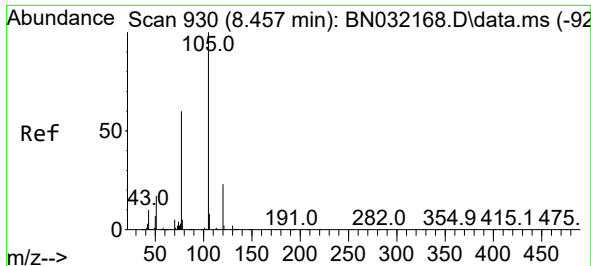

#16
Acetophenone
Concen: 3.498 ng/ul
RT: 8.457 min Scan# 91
Delta R.T. -0.006 min
Lab File: BN032177.D
Acq: 22 Jun 2024 21:50

Instrument :
BNA_N
ClientSampleId :
C0AB9

Tgt Ion:105 Resp: 119466
Ion Ratio Lower Upper
105 100
77 72.7 58.6 87.8
51 21.8 17.2 25.8

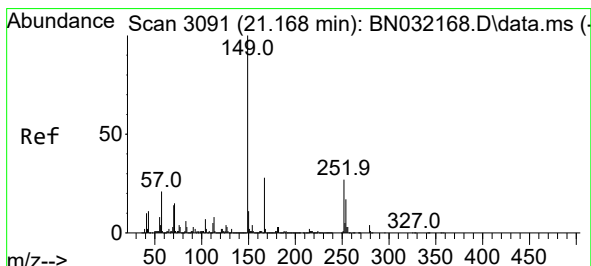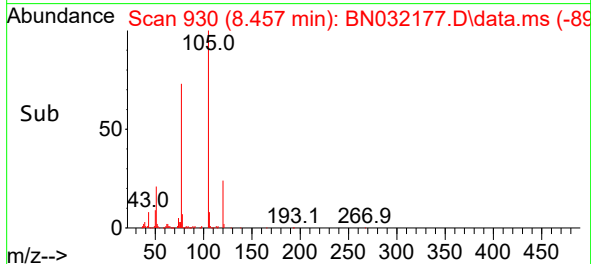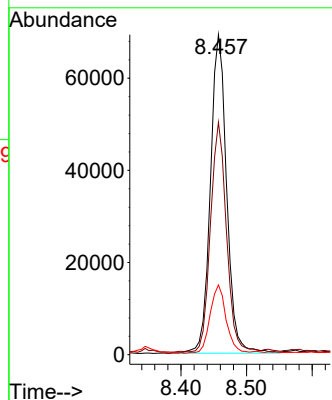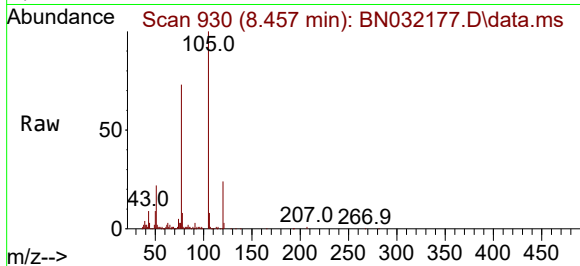

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.753 ng/ul
RT: 21.174 min Scan# 3092
Delta R.T. -0.000 min
Lab File: BN032177.D
Acq: 22 Jun 2024 21:50

Tgt Ion:149 Resp: 100172
Ion Ratio Lower Upper
149 100
167 30.9 21.4 32.0
279 5.0 3.3 4.9#

