

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BN032194.D
 Acq On : 23 Jun 2024 09:39
 Operator : MA/JU
 Sample : P2775-15
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4C97

Quant Time: Jun 24 01:42:18 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 10:49:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	378367	20.000	ng/u1	0.00
20) Naphthalene-d8	10.410	136	1403015	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.275	164	781815	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.028	188	1473061	20.000	ng/u1	0.00
79) Chrysene-d12	21.263	240	1389277	20.000	ng/u1	0.00
88) Perylene-d12	24.180	264	1640235	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	32149	3.515	ng/uL	0.00
4) Pyridine-d5	3.570	84	414744	16.110	ng/u1	0.00
7) Phenol-d5	6.816	99	581488	17.927	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	315634	16.636	ng/u1	0.00
11) 2-Chlorophenol-d4	7.169	132	512017	20.688	ng/u1	0.00
15) 4-Methylphenol-d8	8.346	113	464377	17.563	ng/u1	0.00
21) Nitrobenzene-d5	8.787	128	243533	22.702	ng/u1	0.00
24) 2-Nitrophenol-d4	9.505	143	261258	23.576	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.040	165	428883	20.731	ng/u1	0.00
31) 4-Chloroaniline-d4	10.557	131	619134	20.157	ng/u1	0.00
46) Dimethylphthalate-d6	13.693	166	1234391	22.664	ng/u1	0.00
49) Acenaphthylene-d8	13.969	160	1466100	23.410	ng/u1	0.00
54) 4-Nitrophenol-d4	14.516	143	200675	18.402	ng/u1	0.01
60) Fluorene-d10	15.275	176	1030595	22.363	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.416	200	73532	9.931	ng/u1	0.00
73) Anthracene-d10	17.128	188	1472702	23.352	ng/u1	0.00
81) Pyrene-d10	19.428	212	1727147	23.232	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.986	264	1811339	23.127	ng/u1	0.00
Target Compounds						
80) Fluoranthene	19.092	202	96509	1.086	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032194.D
Acq On : 23 Jun 2024 09:39
Operator : MA/JU
Sample : P2775-15
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4C97

Quant Time: Jun 24 01:42:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 10:49:40 2024
Response via : Initial Calibration

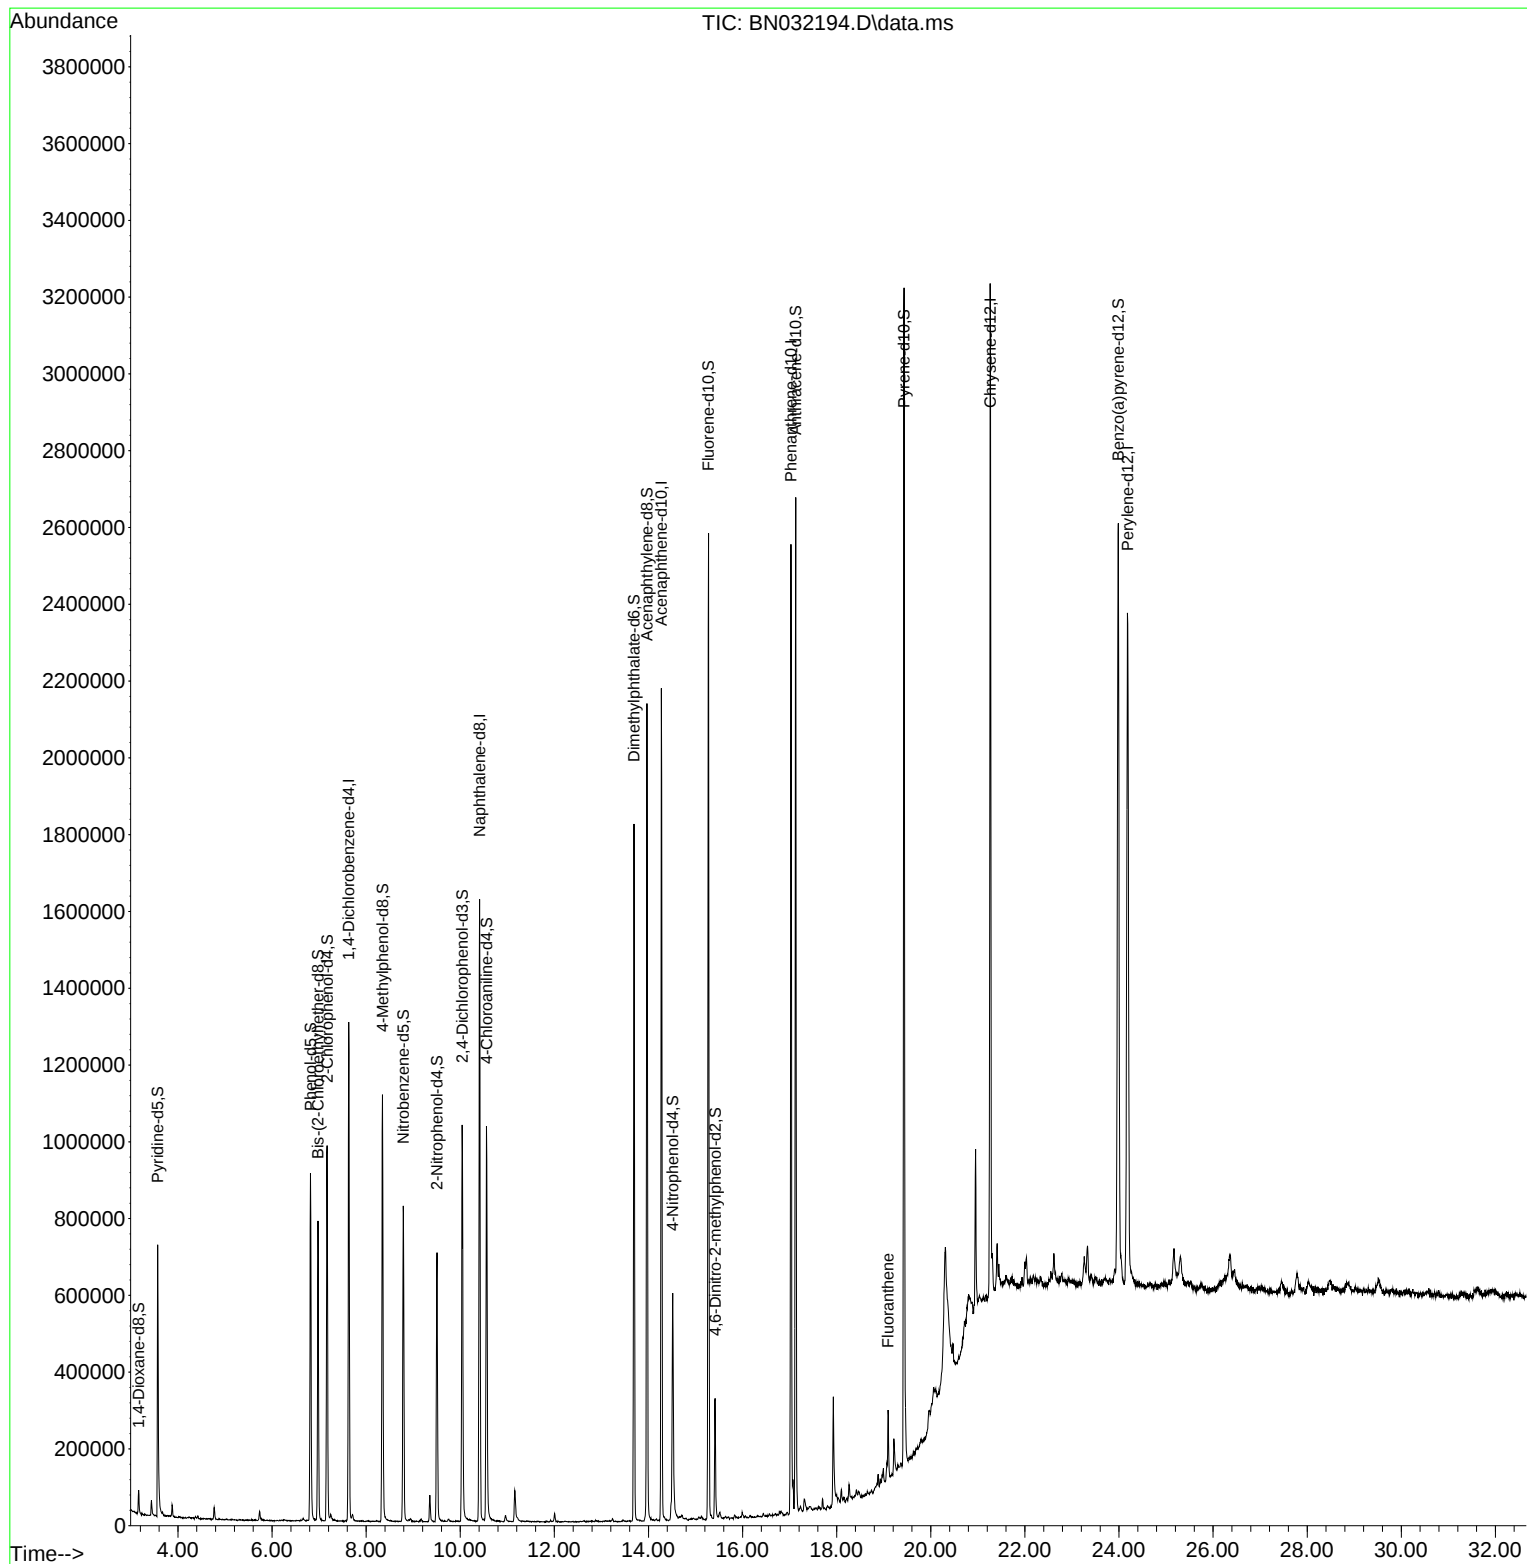

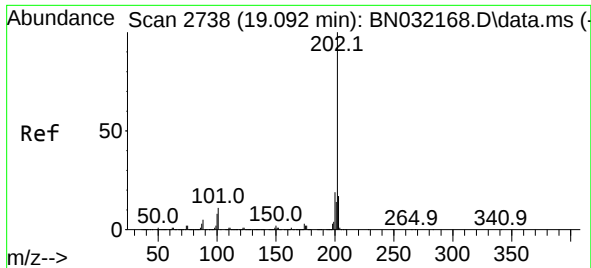

#80
 Fluoranthene
 Concen: 1.086 ng/ul
 RT: 19.092 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BN032194.D
 Acq: 23 Jun 2024 09:39

Instrument :
 BNA_N
 ClientSampleId :
 A4C97

Tgt Ion:	202	Resp:	96509
Ion Ratio	Lower	Upper	
202	100		
101	13.1	10.3	15.5
100	9.6	8.0	12.0

