

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BNCCC200.D
 Acq On : 23 Jun 2024 13:36
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 24 01:44:36 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 10:49:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	356380	20.000	ng/u1	0.00
20) Naphthalene-d8	10.410	136	1405125	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.275	164	793573	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.028	188	1494719	20.000	ng/u1	0.00
79) Chrysene-d12	21.269	240	1312644	20.000	ng/u1	0.00
88) Perylene-d12	24.180	264	1627334	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	67709	7.860	ng/uL	0.00
4) Pyridine-d5	3.564	84	464467	19.154	ng/u1	0.00
7) Phenol-d5	6.816	99	594033	19.443	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	329038	18.412	ng/u1	0.00
11) 2-Chlorophenol-d4	7.169	132	523567	22.459	ng/u1	0.00
15) 4-Methylphenol-d8	8.346	113	484125	19.439	ng/u1	0.00
21) Nitrobenzene-d5	8.787	128	251751	23.433	ng/u1	0.00
24) 2-Nitrophenol-d4	9.504	143	279487	25.184	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.040	165	475225	22.937	ng/u1	0.00
31) 4-Chloroaniline-d4	10.557	131	633180	20.583	ng/u1	0.00
46) Dimethylphthalate-d6	13.692	166	1193153	21.582	ng/u1	0.00
49) Acenaphthylene-d8	13.969	160	1446524	22.755	ng/u1	0.00
54) 4-Nitrophenol-d4	14.510	143	213042	19.246	ng/u1	0.00
60) Fluorene-d10	15.275	176	1025675	21.927	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.416	200	145102	19.313	ng/u1	0.00
73) Anthracene-d10	17.128	188	1484236	23.194	ng/u1	0.00
81) Pyrene-d10	19.427	212	1647173	23.450	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.986	264	1741994	22.418	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.199	88	72561	7.873	ng/uL	93
5) Pyridine	3.587	79	454606	18.750	ng/u1	97
6) Benzaldehyde	6.787	77	323215	22.555	ng/u1	93
8) Phenol	6.846	94	604910	19.455	ng/u1	97
10) Bis(2-Chloroethyl)ether	7.069	93	507527	19.740	ng/u1	94
12) 2-Chlorophenol	7.199	128	541738	22.207	ng/u1	95
13) 2-Methylphenol	8.081	108	472192	19.663	ng/u1	97
14) 2,2'-oxybis(1-Chloropr...	8.152	45	532974	18.008	ng/u1	98
16) Acetophenone	8.457	105	737896	19.551	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.440	70	333075	17.030	ng/u1#	95
18) 4-Methylphenol	8.410	108	495123	19.020	ng/u1	99
19) Hexachloroethane	8.693	117	211606	20.484	ng/u1	88
22) Nitrobenzene	8.834	77	530893	20.741	ng/u1	92
23) Isophorone	9.352	82	967382	18.423	ng/u1	96
25) 2-Nitrophenol	9.534	139	294358	24.277	ng/u1	93
26) 2,4-Dimethylphenol	9.599	107	511623	21.691	ng/u1	98
27) Bis(2-Chloroethoxy)met...	9.834	93	630631	19.271	ng/u1	99
29) 2,4-Dichlorophenol	10.069	162	464040	22.683	ng/u1	98
30) Naphthalene	10.457	128	1631627	22.437	ng/u1	99
32) 4-Chloroaniline	10.581	127	617138	20.664	ng/u1	97
33) Hexachlorobutadiene	10.728	225	312646	25.446	ng/u1	98
34) Caprolactam	11.375	113	113901	14.264	ng/u1	83
35) 4-Chloro-3-methylphenol	11.716	107	462205	19.329	ng/u1	98
36) 2-Methylnaphthalene	12.081	142	1047051	21.065	ng/u1	99


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BNCCC200.D
 Acq On : 23 Jun 2024 13:36
 Operator : MA/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 24 01:44:36 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 10:49:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.298	142	1061157	21.277	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.451	216	544195	25.930	ng/ul	97
40) Hexachlorocyclopentadiene	12.416	237	113491	9.383	ng/ul	93
41) 2,4,6-Trichlorophenol	12.704	196	344485	24.183	ng/ul	98
42) 2,4,5-Trichlorophenol	12.781	196	369472	23.868	ng/ul	97
43) 1,1'-Biphenyl	13.104	154	1322159	23.687	ng/ul	95
44) 2-Chloronaphthalene	13.145	162	1052721	24.079	ng/ul	98
45) 2-Nitroaniline	13.369	65	253086	19.971	ng/ul#	85
47) Dimethylphthalate	13.740	163	1235893	21.859	ng/ul	99
48) 2,6-Dinitrotoluene	13.869	165	256002	22.779	ng/ul	95
50) Acenaphthylene	13.998	152	1649473	22.960	ng/ul	99
51) 3-Nitroaniline	14.198	138	275773	22.950	ng/ul	92
52) Acenaphthene	14.340	153	1102565	23.195	ng/ul	99
53) 2,4-Dinitrophenol	14.422	184	83691	14.751	ng/ul	95
55) 4-Nitrophenol	14.528	109	162676	19.811	ng/ul	87
56) Dibenzofuran	14.681	168	1460069	22.608	ng/ul	100
57) 2,4-Dinitrotoluene	14.663	165	349555	21.197	ng/ul	96
58) 2,3,4,6-Tetrachlorophenol	14.910	232	287071	22.170	ng/ul	100
59) Diethylphthalate	15.110	149	1216506	20.851	ng/ul	99
61) Fluorene	15.328	166	1160808	22.320	ng/ul	97
62) 4-Chlorophenyl-phenyle...	15.328	204	576353	22.880	ng/ul	98
63) 4-Nitroaniline	15.369	138	266350	23.284	ng/ul	97
66) 4,6-Dinitro-2-methylph...	15.428	198	157690	19.743	ng/ul	99
67) N-Nitrosodiphenylamine	15.545	169	996712	24.192	ng/ul	98
68) 4-Bromophenyl-phenylether	16.222	248	346318	23.913	ng/ul	92
69) Hexachlorobenzene	16.328	284	398298	24.265	ng/ul	97
70) Atrazine	16.504	200	266436	20.481	ng/ul	97
71) Pentachlorophenol	16.686	266	223950	21.325	ng/ul	92
72) Phenanthrene	17.069	178	1722213	22.618	ng/ul	99
74) Anthracene	17.163	178	1803727	23.378	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.063	216	522832	27.176	ng/ul	97
76) Pentachlorobenzene	14.592	250	496826	26.513	ng/ul	96
77) Carbazole	17.439	167	1626205	24.719	ng/ul	99
78) Di-n-butylphthalate	17.998	149	2029377	22.421	ng/ul	100
80) Fluoranthene	19.098	202	1962750	23.381	ng/ul	95
82) Pyrene	19.457	202	2025611	23.518	ng/ul	96
83) Butylbenzylphthalate	20.369	149	919579	22.605	ng/ul	88
84) 3,3'-Dichlorobenzidine	21.180	252	602105	23.920	ng/ul	97
85) Benzo(a)anthracene	21.251	228	2017964	22.968	ng/ul	97
86) Bis(2-ethylhexyl)phtha...	21.169	149	1317985	22.226	ng/ul	100
87) Chrysene	21.310	228	1929001	23.505	ng/ul	99
89) Di-n-octyl phthalate	22.269	149	2357275	21.637	ng/ul	100
90) Benzo(b)fluoranthene	23.263	252	2108709	21.679	ng/ul	98
91) Benzo(k)fluoranthene	23.321	252	2098453	21.985	ng/ul	99
93) Benzo(a)pyrene	24.045	252	2019108	22.163	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	27.468	276	2454469	23.380	ng/ul	98
95) Dibenzo(a,h)anthracene	27.515	278	2068258	24.132	ng/ul	97
96) Benzo(g,h,i)perylene	28.492	276	2015838	24.156	ng/ul	95





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 7.873 ng/uL
RT: 3.199 min Scan# 30
Delta R.T. 0.000 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36




Instrument :
BNA_N
ClientSampleId :


Tgt Ion: 88 Resp: 72561
Ion Ratio Lower Upper
88 100
43 21.4 18.5 27.7
58 59.1 52.6 78.8

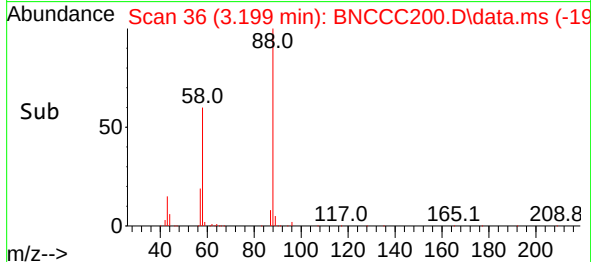

#5
Pyridine
Concen: 18.750 ng/uL
RT: 3.587 min Scan# 102
Delta R.T. 0.000 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36

Tgt Ion: 79 Resp: 454606
Ion Ratio Lower Upper
79 100
52 62.6 53.0 79.6
51 29.3 23.3 34.9


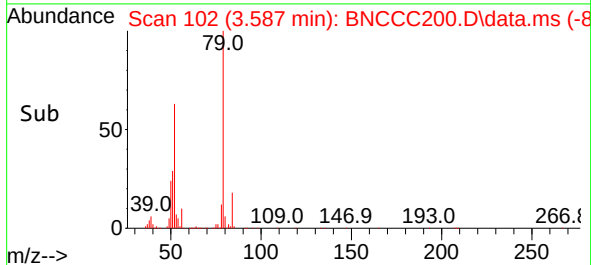

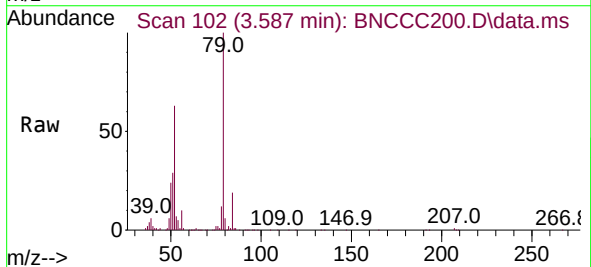




#6
Benzaldehyde
Concen: 22.555 ng/ul
RT: 6.787 min Scan# 646
Delta R.T. -0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36




Instrument :
BNA_N
ClientSampleId :


Tgt Ion: 77 Resp: 323215
Ion Ratio Lower Upper
77 100
105 106.4 80.2 120.4
106 103.2 76.8 115.2

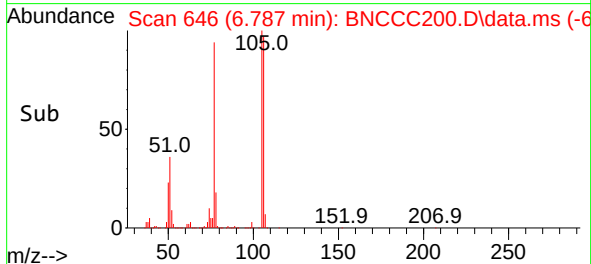

#8
Phenol
Concen: 19.455 ng/ul
RT: 6.846 min Scan# 656
Delta R.T. 0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36


Tgt Ion: 94 Resp: 604910
Ion Ratio Lower Upper
94 100
65 24.6 20.3 30.5
66 34.5 25.8 38.8

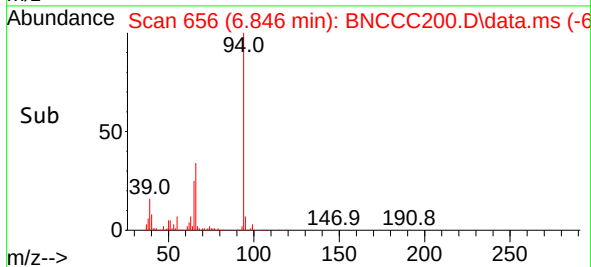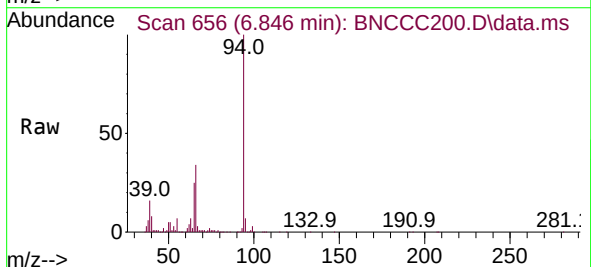






#10
 Bis(2-Chloroethyl)ether
 Concen: 19.740 ng/ul
 RT: 7.069 min Scan# 694
 Delta R.T. -0.006 min
 Lab File: BNCCC200.D
 Acq: 23 Jun 2024 13:36

Instrument :
 BNA_N
 ClientSampleId :



Tgt Ion: 93 Resp: 507527




Ion	Ratio	Lower	Upper
93	100		
63	64.4	56.8	85.2
95	32.1	26.0	39.0

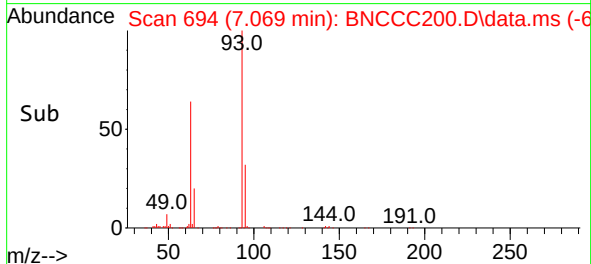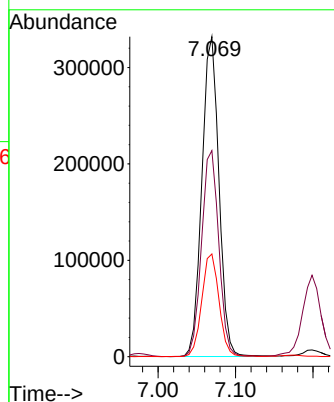


#12
 2-Chlorophenol
 Concen: 22.207 ng/ul
 RT: 7.199 min Scan# 716
 Delta R.T. -0.006 min
 Lab File: BNCCC200.D
 Acq: 23 Jun 2024 13:36

Tgt Ion:128 Resp: 541738

Ion	Ratio	Lower	Upper
128	100		
64	37.9	33.9	50.9
130	31.5	26.3	39.5


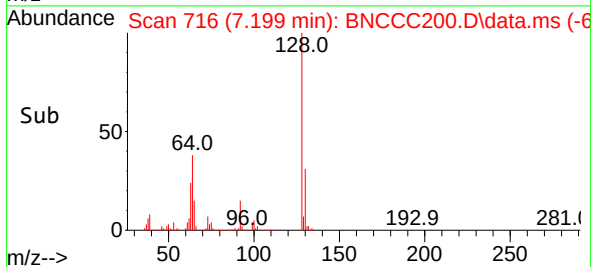
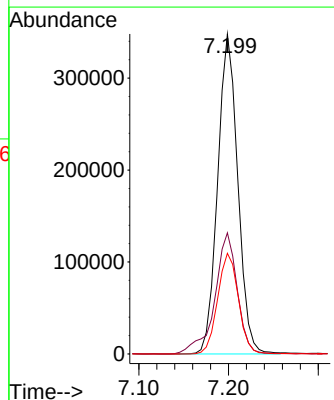
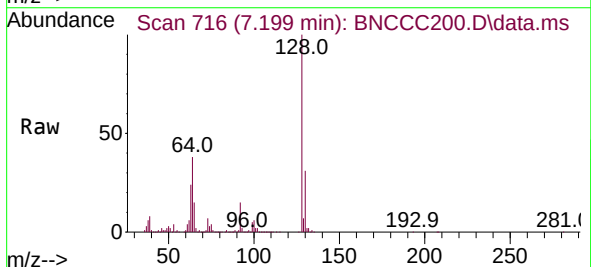




#13
2-Methylphenol
Concen: 19.663 ng/ul
RT: 8.081 min Scan# 865
Delta R.T. 0.000 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:108 Resp: 472192
Ion Ratio Lower Upper
108 100
107 92.8 71.6 107.4

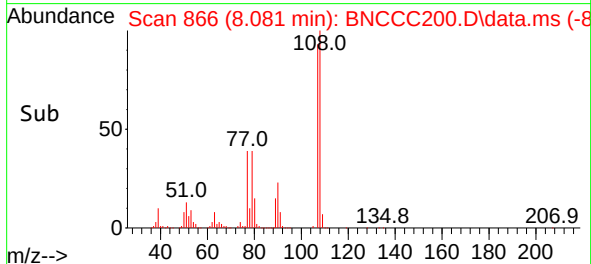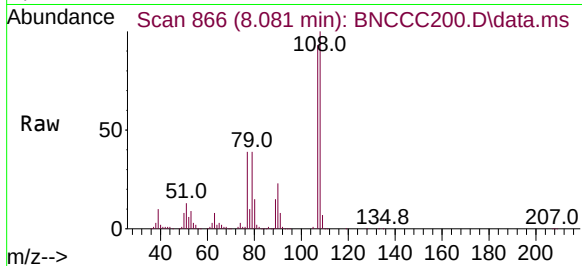

#14
2,2'-oxybis(1-Chloropropane)
Concen: 18.008 ng/ul
RT: 8.152 min Scan# 878
Delta R.T. -0.012 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36


Tgt Ion: 45 Resp: 532974
Ion Ratio Lower Upper
45 100
77 17.7 13.6 20.4
79 13.9 10.6 15.8

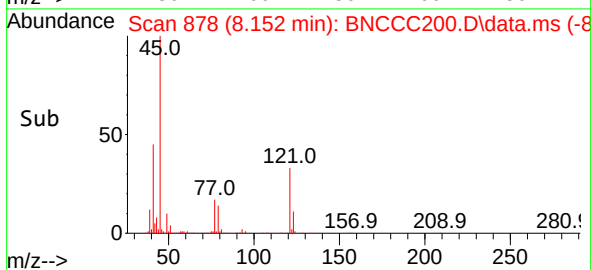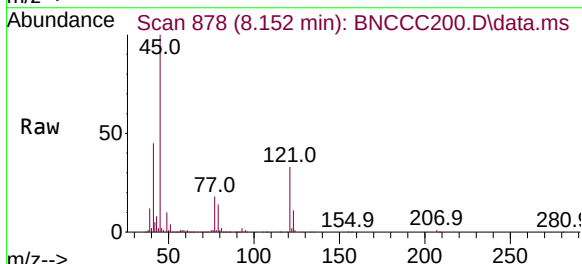






#16
Acetophenone
Concen: 19.551 ng/ul
RT: 8.457 min Scan# 911
Delta R.T. -0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36


Instrument :
BNA_N
ClientSampleId :





Tgt Ion:105 Resp: 737896
Ion Ratio Lower Upper
105 100
77 71.6 58.6 87.8
51 20.2 17.2 25.8

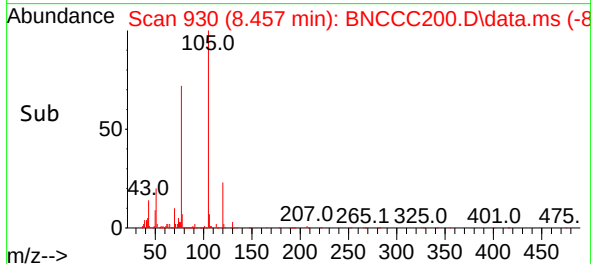


#17
N-Nitroso-di-n-propylamine
Concen: 17.030 ng/ul
RT: 8.440 min Scan# 927
Delta R.T. -0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36

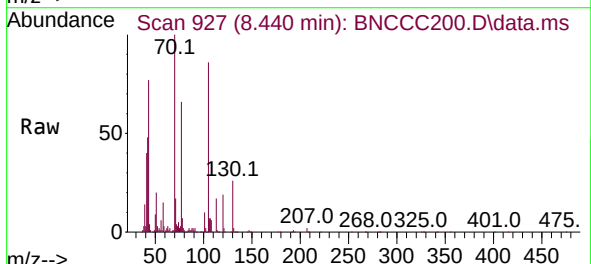

Tgt Ion: 70 Resp: 333075
Ion Ratio Lower Upper
70 100
42 48.2 37.3 55.9
101 10.4 7.8 11.6
130 25.5 16.4 24.6#

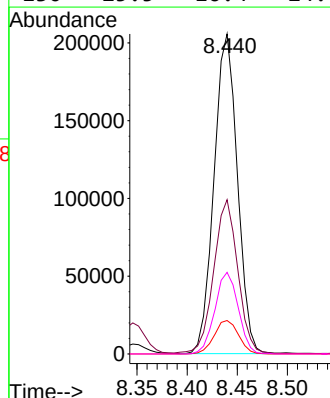

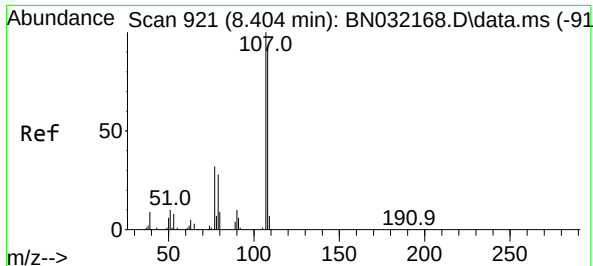

#18

4-Methylphenol

Concen: 19.020 ng/ul

RT: 8.410 min Scan# 91

Delta R.T. 0.000 min

Lab File: BNCCC200.D

Acq: 23 Jun 2024 13:36

Instrument :

BNA_N





ClientSampleId :

Tgt Ion:108 Resp: 495123

Ion Ratio Lower Upper

108 100

107 111.0 89.6 134.4

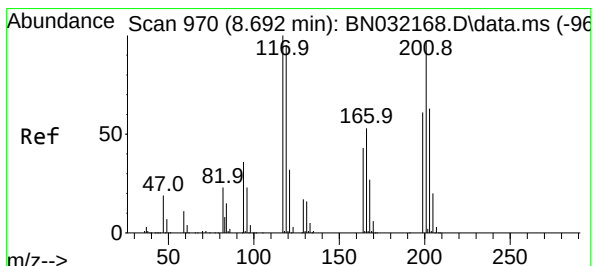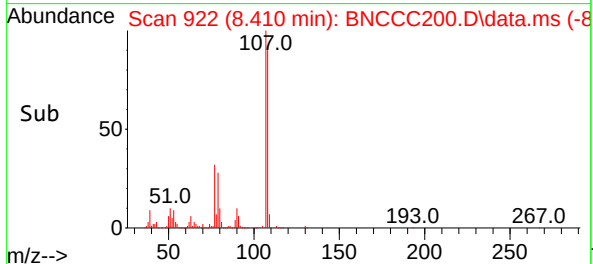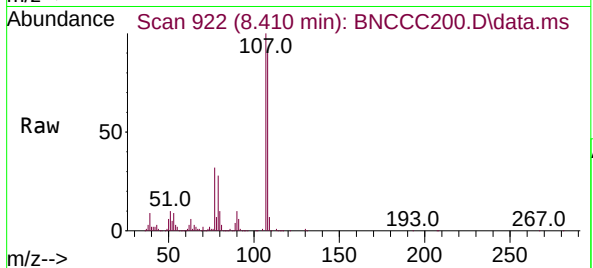

#19

Hexachloroethane

Concen: 20.484 ng/ul

RT: 8.693 min Scan# 970

Delta R.T. -0.006 min

Lab File: BNCCC200.D

Acq: 23 Jun 2024 13:36




Tgt Ion:117 Resp: 211606


Ion Ratio Lower Upper

117 100

201 102.1 71.6 107.4

199 63.8 45.6 68.4


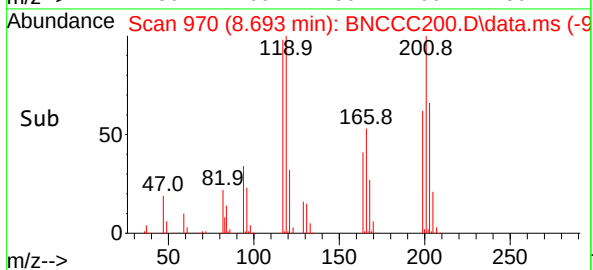

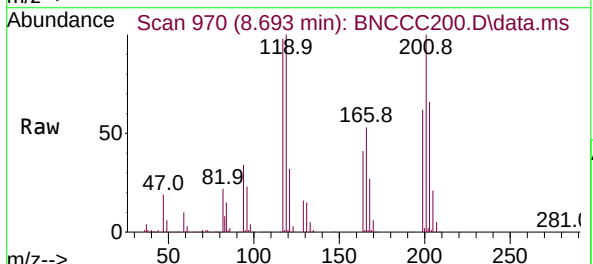




#22
Nitrobenzene
Concen: 20.741 ng/ul
RT: 8.834 min Scan# 993
Delta R.T. -0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36




Instrument :
BNA_N
ClientSampleId :


Tgt Ion: 77 Resp: 530893
Ion Ratio Lower Upper
77 100
123 52.1 36.6 55.0
65 12.6 10.2 15.4

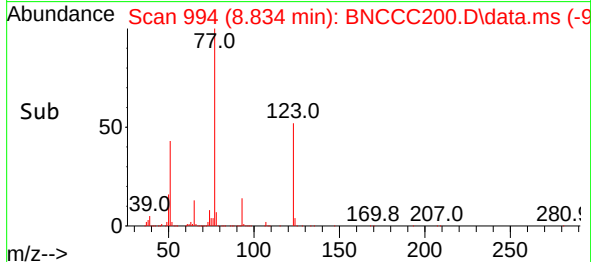

#23
Isophorone
Concen: 18.423 ng/ul
RT: 9.352 min Scan# 1082
Delta R.T. -0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36

Tgt Ion: 82 Resp: 967382
Ion Ratio Lower Upper
82 100
95 7.5 5.5 8.3
138 19.5 14.1 21.1


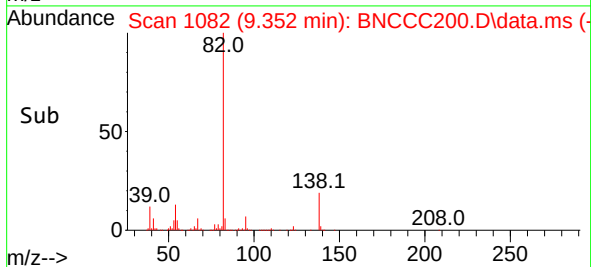

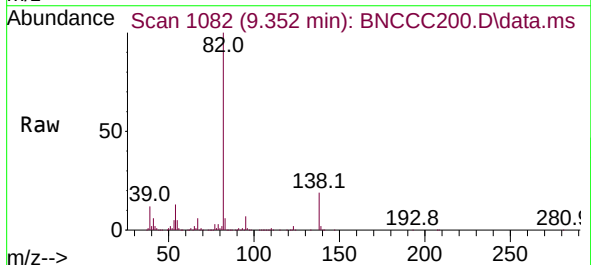




#25
2-Nitrophenol
Concen: 24.277 ng/ul
RT: 9.534 min Scan# 1113
Delta R.T. -0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:139 Resp: 294358
Ion Ratio Lower Upper
139 100
65 42.7 38.3 57.5
109 30.8 22.1 33.1

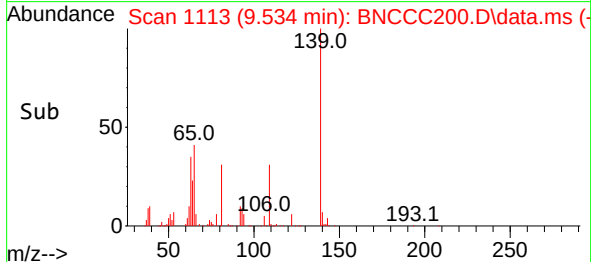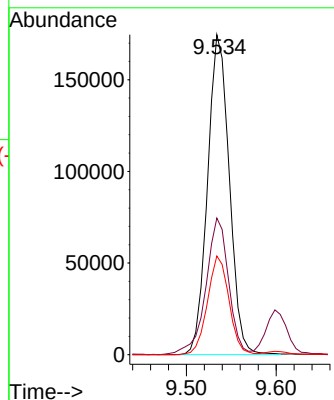

#26
2,4-Dimethylphenol
Concen: 21.691 ng/ul
RT: 9.599 min Scan# 1124
Delta R.T. -0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36

Tgt Ion:107 Resp: 511623
Ion Ratio Lower Upper
107 100
121 51.2 40.8 61.2
122 84.6 70.4 105.6

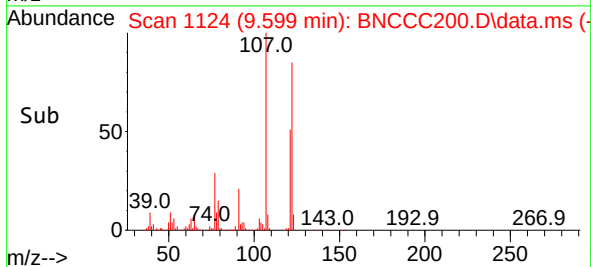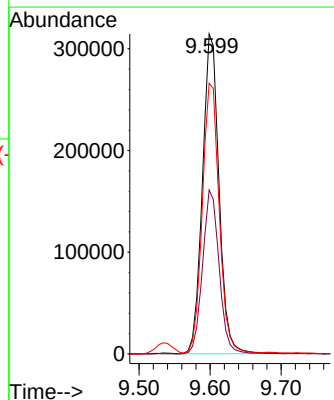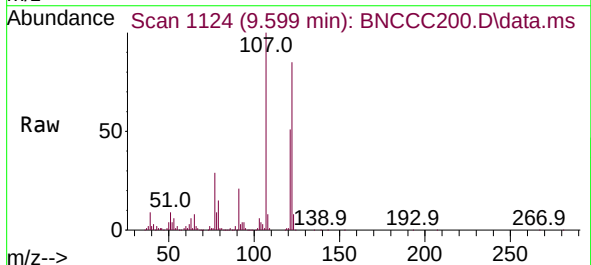



#27

Bis(2-Chloroethoxy)methane

Concen: 19.271 ng/ul

RT: 9.834 min Scan# 1164

Delta R.T. -0.006 min

Lab File: BNCCC200.D

Acq: 23 Jun 2024 13:36

Instrument :

BNA_N

ClientSampleId :





Tgt Ion: 93 Resp: 630631

Ion Ratio Lower Upper

93 100

95 32.2 26.1 39.1

123 11.7 9.0 13.6

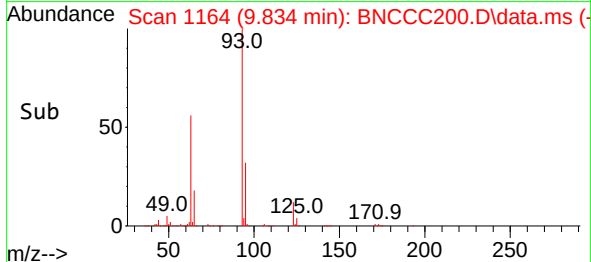

#29

2,4-Dichlorophenol

Concen: 22.683 ng/ul

RT: 10.069 min Scan# 1204

Delta R.T. 0.000 min

Lab File: BNCCC200.D

Acq: 23 Jun 2024 13:36




Tgt Ion:162 Resp: 464040


Ion Ratio Lower Upper

162 100

164 65.2 52.7 79.1


98 35.7 30.5 45.7

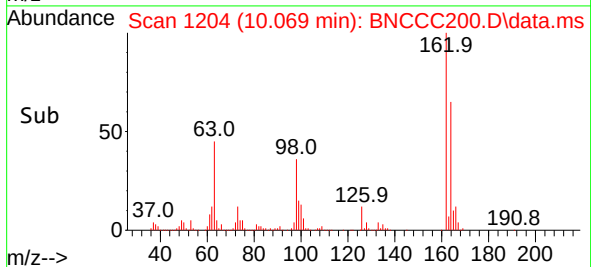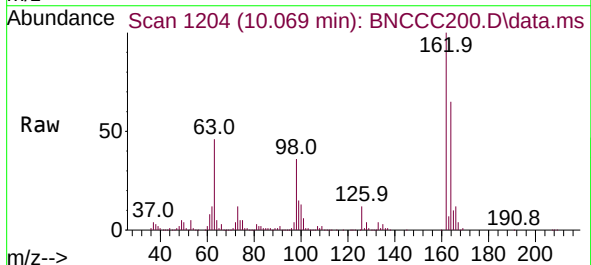






#30
Naphthalene
Concen: 22.437 ng/ul
RT: 10.457 min Scan# 1270
Delta R.T. -0.012 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36

Instrument :
BNA_N
ClientSampleId :







Tgt Ion:128 Resp: 1631627
Ion Ratio Lower Upper
128 100
129 11.1 8.5 12.7
127 13.2 10.3 15.5



#32
4-Chloroaniline
Concen: 20.664 ng/ul
RT: 10.581 min Scan# 1291
Delta R.T. -0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36

Tgt Ion:127 Resp: 617138
Ion Ratio Lower Upper
127 100
129 32.7 25.0 37.4




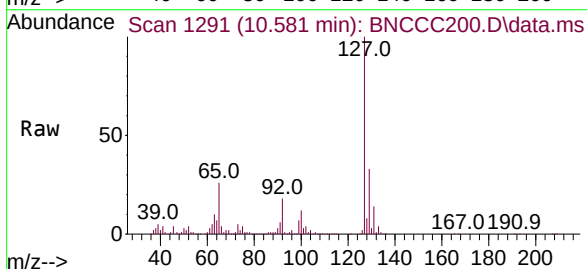




#33
Hexachlorobutadiene
Concen: 25.446 ng/ul
RT: 10.728 min Scan# 1316
Delta R.T. -0.012 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:225 Resp: 312646
Ion Ratio Lower Upper
225 100
223 62.7 52.3 78.5
227 65.0 52.5 78.7

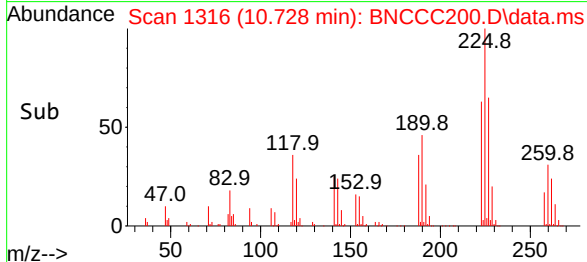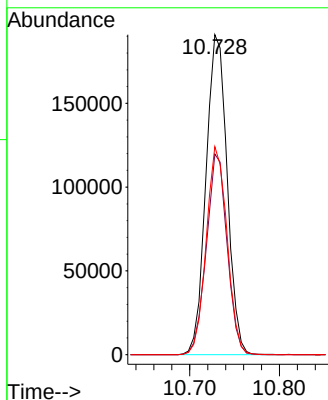

#34
Caprolactam
Concen: 14.264 ng/ul
RT: 11.375 min Scan# 1426
Delta R.T. 0.000 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36

Tgt Ion:113 Resp: 113901
Ion Ratio Lower Upper
113 100
55 125.5 117.2 175.8
56 92.9 89.4 134.0


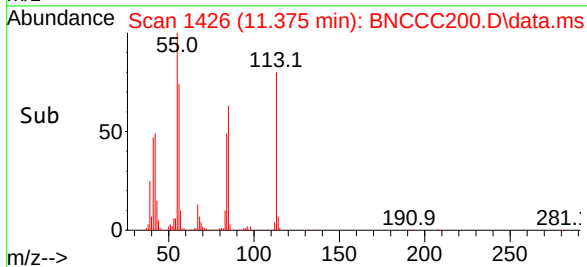
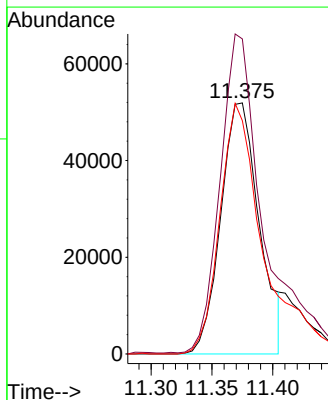
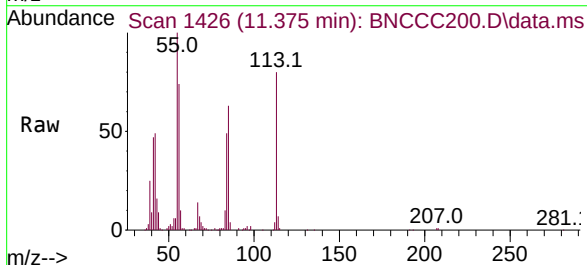




#35
4-Chloro-3-methylphenol
Concen: 19.329 ng/ul
RT: 11.716 min Scan# 1484
Delta R.T. 0.000 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:107 Resp: 462205
Ion Ratio Lower Upper
107 100
144 25.6 20.5 30.7
142 82.8 64.0 96.0

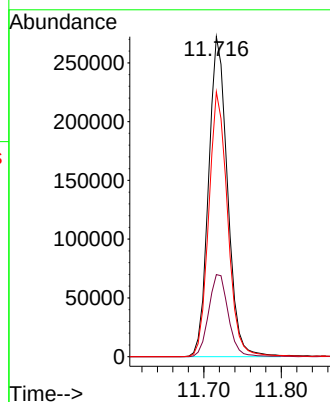

#36
2-Methylnaphthalene
Concen: 21.065 ng/ul
RT: 12.081 min Scan# 1546
Delta R.T. -0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36

Tgt Ion:142 Resp: 1047051
Ion Ratio Lower Upper
142 100
141 89.0 70.1 105.1



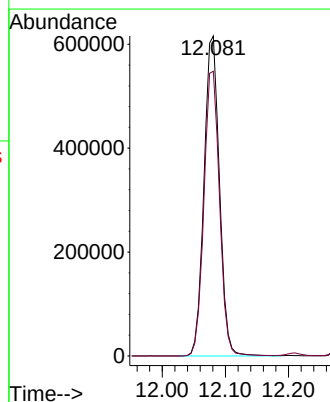





#37
1-Methylnaphthalene
Concen: 21.277 ng/ul
RT: 12.298 min Scan# 11
Delta R.T. -0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:142 Resp: 1061157
Ion Ratio Lower Upper
142 100
141 90.9 71.7 107.5
116 3.5 3.0 4.4

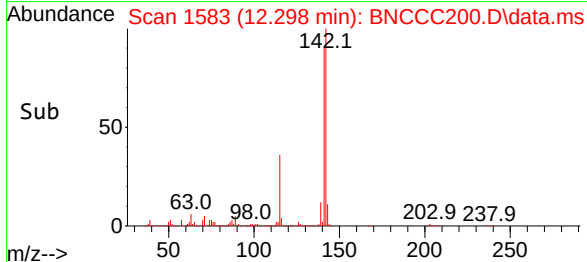

#39
1,2,4,5-Tetrachlorobenzene
Concen: 25.930 ng/ul
RT: 12.451 min Scan# 1609
Delta R.T. -0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36


Tgt Ion:216 Resp: 544195
Ion Ratio Lower Upper
216 100
214 80.1 61.7 92.5
179 21.9 16.7 25.1
108 16.5 14.5 21.7

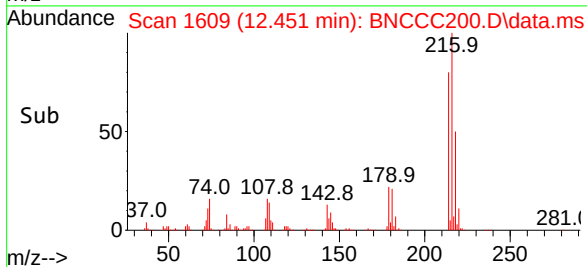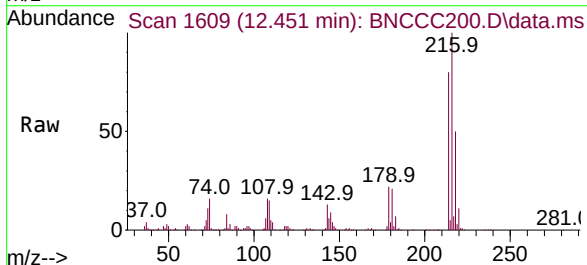






#40
Hexachlorocyclopentadiene
Concen: 9.383 ng/ul
RT: 12.416 min Scan# 1603
Delta R.T. -0.012 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36


Instrument :
BNA_N
ClientSampleId :





Tgt Ion:237 Resp: 113491
Ion Ratio Lower Upper
237 100
235 65.2 47.8 71.6
272 13.8 10.0 15.0




#41
2,4,6-Trichlorophenol
Concen: 24.183 ng/ul
RT: 12.704 min Scan# 1652
Delta R.T. 0.000 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36



Tgt Ion:196 Resp: 344485
Ion Ratio Lower Upper
196 100
198 98.1 76.4 114.6
200 30.0 24.2 36.4









#42
2,4,5-Trichlorophenol
Concen: 23.868 ng/ul
RT: 12.781 min Scan# 1665
Delta R.T. 0.000 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:196 Resp: 369472
Ion Ratio Lower Upper
196 100
198 95.6 73.8 110.6
200 30.6 25.6 38.4



#43
1,1'-Biphenyl
Concen: 23.687 ng/ul
RT: 13.104 min Scan# 1720
Delta R.T. -0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36

Tgt Ion:154 Resp: 1322159
Ion Ratio Lower Upper
154 100
153 40.8 30.6 46.0
76 11.4 11.1 16.7









#44
 2-Chloronaphthalene
 Concen: 24.079 ng/ul
 RT: 13.145 min Scan# 1727
 Delta R.T. -0.006 min
 Lab File: BNCCC200.D
 Acq: 23 Jun 2024 13:36




Instrument :
 BNA_N
 ClientSampleId :


Tgt Ion:162 Resp: 1052721
 Ion Ratio Lower Upper
 162 100
 164 32.0 27.0 40.4
 127 38.9 31.8 47.6

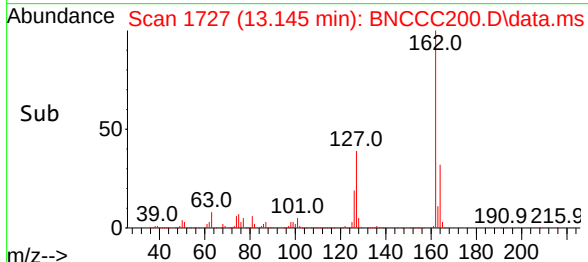

#45
 2-Nitroaniline
 Concen: 19.971 ng/ul
 RT: 13.369 min Scan# 1765
 Delta R.T. 0.000 min
 Lab File: BNCCC200.D
 Acq: 23 Jun 2024 13:36

Tgt Ion: 65 Resp: 253086
 Ion Ratio Lower Upper
 65 100
 92 77.9 58.8 88.2
 138 130.9 86.2 129.4#


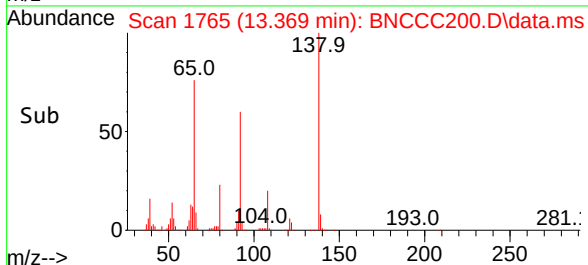






#47
Dimethylphthalate
Concen: 21.859 ng/ul
RT: 13.740 min Scan# 1828
Delta R.T. -0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:163 Resp: 1235893
Ion Ratio Lower Upper
163 100
194 4.0 3.2 4.8
164 9.6 8.2 12.2



#48
2,6-Dinitrotoluene
Concen: 22.779 ng/ul
RT: 13.869 min Scan# 1850
Delta R.T. -0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36

Tgt Ion:165 Resp: 256002
Ion Ratio Lower Upper
165 100
89 50.9 44.6 67.0
121 20.5 17.3 25.9









#50
Acenaphthylene
Concen: 22.960 ng/ul
RT: 13.998 min Scan# 1872
Delta R.T. -0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36

Instrument : BNA_N
ClientSampleId :

Tgt Ion:152 Resp: 1649473




Ion	Ratio	Lower	Upper
152	100		
151	20.4	15.9	23.9
153	13.2	10.4	15.6

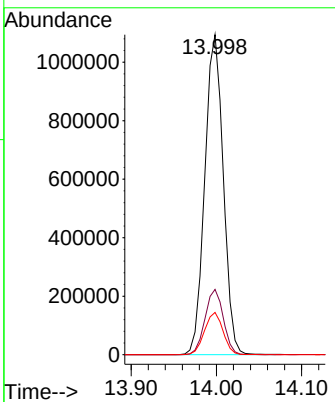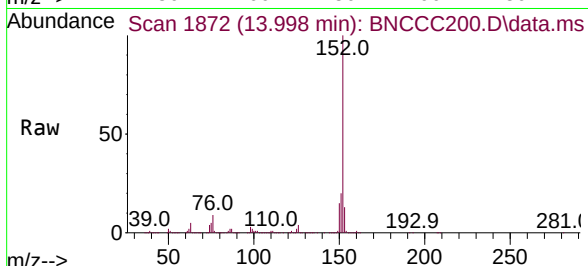


#51
3-Nitroaniline
Concen: 22.950 ng/ul
RT: 14.198 min Scan# 1906
Delta R.T. -0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36

Tgt Ion:138 Resp: 275773

Ion	Ratio	Lower	Upper
138	100		
108	10.6	9.2	13.8
92	107.6	94.0	141.0

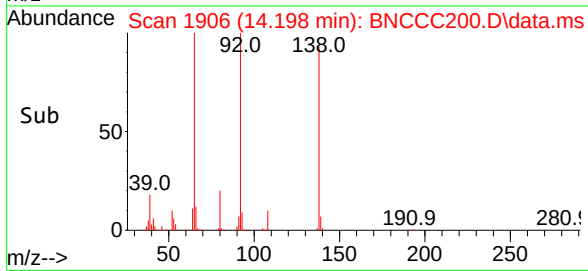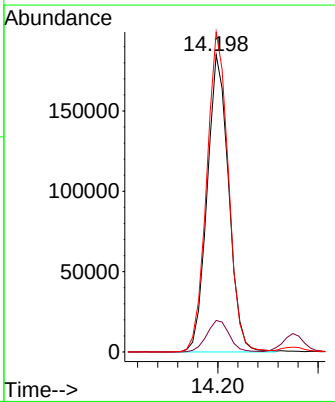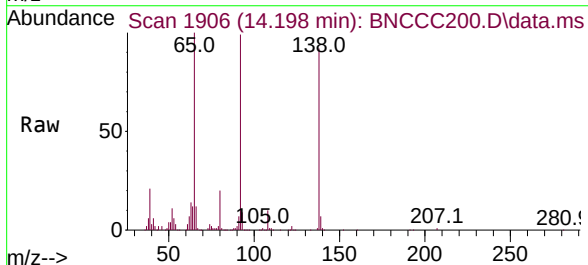



#52

Acenaphthene

Concen: 23.195 ng/ul

RT: 14.340 min Scan# 1930

Delta R.T. -0.006 min

Lab File: BNCCC200.D

Acq: 23 Jun 2024 13:36

Instrument :

BNA_N

ClientSampleId :





Tgt Ion:153 Resp: 1102565

Ion Ratio Lower Upper

153 100

152 47.0 37.8 56.6

154 86.5 69.8 104.8

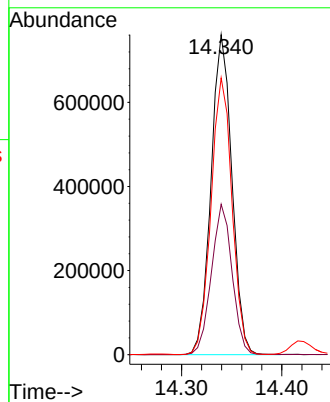

#53

2,4-Dinitrophenol

Concen: 14.751 ng/ul

RT: 14.422 min Scan# 1944

Delta R.T. 0.006 min

Lab File: BNCCC200.D

Acq: 23 Jun 2024 13:36




Tgt Ion:184 Resp: 83691


Ion Ratio Lower Upper

184 100

63 54.5 50.2 75.4

154 61.3 49.1 73.7




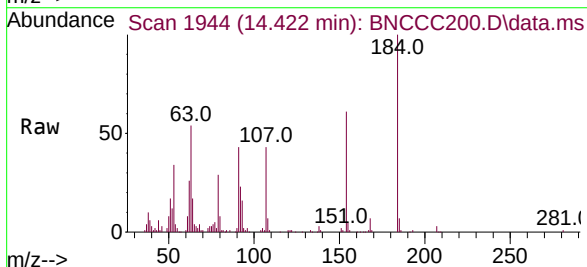




#55
4-Nitrophenol
Concen: 19.811 ng/ul
RT: 14.528 min Scan# 1962
Delta R.T. 0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:109 Resp: 162676
Ion Ratio Lower Upper
109 100
139 133.0 113.4 170.2
65 110.5 106.2 159.2



#56
Dibenzofuran
Concen: 22.608 ng/ul
RT: 14.681 min Scan# 1988
Delta R.T. 0.000 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36

Tgt Ion:168 Resp: 1460069
Ion Ratio Lower Upper
168 100
139 36.5 29.4 44.0




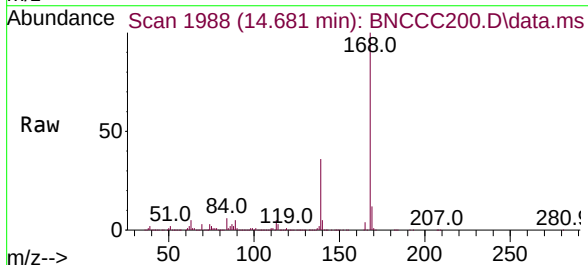




#57
2,4-Dinitrotoluene
Concen: 21.197 ng/ul
RT: 14.663 min Scan# 1984
Delta R.T. 0.000 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:165 Resp: 349555
Ion Ratio Lower Upper
165 100
63 42.6 32.2 48.2
182 3.0 2.3 3.5



#58
2,3,4,6-Tetrachlorophenol
Concen: 22.170 ng/ul
RT: 14.910 min Scan# 2027
Delta R.T. 0.000 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36

Tgt Ion:232 Resp: 287071
Ion Ratio Lower Upper
232 100
131 45.9 36.6 55.0
130 2.4 1.8 2.8
166 31.5 25.0 37.4

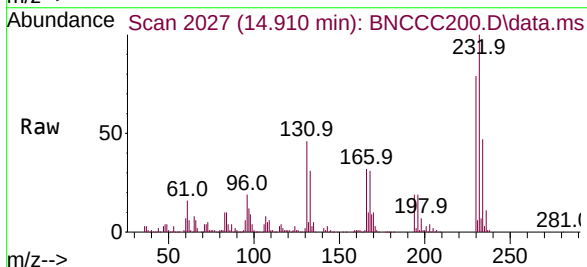



#59

Diethylphthalate

Concen: 20.851 ng/ul

RT: 15.110 min Scan# 2061

Delta R.T. -0.006 min


Lab File: BNCCC200.D

Acq: 23 Jun 2024 13:36

Instrument :

BNA_N

ClientSampleId :






Tgt Ion:149 Resp: 1216506

Ion Ratio Lower Upper

149 100

177 22.0 17.1 25.7

150 12.1 10.0 15.0



#61

Fluorene

Concen: 22.320 ng/ul

RT: 15.328 min Scan# 2098

Delta R.T. -0.006 min

Lab File: BNCCC200.D

Acq: 23 Jun 2024 13:36




Tgt Ion:166 Resp: 1160808


Ion Ratio Lower Upper

166 100

165 96.8 80.3 120.5

167 13.4 11.3 16.9


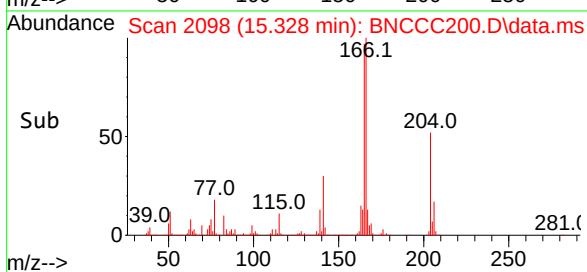






#62
4-Chlorophenyl-phenylether
Concen: 22.880 ng/ul
RT: 15.328 min Scan# 2098
Delta R.T. -0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:204 Resp: 576353
Ion Ratio Lower Upper
204 100
206 33.0 25.7 38.5
141 58.1 47.7 71.5



#63
4-Nitroaniline
Concen: 23.284 ng/ul
RT: 15.369 min Scan# 2105
Delta R.T. 0.000 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36

Tgt Ion:138 Resp: 266350
Ion Ratio Lower Upper
138 100
92 49.7 41.0 61.4
108 78.6 60.1 90.1









#66
4,6-Dinitro-2-methylphenol
Concen: 19.743 ng/ul
RT: 15.428 min Scan# 2114
Delta R.T. 0.000 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:198 Resp: 157690
Ion Ratio Lower Upper
198 100
182 4.5 3.0 4.6
77 23.6 19.4 29.2

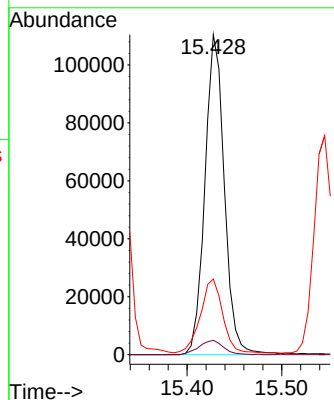

#67
N-Nitrosodiphenylamine
Concen: 24.192 ng/ul
RT: 15.545 min Scan# 2135
Delta R.T. -0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36


Tgt Ion:169 Resp: 996712
Ion Ratio Lower Upper
169 100
168 67.6 52.7 79.1
167 35.6 29.6 44.4

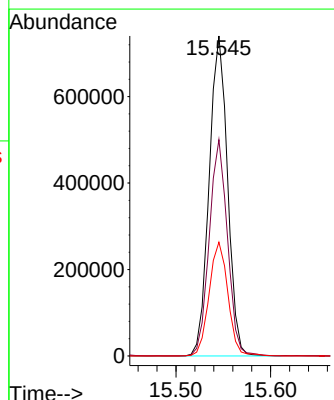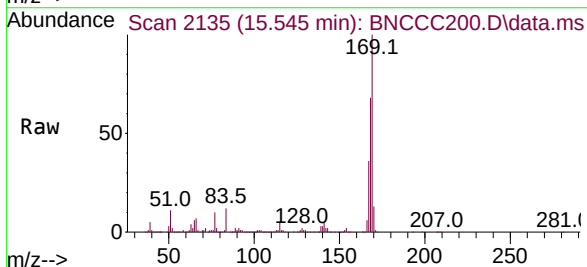






#68
4-Bromophenyl-phenylether
Concen: 23.913 ng/ul
RT: 16.222 min Scan# 21
Delta R.T. -0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36


Instrument :
BNA_N
ClientSampleId :





Tgt Ion:248 Resp: 346318
Ion Ratio Lower Upper
248 100
250 108.8 76.5 114.7
141 82.0 63.9 95.9

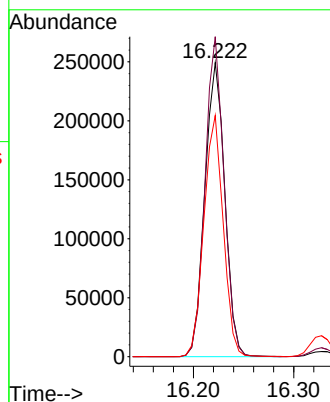


#69
Hexachlorobenzene
Concen: 24.265 ng/ul
RT: 16.328 min Scan# 2268
Delta R.T. -0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36

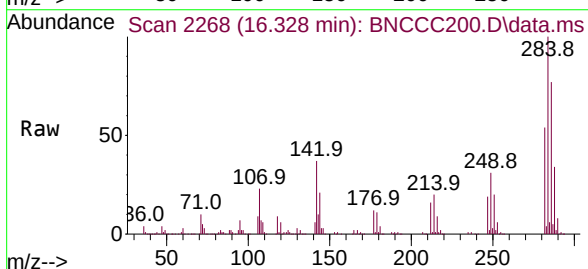

Tgt Ion:284 Resp: 398298
Ion Ratio Lower Upper
284 100
142 37.2 31.1 46.7
249 30.5 25.7 38.5





#70

Atrazine

Concen: 20.481 ng/ul

RT: 16.504 min Scan# 21

Delta R.T. 0.000 min


Lab File: BNCCC200.D

Acq: 23 Jun 2024 13:36

Instrument :

BNA_N

ClientSampleId :






Tgt Ion:200 Resp: 266436

Ion Ratio Lower Upper

200 100

173 28.3 21.2 31.8

215 50.3 38.9 58.3



#71

Pentachlorophenol

Concen: 21.325 ng/ul

RT: 16.686 min Scan# 2329

Delta R.T. 0.000 min

Lab File: BNCCC200.D

Acq: 23 Jun 2024 13:36




Tgt Ion:266 Resp: 223950


Ion Ratio Lower Upper

266 100

264 61.2 54.7 82.1

268 61.6 53.4 80.2


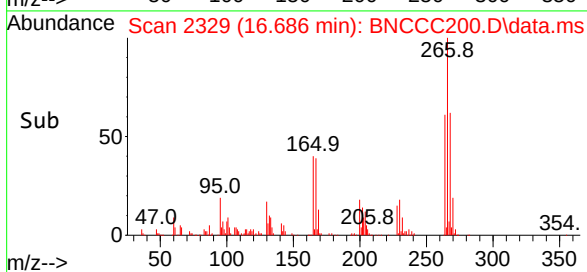

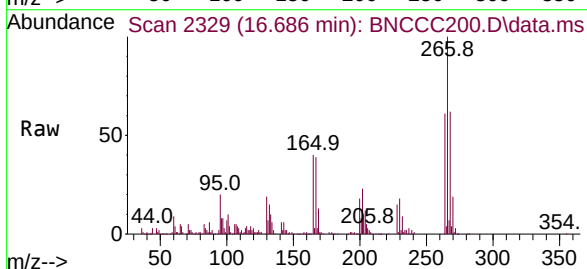




#72
Phenanthrene
Concen: 22.618 ng/u1
RT: 17.069 min Scan# 21
Delta R.T. -0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:178 Resp: 1722213
Ion Ratio Lower Upper
178 100
179 15.5 12.6 19.0
176 19.0 15.8 23.6

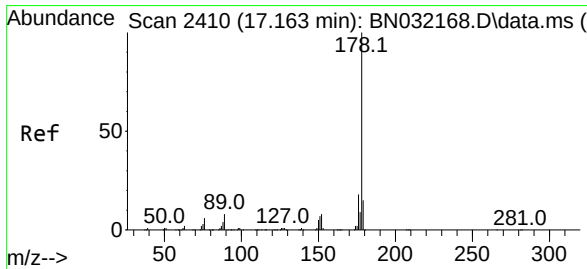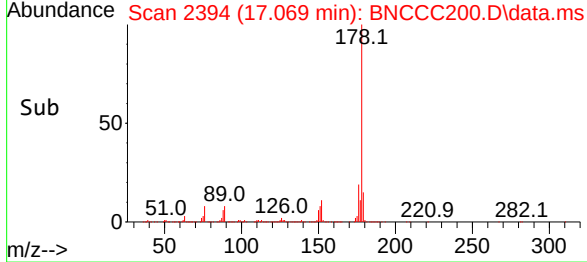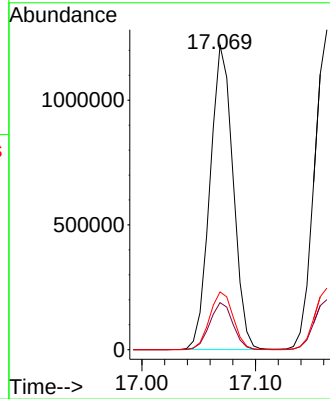

#74
Anthracene
Concen: 23.378 ng/u1
RT: 17.163 min Scan# 2410
Delta R.T. 0.000 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36

Tgt Ion:178 Resp: 1803727
Ion Ratio Lower Upper
178 100
179 15.6 11.8 17.6
176 19.3 14.8 22.2


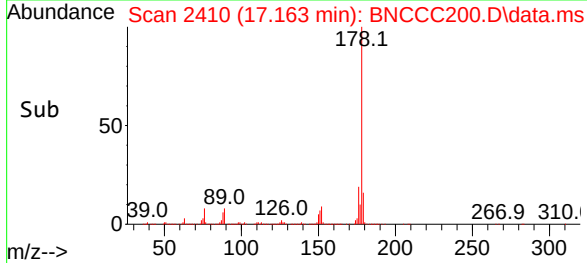

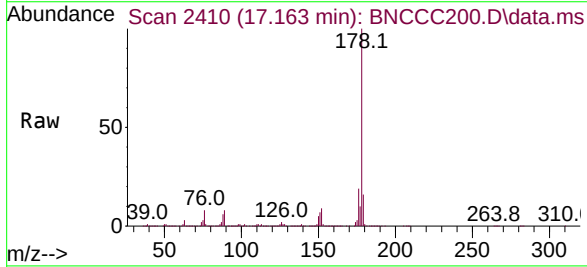




#75
1,2,3,4-Tetrachlorobenzene
Concen: 27.176 ng/uL
RT: 13.063 min Scan# 1713
Delta R.T. -0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:216 Resp: 522832
Ion Ratio Lower Upper
216 100
214 76.5 62.1 93.1
218 47.2 40.2 60.4

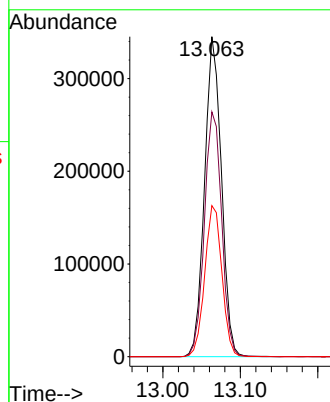

#76
Pentachlorobenzene
Concen: 26.513 ng/uL
RT: 14.592 min Scan# 1973
Delta R.T. -0.006 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36


Tgt Ion:250 Resp: 496826
Ion Ratio Lower Upper
250 100
248 61.0 49.8 74.6
252 60.5 52.3 78.5

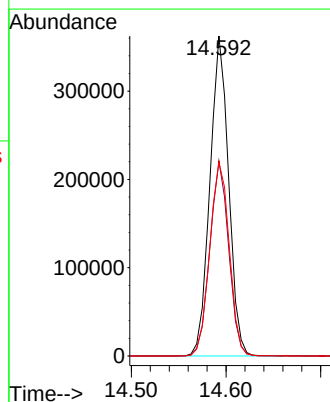






#77
 Carbazole
 Concen: 24.719 ng/ul
 RT: 17.439 min Scan# 2457
 Delta R.T. 0.000 min
 Lab File: BNCCC200.D
 Acq: 23 Jun 2024 13:36

Instrument :
 BNA_N
 ClientSampleId :







Tgt Ion:167 Resp: 1626205
 Ion Ratio Lower Upper
 167 100
 166 22.1 17.9 26.9
 139 13.2 10.5 15.7

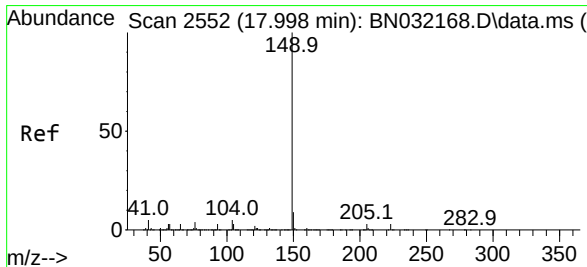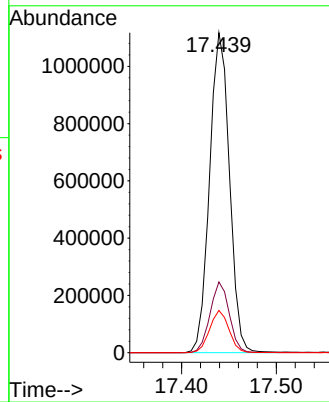

#78
 Di-n-butylphthalate
 Concen: 22.421 ng/ul
 RT: 17.998 min Scan# 2552
 Delta R.T. -0.006 min
 Lab File: BNCCC200.D
 Acq: 23 Jun 2024 13:36

Tgt Ion:149 Resp: 2029377
 Ion Ratio Lower Upper
 149 100
 150 9.1 7.4 11.0
 104 4.9 4.1 6.1

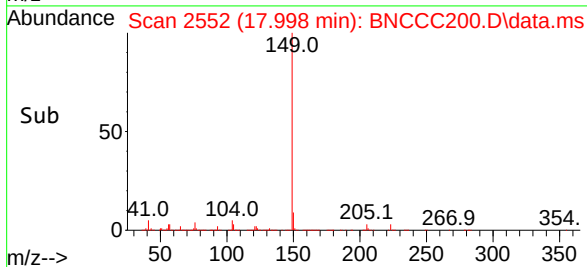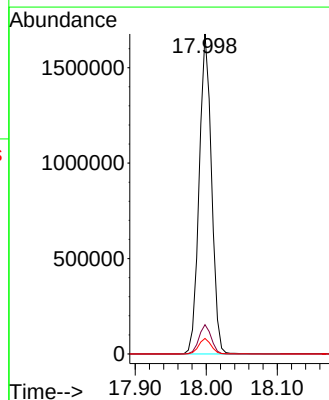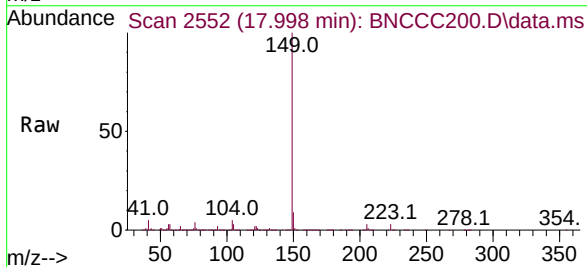







#80
 Fluoranthene
 Concen: 23.381 ng/u1
 RT: 19.098 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BNCCC200.D
 Acq: 23 Jun 2024 13:36

Instrument :
 BNA_N
 ClientSampleId :

Tgt Ion:202 Resp: 1962750




Ion	Ratio	Lower	Upper
202	100		
101	10.7	10.3	15.5
100	8.1	8.0	12.0

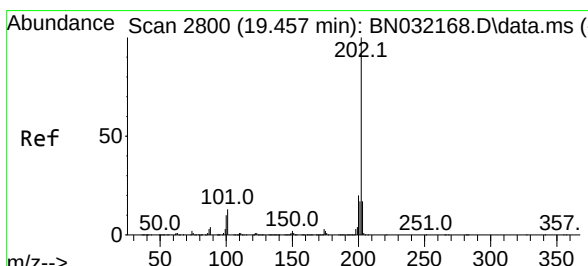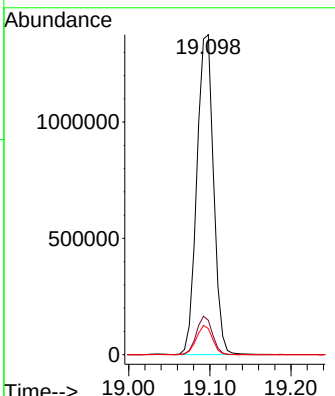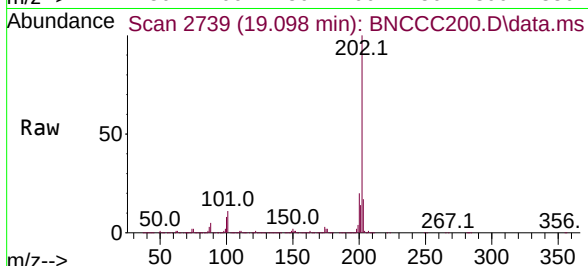


#82
 Pyrene
 Concen: 23.518 ng/u1
 RT: 19.457 min Scan# 2800
 Delta R.T. -0.006 min
 Lab File: BNCCC200.D
 Acq: 23 Jun 2024 13:36

Tgt Ion:202 Resp: 2025611

Ion	Ratio	Lower	Upper
202	100		
101	13.4	12.6	18.8
100	11.5	10.2	15.2


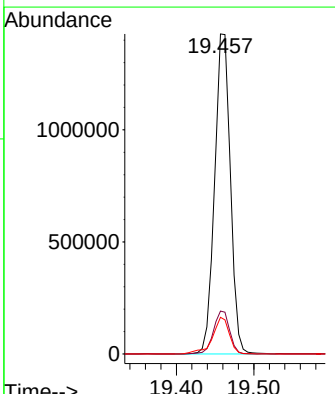
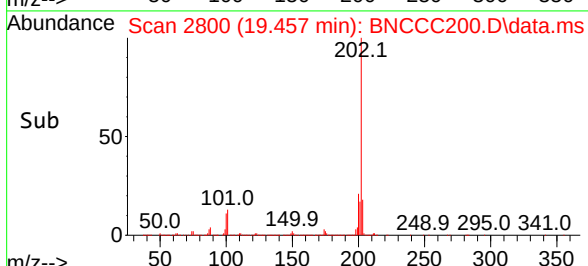





#83
Butylbenzylphthalate
Concen: 22.605 ng/ul
RT: 20.369 min Scan# 2954
Delta R.T. 0.000 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:	149	Resp:	919579
Ion Ratio	Lower	Upper	
149	100		
91	63.4	61.0	91.4
206	21.2	16.5	24.7

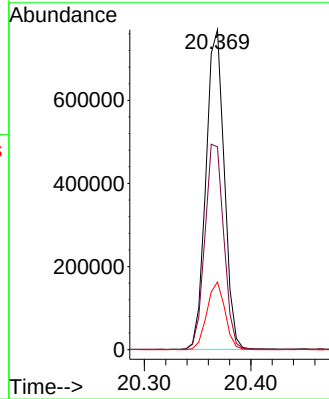

#84
3,3'-Dichlorobenzidine
Concen: 23.920 ng/ul
RT: 21.180 min Scan# 3093
Delta R.T. 0.000 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36

Tgt Ion:	252	Resp:	602105
Ion Ratio	Lower	Upper	
252	100		
254	69.6	53.6	80.4
126	12.4	10.2	15.4

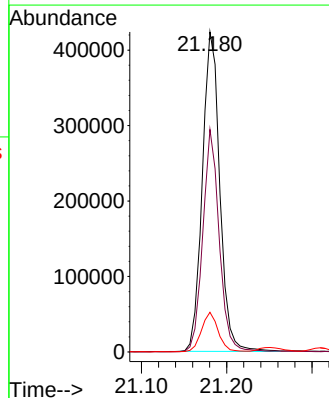



#85

Benzo(a)anthracene

Concen: 22.968 ng/ul

RT: 21.251 min Scan# 3105

Delta R.T. 0.000 min


Lab File: BNCCC200.D

Acq: 23 Jun 2024 13:36

Instrument :

BNA_N

ClientSampleId :






Tgt Ion:228 Resp: 2017964

Ion Ratio Lower Upper

228 100

229 19.5 16.7 25.1

226 27.4 22.8 34.2



#86

Bis(2-ethylhexyl)phthalate

Concen: 22.226 ng/ul

RT: 21.169 min Scan# 3091

Delta R.T. -0.006 min

Lab File: BNCCC200.D

Acq: 23 Jun 2024 13:36




Tgt Ion:149 Resp: 1317985


Ion Ratio Lower Upper

149 100

167 26.9 21.4 32.0

279 3.9 3.3 4.9

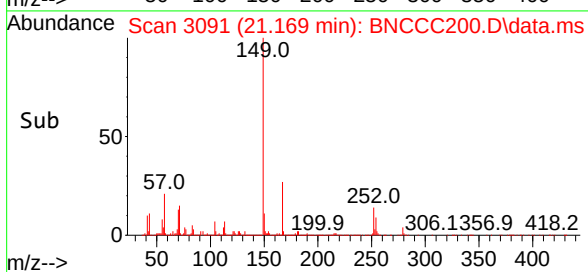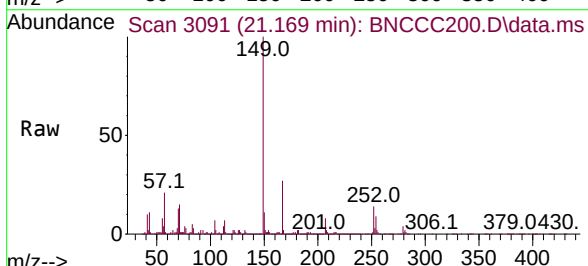







#87
 Chrysene
 Concen: 23.505 ng/u1
 RT: 21.310 min Scan# 3115
 Delta R.T. 0.000 min
 Lab File: BNCCC200.D
 Acq: 23 Jun 2024 13:36

Instrument :
 BNA_N
 ClientSampleId :




Tgt Ion:228 Resp: 1929001


Ion	Ratio	Lower	Upper
228	100		
226	30.4	23.7	35.5
229	19.5	15.1	22.7

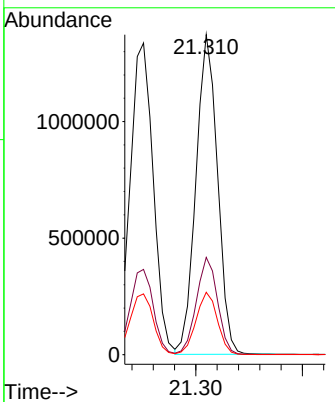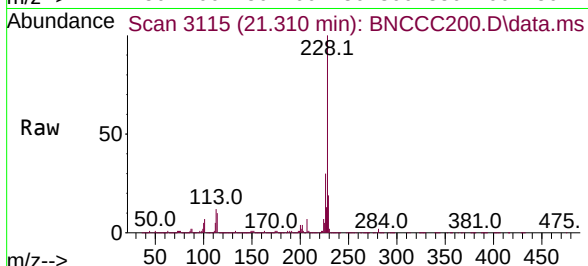

#89
 Di-n-octyl phthalate
 Concen: 21.637 ng/u1
 RT: 22.269 min Scan# 3278
 Delta R.T. -0.006 min
 Lab File: BNCCC200.D
 Acq: 23 Jun 2024 13:36

Tgt Ion:149 Resp: 2357275


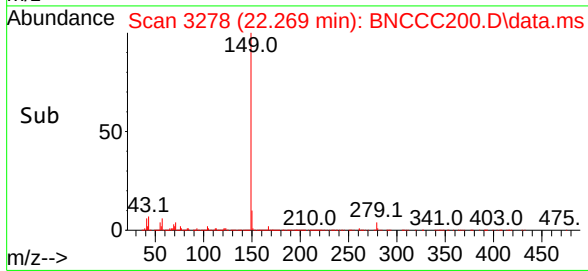
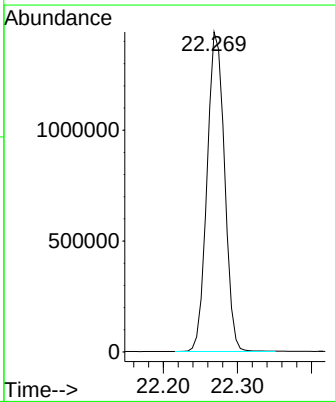
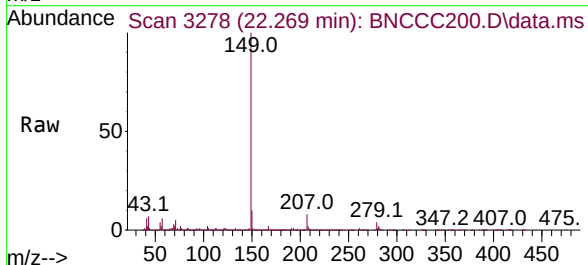




#90
Benzo(b)fluoranthene
Concen: 21.679 ng/ul
RT: 23.263 min Scan# 3445
Delta R.T. 0.000 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:252 Resp: 2108709
Ion Ratio Lower Upper
252 100
253 22.6 17.0 25.6
125 11.2 9.2 13.8



#91
Benzo(k)fluoranthene
Concen: 21.985 ng/ul
RT: 23.321 min Scan# 3457
Delta R.T. 0.000 min
Lab File: BNCCC200.D
Acq: 23 Jun 2024 13:36

Tgt Ion:252 Resp: 2098453
Ion Ratio Lower Upper
252 100
253 22.1 17.6 26.4
125 10.6 9.4 14.2





#93

Benzo(a)pyrene

Concen: 22.163 ng/ul

RT: 24.045 min Scan# 31

Delta R.T. 0.006 min

Lab File: BNCCC200.D

Acq: 23 Jun 2024 13:36

Instrument :

BNA_N

ClientSampleId :





Tgt Ion:252 Resp: 2019108

Ion Ratio Lower Upper

252 100

253 21.7 16.6 24.8

125 11.8 9.8 14.8



#94

Indeno(1,2,3-cd)pyrene

Concen: 23.380 ng/ul

RT: 27.468 min Scan# 4162

Delta R.T. 0.024 min

Lab File: BNCCC200.D

Acq: 23 Jun 2024 13:36




Tgt Ion:276 Resp: 2454469


Ion Ratio Lower Upper

276 100

138 21.7 18.1 27.1

277 23.4 18.2 27.2





#95

Dibenzo(a,h)anthracene

Concen: 24.132 ng/ul

RT: 27.515 min Scan# 41

Delta R.T. 0.012 min

Lab File: BNCCC200.D

Acq: 23 Jun 2024 13:36

Instrument :

BNA_N

ClientSampleId :





Tgt Ion:278 Resp: 2068258

Ion Ratio Lower Upper

278 100

139 17.5 15.0 22.6

279 22.8 17.4 26.0



#96

Benzo(g,h,i)perylene

Concen: 24.156 ng/ul

RT: 28.492 min Scan# 4336

Delta R.T. 0.024 min

Lab File: BNCCC200.D

Acq: 23 Jun 2024 13:36

Tgt Ion:276 Resp: 2015838

Ion Ratio Lower Upper

276 100

138 22.4 20.9 31.3

277 23.9 18.0 27.0

