




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032183.D
Acq On : 23 Jun 2024 01:47
Operator : MA/JU
Sample : PB161556BS
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLCS556

Manual IntegrationsAPPROVED

Quant Time: Jun 23 02:27:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 10:49:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/26/2024

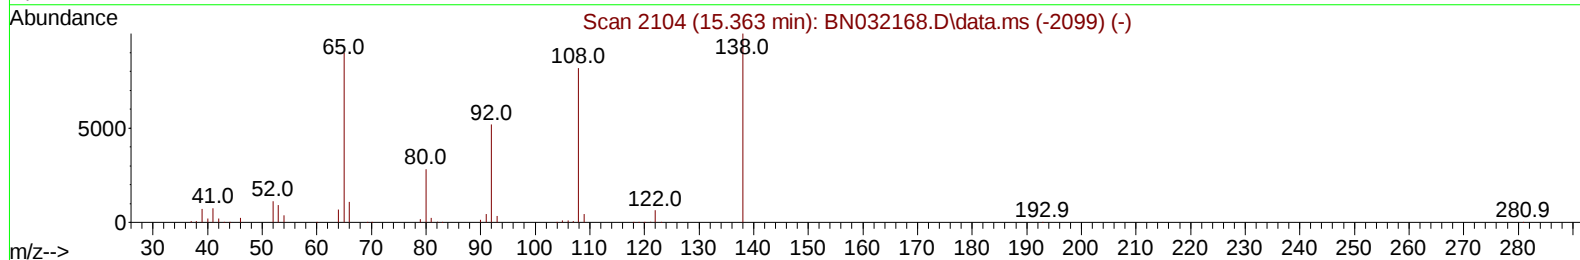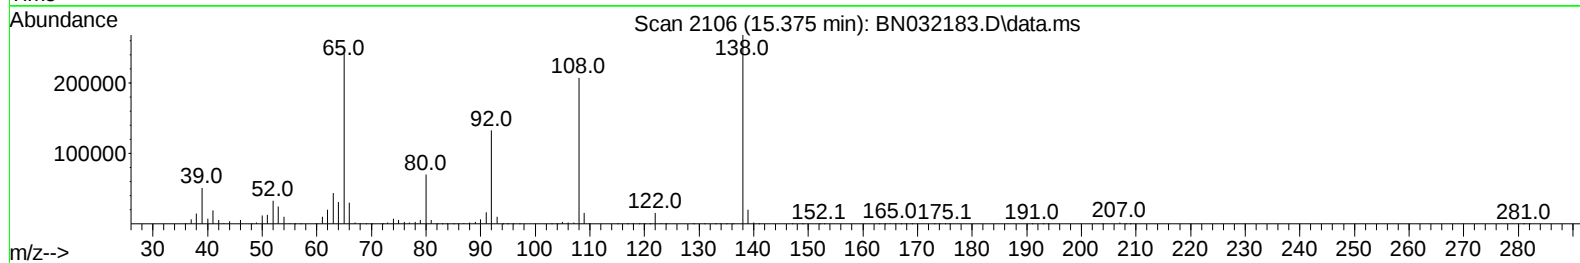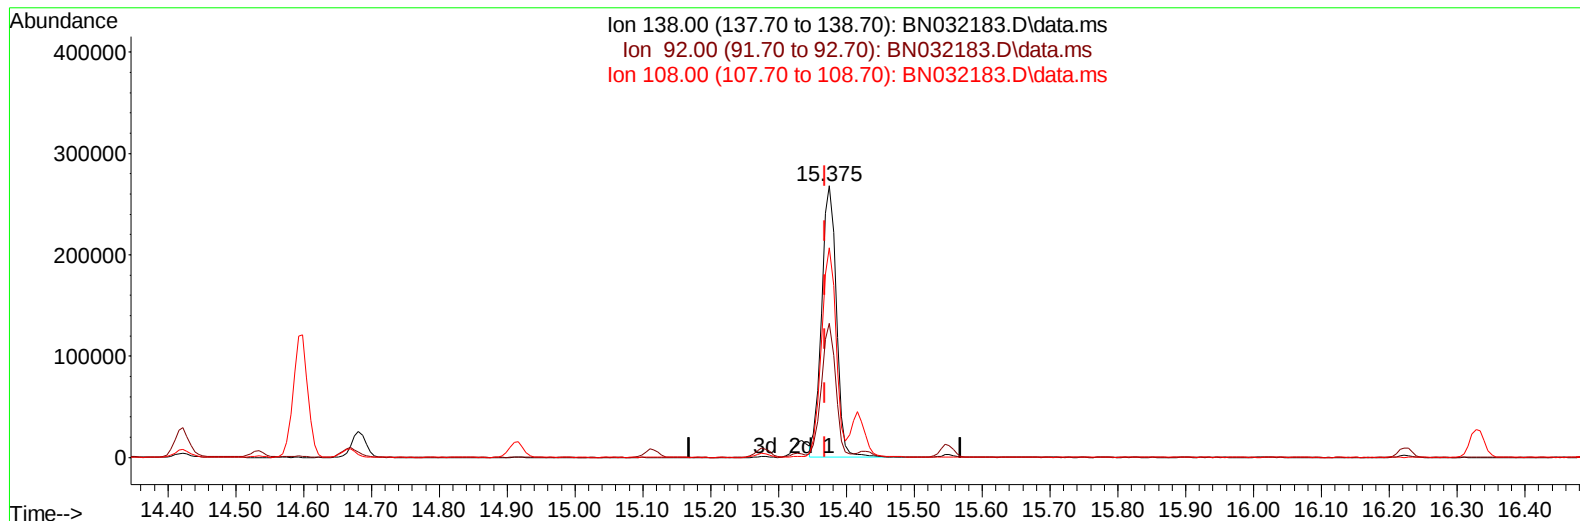

TIC: BN032183.D\data.ms

(63) 4-Nitroaniline

15.375min (+ 0.006) 33.64 ng/ul

response 406131

Ion	Exp%	Act%
138.00	100.00	100.00
92.00	51.20	49.37
108.00	75.10	77.29
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BN032183.D
 Acq On : 23 Jun 2024 01:47
 Operator : MA/JU
 Sample : PB161556BS
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLCS556

Manual IntegrationsAPPROVED

Quant Time: Jun 23 02:27:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 10:49:40 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
 Supervised By :mohammad ahmed 06/26/2024

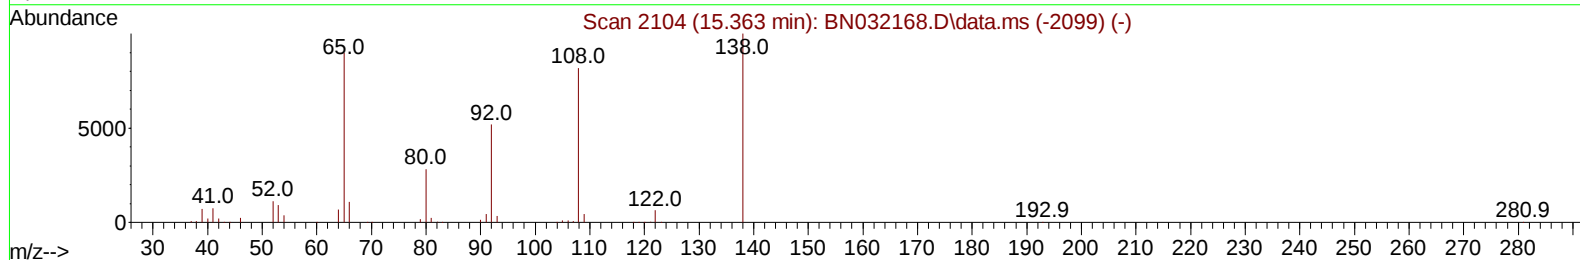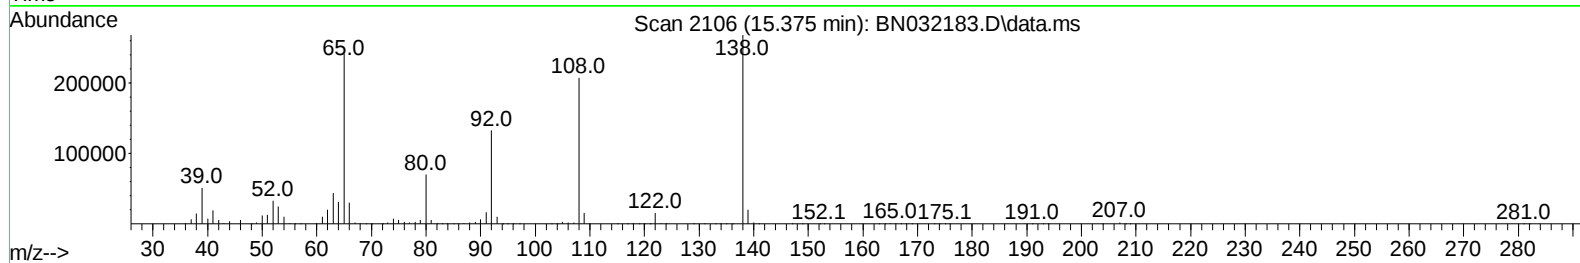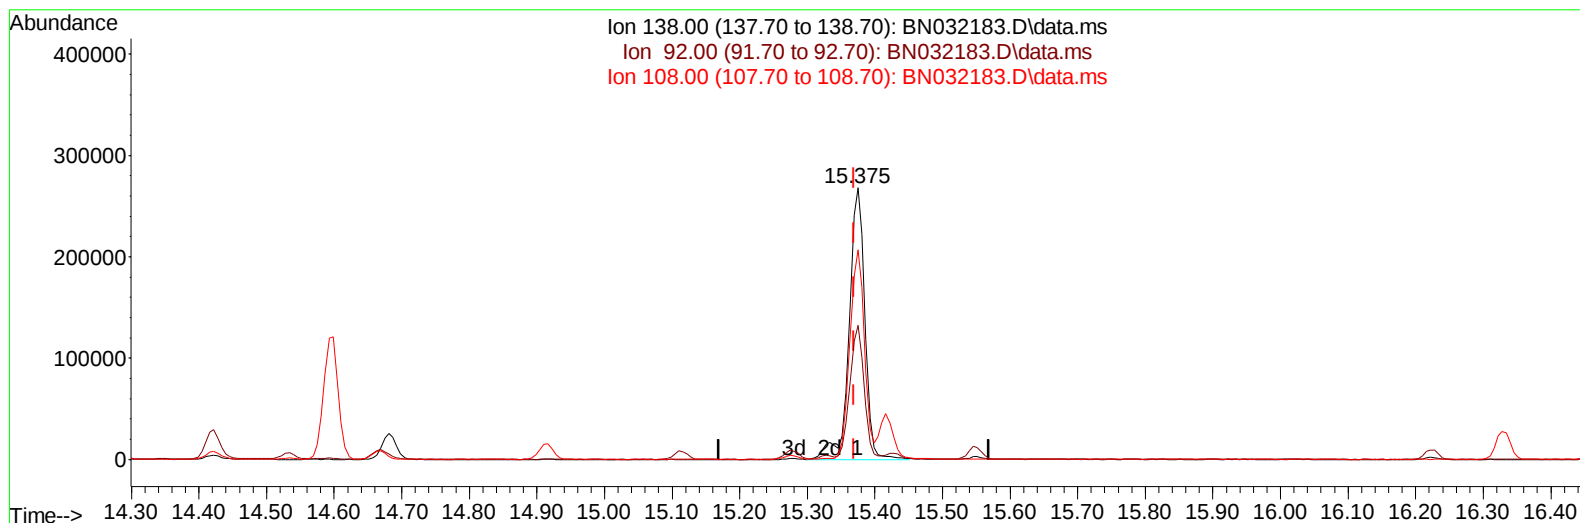

TIC: BN032183.D\data.ms

(63) 4-Nitroaniline

15.375min (+ 0.006) 35.83 ng/ul m

response 432557

Ion	Exp%	Act%
138.00	100.00	100.00
92.00	51.20	49.37
108.00	75.10	77.29
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BN032183.D
 Acq On : 23 Jun 2024 01:47
 Operator : MA/JU
 Sample : PB161556BS
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLCS556

Manual IntegrationsAPPROVED

Quant Time: Jun 23 02:30:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 10:49:40 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
 Supervised By :mohammad ahmed 06/26/2024

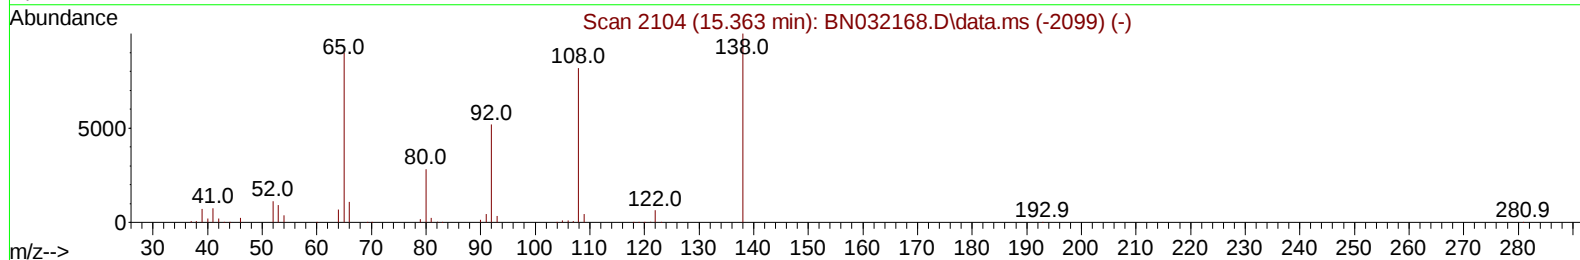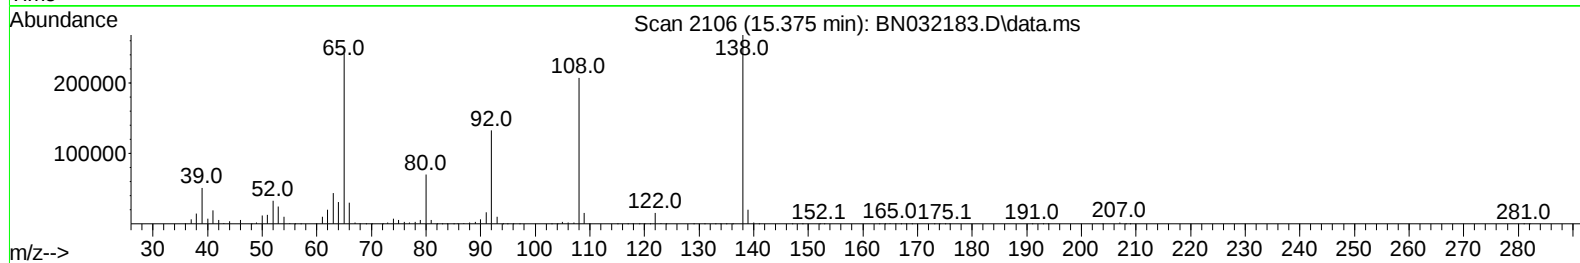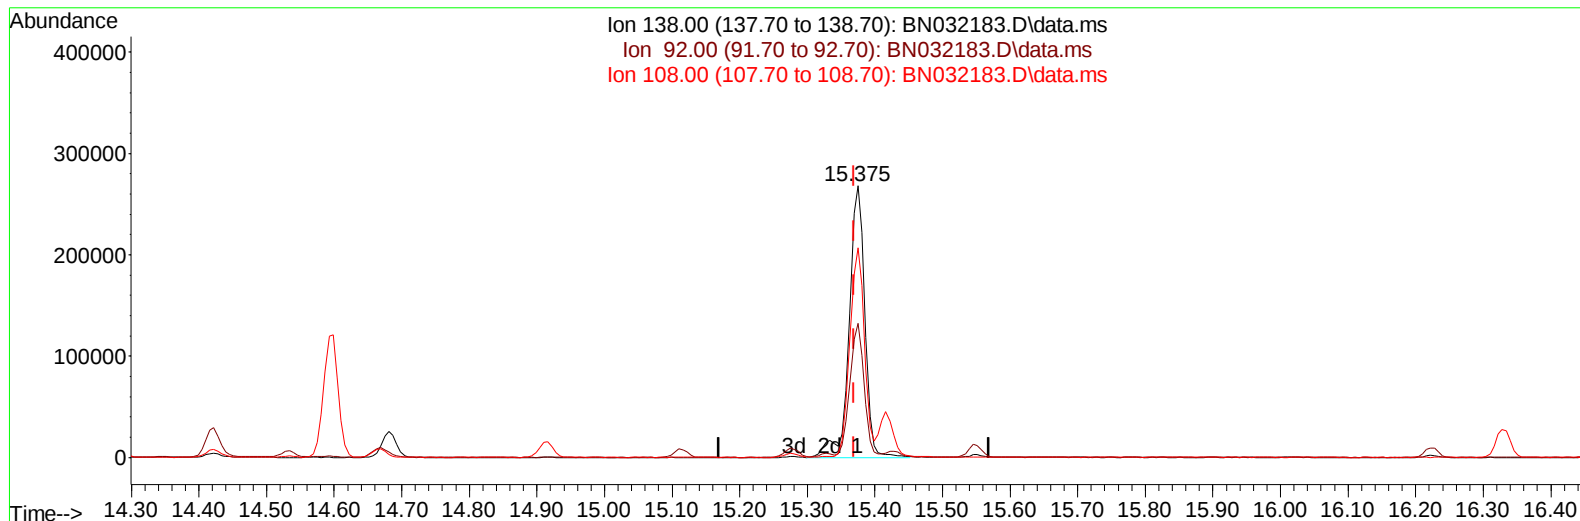

TIC: BN032183.D\data.ms

(63) 4-Nitroaniline

15.375min (+ 0.006) 35.83 ng/ul m

response 432557

Ion	Exp%	Act%
138.00	100.00	100.00
92.00	51.20	49.37
108.00	75.10	77.29
0.00	0.00	0.00