




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032187.D
Acq On : 23 Jun 2024 05:04
Operator : MA/JU
Sample : P2775-24
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4D56

Manual IntegrationsAPPROVED

Quant Time: Jun 23 05:34:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 10:49:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/26/2024

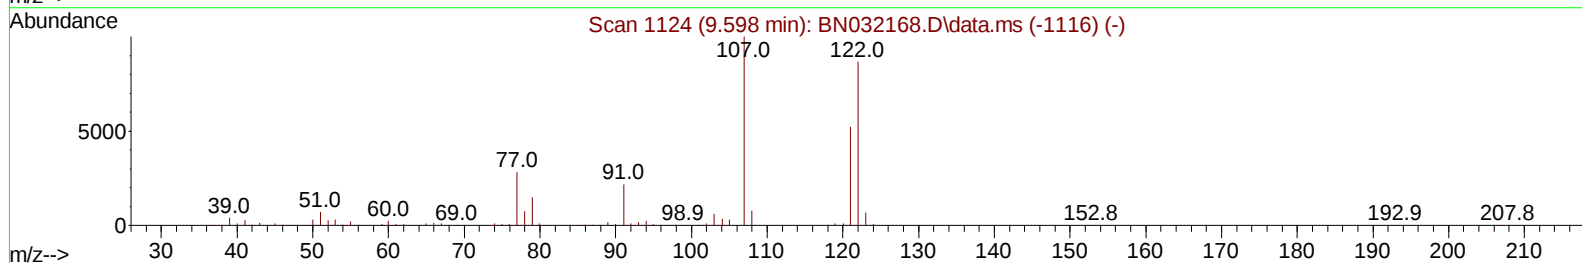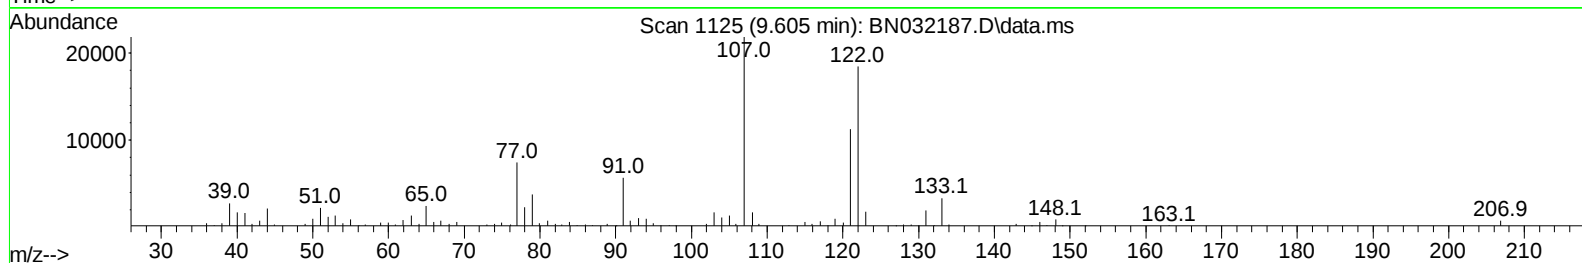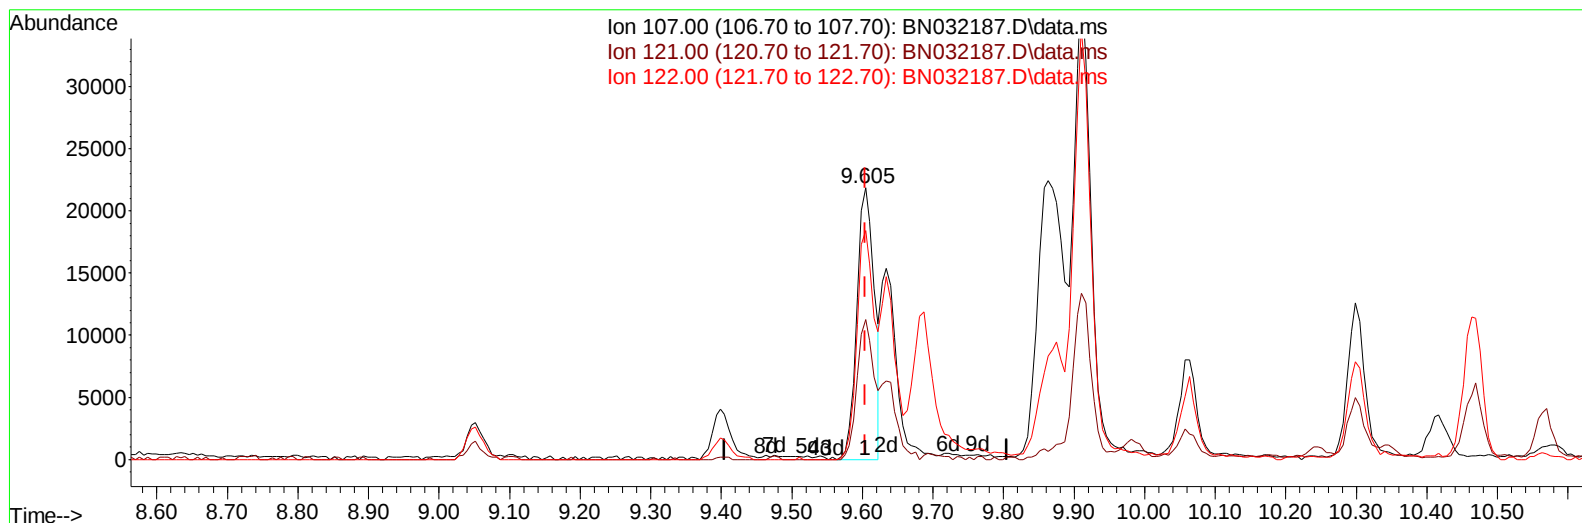

TIC: BN032187.D\data.ms

(26) 2,4-Dimethylphenol

9.605min (+ 0.000) 1.82 ng/u1

response 38185

Ion	Exp%	Act%
107.00	100.00	100.00
121.00	51.00	51.48
122.00	88.00	84.37
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BN032187.D
 Acq On : 23 Jun 2024 05:04
 Operator : MA/JU
 Sample : P2775-24
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4D56

Manual IntegrationsAPPROVED

Quant Time: Jun 23 05:34:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 10:49:40 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
 Supervised By :mohammad ahmed 06/26/2024

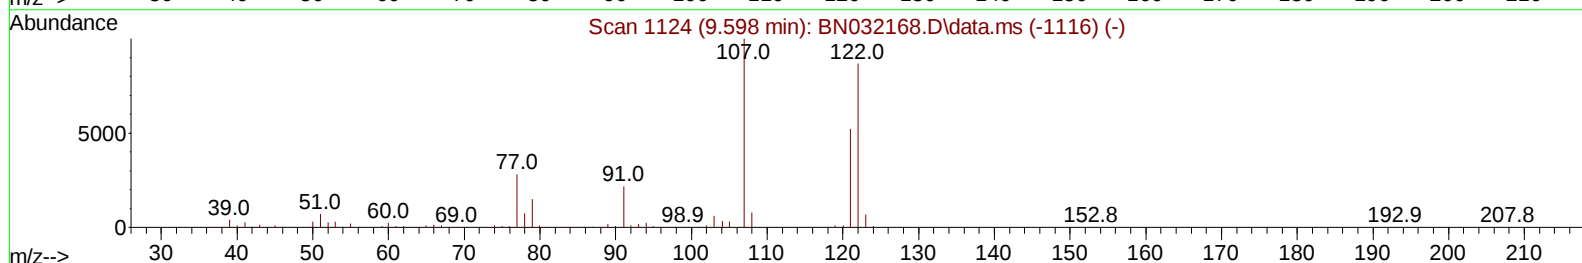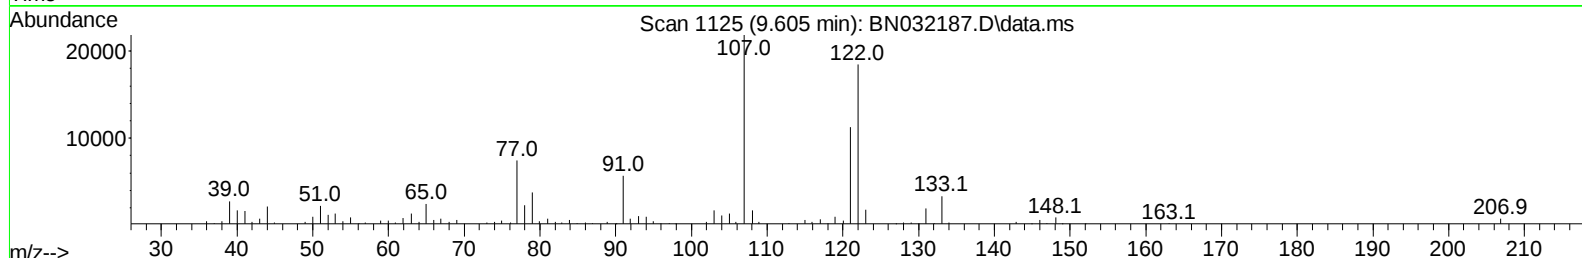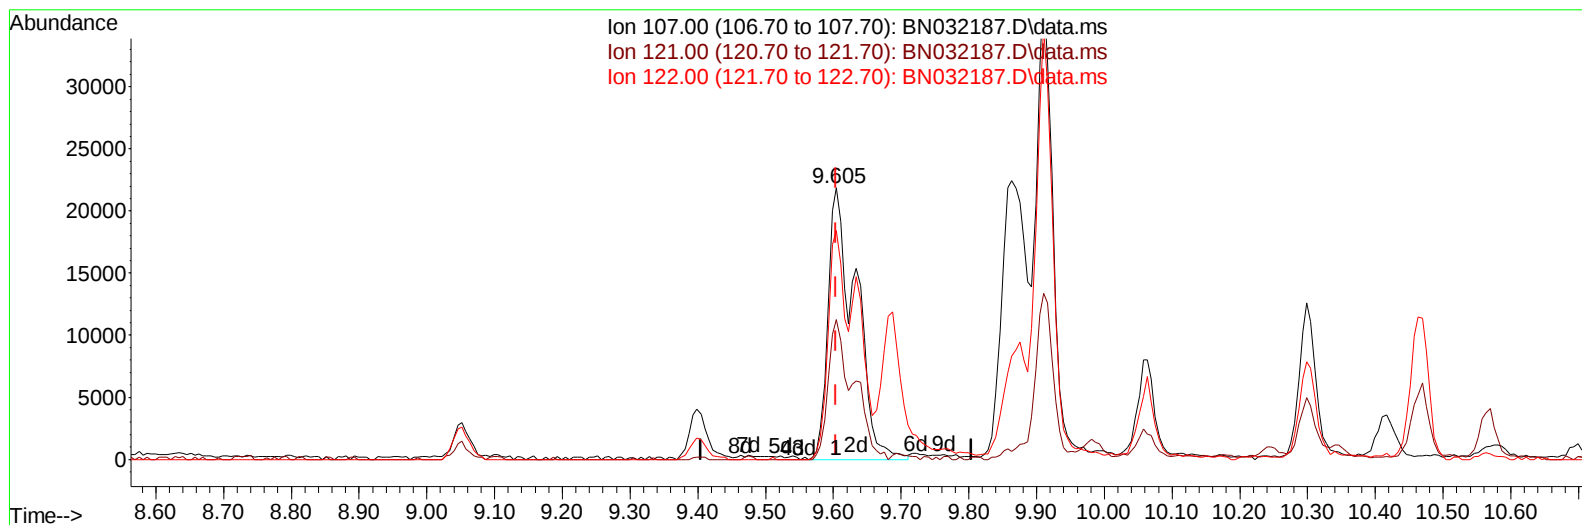

TIC: BN032187.D\data.ms

(26) 2,4-Dimethylphenol

9.605min (+ 0.000) 2.95 ng/u1 m

response 62026

Ion	Exp%	Act%
107.00	100.00	100.00
121.00	51.00	51.48
122.00	88.00	84.37
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032187.D
Acq On : 23 Jun 2024 05:04
Operator : MA/JU
Sample : P2775-24
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4D56

Manual IntegrationsAPPROVED

Quant Time: Jun 23 05:36:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 10:49:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/26/2024

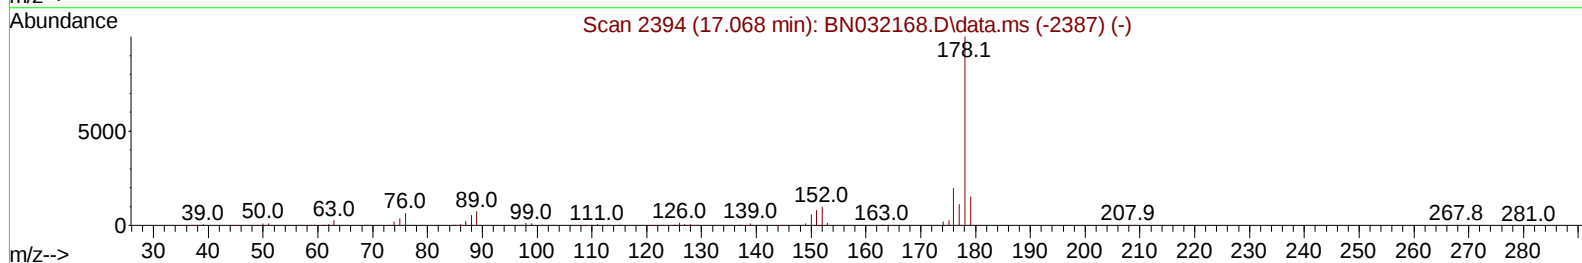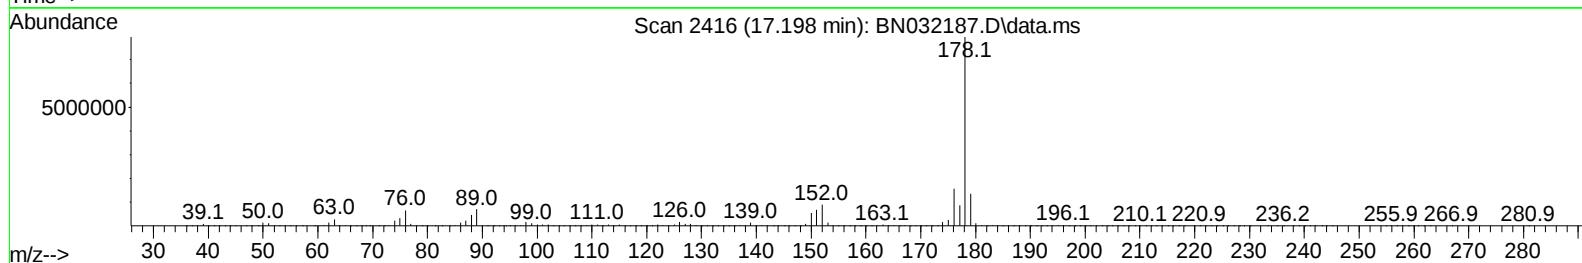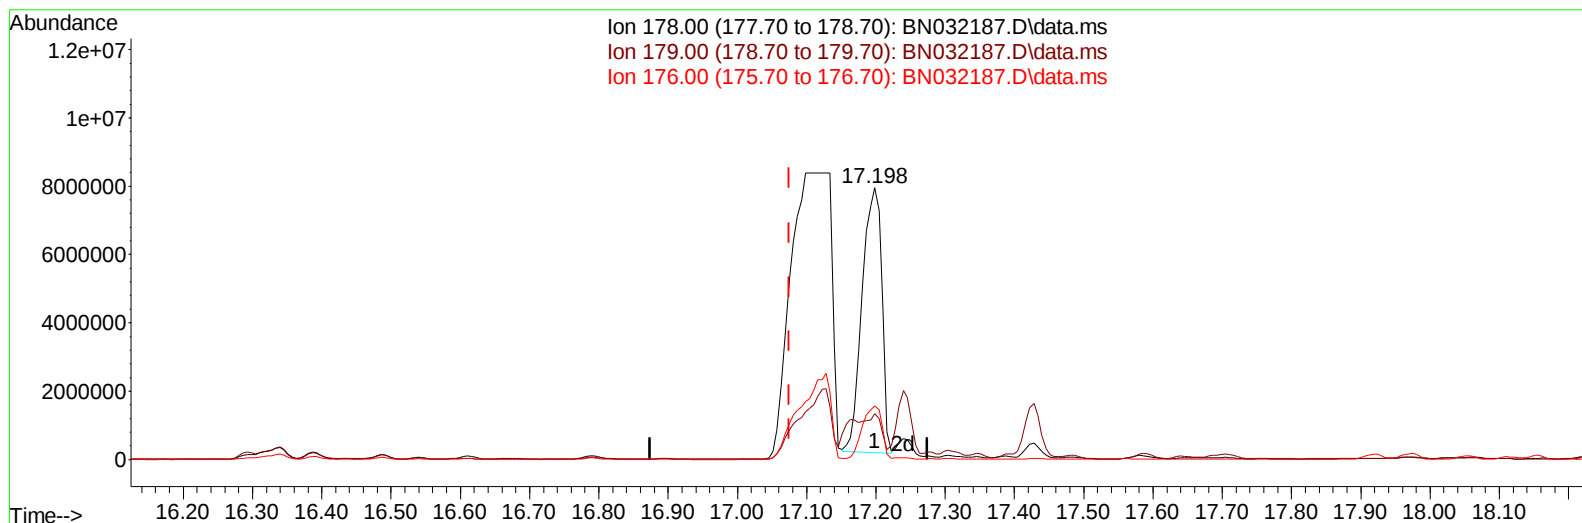

TIC: BN032187.D\data.ms

(72) Phenanthrene

17.198min (+ 0.124) 254.20 ng/u1

response 15213334

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.80	16.91
176.00	19.70	19.68
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032187.D
Acq On : 23 Jun 2024 05:04
Operator : MA/JU
Sample : P2775-24
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4D56

Manual IntegrationsAPPROVED

Quant Time: Jun 23 05:36:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 10:49:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/26/2024

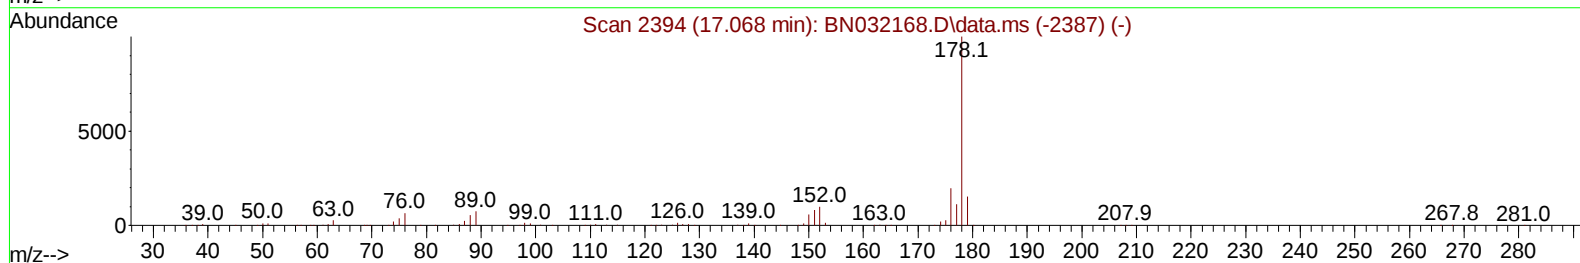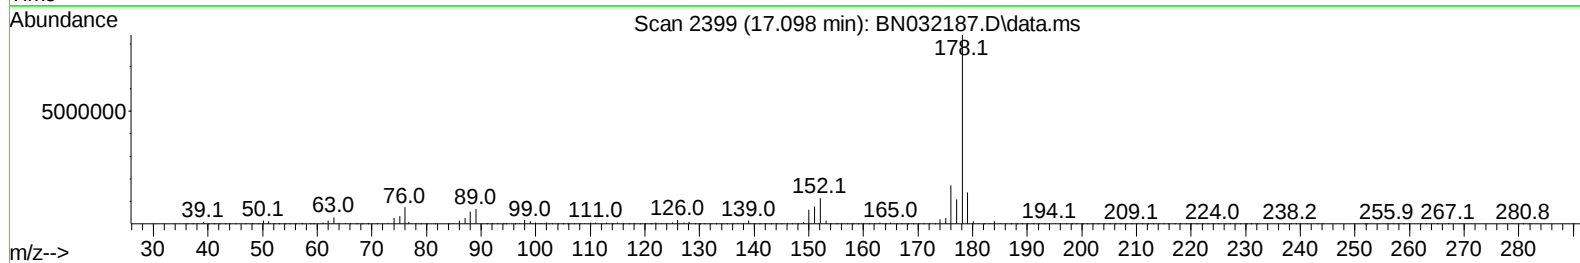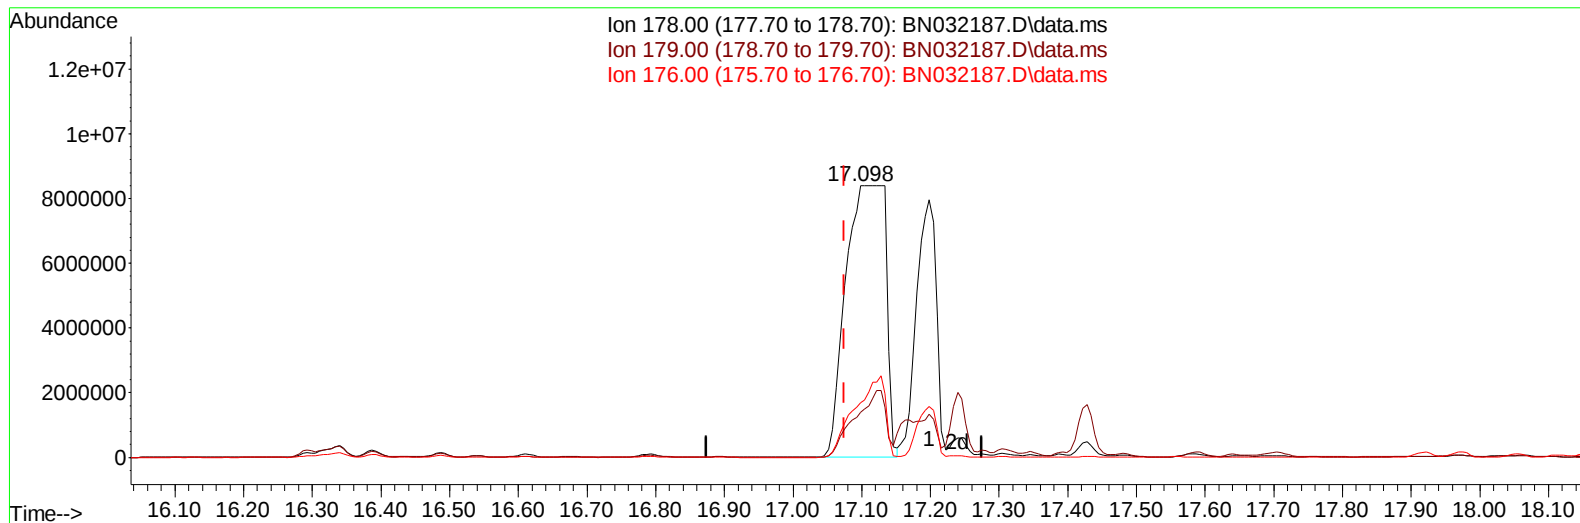

TIC: BN032187.D\data.ms

(72) Phenanthrene

17.098min (+ 0.024) 565.72 ng/u1 m

response 33857387

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.80	16.60
176.00	19.70	20.30
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BN032187.D
 Acq On : 23 Jun 2024 05:04
 Operator : MA/JU
 Sample : P2775-24
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4D56

Manual IntegrationsAPPROVED

Quant Time: Jun 23 05:37:00 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 10:49:40 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
 Supervised By :mohammad ahmed 06/26/2024

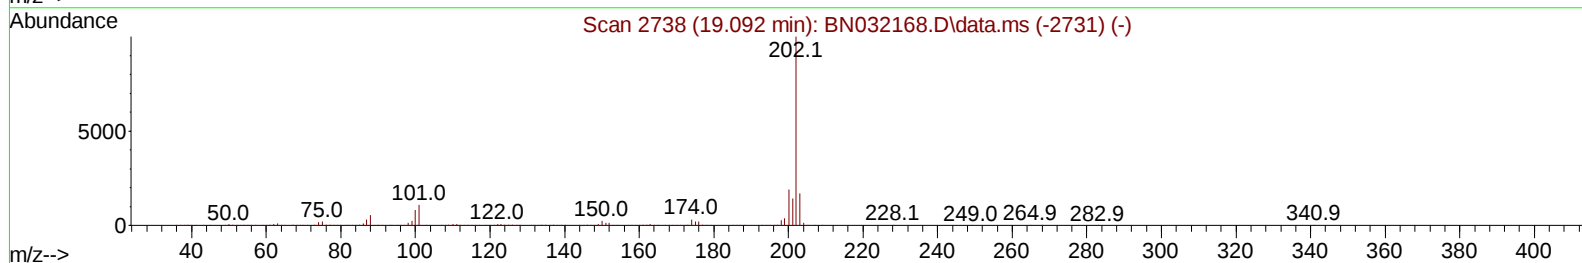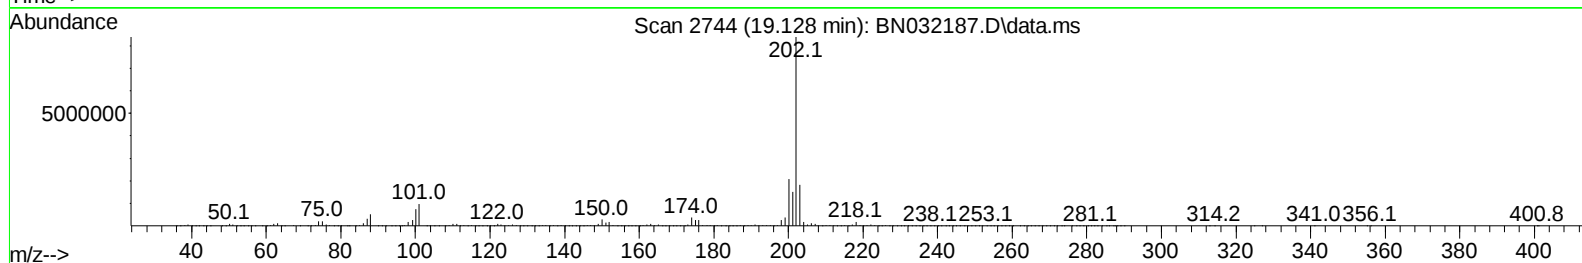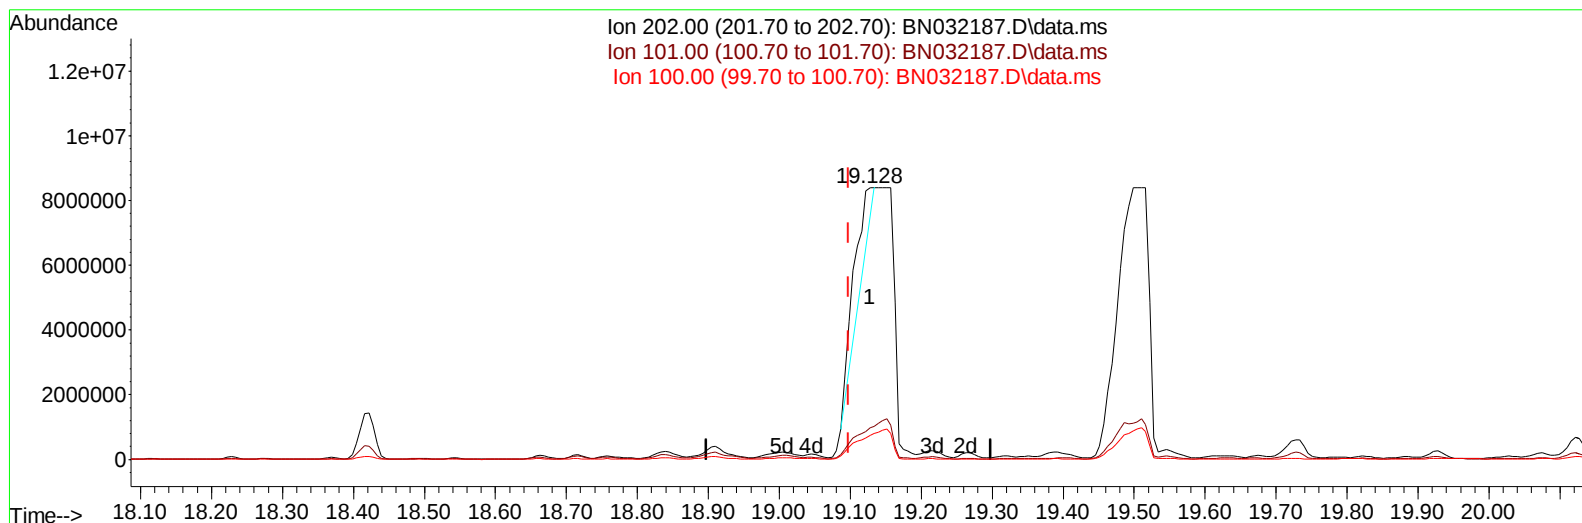

TIC: BN032187.D\data.ms

(80) Fluoranthene

19.128min (+ 0.030) 144.18 ng/u1

response 5241288

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	12.90	11.66
100.00	10.00	8.85
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BN032187.D
 Acq On : 23 Jun 2024 05:04
 Operator : MA/JU
 Sample : P2775-24
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4D56

Manual IntegrationsAPPROVED

Quant Time: Jun 23 05:37:00 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 10:49:40 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
 Supervised By :mohammad ahmed 06/26/2024

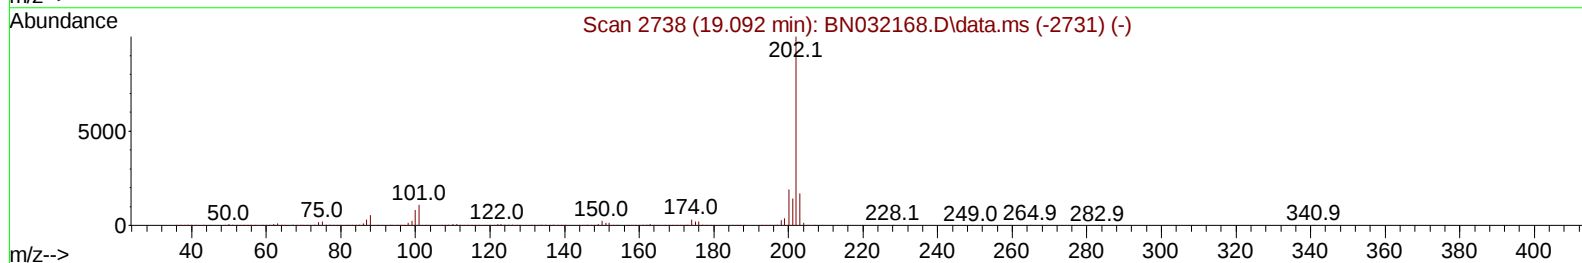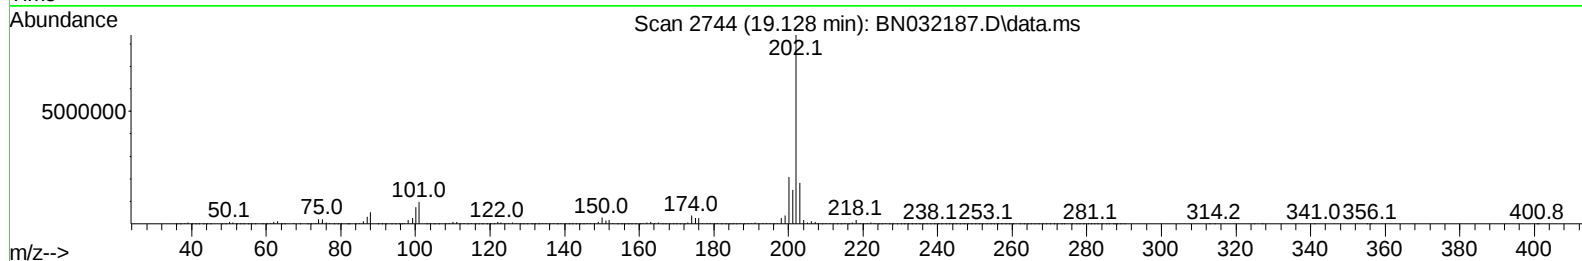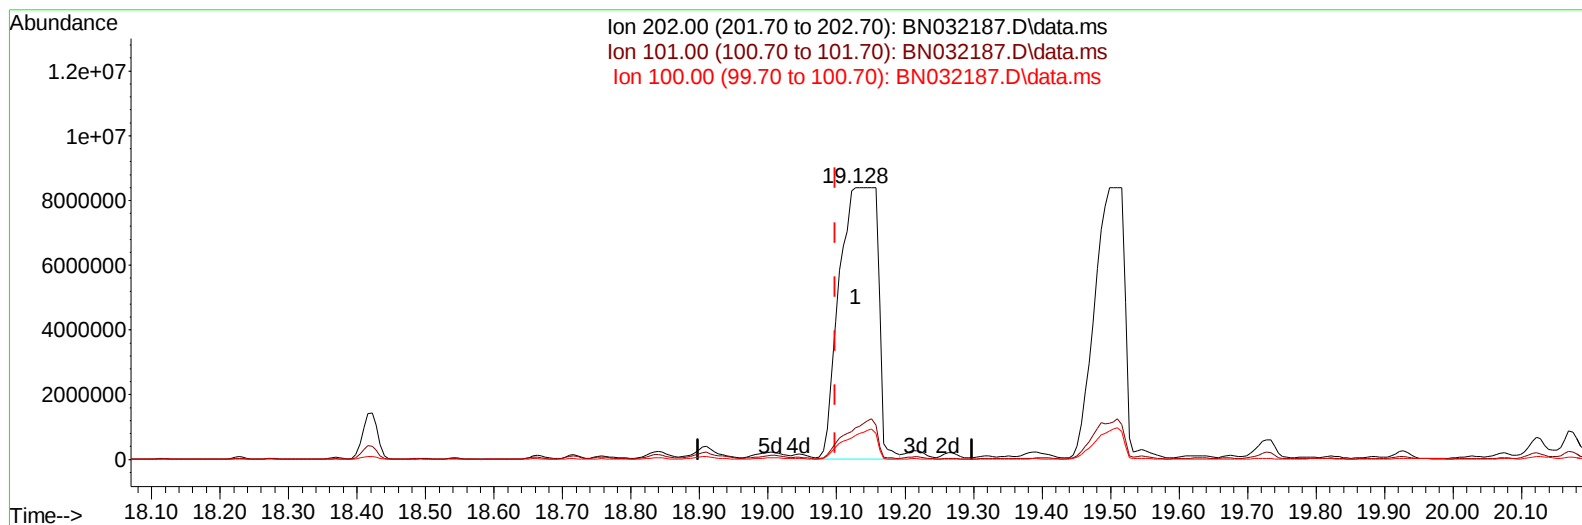

TIC: BN032187.D\data.ms

(80) Fluoranthene

19.128min (+ 0.030) 896.27 ng/u1 m

response 32581142

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	12.90	11.66
100.00	10.00	8.85
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BN032187.D
 Acq On : 23 Jun 2024 05:04
 Operator : MA/JU
 Sample : P2775-24
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4D56

Manual IntegrationsAPPROVED

Quant Time: Jun 23 05:37:00 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 10:49:40 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
 Supervised By :mohammad ahmed 06/26/2024

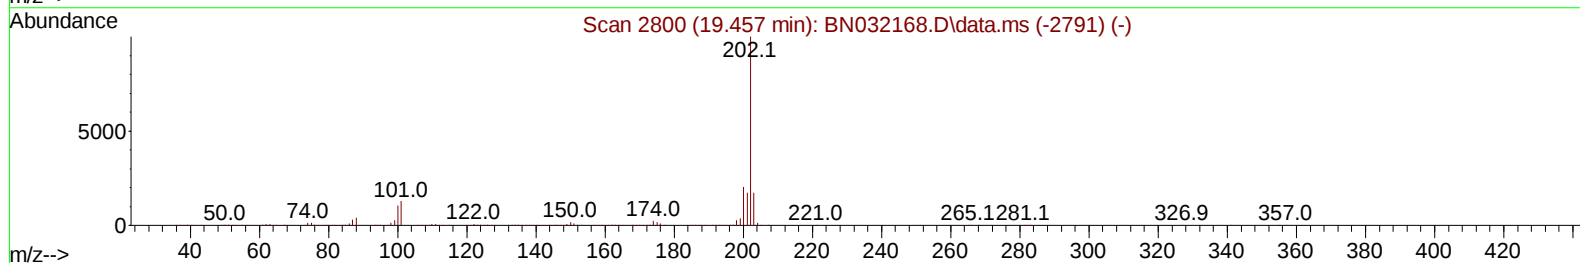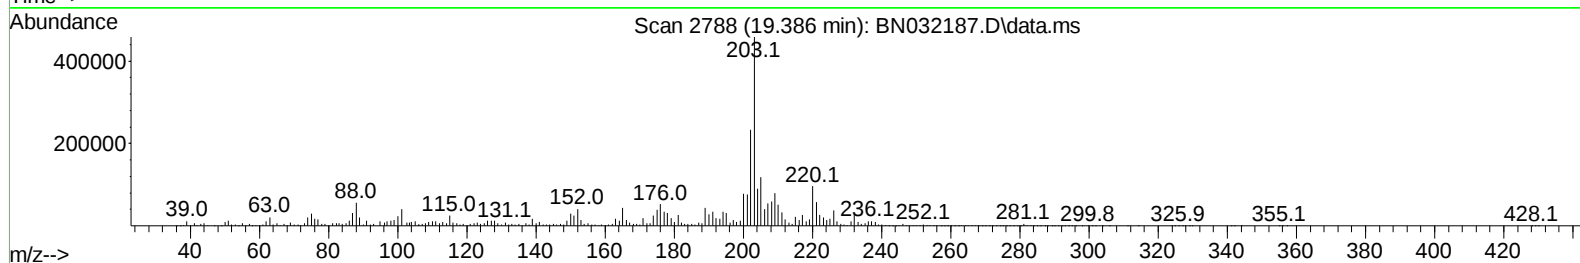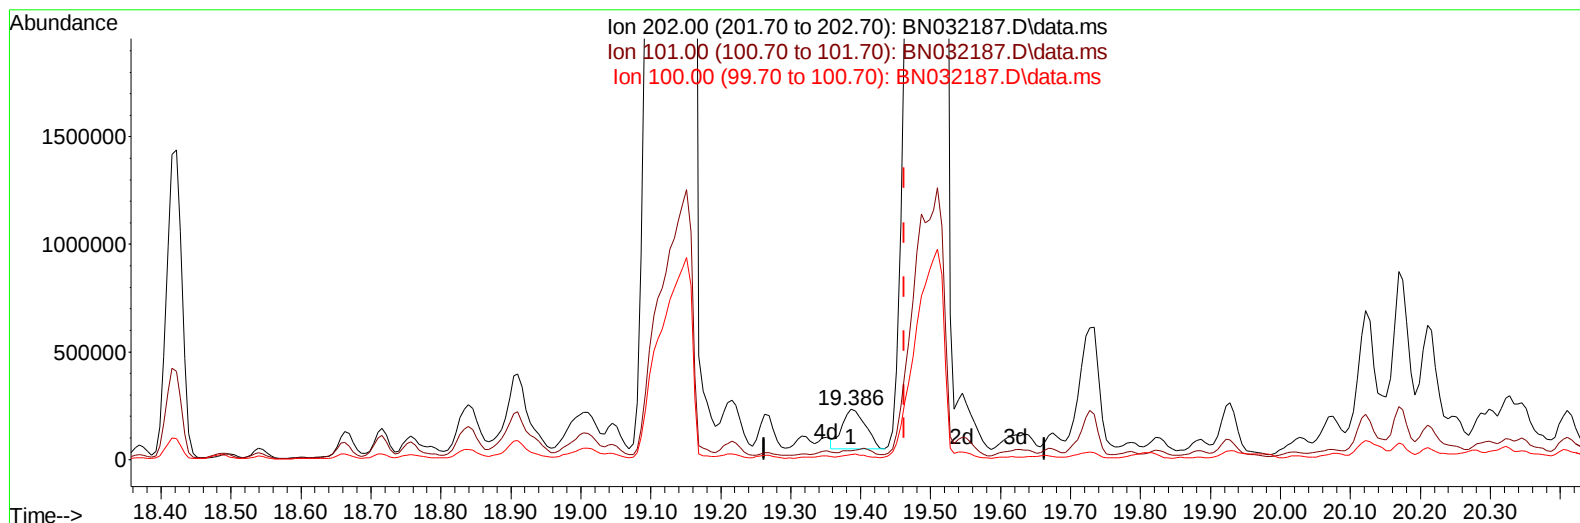

TIC: BN032187.D\data.ms

(82) Pyrene

19.386min (-0.076) 11.37 ng/u1

response 423923

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.70	17.08
100.00	12.70	10.28
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BN032187.D
 Acq On : 23 Jun 2024 05:04
 Operator : MA/JU
 Sample : P2775-24
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4D56

Manual IntegrationsAPPROVED

Quant Time: Jun 23 05:37:00 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 10:49:40 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
 Supervised By :mohammad ahmed 06/26/2024

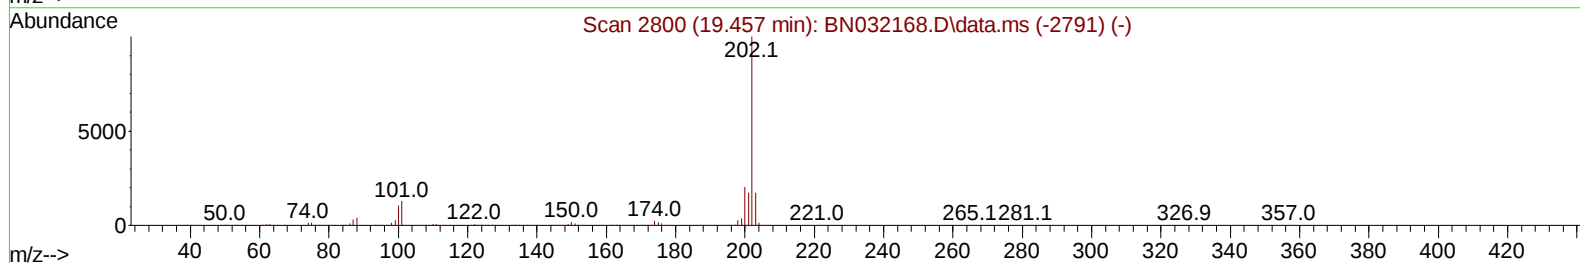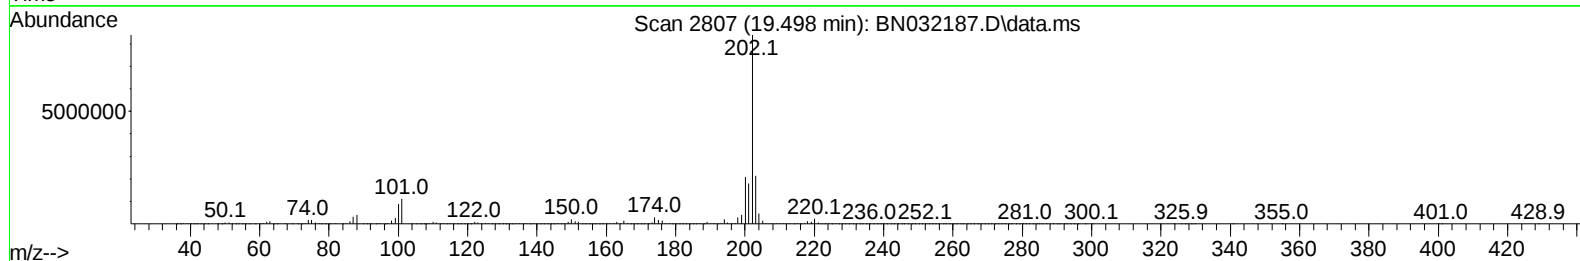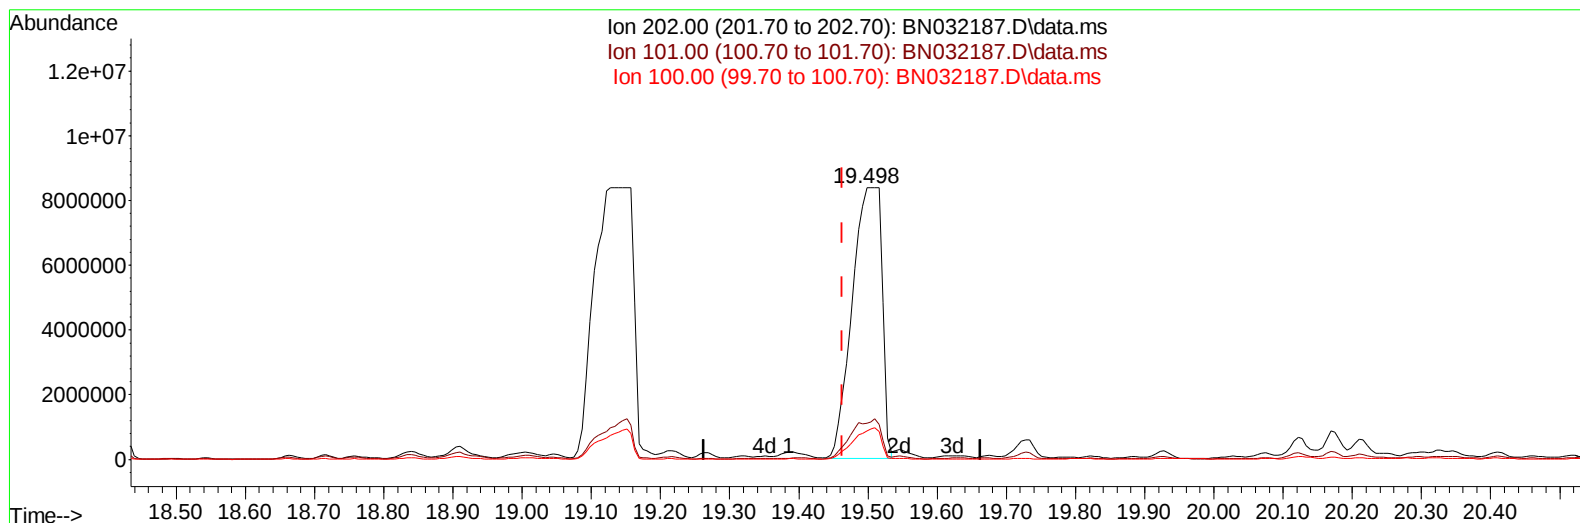

TIC: BN032187.D\data.ms

(82) Pyrene

19.498min (+ 0.036) 668.37 ng/u1 m

response 24928312

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.70	13.29
100.00	12.70	10.53
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BN032187.D
 Acq On : 23 Jun 2024 05:04
 Operator : MA/JU
 Sample : P2775-24
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4D56

Manual IntegrationsAPPROVED

Quant Time: Jun 23 05:38:06 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 10:49:40 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
 Supervised By :mohammad ahmed 06/26/2024

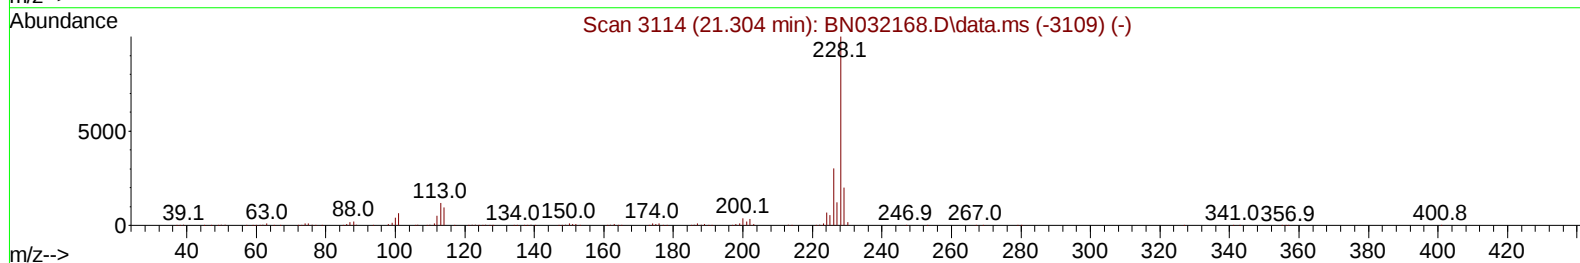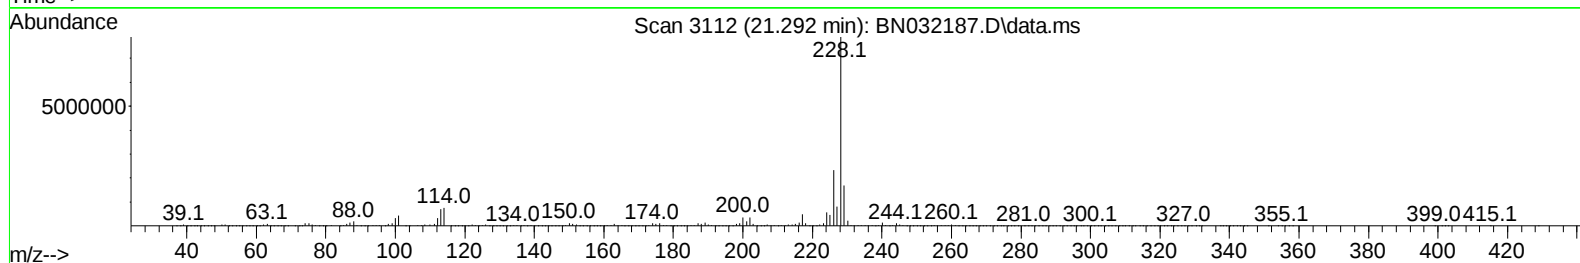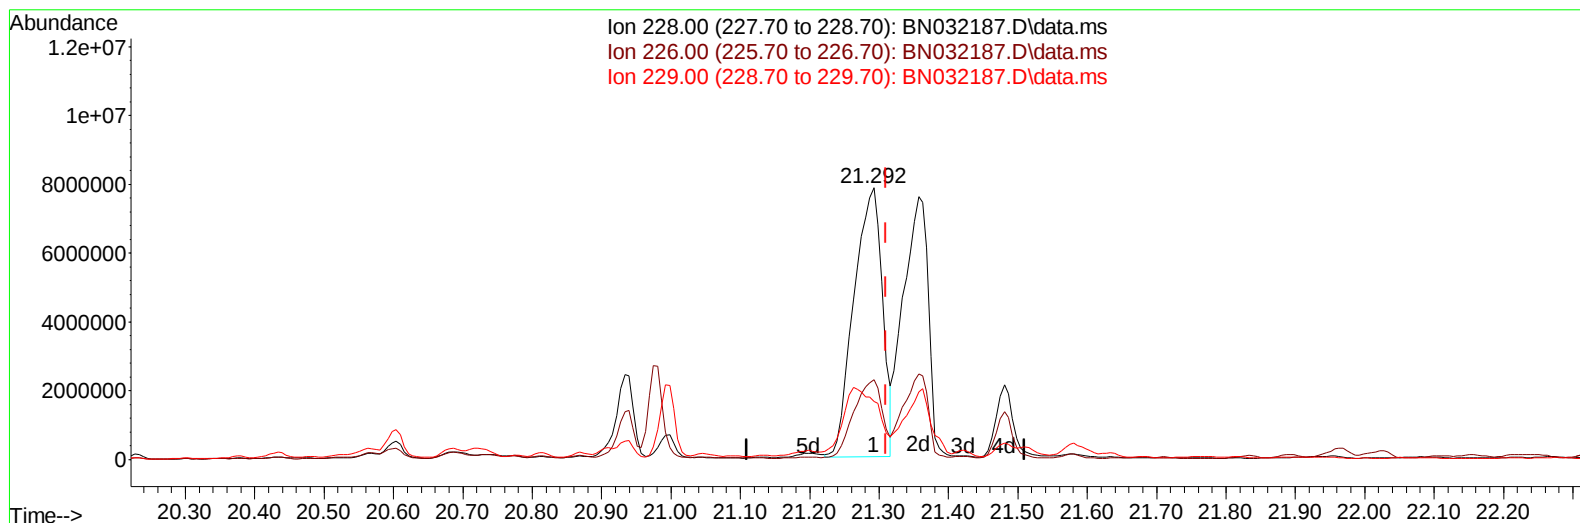

TIC: BN032187.D\data.ms

(87) Chrysene

21.292min (-0.017) 627.60 ng/u1

response 22303849

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	29.60	29.34
229.00	18.90	21.35
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032187.D
Acq On : 23 Jun 2024 05:04
Operator : MA/JU
Sample : P2775-24
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4D56

Manual IntegrationsAPPROVED

Quant Time: Jun 23 05:38:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 10:49:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/26/2024

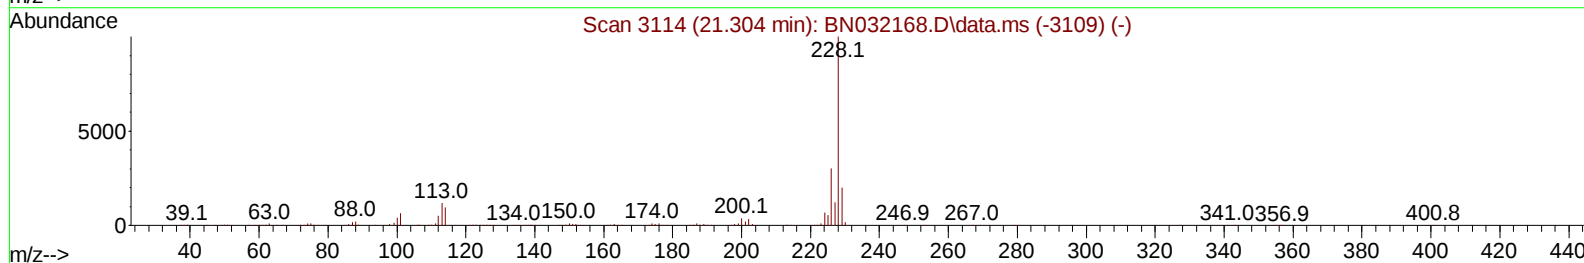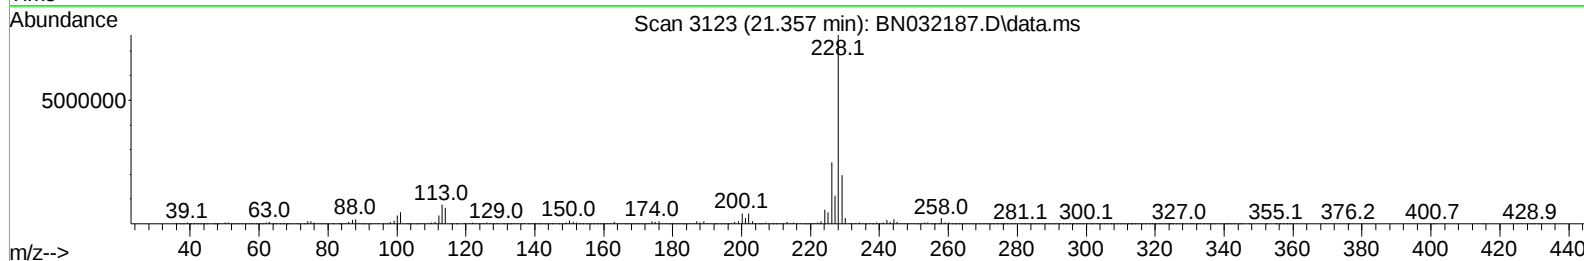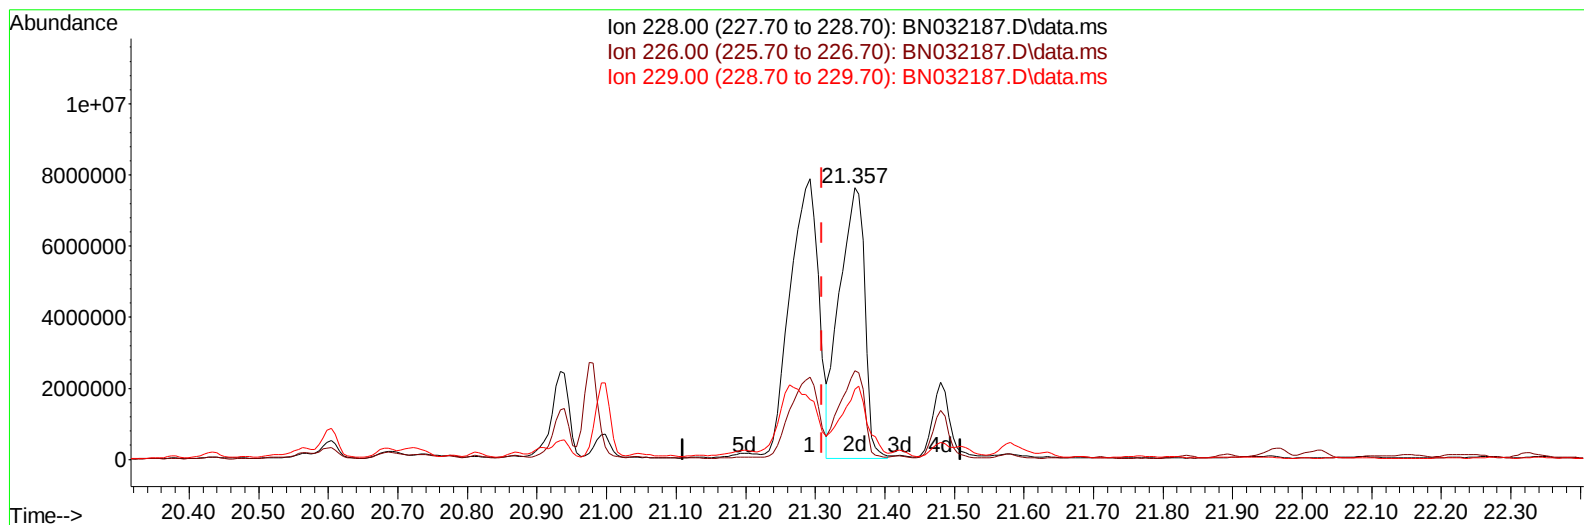

TIC: BN032187.D\data.ms

(87) Chrysene

21.357min (+ 0.047) 540.22 ng/u1 m

response 19198456

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	29.60	32.62
229.00	18.90	25.76#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032187.D
Acq On : 23 Jun 2024 05:04
Operator : MA/JU
Sample : P2775-24
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4D56

Manual IntegrationsAPPROVED

Quant Time: Jun 23 05:38:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 10:49:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/26/2024

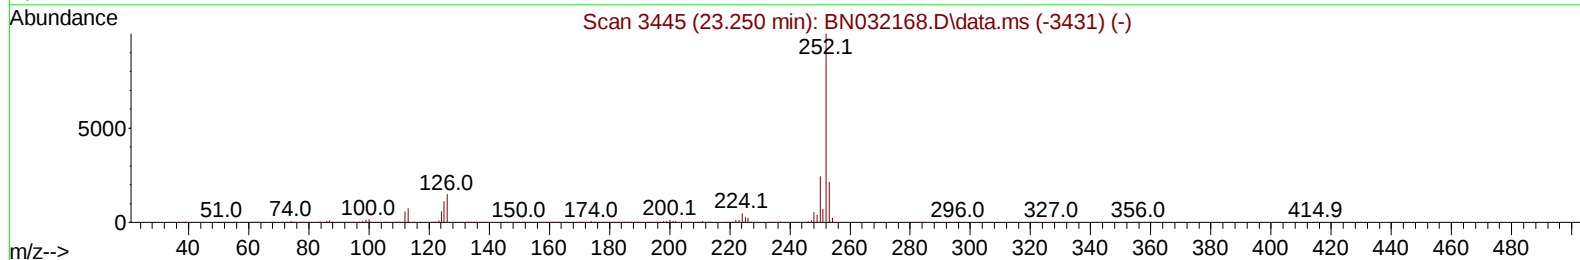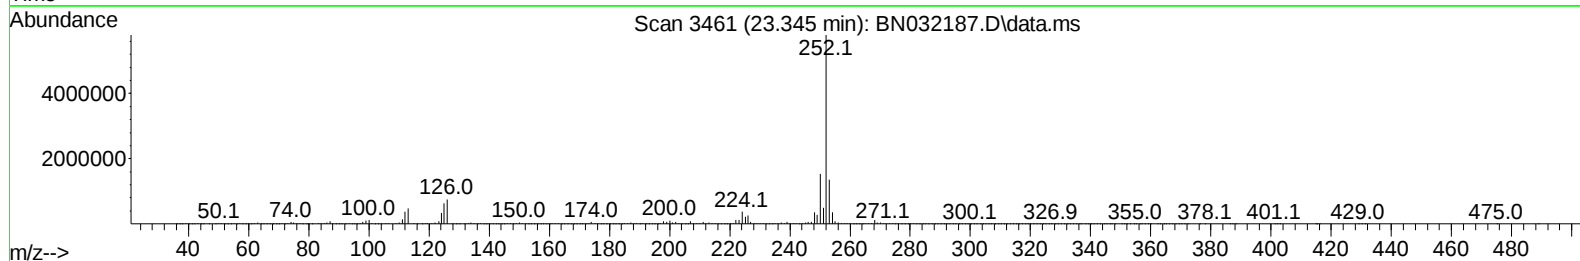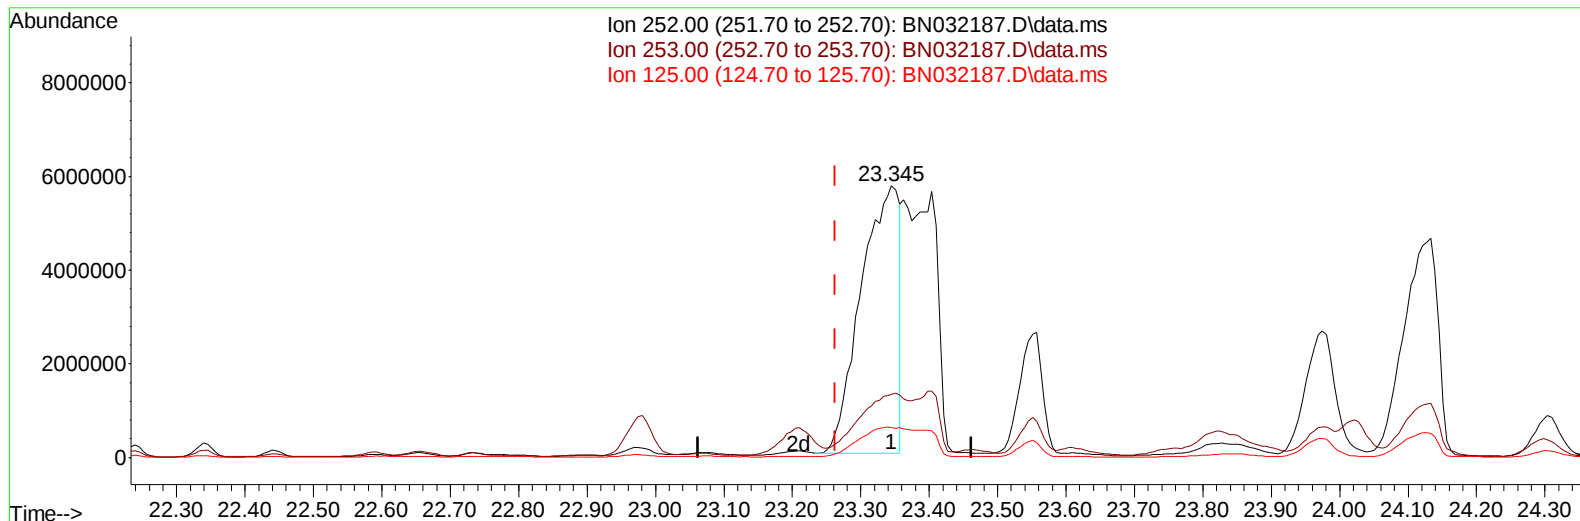

TIC: BN032187.D\data.ms

(90) Benzo(b)fluoranthene

23.345min (+ 0.083) 253.15 ng/u1

response 22194477

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.30	23.27
125.00	11.50	10.98
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032187.D
Acq On : 23 Jun 2024 05:04
Operator : MA/JU
Sample : P2775-24
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4D56

Manual IntegrationsAPPROVED

Quant Time: Jun 23 05:38:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 10:49:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/26/2024

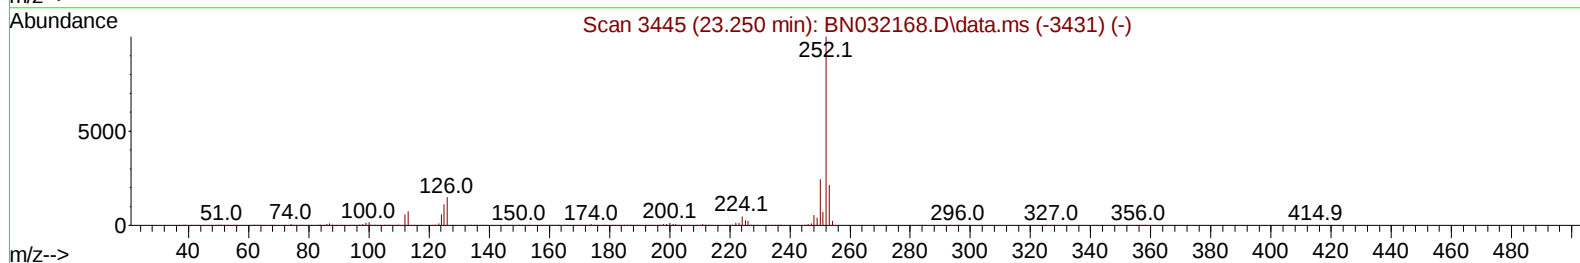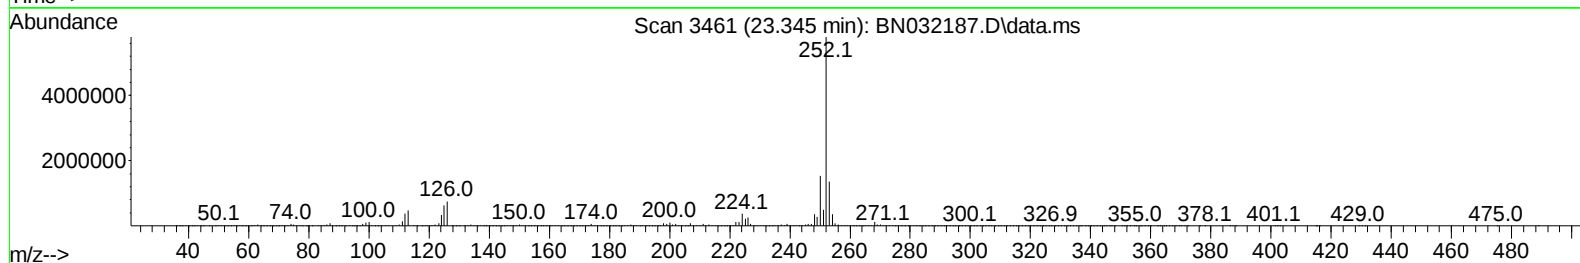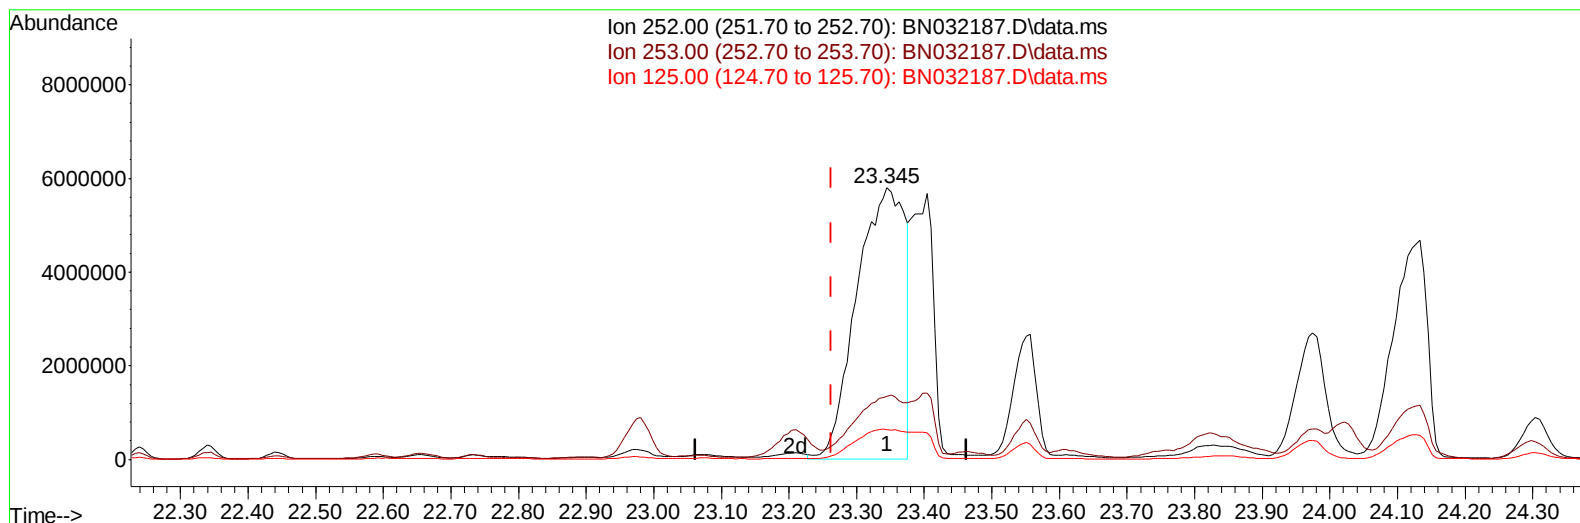

TIC: BN032187.D\data.ms

(90) Benzo(b)fluoranthene

23.345min (+ 0.083) 323.47 ng/u1 m

response 28359061

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.30	23.27
125.00	11.50	10.98
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032187.D
Acq On : 23 Jun 2024 05:04
Operator : MA/JU
Sample : P2775-24
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4D56

Manual IntegrationsAPPROVED

Quant Time: Jun 23 05:38:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 10:49:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/26/2024

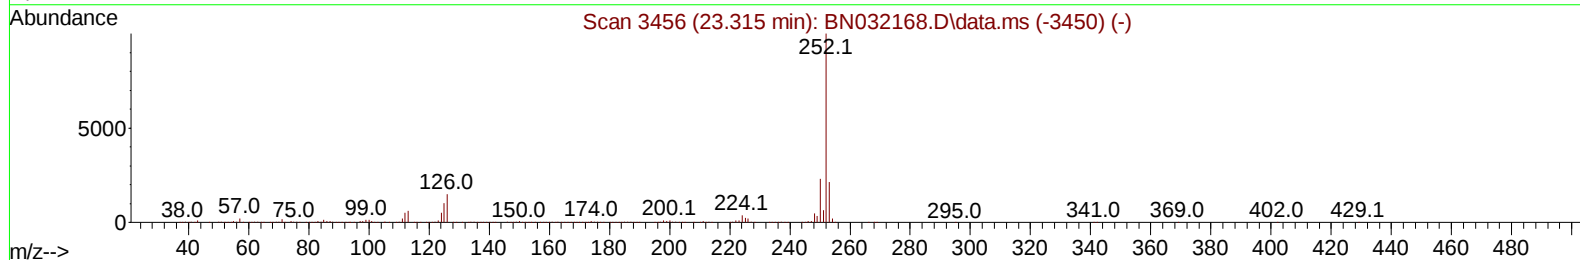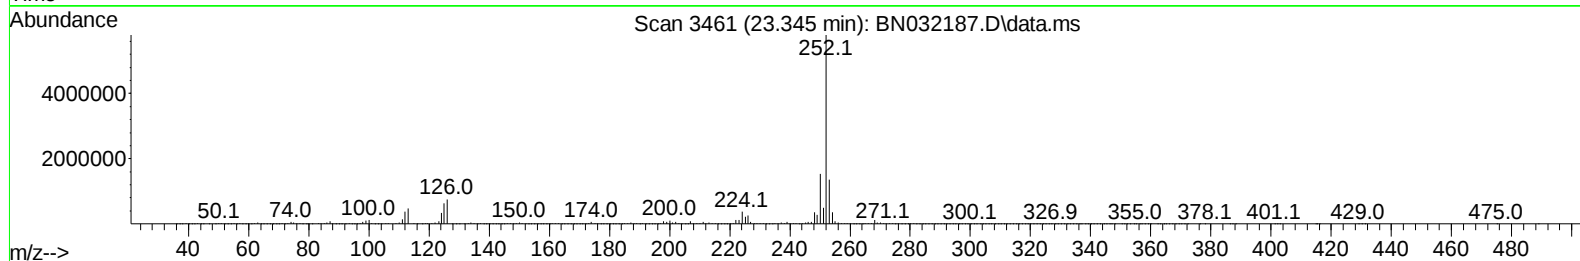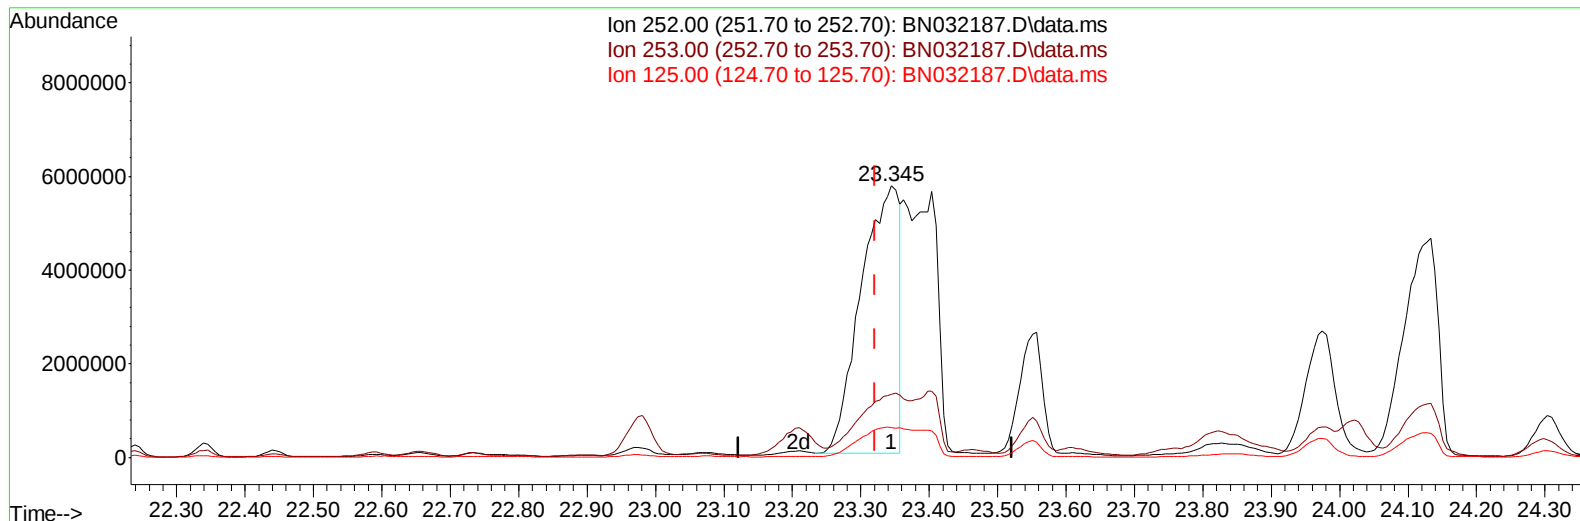

TIC: BN032187.D\data.ms

(91) Benzo(k)fluoranthene

23.345min (+ 0.024) 257.99 ng/u1

response 22194477

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.00	23.27
125.00	11.80	10.98
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032187.D
Acq On : 23 Jun 2024 05:04
Operator : MA/JU
Sample : P2775-24
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4D56

Manual IntegrationsAPPROVED

Quant Time: Jun 23 05:38:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 10:49:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/26/2024

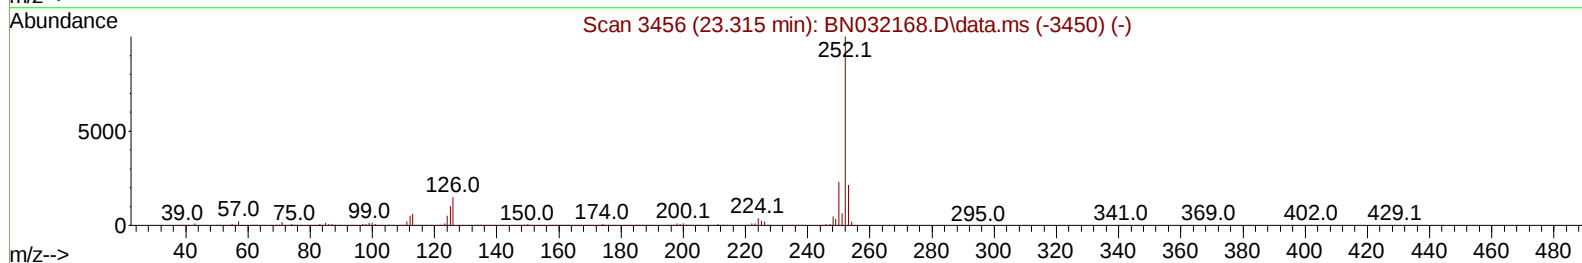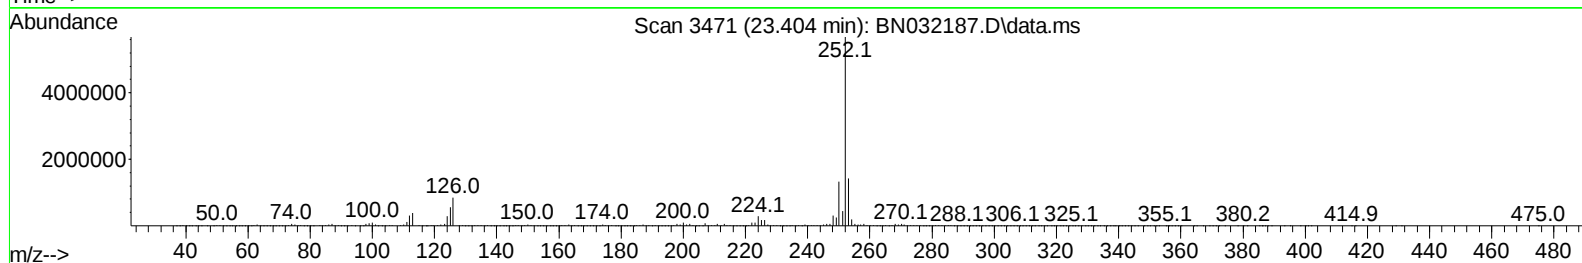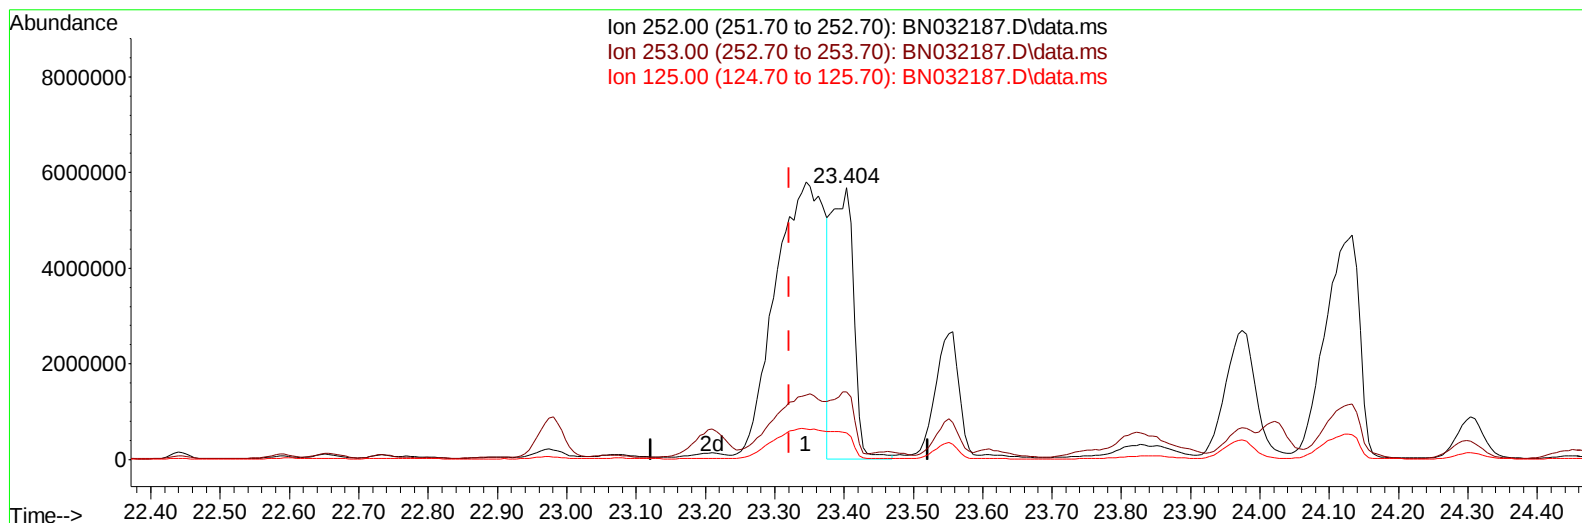

TIC: BN032187.D\data.ms

(91) Benzo(k)fluoranthene

23.404min (+ 0.083) 147.48 ng/ul m

response 12687335

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.00	25.00
125.00	11.80	9.91
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032187.D
Acq On : 23 Jun 2024 05:04
Operator : MA/JU
Sample : P2775-24
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4D56

Manual IntegrationsAPPROVED

Quant Time: Jun 23 05:38:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 10:49:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/26/2024

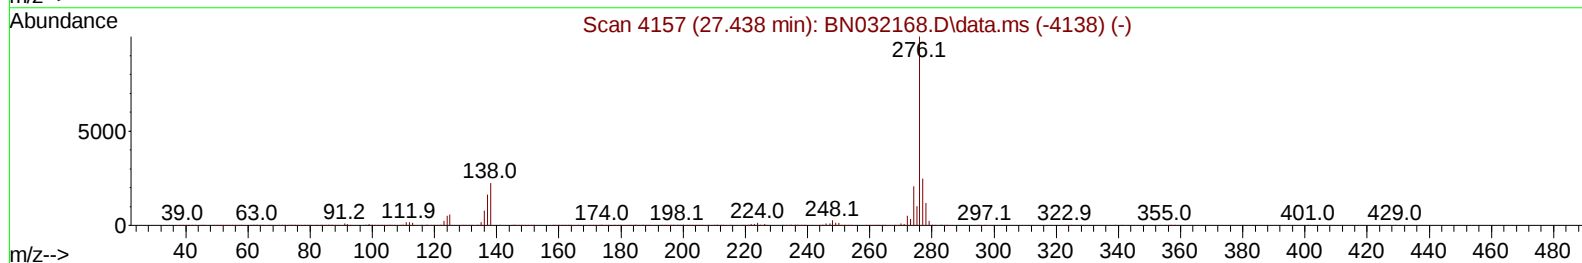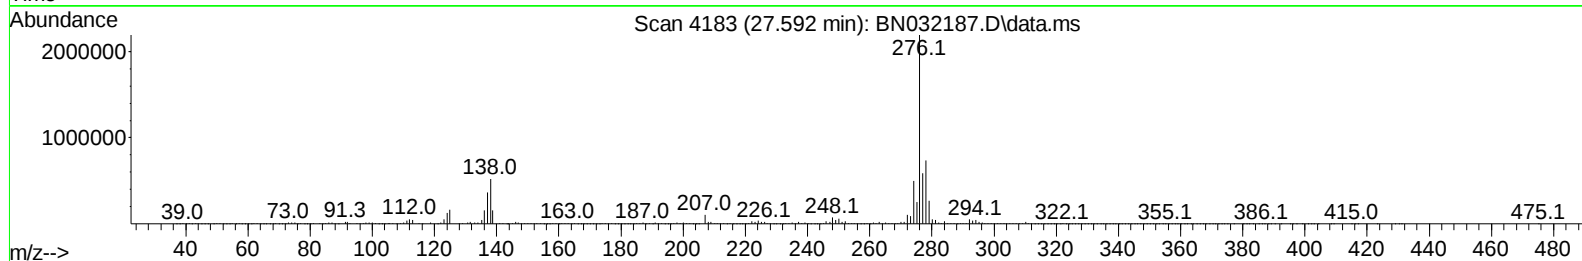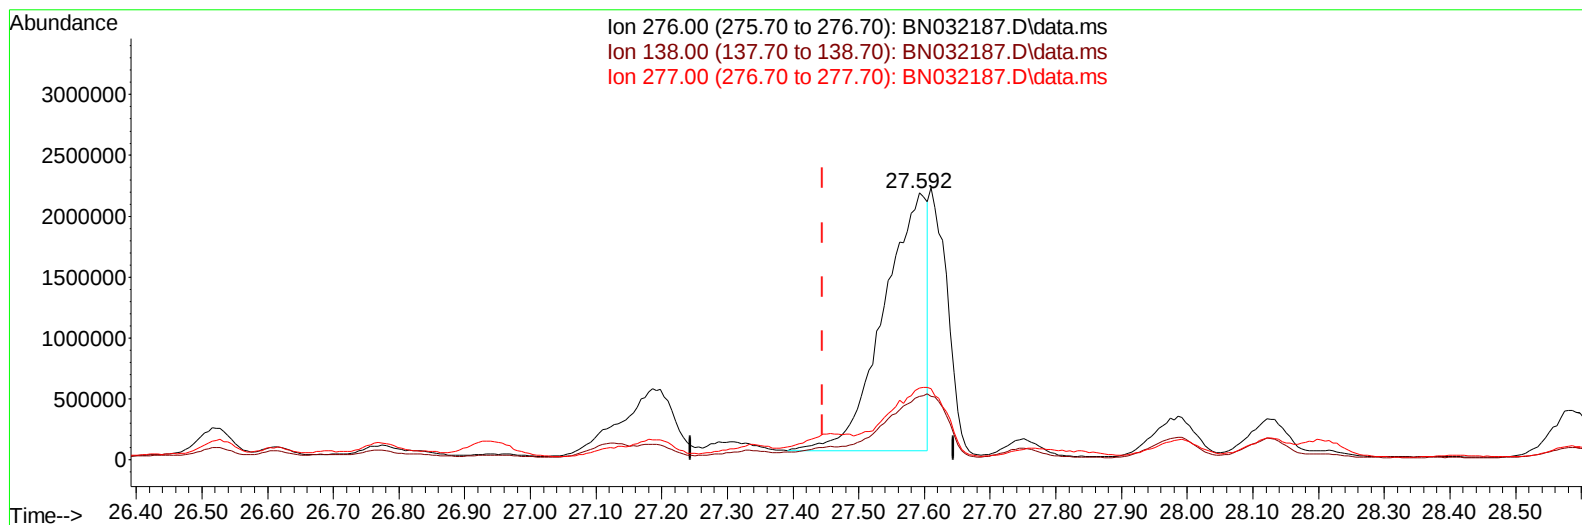

TIC: BN032187.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

27.592min (+ 0.147) 101.52 ng/u1

response 9605669

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	22.60	23.74
277.00	22.70	26.83
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BN032187.D
 Acq On : 23 Jun 2024 05:04
 Operator : MA/JU
 Sample : P2775-24
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4D56

Manual IntegrationsAPPROVED

Quant Time: Jun 23 05:38:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 10:49:40 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
 Supervised By :mohammad ahmed 06/26/2024

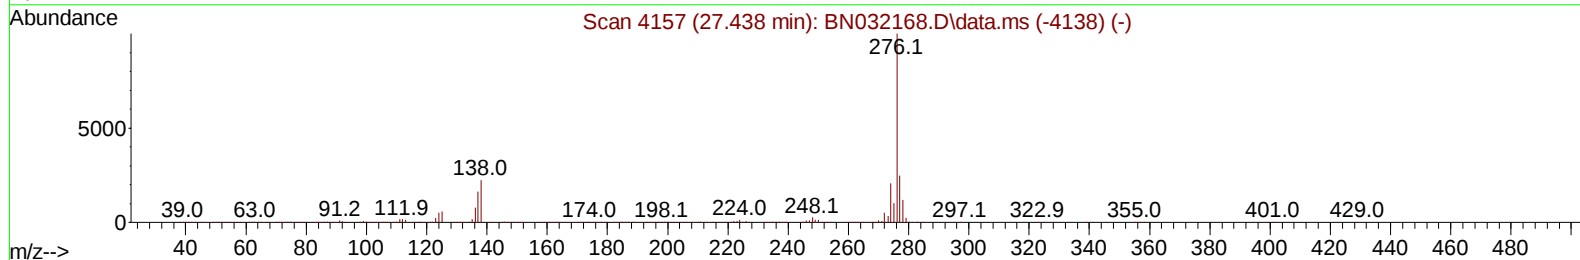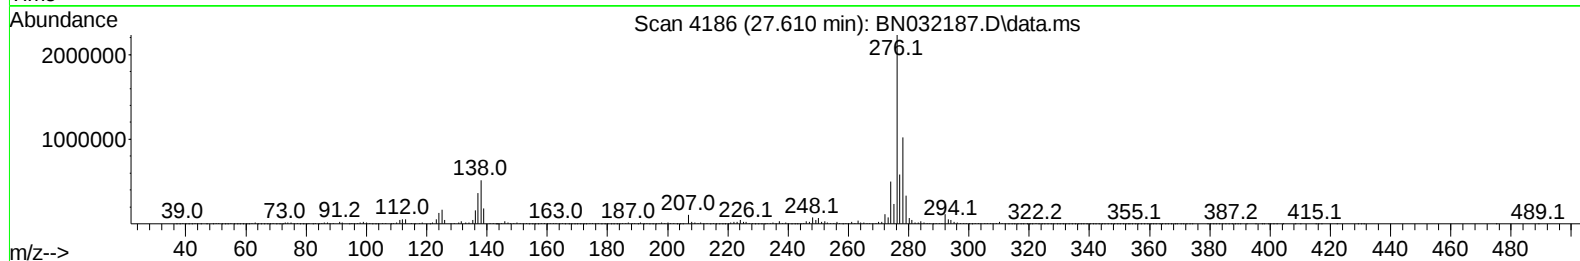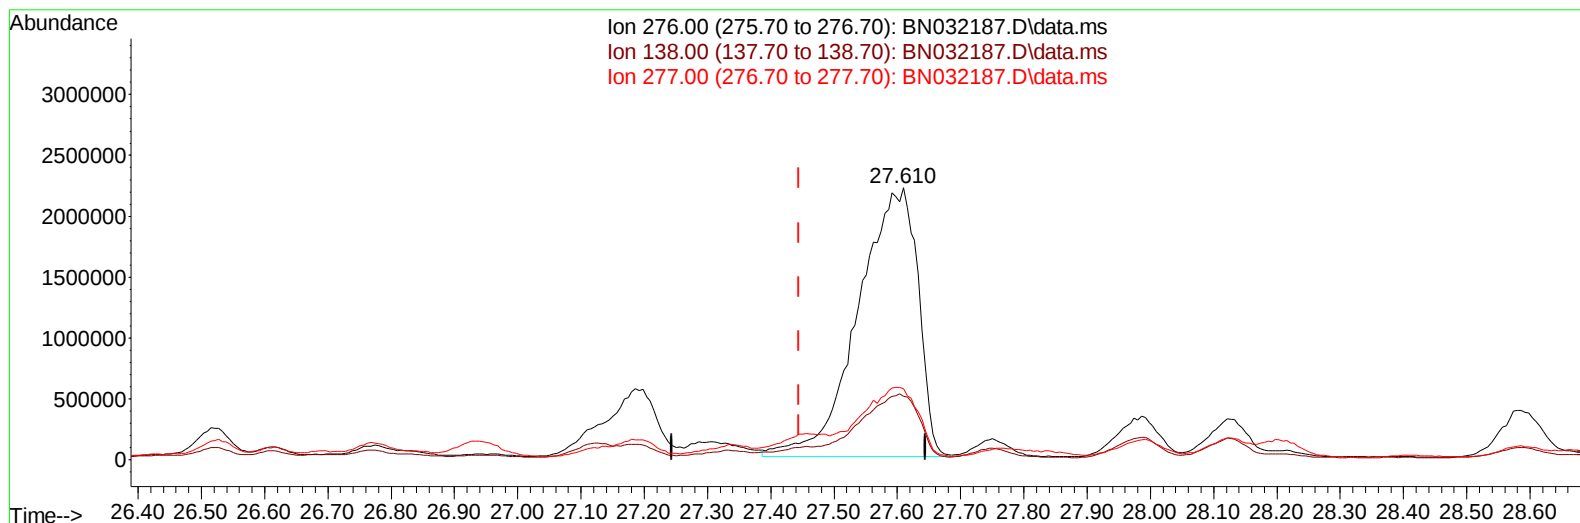

TIC: BN032187.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

27.610min (+ 0.165) 152.19 ng/u1 m

response 14400290

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	22.60	23.17
277.00	22.70	26.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BN032187.D
 Acq On : 23 Jun 2024 05:04
 Operator : MA/JU
 Sample : P2775-24
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4D56

Manual IntegrationsAPPROVED

Quant Time: Jun 23 05:39:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 10:49:40 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
 Supervised By :mohammad ahmed 06/26/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	328731	20.000	ng/ul	0.00
20) Naphthalene-d8	10.410	136	1252098	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.281	164	713333	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.045	188	1174844	20.000	ng/ul	0.01
79) Chrysene-d12	21.310	240	568421	20.000	ng/ul	0.04
88) Perylene-d12	24.233	264	1466761	20.000	ng/ul	# 0.05
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	32601	4.103	ng/uL	0.00
4) Pyridine-d5	3.570	84	252725	11.299	ng/ul	0.00
7) Phenol-d5	6.817	99	658798	23.377	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	337668	20.484	ng/ul	0.00
11) 2-Chlorophenol-d4	7.169	132	577893	26.875	ng/ul	0.00
15) 4-Methylphenol-d8	8.346	113	536423	23.351	ng/ul	0.00
21) Nitrobenzene-d5	8.793	128	269478	28.148	ng/ul	0.00
24) 2-Nitrophenol-d4	9.505	143	298679	30.202	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.046	165	505383	27.374	ng/ul	0.00
31) 4-Chloroaniline-d4	10.563	131	465201	16.971	ng/ul	0.00
46) Dimethylphthalate-d6	13.699	166	1348178	27.129	ng/ul	0.00
49) Acenaphthylene-d8	13.969	160	1596197	27.934	ng/ul	0.00
54) 4-Nitrophenol-d4	14.540	143	208823	20.987	ng/ul	0.04
60) Fluorene-d10	15.275	176	1122995	26.707	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.457	200	82099	13.903	ng/ul	0.04
73) Anthracene-d10	17.157	188	1521664	30.253	ng/ul	0.03
81) Pyrene-d10	19.451	212	1224687	40.263	ng/ul	0.02
92) Benzo(a)pyrene-d12	24.039	264	1323959	18.903	ng/ul	0.06
Target Compounds						
					Qvalue	
8) Phenol	6.846	94	75315	2.626	ng/ul	94
13) 2-Methylphenol	8.081	108	35109	1.585	ng/ul	98
16) Acetophenone	8.458	105	202094	5.805	ng/ul	98
18) 4-Methylphenol	8.416	108	77386	3.223	ng/ul	91
26) 2,4-Dimethylphenol	9.605	107	62026m	2.951	ng/ul	
30) Naphthalene	10.463	128	8375664	129.252	ng/ul	98
36) 2-Methylnaphthalene	12.081	142	3257647	73.547	ng/ul	96
37) 1-Methylnaphthalene	12.305	142	2199471	49.490	ng/ul	97
43) 1,1'-Biphenyl	13.104	154	926401	18.464	ng/ul	97
50) Acenaphthylene	13.999	152	543701	8.419	ng/ul#	87
52) Acenaphthene	14.351	153	7686656	179.893	ng/ul	98
56) Dibenzofuran	14.687	168	8086600	139.297	ng/ul	89
61) Fluorene	15.346	166	8432953	180.389	ng/ul	98
72) Phenanthrene	17.098	178	33857387m	565.722	ng/ul	
74) Anthracene	17.198	178	15115819	249.260	ng/ul	96
77) Carbazole	17.463	167	9381303	181.424	ng/ul	99
80) Fluoranthene	19.128	202	32581142m	896.272	ng/ul	
82) Pyrene	19.498	202	24928312m	668.375	ng/ul	
85) Benzo(a)anthracene	21.292	228	22463543	590.417	ng/ul	99
87) Chrysene	21.357	228	19198456m	540.216	ng/ul	
90) Benzo(b)fluoranthene	23.345	252	28359061m	323.469	ng/ul	
91) Benzo(k)fluoranthene	23.404	252	12687335m	147.477	ng/ul	
93) Benzo(a)pyrene	24.133	252	16054547	195.519	ng/ul	93

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BN032187.D
 Acq On : 23 Jun 2024 05:04
 Operator : MA/JU
 Sample : P2775-24
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4D56

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/24/2024
 Supervised By :mohammad ahmed 06/26/2024

Quant Time: Jun 23 05:39:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 10:49:40 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
94) Indeno(1,2,3-cd)pyrene	27.610	276	14400290m	152.189	ng/ul		
95) Dibenzo(a,h)anthracene	27.621	278	5277112	68.312	ng/ul#		86
96) Benzo(g,h,i)perylene	28.586	276	1945385	25.864	ng/ul#		93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032187.D
Acq On : 23 Jun 2024 05:04
Operator : MA/JU
Sample : P2775-24
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4D56

Manual IntegrationsAPPROVED

Quant Time: Jun 23 05:39:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 10:49:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/24/2024
Supervised By :mohammad ahmed 06/26/2024

