

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BN032171.D
 Acq On : 22 Jun 2024 17:54
 Operator : MA/JU
 Sample : P2899-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB3

Quant Time: Jun 22 23:48:46 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 10:49:40 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	314473	20.000	ng/u1	0.00
20) Naphthalene-d8	10.410	136	1256714	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.275	164	737336	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.028	188	1359196	20.000	ng/u1	0.00
79) Chrysene-d12	21.263	240	1162395	20.000	ng/u1	0.00
88) Perylene-d12	24.174	264	1281076	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	22874	3.009	ng/uL	0.00
4) Pyridine-d5	3.569	84	217598	10.169	ng/u1	0.00
7) Phenol-d5	6.810	99	509294	18.891	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	273942	17.372	ng/u1	0.00
11) 2-Chlorophenol-d4	7.163	132	446869	21.724	ng/u1	0.00
15) 4-Methylphenol-d8	8.340	113	387692	17.642	ng/u1	0.00
21) Nitrobenzene-d5	8.787	128	217597	22.645	ng/u1	0.00
24) 2-Nitrophenol-d4	9.504	143	241342	24.315	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.040	165	420575	22.697	ng/u1	0.00
31) 4-Chloroaniline-d4	10.563	131	121526	4.417	ng/u1	0.00
46) Dimethylphthalate-d6	13.692	166	1241211	24.163	ng/u1	0.00
49) Acenaphthylene-d8	13.969	160	1449979	24.549	ng/u1	0.00
54) 4-Nitrophenol-d4	14.504	143	190487	18.521	ng/u1	0.00
60) Fluorene-d10	15.269	176	1059859	24.385	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.410	200	140059	20.501	ng/u1	0.00
73) Anthracene-d10	17.122	188	1521247	26.143	ng/u1	0.00
81) Pyrene-d10	19.427	212	1625936	26.139	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.974	264	1586352	25.933	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.168	149	62141	1.183	ng/u1	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032171.D
Acq On : 22 Jun 2024 17:54
Operator : MA/JU
Sample : P2899-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB3


Quant Time: Jun 22 23:48:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 10:49:40 2024
Response via : Initial Calibration

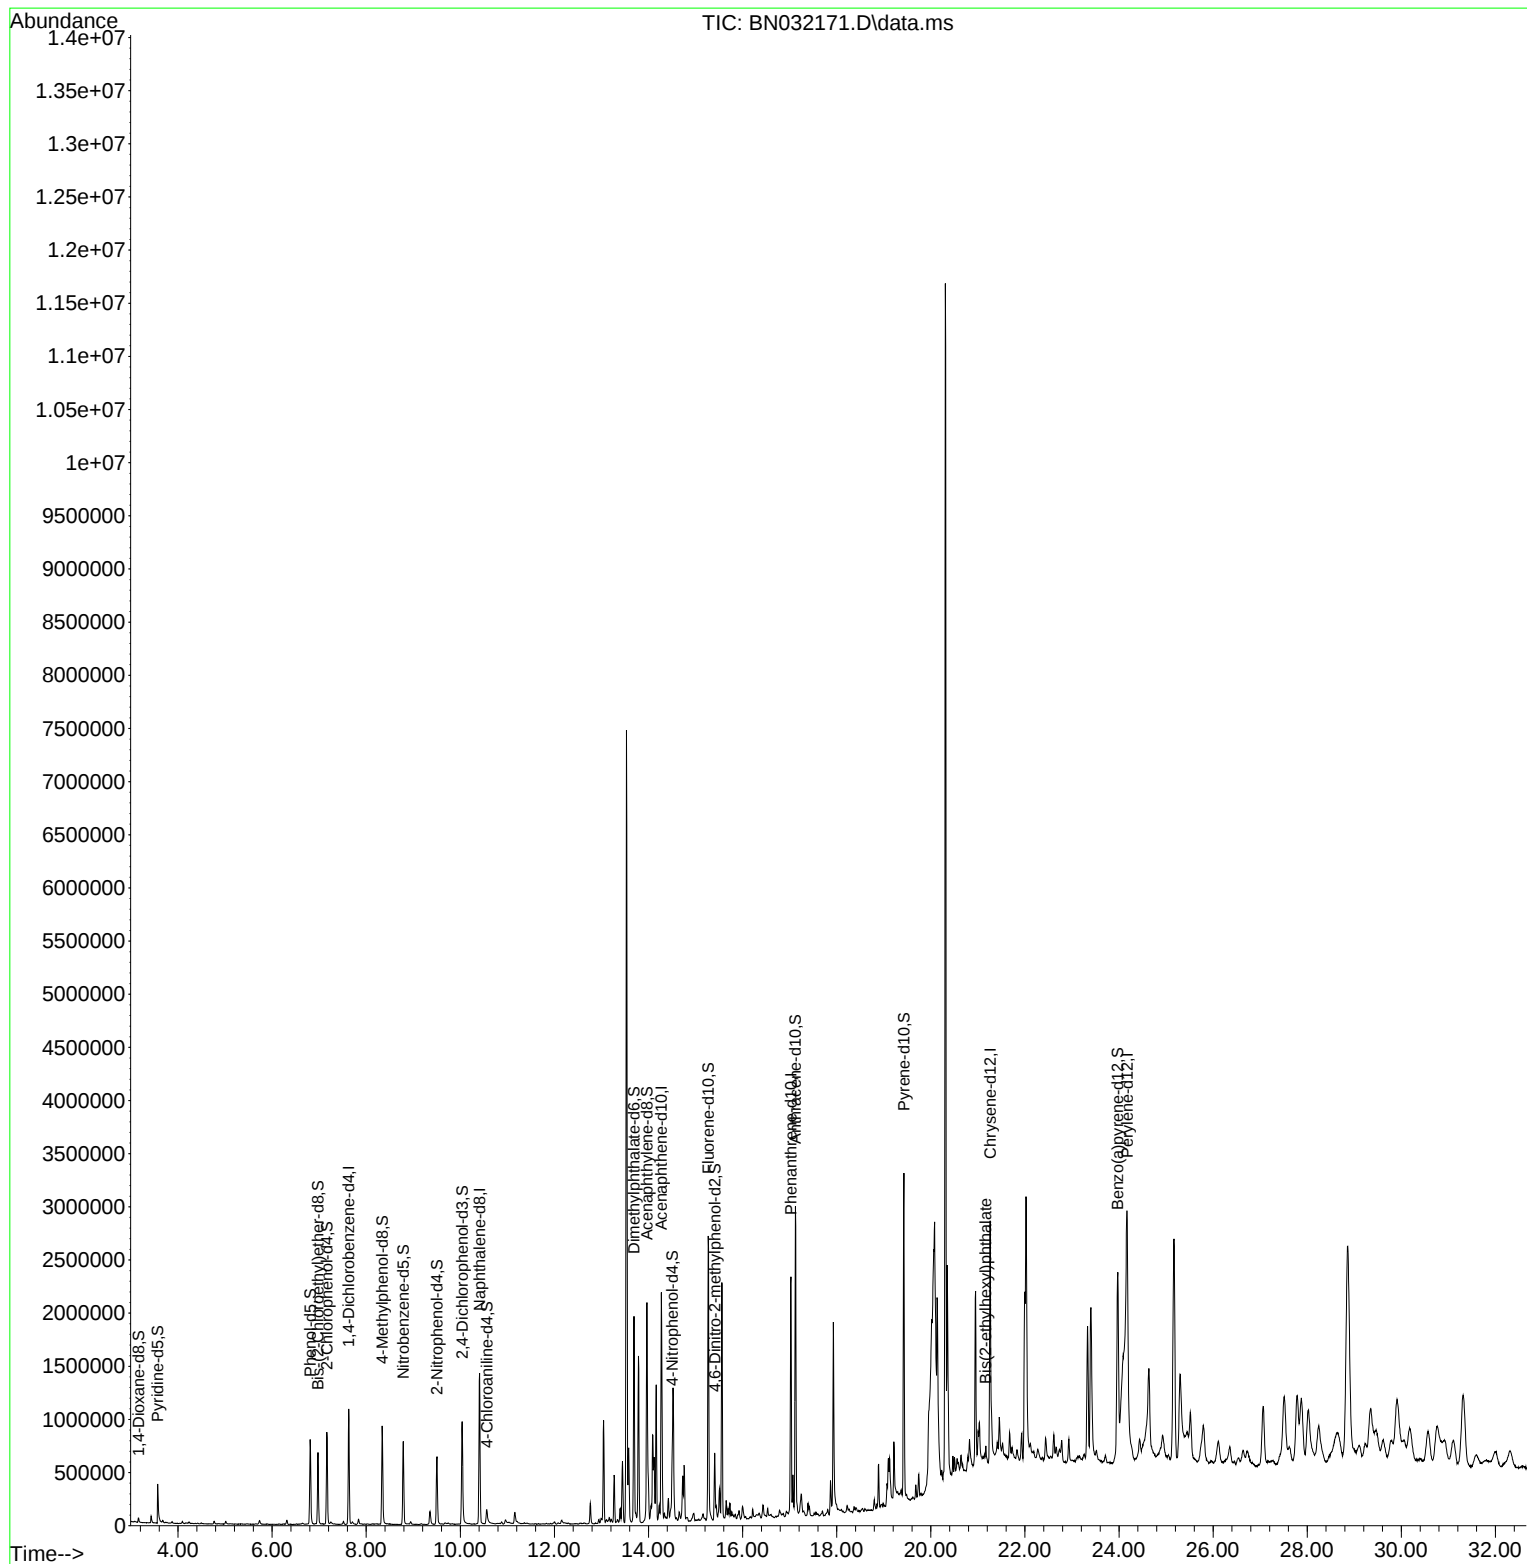

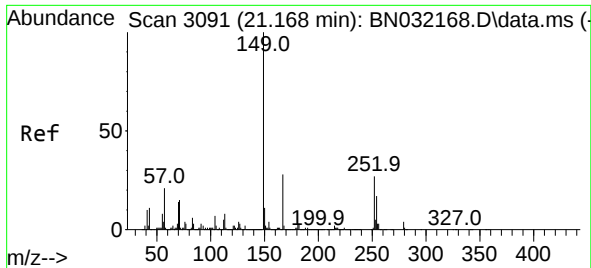

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.183 ng/ul
 RT: 21.168 min Scan# 3091
 Delta R.T. -0.006 min
 Lab File: BN032171.D
 Acq: 22 Jun 2024 17:54

Instrument :
 BNA_N
 ClientSampleId :
 C0AB3

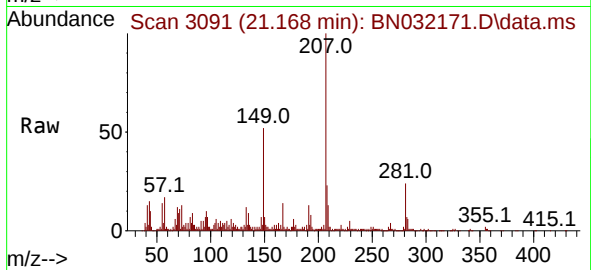

Tgt Ion:	149	Resp:	62141
Ion Ratio	100	Lower	Upper
149	100		
167	26.6	21.4	32.0
279	4.6	3.3	4.9

