

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BN032173.D
 Acq On : 22 Jun 2024 19:13
 Operator : MA/JU
 Sample : P2899-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA4

Quant Time: Jun 22 23:43:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 10:49:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	366747	20.000	ng/u1	0.00
20) Naphthalene-d8	10.410	136	1439444	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.275	164	794473	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.027	188	1366226	20.000	ng/u1	0.00
79) Chrysene-d12	21.262	240	1092196	20.000	ng/u1	0.00
88) Perylene-d12	24.180	264	1292449	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.163	96	27882	3.145	ng/uL	0.00
4) Pyridine-d5	3.599	84	11370	0.456	ng/u1	0.03
7) Phenol-d5	6.816	99	604709	19.233	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	327091	17.786	ng/u1	0.00
11) 2-Chlorophenol-d4	7.169	132	535643	22.328	ng/u1	0.00
15) 4-Methylphenol-d8	8.345	113	488640	19.066	ng/u1	0.00
21) Nitrobenzene-d5	8.792	128	258624	23.498	ng/u1	0.00
24) 2-Nitrophenol-d4	9.504	143	282414	24.841	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.039	165	467485	22.025	ng/u1	0.00
31) 4-Chloroaniline-d4	10.575	131	38542	1.223	ng/u1	0.01
46) Dimethylphthalate-d6	13.692	166	1279653	23.120	ng/u1	0.00
49) Acenaphthylene-d8	13.969	160	1475376	23.183	ng/u1	0.00
54) 4-Nitrophenol-d4	14.516	143	174546	15.751	ng/u1	0.01
60) Fluorene-d10	15.274	176	1038748	22.181	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.410	200	116152	16.914	ng/u1	0.00
73) Anthracene-d10	17.127	188	1394416	23.840	ng/u1	0.00
81) Pyrene-d10	19.427	212	1261807	21.589	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.986	264	939312	15.220	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.451	105	56222	1.448	ng/u1	99
86) Bis(2-ethylhexyl)phtha...	21.168	149	108930	2.208	ng/u1#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032173.D
Acq On : 22 Jun 2024 19:13
Operator : MA/JU
Sample : P2899-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AA4

Quant Time: Jun 22 23:43:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 10:49:40 2024
Response via : Initial Calibration




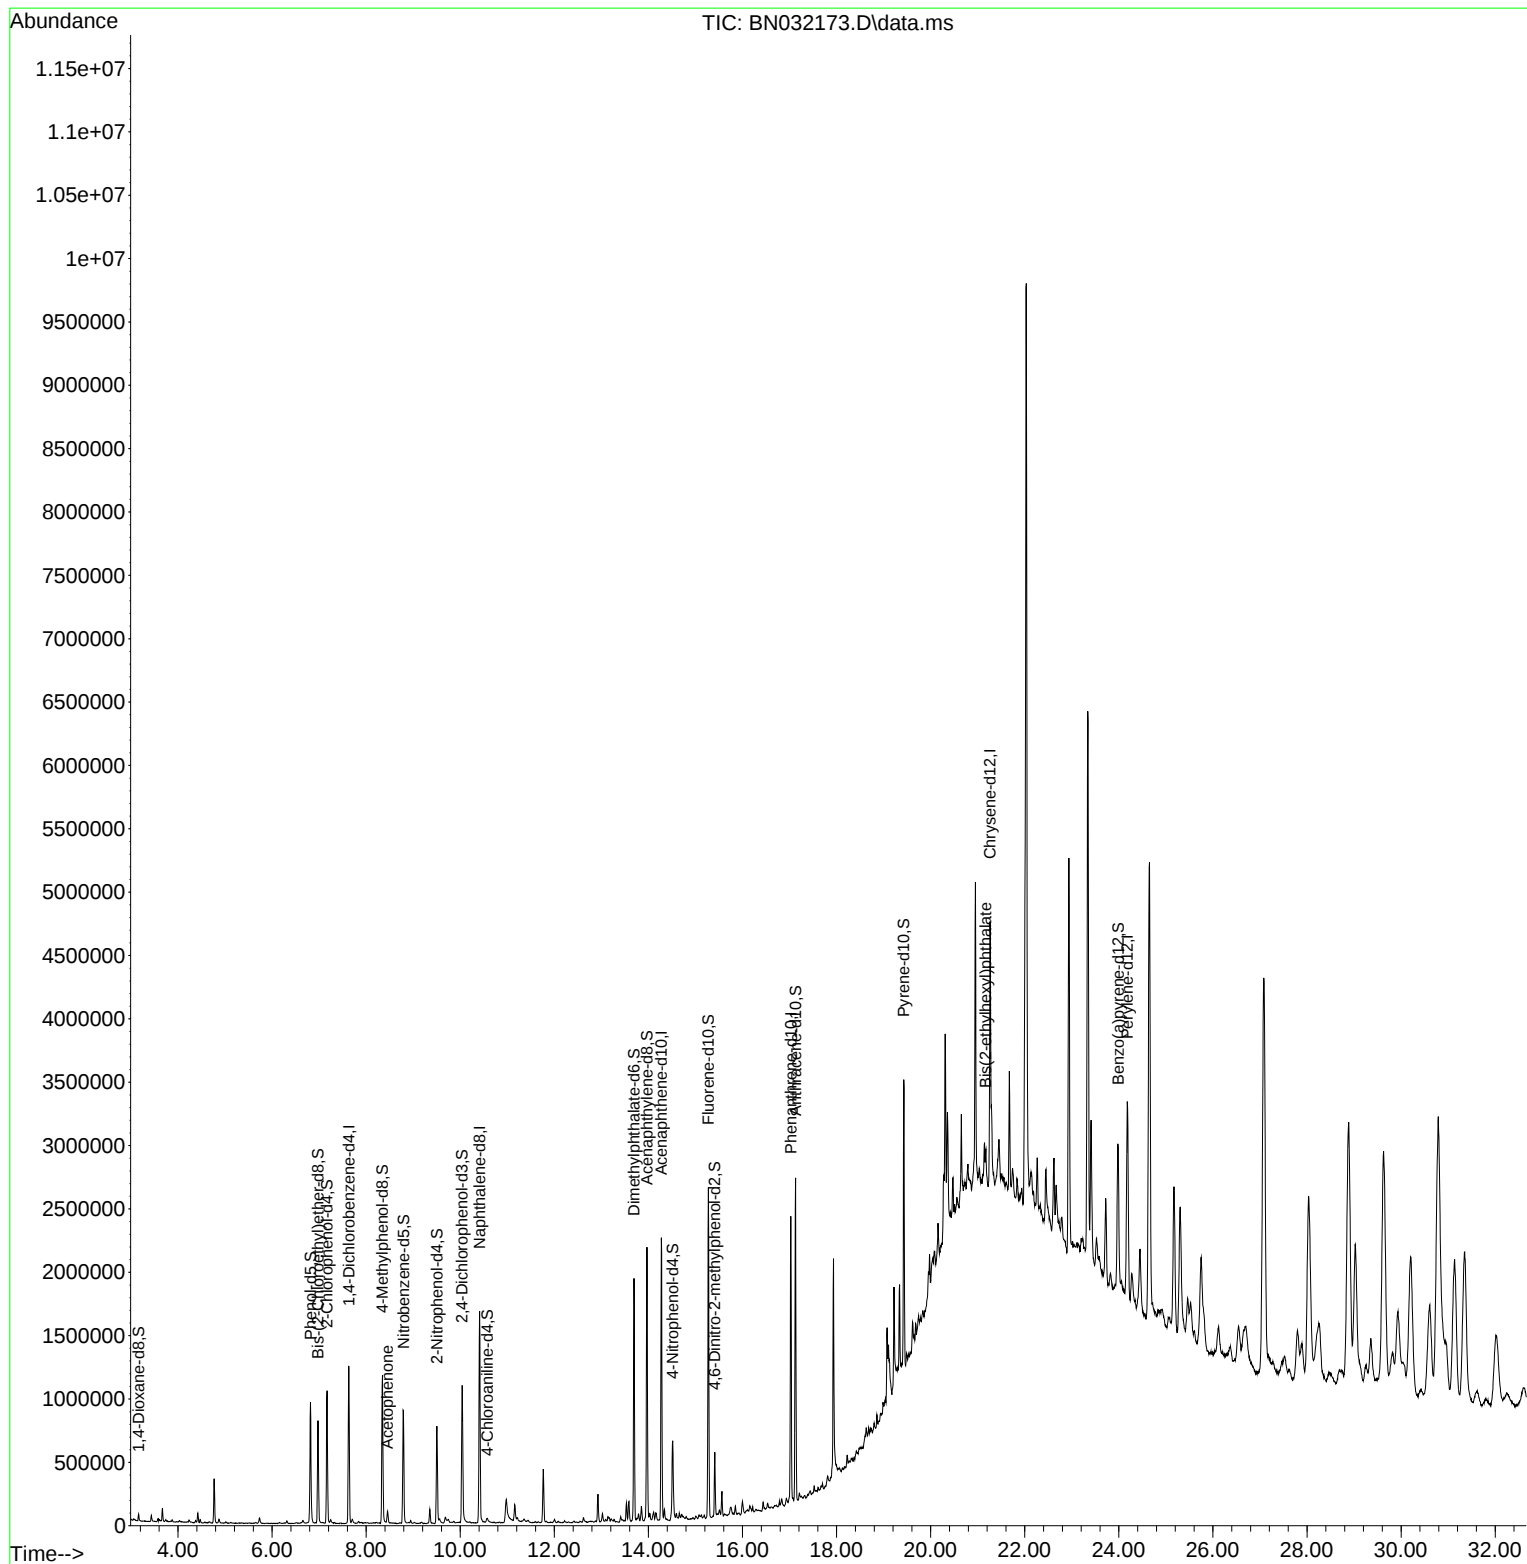


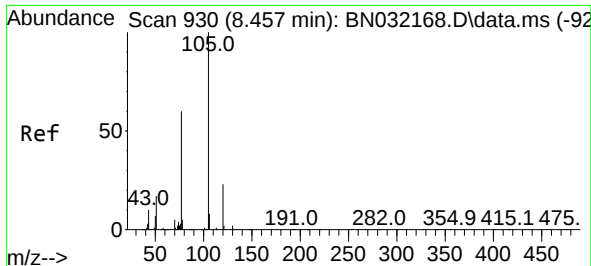

#16
Acetophenone
Concen: 1.448 ng/ul
RT: 8.451 min Scan# 91
Delta R.T. -0.012 min
Lab File: BN032173.D
Acq: 22 Jun 2024 19:13

Instrument :
BNA_N
ClientSampleId :
C0AA4

Tgt Ion:105 Resp: 56222
Ion Ratio Lower Upper
105 100
77 72.7 58.6 87.8
51 23.0 17.2 25.8

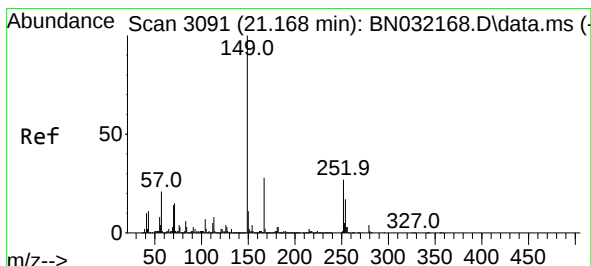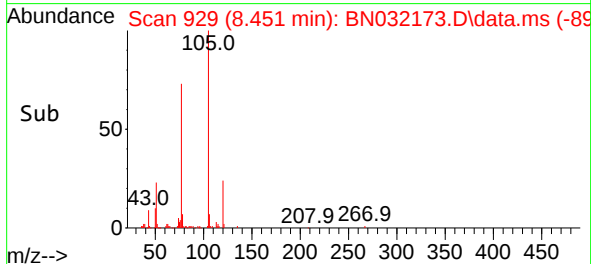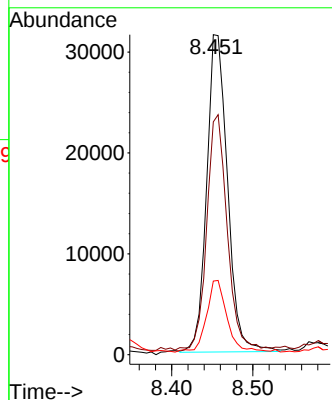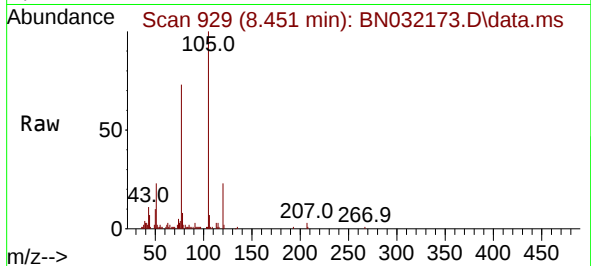

#86
Bis(2-ethylhexyl)phthalate
Concen: 2.208 ng/ul
RT: 21.168 min Scan# 3091
Delta R.T. -0.006 min
Lab File: BN032173.D
Acq: 22 Jun 2024 19:13

Tgt Ion:149 Resp: 108930
Ion Ratio Lower Upper
149 100
167 29.1 21.4 32.0
279 5.0 3.3 4.9#

