

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BN032161.D
 Acq On : 22 Jun 2024 10:39
 Operator : MA/JU
 Sample : PB161647BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK647

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN032161.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	25	30	38	rVB	74979	104225	1.43%	0.134%
2	3.564	95	98	124	rBV	844166	1279078	17.55%	1.642%
3	3.875	147	151	155	rVB	15805	20977	0.29%	0.027%
4	6.811	643	650	663	rBV	1090039	1785150	24.50%	2.292%
5	6.975	671	678	691	rVB	939830	1501407	20.61%	1.928%
6	7.164	703	710	728	rBV	1152120	1896204	26.02%	2.435%
7	7.628	781	789	800	rBV	1059695	1711244	23.49%	2.197%
8	8.340	902	910	924	rBV	1414908	2410178	33.08%	3.095%
9	8.787	979	986	998	rBV	1087198	1839242	25.24%	2.362%
10	9.505	1098	1108	1124	rBV	920146	1575340	21.62%	2.023%
11	10.034	1191	1198	1226	rBV	1354286	2455095	33.69%	3.153%
12	10.410	1253	1262	1272	rBV	1529567	2564285	35.19%	3.293%
13	10.557	1279	1287	1306	rBV	1166735	2139821	29.37%	2.748%
14	12.010	1528	1534	1539	rBV	17547	34650	0.48%	0.044%
15	13.240	1739	1743	1747	rBV6	5461	7733	0.11%	0.010%
16	13.693	1813	1820	1834	rBV	2867827	4051771	55.61%	5.203%
17	13.969	1859	1867	1882	rBV	3095388	4831563	66.31%	6.204%
18	14.275	1910	1919	1933	rBV	2458028	3690911	50.66%	4.739%
19	14.498	1950	1957	1979	rBV	1096681	1928627	26.47%	2.477%
20	15.269	2080	2088	2101	rBV	4059149	6079576	83.44%	7.807%
21	15.410	2105	2112	2125	rBV	1203109	1824845	25.04%	2.343%
22	15.510	2125	2129	2136	rVB3	20975	36402	0.50%	0.047%
23	15.781	2171	2175	2181	rBV2	9316	12154	0.17%	0.016%
24	16.057	2217	2222	2229	rBV2	13320	20453	0.28%	0.026%
25	16.704	2328	2332	2336	rVB4	5740	7873	0.11%	0.010%
26	16.816	2343	2351	2357	rBV3	7684	20271	0.28%	0.026%
27	17.028	2380	2387	2396	rBV	2957206	4403050	60.43%	5.654%
28	17.122	2397	2403	2418	rVV	4390252	6543064	89.80%	8.402%
29	17.698	2496	2501	2509	rBV10	13162	24274	0.33%	0.031%
30	17.922	2535	2539	2550	rBV2	94439	207727	2.85%	0.267%
31	18.475	2629	2633	2636	rBV6	8005	11710	0.16%	0.015%
32	18.986	2716	2720	2727	rBV	59844	90672	1.24%	0.116%
33	19.063	2728	2733	2739	rBV	48753	80971	1.11%	0.104%
34	19.216	2755	2759	2767	rBV4	69783	135430	1.86%	0.174%
35	19.428	2788	2795	2807	rBV	5415185	7286316	100.00%	9.356%
36	21.263	3101	3107	3115	rBV	2912387	4329259	59.42%	5.559%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032161.D
Acq On : 22 Jun 2024 10:39
Operator : MA/JU
Sample : PB161647BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK647

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION

37	23.969	3559	3567	3586	rVB2	2672481	6634802	91.06%	8.520%
38	24.169	3593	3601	3615	rVB2	1714570	4300731	59.02%	5.522%




Sum of corrected areas: 77877081

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032161.D
Acq On : 22 Jun 2024 10:39
Operator : MA/JU
Sample : PB161647BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK647

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

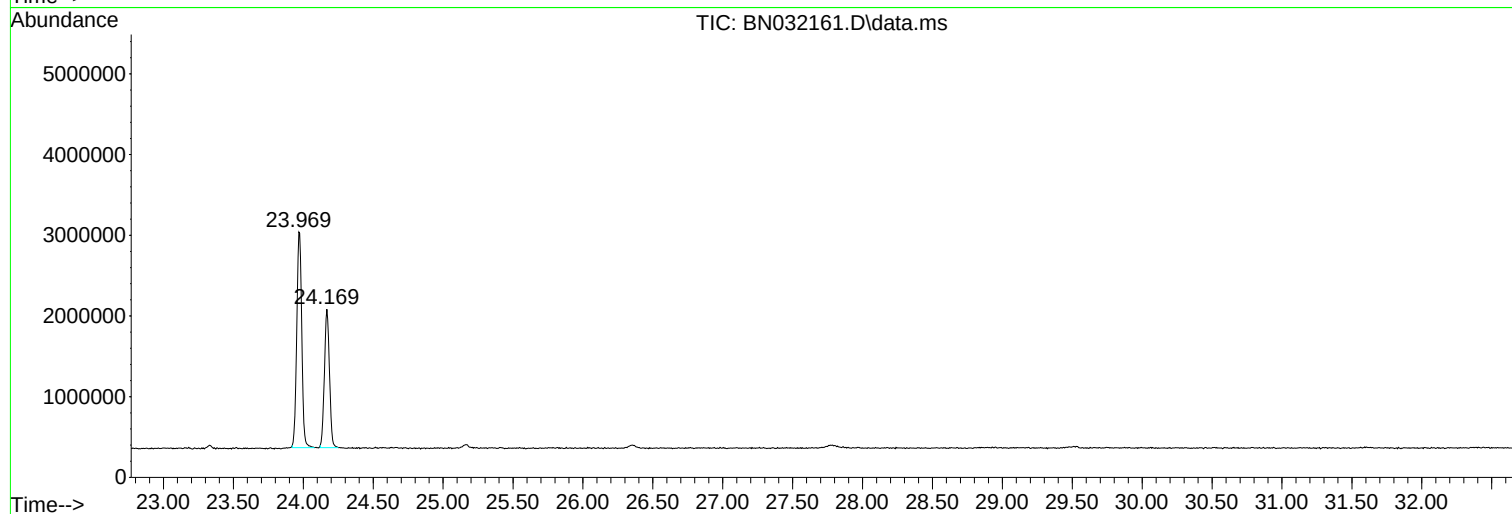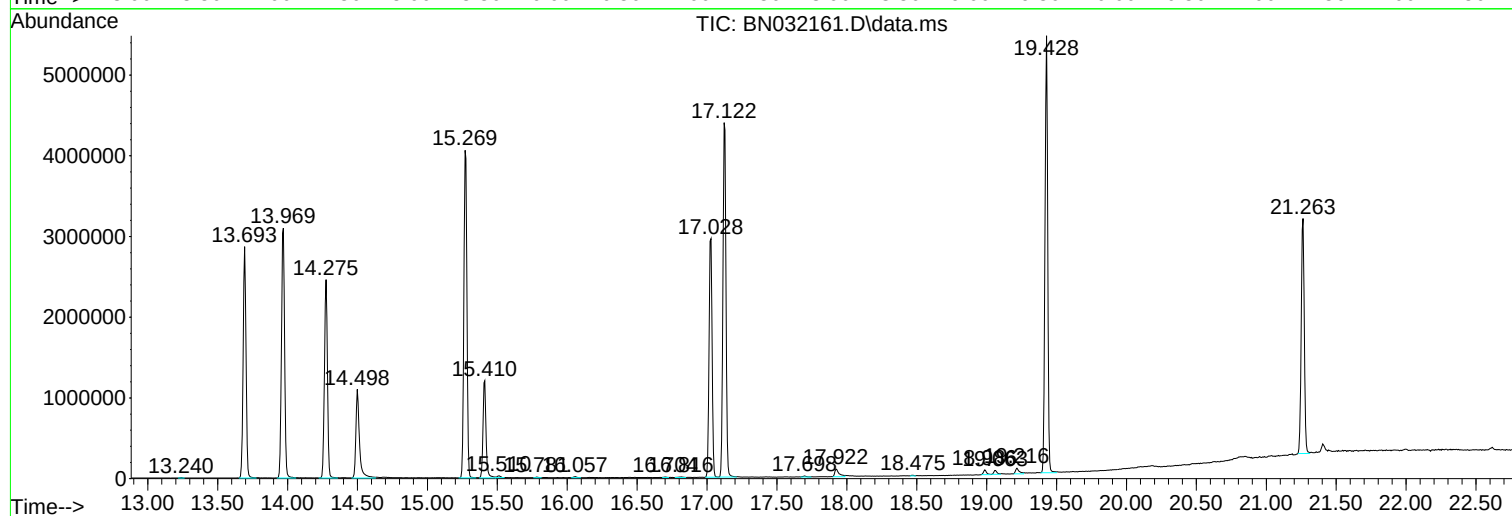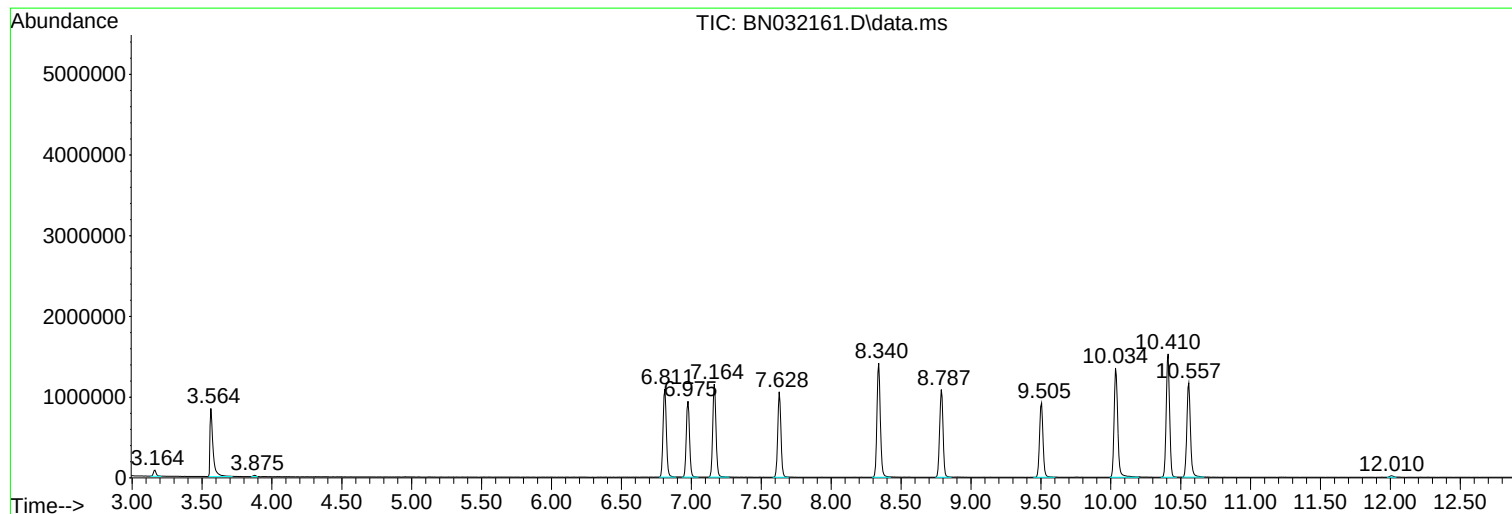

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032161.D
Acq On : 22 Jun 2024 10:39
Operator : MA/JU
Sample : PB161647BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK647

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032161.D
Acq On : 22 Jun 2024 10:39
Operator : MA/JU
Sample : PB161647BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK647

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------