

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BN032163.D
 Acq On : 22 Jun 2024 11:58
 Operator : MA/JU
 Sample : P2961-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1G86

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN032163.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	19	24	27	rBV	73772	105328	1.25%	0.134%
2	3.164	27	30	36	rVB	65854	90573	1.07%	0.115%
3	3.575	98	100	116	rBV	93475	151900	1.80%	0.193%
4	3.875	147	151	161	rVB	24056	41075	0.49%	0.052%
5	4.416	240	243	251	rVB	8472	12811	0.15%	0.016%
6	4.769	299	303	310	rVB	27055	40881	0.48%	0.052%
7	6.810	643	650	659	rBV	352553	582403	6.89%	0.739%
8	6.975	671	678	691	rBV	1049024	1665599	19.72%	2.112%
9	7.163	703	710	721	rBV	1193246	1962797	23.24%	2.489%
10	7.240	721	723	733	rVB8	8274	16661	0.20%	0.021%
11	7.628	782	789	797	rBV	1084627	1771255	20.97%	2.246%
12	7.693	797	800	806	rVB2	14868	24621	0.29%	0.031%
13	8.340	903	910	926	rBV	1040685	1764305	20.89%	2.237%
14	8.787	978	986	1001	rVV	1209122	2020609	23.92%	2.562%
15	9.504	1100	1108	1120	rBV	987145	1679189	19.88%	2.129%
16	10.034	1190	1198	1223	rBV	1453894	2695742	31.91%	3.418%
17	10.410	1253	1262	1277	rBV	1523765	2577866	30.52%	3.269%
18	10.557	1279	1287	1304	rBV	1039952	1907191	22.58%	2.419%
19	11.216	1394	1399	1404	rBV5	6574	13756	0.16%	0.017%
20	12.004	1528	1533	1544	rBV2	21976	44552	0.53%	0.056%
21	12.875	1675	1681	1691	rBV7	8649	20460	0.24%	0.026%
22	13.169	1725	1731	1738	rVB3	33213	55138	0.65%	0.070%
23	13.245	1738	1744	1746	rBV5	5659	10430	0.12%	0.013%
24	13.287	1746	1751	1758	rVB4	7187	14889	0.18%	0.019%
25	13.692	1813	1820	1832	rBV	3205286	4479753	53.03%	5.681%
26	13.969	1857	1867	1884	rBV	3402488	5209477	61.67%	6.606%
27	14.275	1912	1919	1930	rBV	2307823	3468570	41.06%	4.399%
28	14.404	1938	1941	1949	rVB7	5605	9635	0.11%	0.012%
29	14.504	1949	1958	1972	rBV	277564	591462	7.00%	0.750%
30	14.704	1986	1992	2001	rVB10	10641	28388	0.34%	0.036%
31	15.075	2051	2055	2058	rBV	12349	14545	0.17%	0.018%
32	15.104	2058	2060	2066	rVB2	7514	11537	0.14%	0.015%
33	15.275	2080	2089	2095	rBV	4350551	6560268	77.66%	8.319%
34	15.322	2095	2097	2105	rVB7	19940	34373	0.41%	0.044%
35	15.404	2105	2111	2125	rBV	1383877	2045670	24.22%	2.594%
36	15.510	2125	2129	2135	rVB2	22388	36359	0.43%	0.046%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BN032163.D
 Acq On : 22 Jun 2024 11:58
 Operator : MA/JU
 Sample : P2961-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1G86

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

37	16.157	2235	2239	2246	rBV10	3810	8635	0.10%	0.011%
38	16.292	2258	2262	2268	rBV3	4080	10036	0.12%	0.013%
39	16.439	2284	2287	2294	rVB9	5431	10298	0.12%	0.013%
40	16.704	2326	2332	2334	rBV5	7476	9335	0.11%	0.012%
41	17.028	2380	2387	2396	rBV	2676144	3902652	46.20%	4.949%
42	17.128	2397	2404	2417	rBV	4970486	7388168	87.46%	9.369%
43	17.422	2450	2454	2459	rBV4	6296	11010	0.13%	0.014%
44	17.698	2497	2501	2507	rVB8	9984	18168	0.22%	0.023%
45	17.928	2535	2540	2549	rVV	202039	364324	4.31%	0.462%
46	17.998	2549	2552	2556	rVB	21001	31260	0.37%	0.040%
47	18.351	2610	2612	2616	rBV5	8287	9777	0.12%	0.012%
48	18.469	2628	2632	2636	rBV6	10786	15091	0.18%	0.019%
49	18.986	2716	2720	2726	rBV	65222	95523	1.13%	0.121%
50	19.063	2728	2733	2736	rBV	62948	98141	1.16%	0.124%
51	19.216	2754	2759	2766	rBV2	166216	281121	3.33%	0.356%
52	19.427	2789	2795	2803	rBV	5779656	8069032	95.52%	10.232%
53	19.663	2832	2835	2839	rBV2	28896	40160	0.48%	0.051%
54	21.263	3101	3107	3115	rBV	2703105	3907960	46.26%	4.956%
55	21.404	3129	3131	3136	rVB	79836	99511	1.18%	0.126%
56	23.974	3559	3568	3586	rVB3	3446694	8447167	100.00%	10.712%
57	24.174	3593	3602	3616	rVB	1761613	4280401	50.67%	5.428%




Sum of corrected areas: 78857838

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032163.D
Acq On : 22 Jun 2024 11:58
Operator : MA/JU
Sample : P2961-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1G86

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

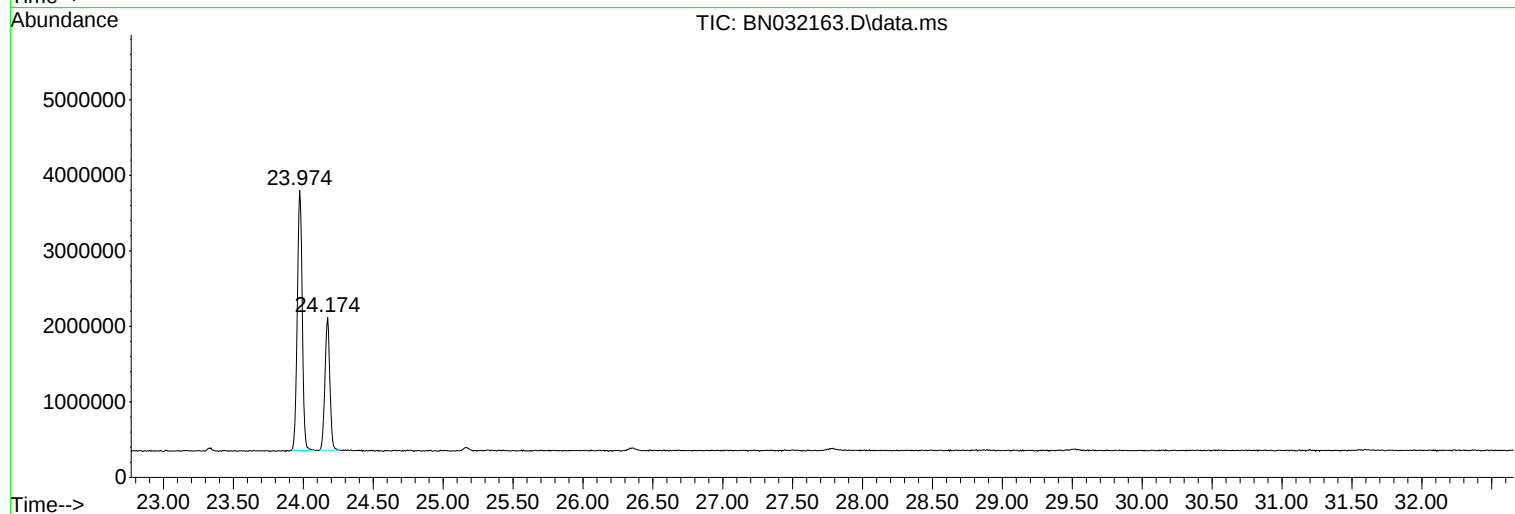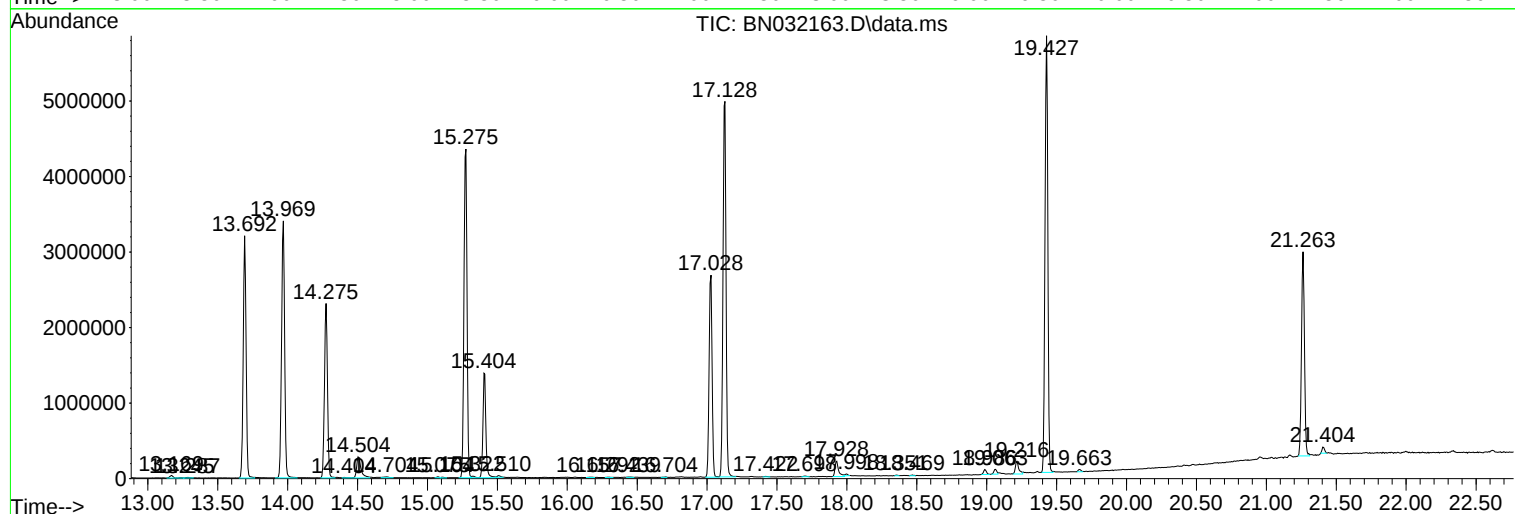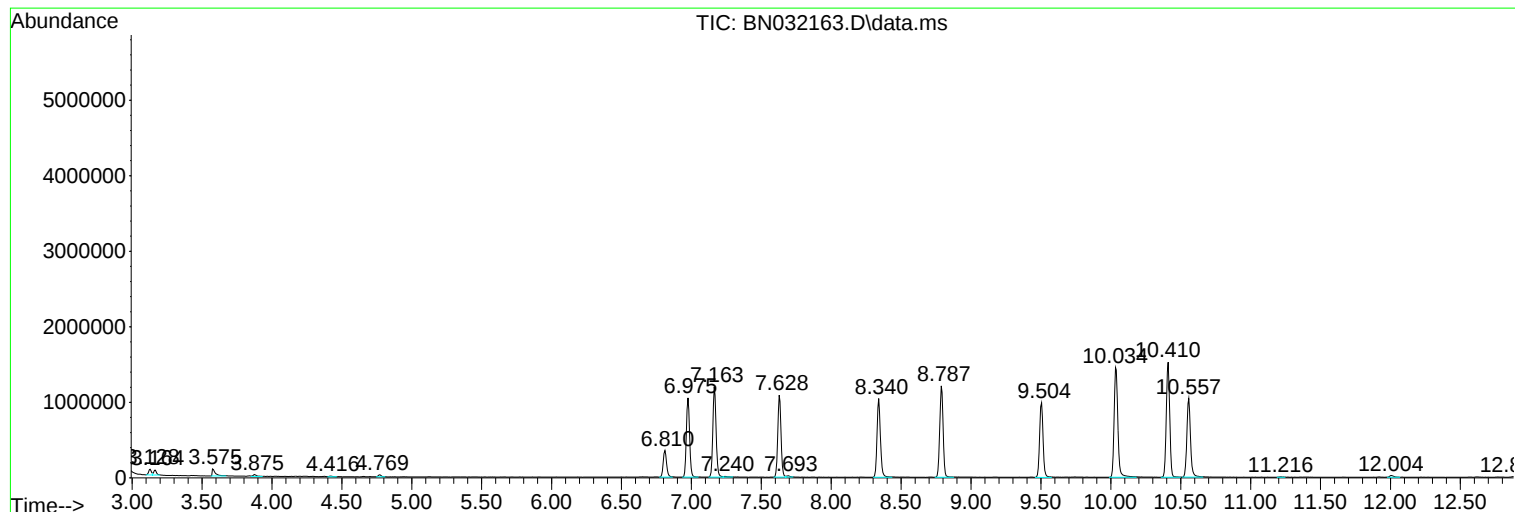

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032163.D
Acq On : 22 Jun 2024 11:58
Operator : MA/JU
Sample : P2961-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1G86

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032163.D
Acq On : 22 Jun 2024 11:58
Operator : MA/JU
Sample : P2961-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1G86

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc