

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BN032165.D
 Acq On : 22 Jun 2024 13:17
 Operator : MA/JU
 Sample : P2961-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1G88

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN032165.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	26	30	39	rVB	49747	67743	0.87%	0.103%
2	3.570	97	99	122	rBV	192575	321813	4.15%	0.491%
3	3.875	147	151	156	rVB	27822	36630	0.47%	0.056%
4	4.417	240	243	249	rVB	8353	12026	0.16%	0.018%
5	4.770	299	303	310	rVB	21376	33885	0.44%	0.052%
6	6.811	643	650	662	rBV	284237	467956	6.03%	0.714%
7	6.975	669	678	691	rBV	872611	1403798	18.10%	2.142%
8	7.164	703	710	720	rBV	990359	1631712	21.04%	2.489%
9	7.628	782	789	797	rBV	934633	1500652	19.35%	2.289%
10	7.693	797	800	804	rVB2	12267	17765	0.23%	0.027%
11	8.340	903	910	927	rBV	820509	1363082	17.57%	2.080%
12	8.787	977	986	996	rBV	996896	1672734	21.56%	2.552%
13	9.505	1099	1108	1121	rBV	790134	1371538	17.68%	2.093%
14	9.693	1134	1140	1143	rBV6	5207	10618	0.14%	0.016%
15	10.034	1191	1198	1215	rBV	1160017	2132998	27.50%	3.254%
16	10.410	1253	1262	1273	rBV	1217617	2105669	27.15%	3.213%
17	10.557	1278	1287	1304	rBV	940106	1727961	22.28%	2.636%
18	11.210	1393	1398	1401	rBV5	4926	8649	0.11%	0.013%
19	11.657	1470	1474	1479	rVB3	6666	9868	0.13%	0.015%
20	12.004	1526	1533	1544	rVB2	18704	39703	0.51%	0.061%
21	13.087	1709	1717	1721	rBV5	6136	9904	0.13%	0.015%
22	13.693	1811	1820	1836	rBV	2389690	3311350	42.69%	5.052%
23	13.969	1857	1867	1882	rBV	2632908	4008088	51.67%	6.115%
24	14.175	1896	1902	1908	rVB4	13761	22292	0.29%	0.034%
25	14.275	1911	1919	1931	rBV	1875563	2778317	35.82%	4.239%
26	14.510	1951	1959	1979	rBV	196155	444685	5.73%	0.678%
27	15.075	2050	2055	2058	rBV2	8750	12880	0.17%	0.020%
28	15.128	2058	2064	2073	rVB8	10787	20845	0.27%	0.032%
29	15.269	2081	2088	2096	rBV	3381023	5082242	65.52%	7.754%
30	15.404	2105	2111	2124	rBV	1016200	1539937	19.85%	2.349%
31	15.510	2126	2129	2135	rVB4	19410	31995	0.41%	0.049%
32	15.992	2207	2211	2219	rBV8	6233	15266	0.20%	0.023%
33	16.810	2348	2350	2359	rVB5	6920	15641	0.20%	0.024%
34	17.022	2380	2386	2396	rBV	2124482	3206218	41.33%	4.892%
35	17.122	2397	2403	2416	rVV2	4103581	5968300	76.94%	9.106%
36	17.322	2435	2437	2444	rVB5	13120	17181	0.22%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032165.D
Acq On : 22 Jun 2024 13:17
Operator : MA/JU
Sample : P2961-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1G88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION

37	17.704	2498	2502	2505	rVB6	8084	11787	0.15%	0.018%
38	17.922	2535	2539	2549	rBV	139719	254964	3.29%	0.389%
39	18.986	2716	2720	2725	rBV3	62677	85741	1.11%	0.131%
40	19.063	2729	2733	2737	rVV	52537	79914	1.03%	0.122%
41	19.216	2755	2759	2768	rBV2	75682	138791	1.79%	0.212%
42	19.428	2789	2795	2804	rBV	5113552	6959501	89.72%	10.618%
43	21.263	3101	3107	3116	rBV	2502105	3606296	46.49%	5.502%
44	23.974	3559	3568	3587	rVB2	3123066	7756948	100.00%	11.834%
45	24.169	3593	3601	3617	rVB	1659531	4229342	54.52%	6.453%




Sum of corrected areas: 65545225

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032165.D
Acq On : 22 Jun 2024 13:17
Operator : MA/JU
Sample : P2961-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1G88

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

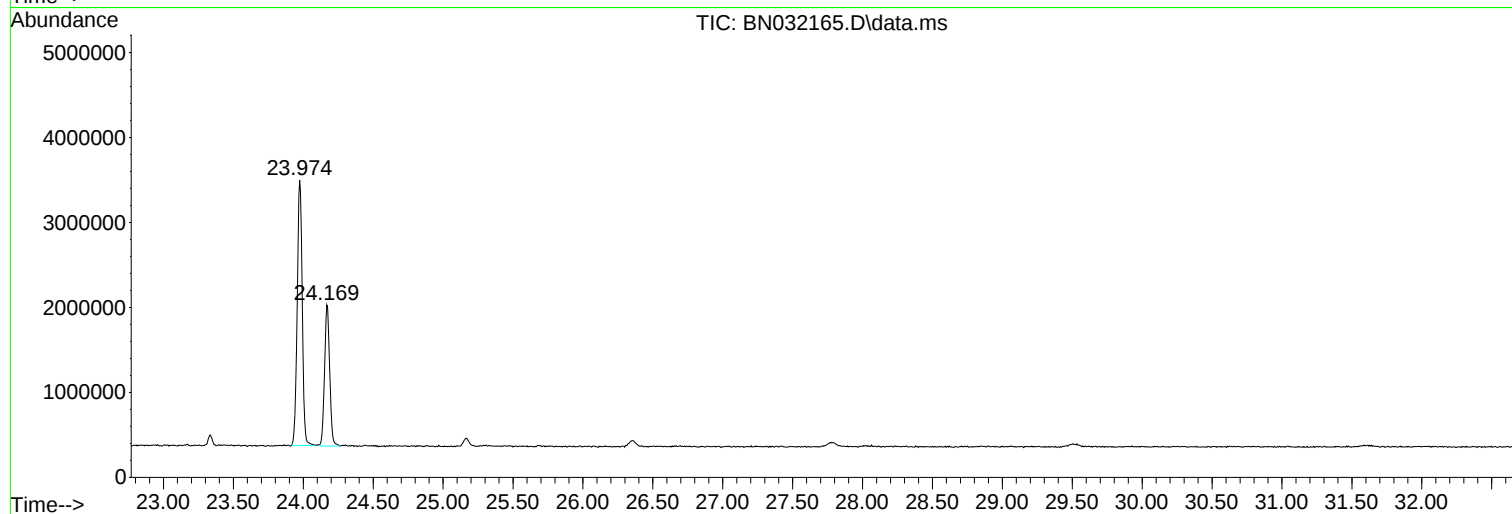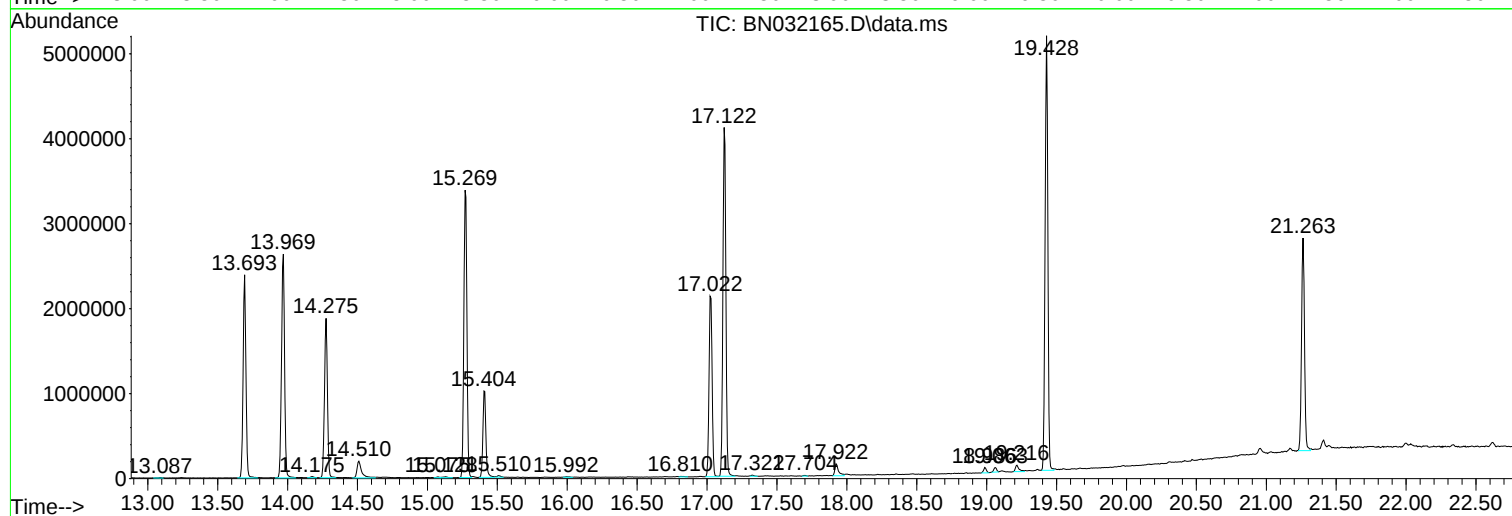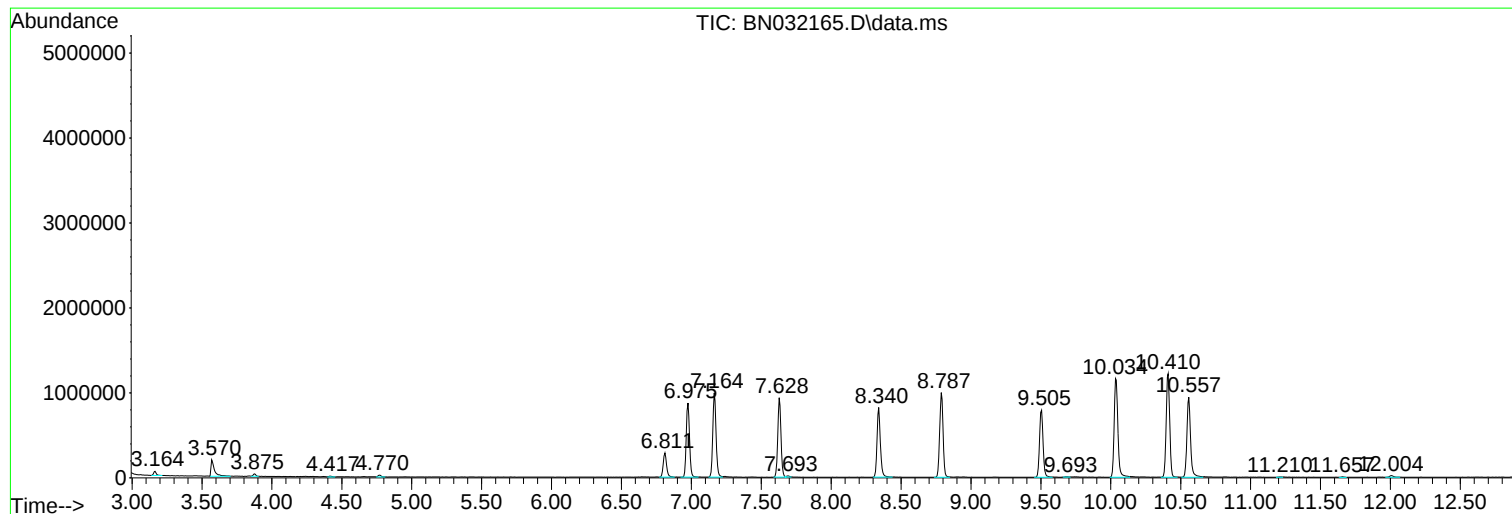

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032165.D
Acq On : 22 Jun 2024 13:17
Operator : MA/JU
Sample : P2961-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1G88

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032165.D
Acq On : 22 Jun 2024 13:17
Operator : MA/JU
Sample : P2961-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1G88

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc