

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BN032166.D
 Acq On : 22 Jun 2024 13:56
 Operator : MA/JU
 Sample : P3017-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E08C0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN032166.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	26	30	40	rVB	58568	81638	0.91%	0.106%
2	3.428	72	75	84	rBV	55742	82279	0.92%	0.107%
3	3.570	96	99	118	rBV	243564	389413	4.35%	0.504%
4	3.875	147	151	155	rVV	15452	20484	0.23%	0.027%
5	4.240	208	213	219	rVB6	8940	13331	0.15%	0.017%
6	4.417	240	243	249	rVB2	10440	16801	0.19%	0.022%
7	4.769	298	303	311	rVB	34061	54637	0.61%	0.071%
8	5.658	447	454	460	rBV	51566	79016	0.88%	0.102%
9	6.652	618	623	631	rVB6	6604	13548	0.15%	0.018%
10	6.811	643	650	664	rVB	416978	705006	7.88%	0.913%
11	6.975	671	678	694	rVB	1114086	1743322	19.48%	2.257%
12	7.163	703	710	720	rBV	1273967	2078557	23.22%	2.691%
13	7.246	722	724	734	rVB5	11490	24161	0.27%	0.031%
14	7.628	782	789	797	rBV	951281	1524079	17.03%	1.973%
15	8.340	903	910	927	rBV	1171297	1951095	21.80%	2.526%
16	8.787	978	986	999	rBV	1269573	2102919	23.49%	2.723%
17	8.952	1010	1014	1020	rVB7	5065	9094	0.10%	0.012%
18	9.169	1045	1051	1057	rBV	18464	30531	0.34%	0.040%
19	9.352	1077	1082	1091	rBV	26595	48899	0.55%	0.063%
20	9.505	1100	1108	1119	rBV	1005451	1730619	19.33%	2.241%
21	9.746	1144	1149	1158	rBV7	5785	13386	0.15%	0.017%
22	10.034	1189	1198	1220	rBV	1482585	2737686	30.59%	3.544%
23	10.410	1252	1262	1272	rBV	1263232	2147209	23.99%	2.780%
24	10.557	1276	1287	1307	rBV	1277082	2335086	26.09%	3.023%
25	10.975	1351	1358	1360	rBV7	6159	10428	0.12%	0.014%
26	11.163	1382	1390	1396	rBV2	47497	112905	1.26%	0.146%
27	11.828	1497	1503	1509	rBV7	6006	10251	0.11%	0.013%
28	12.004	1524	1533	1541	rBV2	24619	45604	0.51%	0.059%
29	13.116	1714	1722	1730	rVB	73084	129691	1.45%	0.168%
30	13.240	1739	1743	1750	rVB5	6487	9589	0.11%	0.012%
31	13.693	1813	1820	1834	rBV	3030708	4156382	46.43%	5.381%
32	13.787	1834	1836	1842	rVB6	5954	9553	0.11%	0.012%
33	13.969	1853	1867	1884	rBV	3327075	5158880	57.63%	6.679%
34	14.175	1895	1902	1907	rVB8	7325	13885	0.16%	0.018%
35	14.275	1911	1919	1931	rBV	1933348	2821823	31.53%	3.653%
36	14.504	1950	1958	1972	rBV	312726	659879	7.37%	0.854%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BN032166.D
 Acq On : 22 Jun 2024 13:56
 Operator : MA/JU
 Sample : P3017-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E08C0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

37	14.798	2002	2008	2013	rVB7	4167	9110	0.10%	0.012%
38	15.069	2049	2054	2059	rBV4	6105	9757	0.11%	0.013%
39	15.275	2080	2089	2104	rBV	4210351	6380246	71.28%	8.260%
40	15.404	2105	2111	2124	rVV	1249596	1896299	21.19%	2.455%
41	15.510	2125	2129	2137	rVB3	23742	45490	0.51%	0.059%
42	15.834	2180	2184	2189	rBV4	7910	13719	0.15%	0.018%
43	15.992	2207	2211	2219	rVB7	10862	19147	0.21%	0.025%
44	16.169	2235	2241	2245	rBV9	5946	14302	0.16%	0.019%
45	16.816	2348	2351	2358	rVB5	7053	12957	0.14%	0.017%
46	16.951	2371	2374	2379	rBV6	9204	14063	0.16%	0.018%
47	17.028	2380	2387	2396	rBV	2257005	3243597	36.24%	4.199%
48	17.128	2396	2404	2417	rBV	4733757	7000058	78.20%	9.063%
49	17.316	2434	2436	2445	rVB5	5150	10173	0.11%	0.013%
50	17.704	2497	2502	2506	rBV3	13892	19771	0.22%	0.026%
51	17.928	2535	2540	2550	rBV	144537	256290	2.86%	0.332%
52	18.986	2716	2720	2724	rBV	64523	89428	1.00%	0.116%
53	19.063	2728	2733	2738	rBV	58909	96484	1.08%	0.125%
54	19.216	2755	2759	2766	rBV2	70691	113972	1.27%	0.148%
55	19.428	2789	2795	2808	rBV	5914299	8090747	90.39%	10.475%
56	20.957	3051	3055	3064	rVB3	145316	247851	2.77%	0.321%
57	21.263	3101	3107	3117	rBV	2423935	3620422	40.45%	4.687%
58	23.974	3559	3568	3585	rVB2	3690542	8950971	100.00%	11.589%
59	24.168	3593	3601	3612	rVB	1604014	4012136	44.82%	5.194%




Sum of corrected areas: 77238656

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032166.D
Acq On : 22 Jun 2024 13:56
Operator : MA/JU
Sample : P3017-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E08C0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

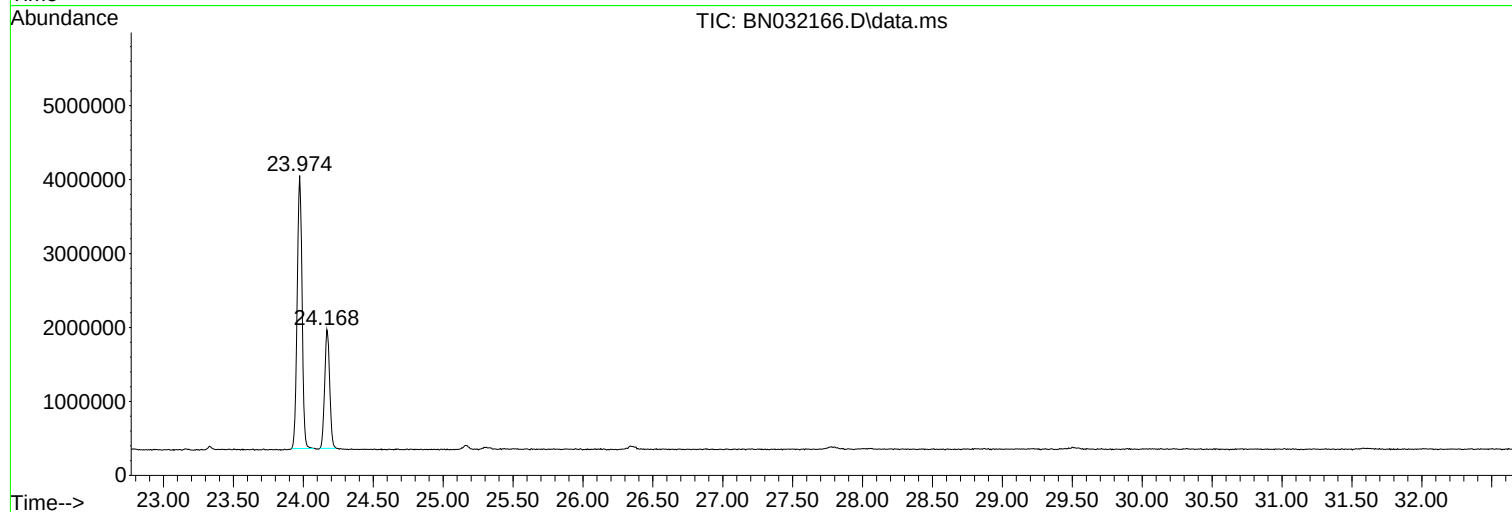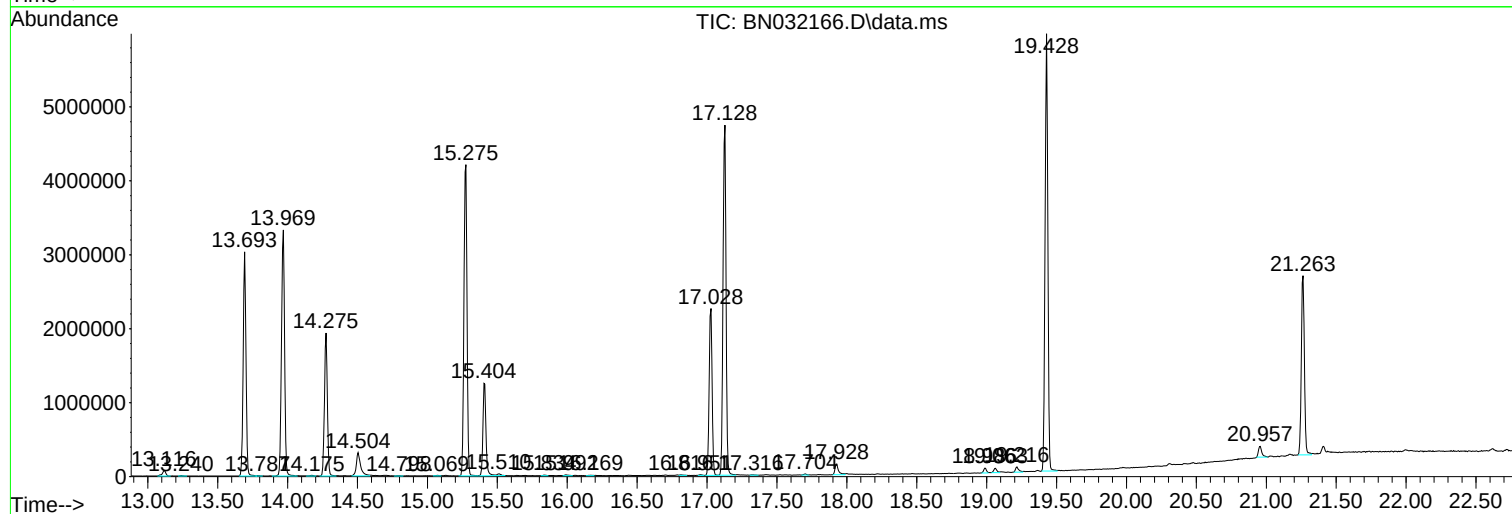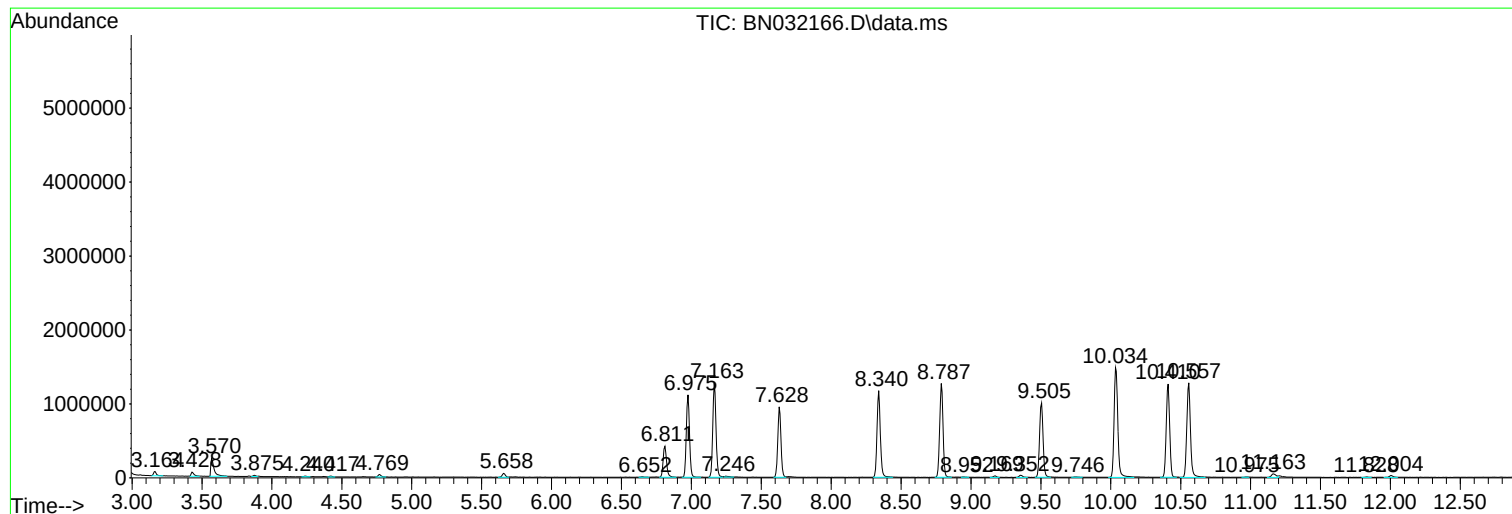

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032166.D
Acq On : 22 Jun 2024 13:56
Operator : MA/JU
Sample : P3017-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E08C0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032166.D
Acq On : 22 Jun 2024 13:56
Operator : MA/JU
Sample : P3017-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E08C0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc