

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BN032169.D
 Acq On : 22 Jun 2024 16:35
 Operator : MA/JU
 Sample : PB161556BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK556

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN032169.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	25	29	37	rVB	70967	93997	1.29%	0.123%
2	3.564	94	98	119	rBV	842637	1301344	17.89%	1.696%
3	3.875	146	151	159	rVB	15028	24718	0.34%	0.032%
4	6.811	643	650	668	rBV	1037096	1702421	23.40%	2.219%
5	6.975	671	678	688	rVV	918557	1439792	19.79%	1.876%
6	7.164	703	710	725	rBV	1169068	1850619	25.44%	2.412%
7	7.628	779	789	799	rBV	1021213	1668865	22.94%	2.175%
8	8.340	902	910	926	rBV	1378636	2306134	31.70%	3.005%
9	8.787	979	986	999	rBV	1067776	1767406	24.30%	2.303%
10	9.505	1099	1108	1126	rBV	871500	1472640	20.24%	1.919%
11	10.034	1191	1198	1223	rBV	1255981	2340280	32.17%	3.050%
12	10.410	1254	1262	1273	rBV	1490130	2524548	34.70%	3.290%
13	10.557	1279	1287	1306	rBV	1377935	2532759	34.82%	3.301%
14	12.010	1527	1534	1541	rBV2	17850	39488	0.54%	0.051%
15	13.693	1813	1820	1830	rBV	2822313	3959588	54.43%	5.160%
16	13.969	1859	1867	1884	rBV	2936895	4661384	64.08%	6.075%
17	14.275	1912	1919	1936	rBV	2472074	3672810	50.49%	4.787%
18	14.498	1951	1957	1979	rBV	1021261	1822342	25.05%	2.375%
19	15.275	2081	2089	2105	rBV	3850168	5834740	80.21%	7.604%
20	15.410	2105	2112	2124	rVV	1124993	1702255	23.40%	2.218%
21	15.510	2125	2129	2135	rVB	21352	35736	0.49%	0.047%
22	16.810	2346	2350	2355	rBV2	7501	10563	0.15%	0.014%
23	17.028	2380	2387	2397	rBV	3038678	4427379	60.86%	5.770%
24	17.122	2397	2403	2420	rVV	4198252	6381564	87.72%	8.317%
25	17.934	2536	2541	2545	rBV6	15596	27723	0.38%	0.036%
26	18.986	2716	2720	2725	rBV2	56581	76360	1.05%	0.100%
27	19.063	2728	2733	2737	rBV	50091	74585	1.03%	0.097%
28	19.428	2789	2795	2803	rBV	5106944	7274669	100.00%	9.481%
29	21.263	3101	3107	3116	rBV	3046844	4588311	63.07%	5.980%
30	23.974	3559	3568	3582	rVB	2677605	6488356	89.19%	8.456%
31	24.169	3593	3601	3613	rVB	1891893	4627689	63.61%	6.031%




Sum of corrected areas: 76731065

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032169.D
Acq On : 22 Jun 2024 16:35
Operator : MA/JU
Sample : PB161556BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK556

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

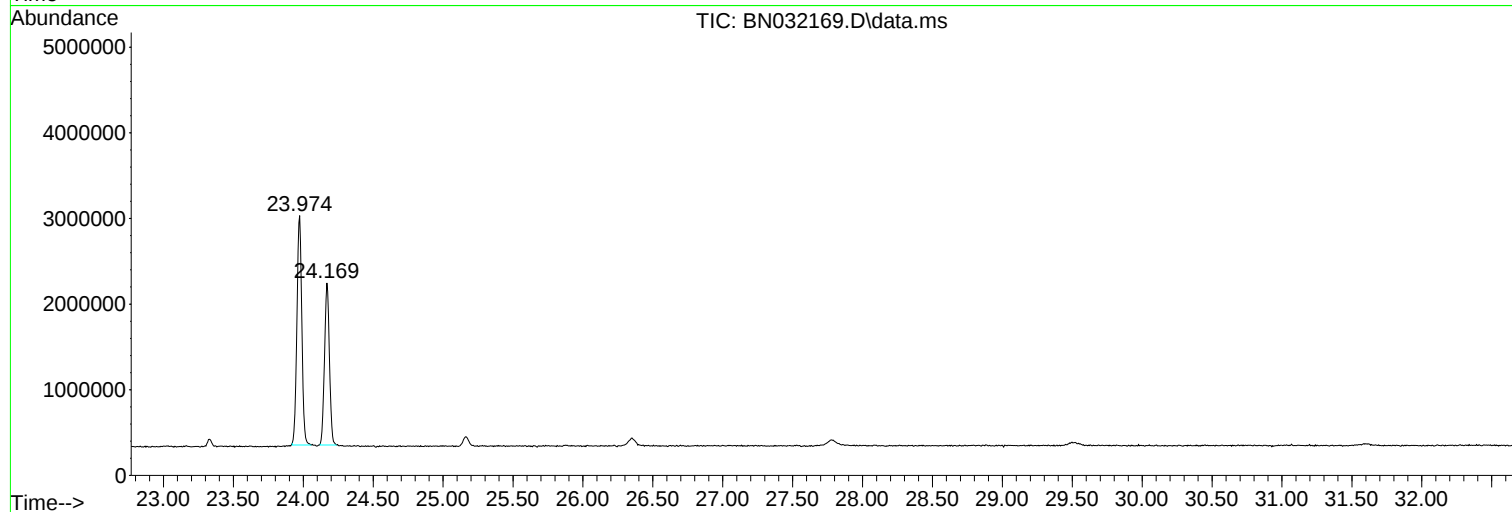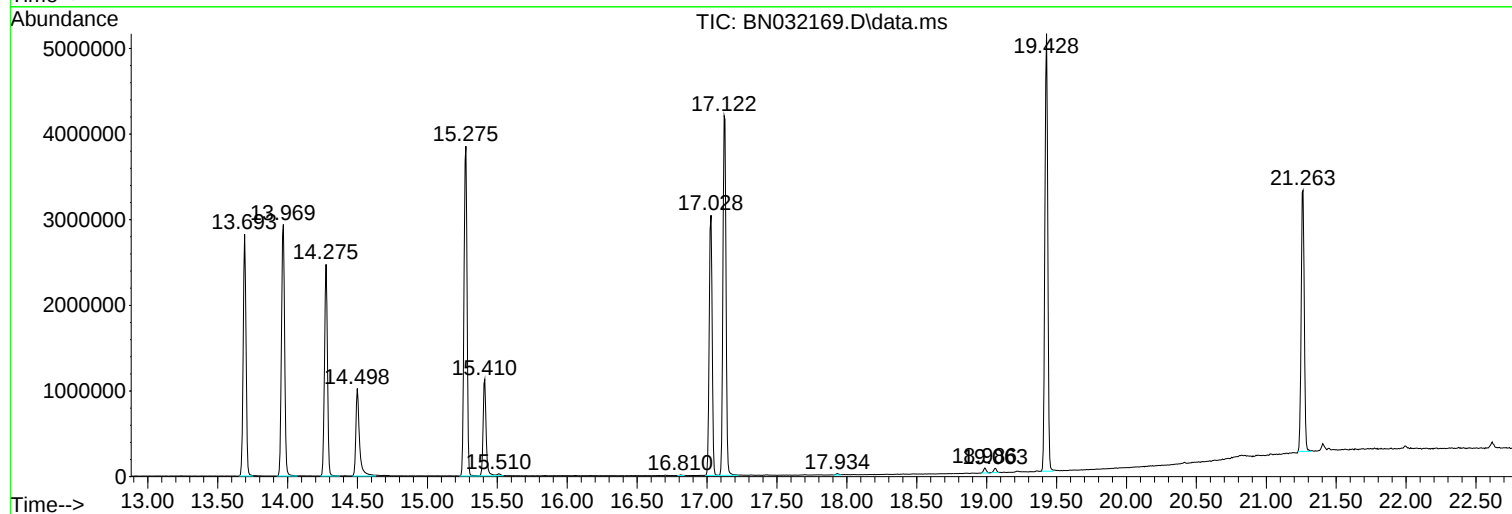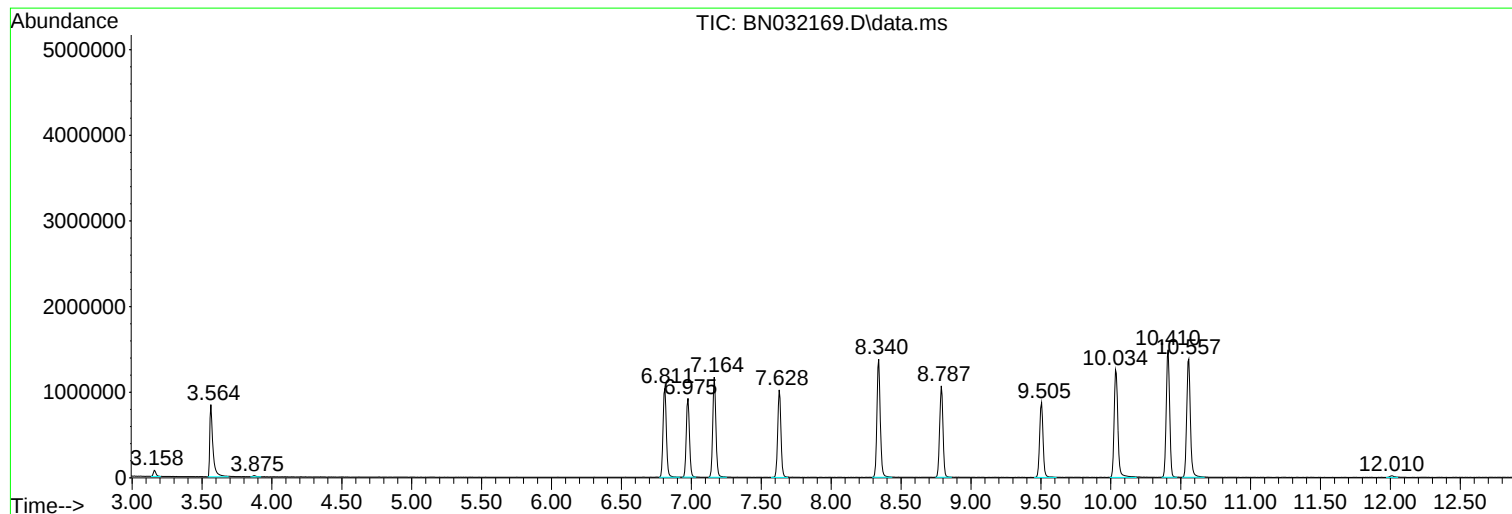

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032169.D
Acq On : 22 Jun 2024 16:35
Operator : MA/JU
Sample : PB161556BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK556

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032169.D
Acq On : 22 Jun 2024 16:35
Operator : MA/JU
Sample : PB161556BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK556

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc