

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
 Data File : BN032185.D
 Acq On : 23 Jun 2024 03:45
 Operator : MA/JU
 Sample : PB161462BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK462

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN032185.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	25	30	37	rVB	83703	109435	2.04%	0.154%
2	3.564	95	98	114	rBV	1060594	1563236	29.11%	2.195%
3	3.875	147	151	156	rVB	16606	24943	0.46%	0.035%
4	6.816	644	651	663	rBV	1294985	2124881	39.58%	2.984%
5	6.975	672	678	691	rVB	1059638	1707562	31.80%	2.398%
6	7.169	704	711	723	rBV	1410145	2296640	42.77%	3.225%
7	7.634	781	790	804	rBV	1165364	1934582	36.03%	2.717%
8	8.346	903	911	926	rBV	1684659	2853847	53.15%	4.008%
9	8.793	979	987	999	rBV	1241841	2144384	39.94%	3.011%
10	9.505	1100	1108	1123	rBV	1083998	1854933	34.55%	2.605%
11	10.040	1192	1199	1220	rBV	1556521	2892934	53.88%	4.063%
12	10.410	1254	1262	1273	rBV	1689759	2868612	53.43%	4.029%
13	10.563	1280	1288	1308	rBV	1621629	2926979	54.51%	4.111%
14	12.010	1527	1534	1542	rBV	27074	53667	1.00%	0.075%
15	13.063	1709	1713	1717	rBV6	3870	7755	0.14%	0.011%
16	13.240	1739	1743	1750	rVB7	5924	12859	0.24%	0.018%
17	13.693	1813	1820	1834	rBV	2598834	3767996	70.18%	5.292%
18	13.787	1834	1836	1842	rVB7	4803	7388	0.14%	0.010%
19	13.969	1859	1867	1879	rBV	3054150	4754254	88.55%	6.677%
20	14.275	1912	1919	1930	rBV	2329289	3576999	66.62%	5.023%
21	14.516	1953	1960	1978	rBV	755691	1456016	27.12%	2.045%
22	14.634	1978	1980	1984	rVV4	9518	14209	0.26%	0.020%
23	14.692	1986	1990	1994	rVB6	3834	7556	0.14%	0.011%
24	15.275	2082	2089	2102	rBV	3665814	5369220	100.00%	7.540%
25	15.410	2106	2112	2125	rVV	764177	1115457	20.78%	1.566%
26	15.516	2125	2130	2141	rVB3	22130	44396	0.83%	0.062%
27	16.063	2218	2223	2224	rBV5	6651	8520	0.16%	0.012%
28	16.710	2328	2333	2337	rBV7	6355	10196	0.19%	0.014%
29	16.816	2347	2351	2356	rVB4	6120	10531	0.20%	0.015%
30	17.028	2381	2387	2397	rBV	2402225	3442151	64.11%	4.834%
31	17.128	2397	2404	2418	rVV2	3500790	5057627	94.20%	7.103%
32	17.322	2433	2437	2440	rBV5	8892	14773	0.28%	0.021%
33	17.928	2538	2540	2548	rVB8	9007	15865	0.30%	0.022%
34	18.263	2595	2597	2603	rBV7	7053	12543	0.23%	0.018%
35	18.992	2717	2721	2728	rVB3	41690	64139	1.19%	0.090%
36	19.063	2729	2733	2738	rVV	43209	59668	1.11%	0.084%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032185.D
Acq On : 23 Jun 2024 03:45
Operator : MA/JU
Sample : PB161462BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK462

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION

37	19.428	2790	2795	2803	rBV	3497432	4973173	92.62%	6.984%
38	21.263	3102	3107	3116	rVB	2016837	3065704	57.10%	4.305%
39	23.980	3561	3569	3584	rVB2	2159812	5287015	98.47%	7.425%
40	24.180	3595	3603	3615	rVB	1426057	3694710	68.81%	5.189%




Sum of corrected areas: 71207355

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032185.D
Acq On : 23 Jun 2024 03:45
Operator : MA/JU
Sample : PB161462BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK462

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

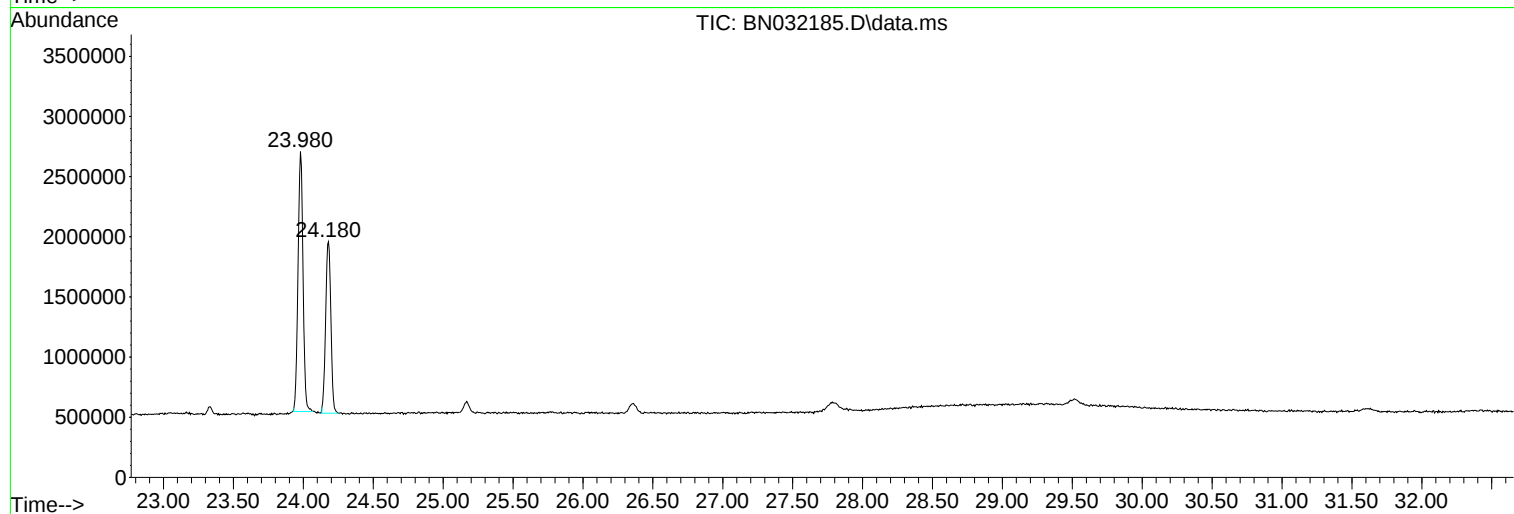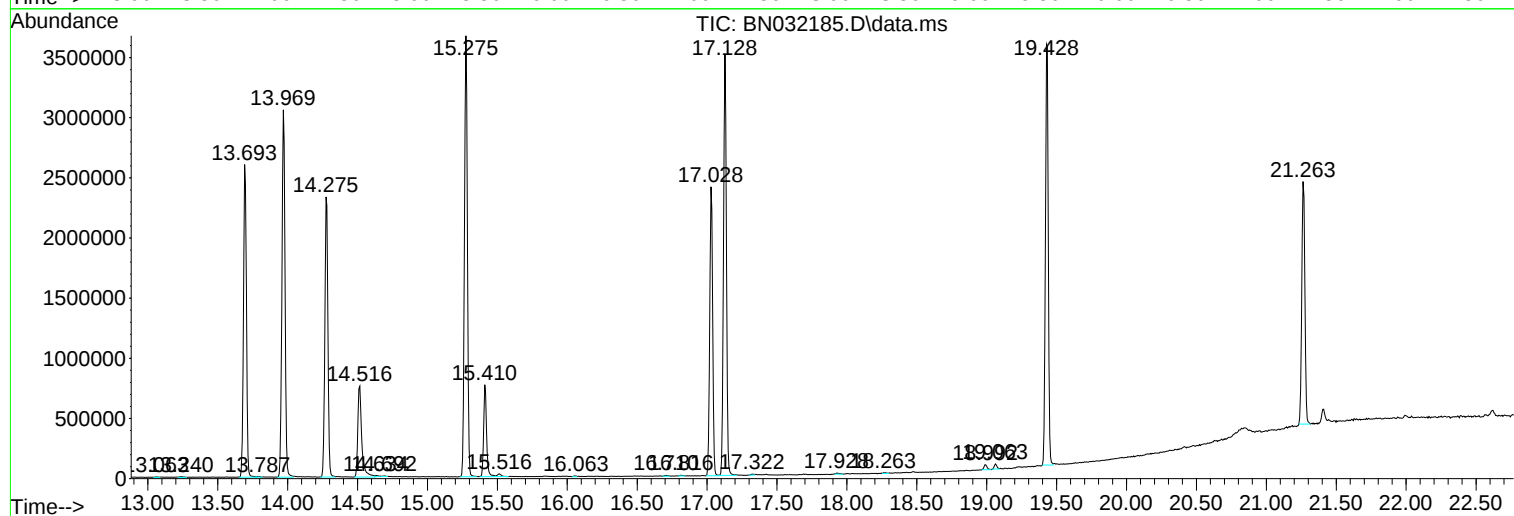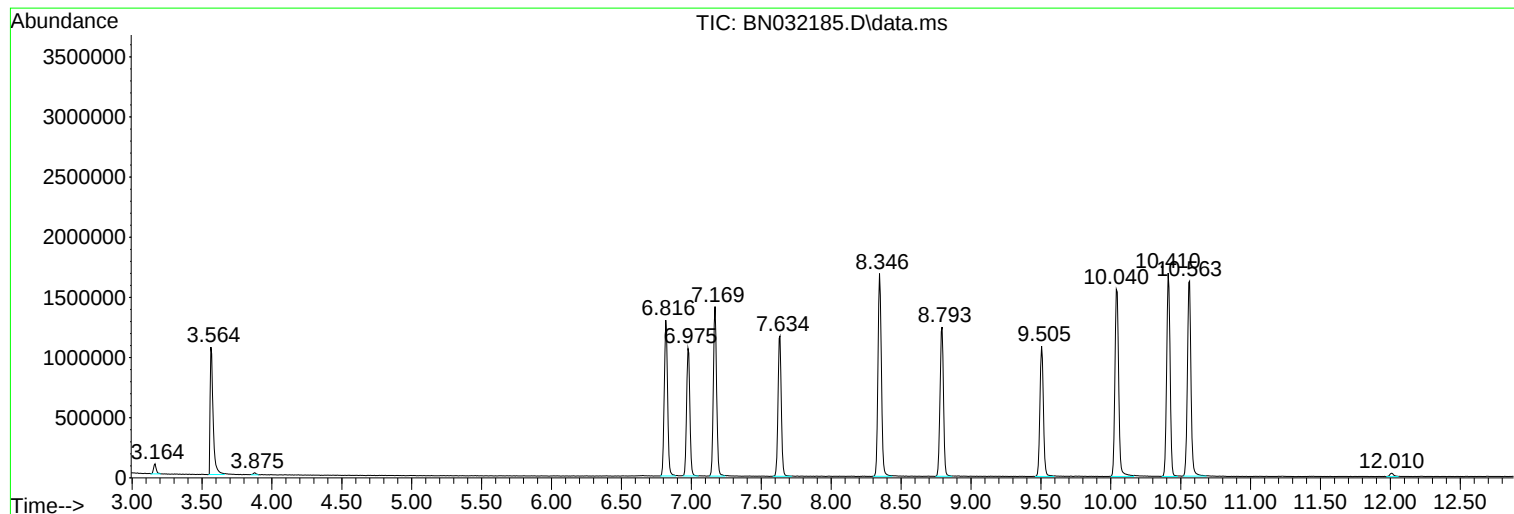

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032185.D
Acq On : 23 Jun 2024 03:45
Operator : MA/JU
Sample : PB161462BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK462

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062224\
Data File : BN032185.D
Acq On : 23 Jun 2024 03:45
Operator : MA/JU
Sample : PB161462BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK462

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------