
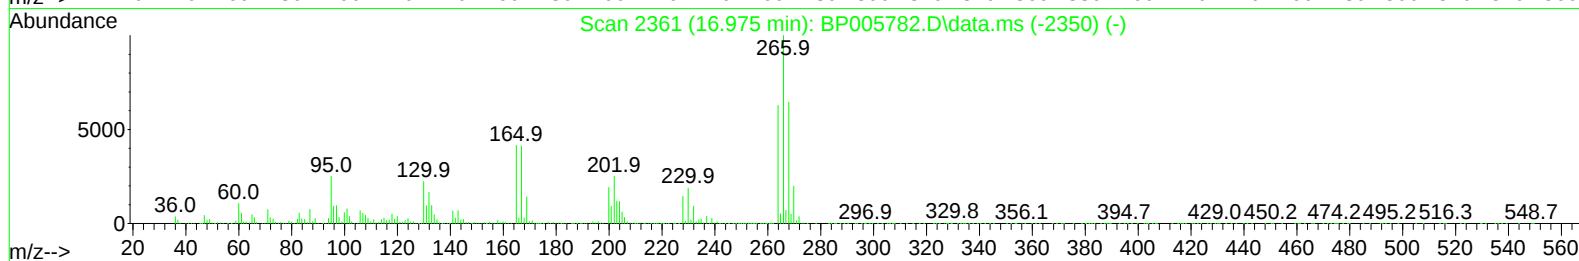
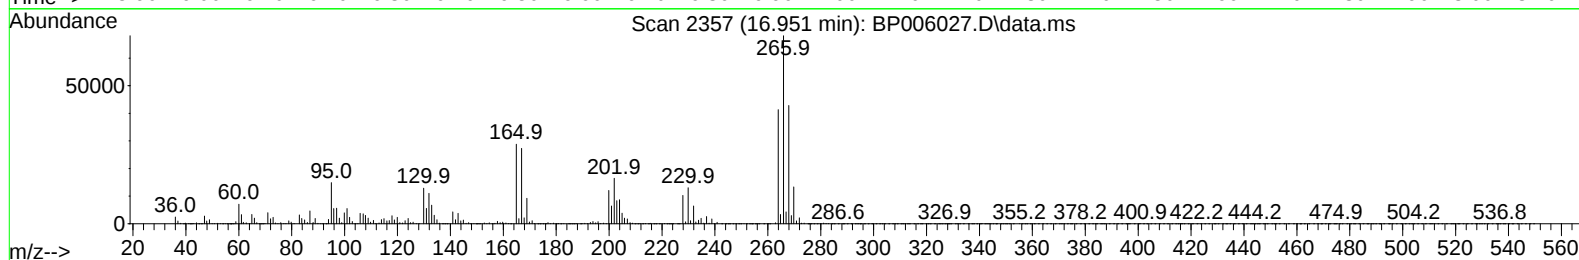


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP062321\
Data File : BP006027.D
Acq On : 23 Jun 2021 09:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 11:22:50 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 22 17:52:38 2021
Response via : Initial Calibration

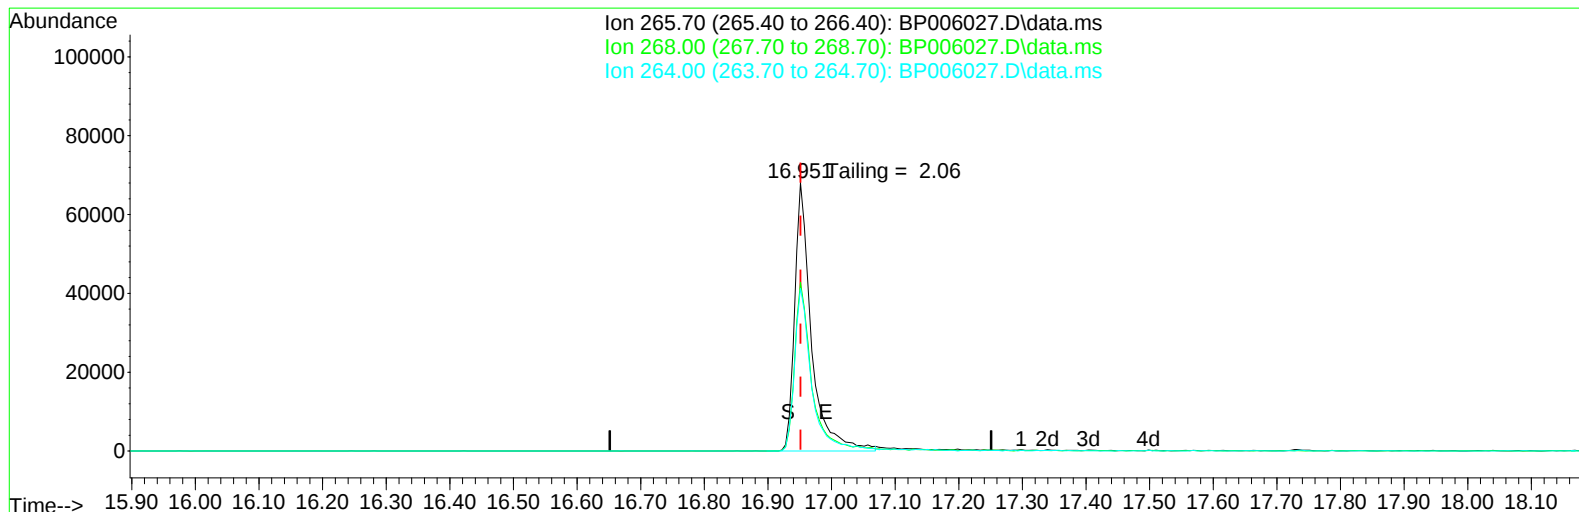

TIC: BP006027.D\data.ms

(70) Pentachlorophenol (C)

16.951min (-0.000) 289081.46 ng m

response 121173

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.86
264.00	62.90	60.70
0.00	0.00	0.00