
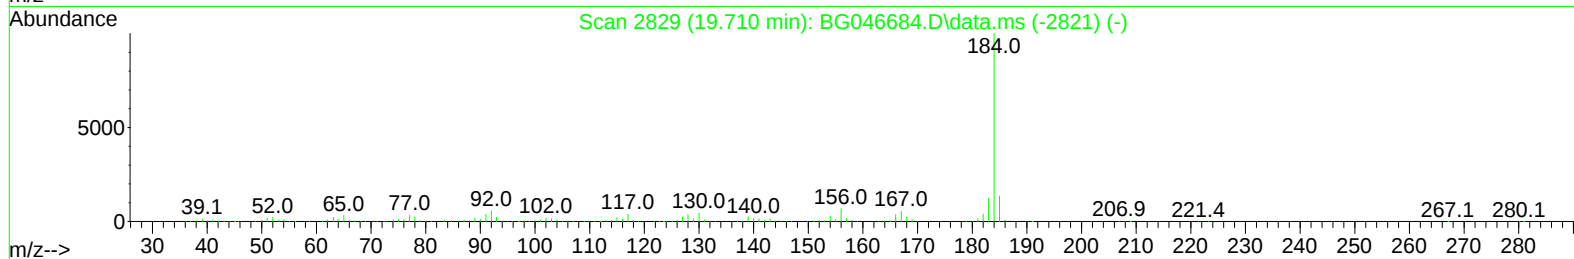
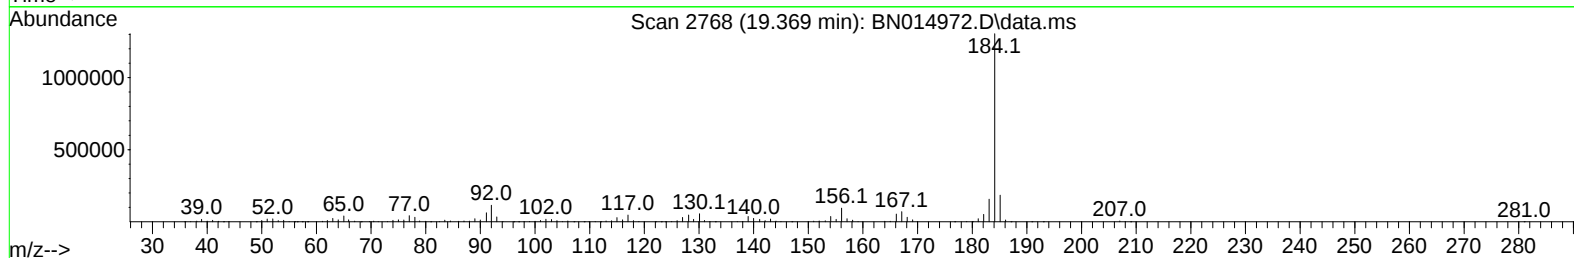


Quant Time: Jun 22 14:58:24 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 22 07:55:10 2021
Response via : Initial Calibration

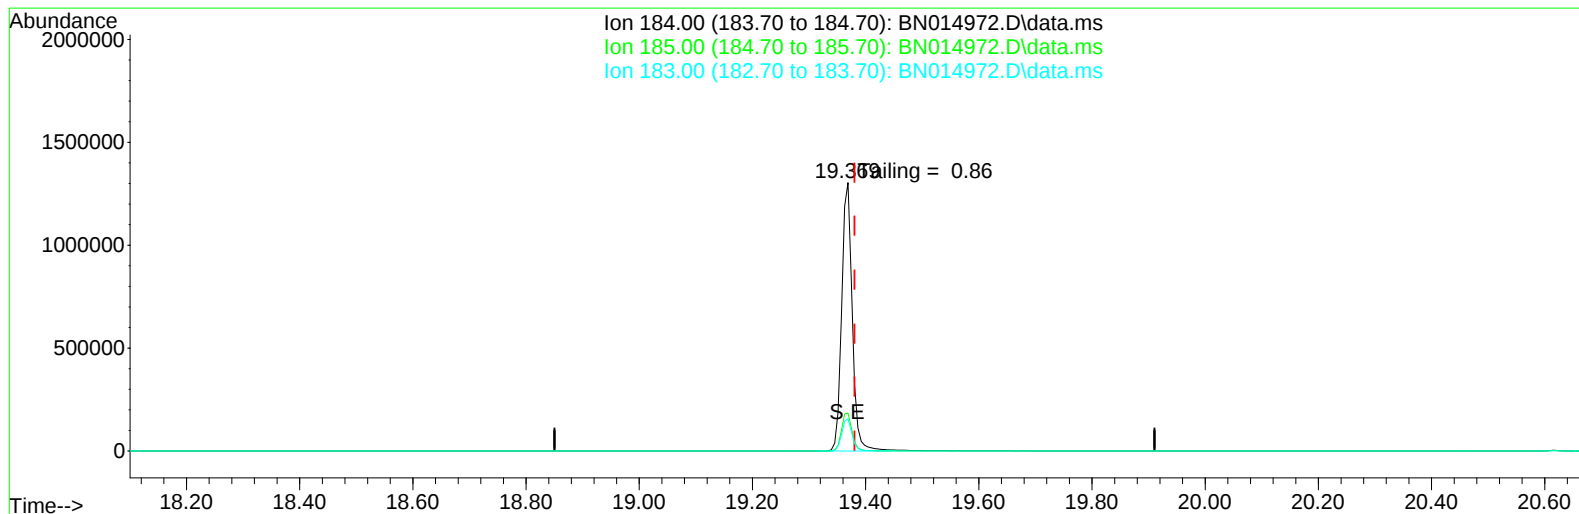

TIC: BN014972.D\data.ms

(77) Benzidine




19.369min (-0.011) 0.00 ng

response **1702141**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.18
183.00	13.20	12.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062321\
 Data File : BN014972.D
 Acq On : 22 Jun 2021 13:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 14:58:24 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 22 07:55:10 2021
 Response via : Initial Calibration

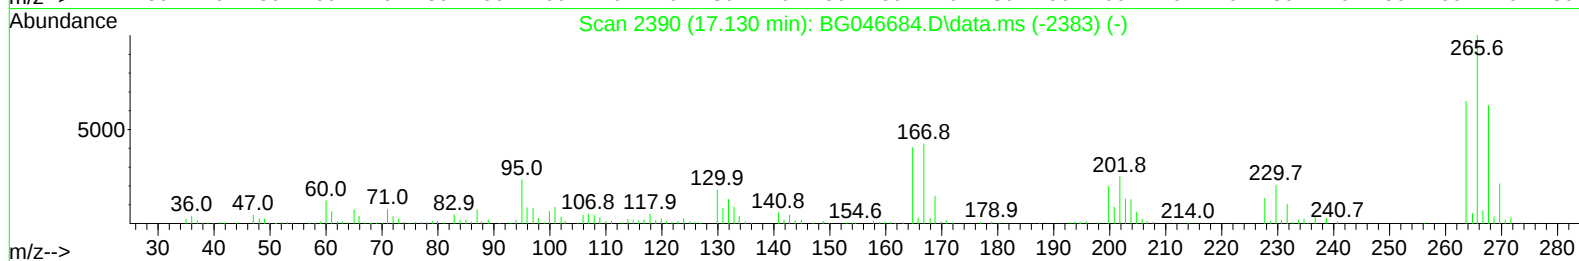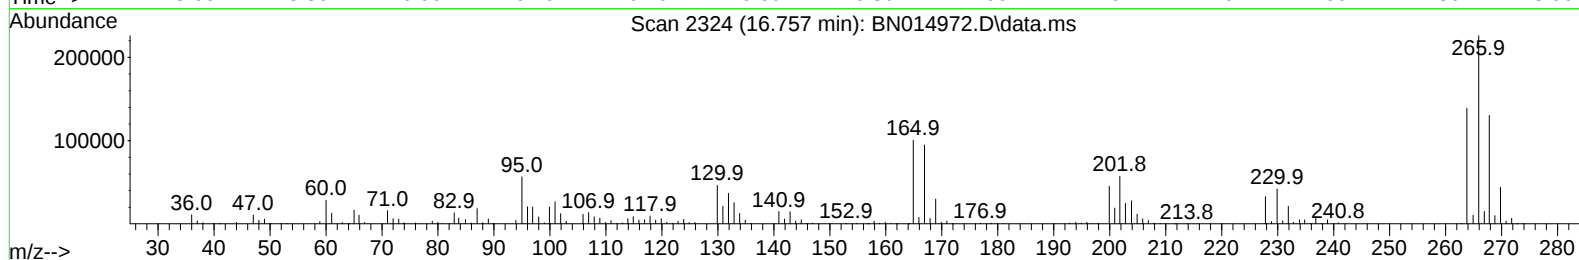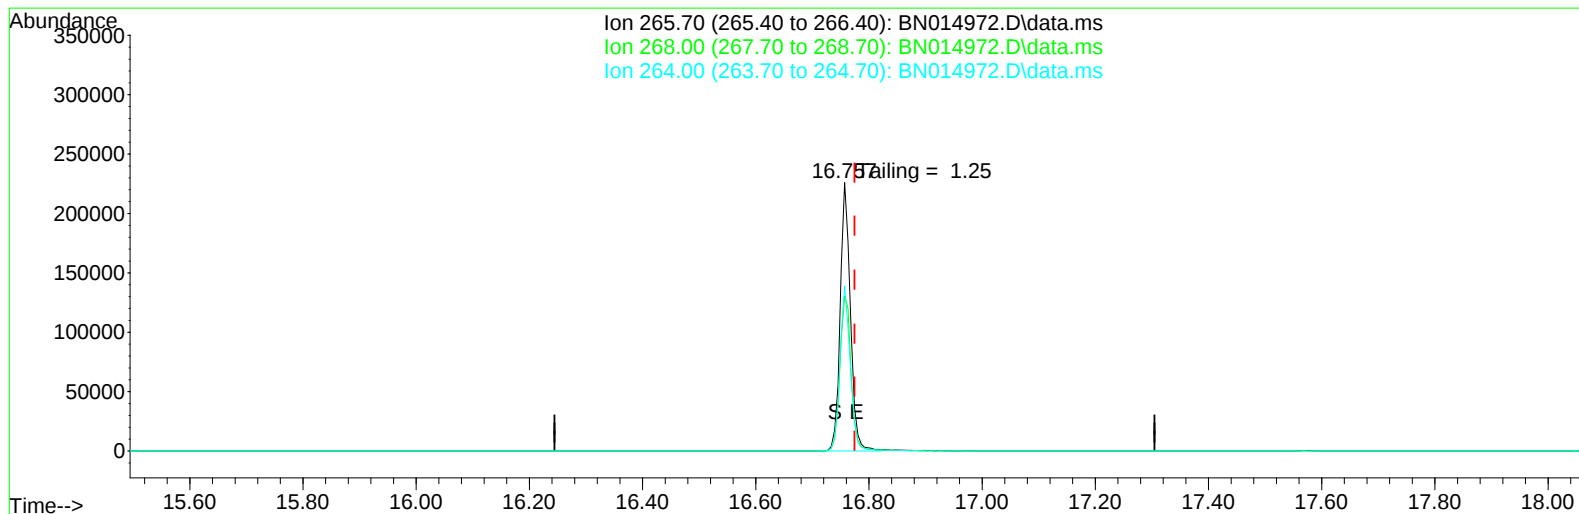

TIC: BN014972.D\data.ms

(70) Pentachlorophenol (C)

16.757min (-0.017) 25658.87 ng

response 285736

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.69
264.00	61.60	61.48
0.00	0.00	0.00