
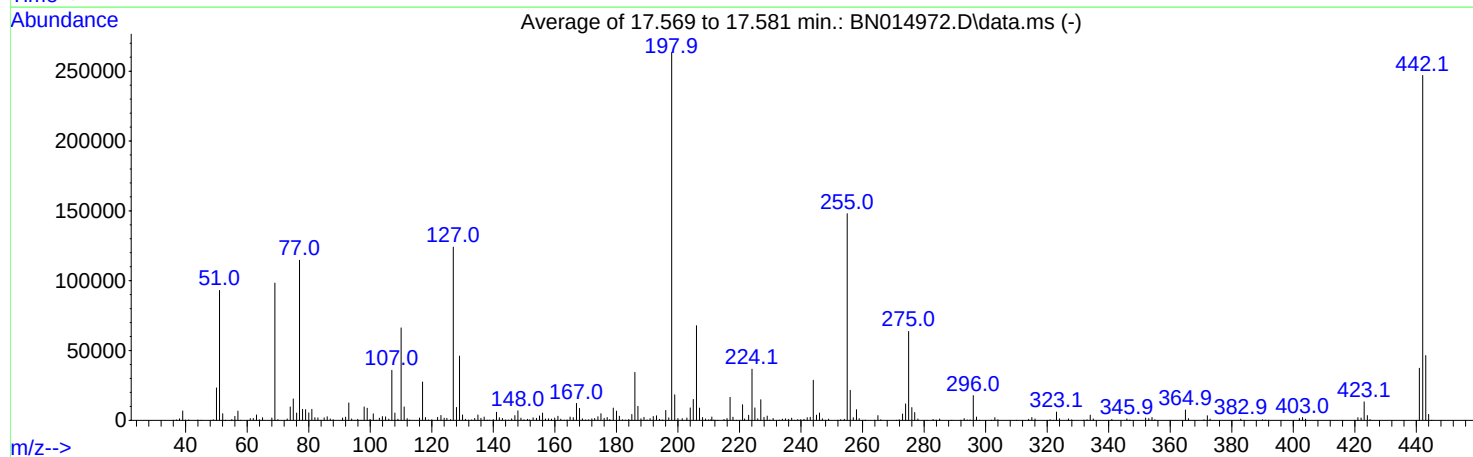


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062321\
 Data File : BN014972.D
 Acq On : 22 Jun 2021 13:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN061621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 23 16:24:59 2021

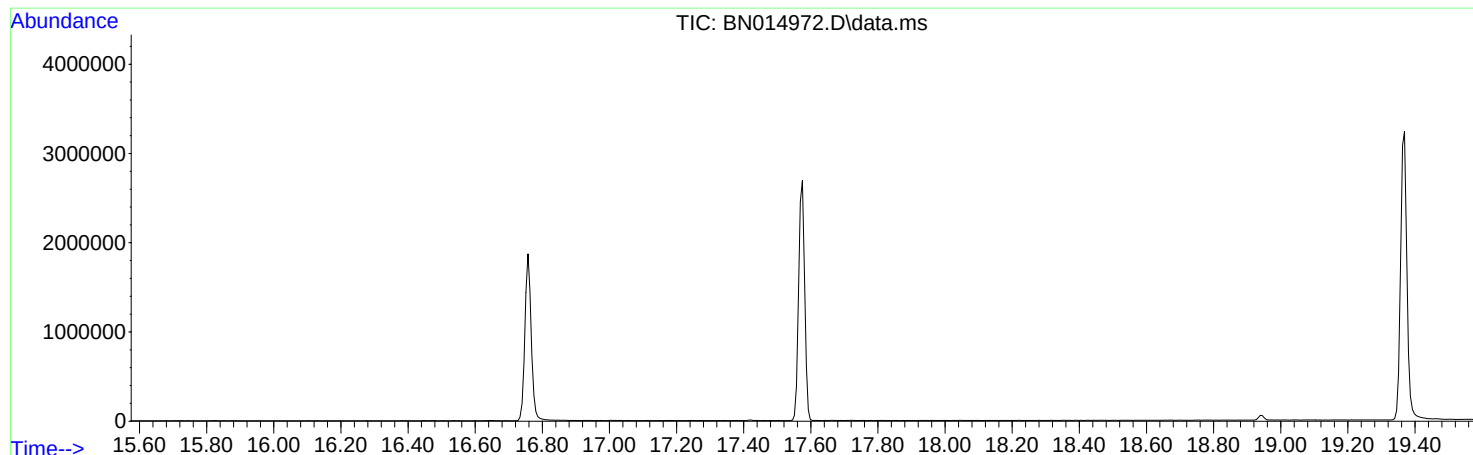




AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	93064	PASS
68	69	0.00	2	1.7	1693	PASS
69	198	0.00	100	37.3	98323	PASS
70	69	0.00	2	0.6	578	PASS
127	198	10	80	47.1	124120	PASS
197	198	0.00	2	0.7	1895	PASS
198	198	100	100	100.0	263360	PASS
199	198	5	9	7.0	18365	PASS
275	198	10	60	24.2	63757	PASS
365	198	1	100	2.8	7451	PASS
441	198	0.01	100	14.2	37371	PASS
442	442	50	100	100.0	246933	PASS
443	442	15	24	18.8	46443	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062321\
Data File : BN014972.D
Acq On : 22 Jun 2021 13:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 22 14:58:24 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 22 07:55:10 2021
Response via : Initial Calibration

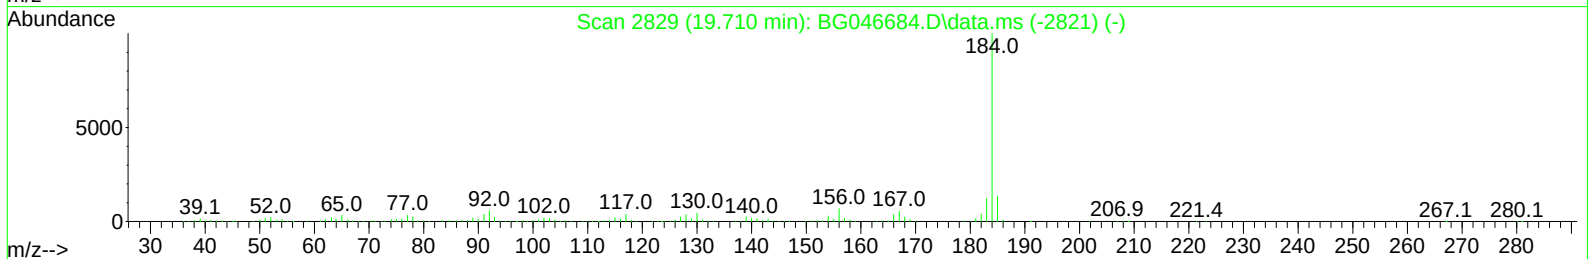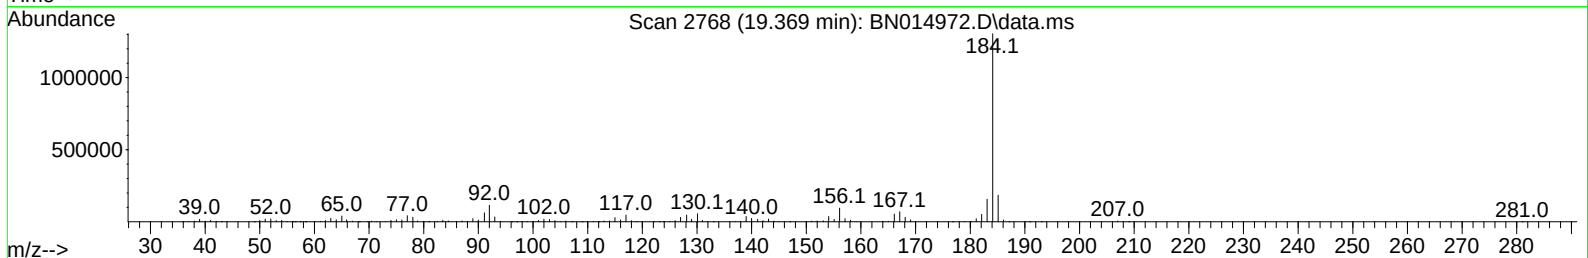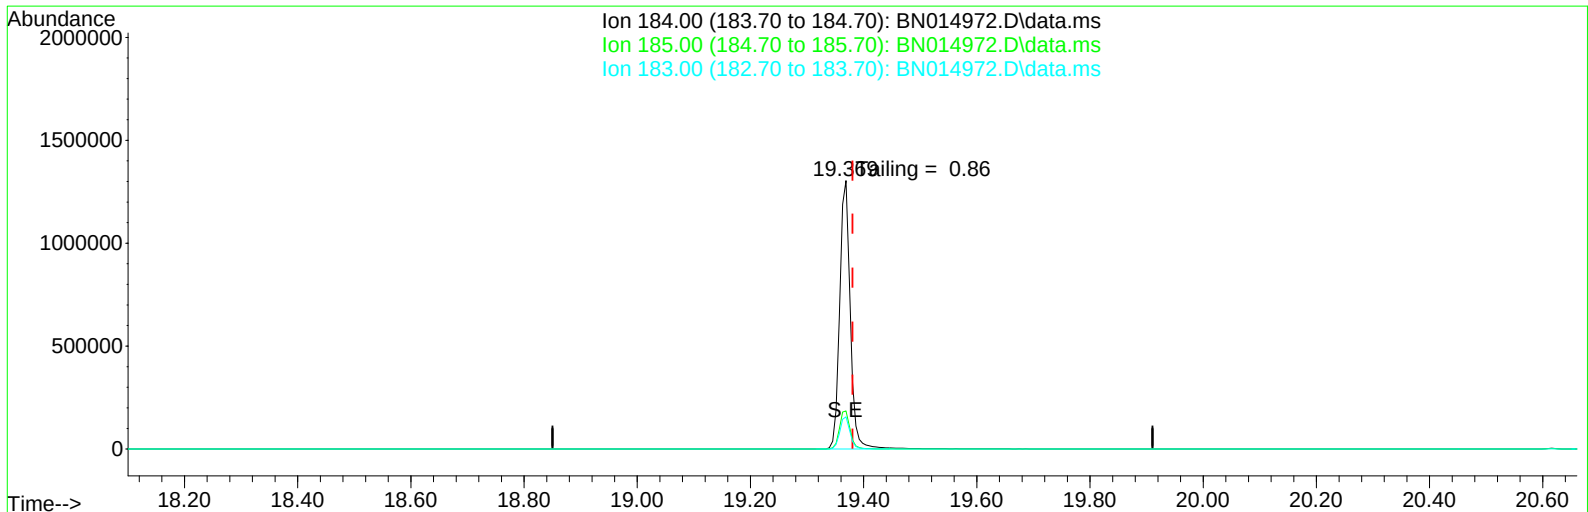

TIC: BN014972.D\data.ms

(77) Benzidine

19.369min (-0.011) 0.00 ng




response 1702141

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.18
183.00	13.20	12.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062321\
 Data File : BN014972.D
 Acq On : 22 Jun 2021 13:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jun 22 14:58:24 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 22 07:55:10 2021
 Response via : Initial Calibration

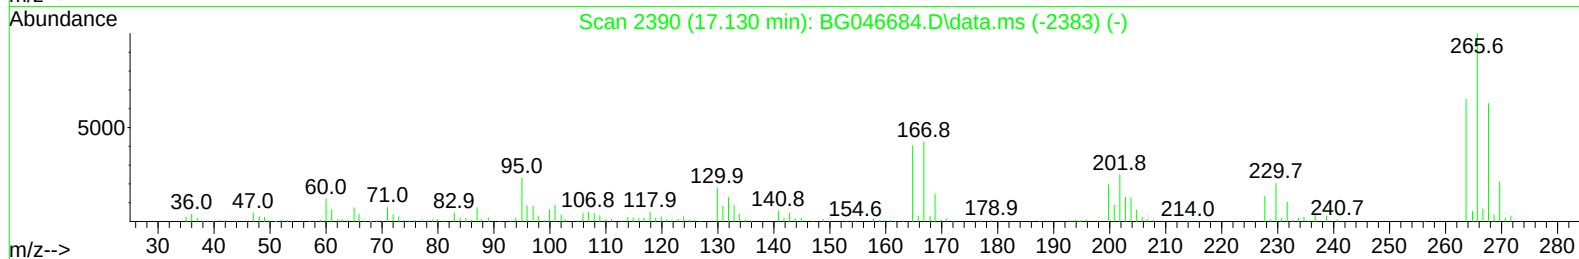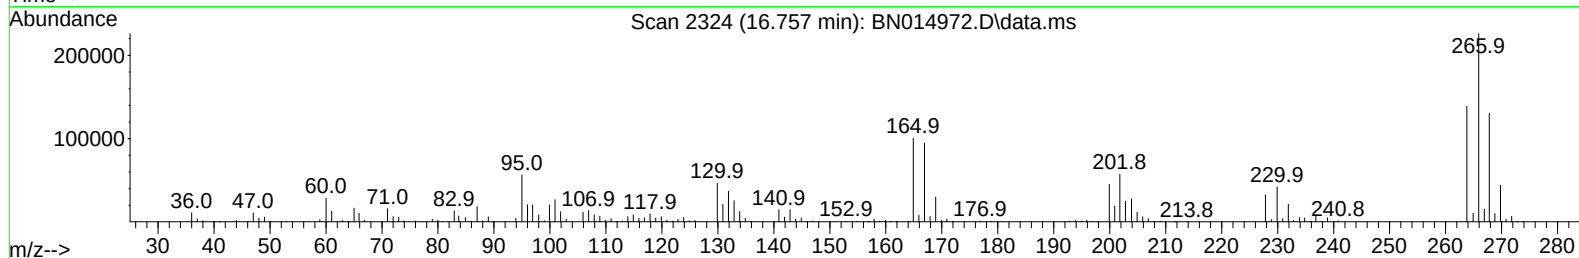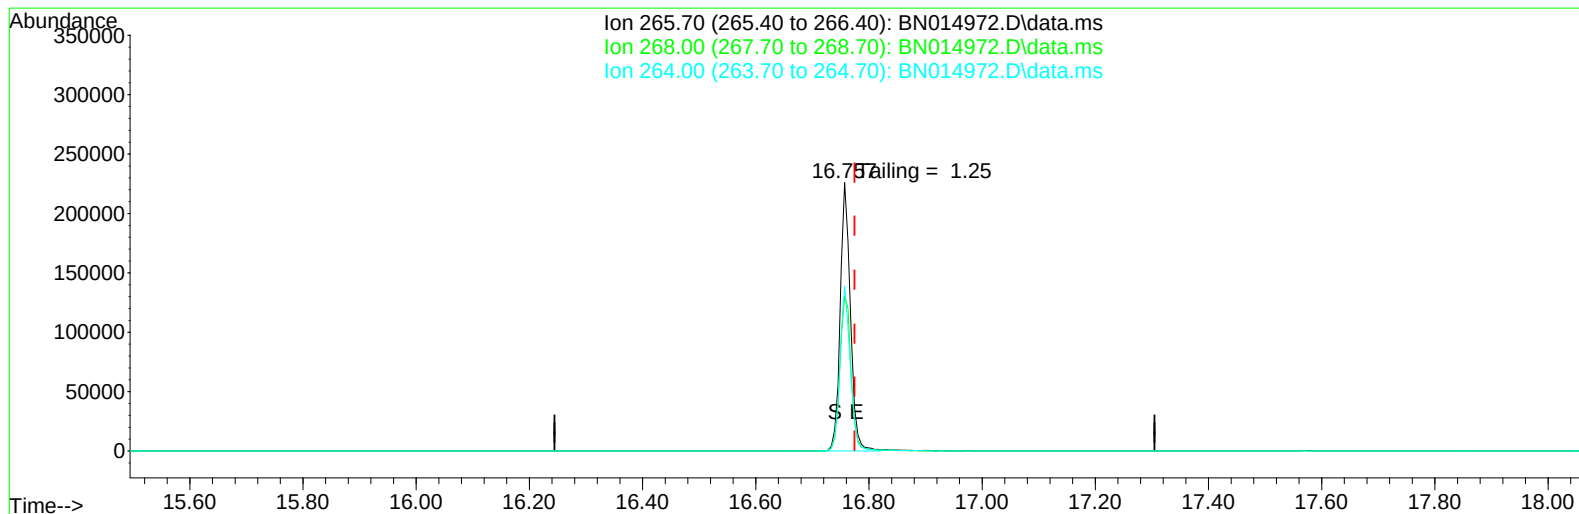

TIC: BN014972.D\data.ms

(70) Pentachlorophenol (C)

16.757min (-0.017) 25658.87 ng

response 285736

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.69
264.00	61.60	61.48
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/23/2021	BNA_N	<u>BN014972.D</u>
Compound Name	Response	Retention Time
DDT	879256	20.61
DDD	6362	20.16
DDE	1236	19.66
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7598	886854	0.86

Instrument :
BNA_N
ClientSampleId :
DFTPP