
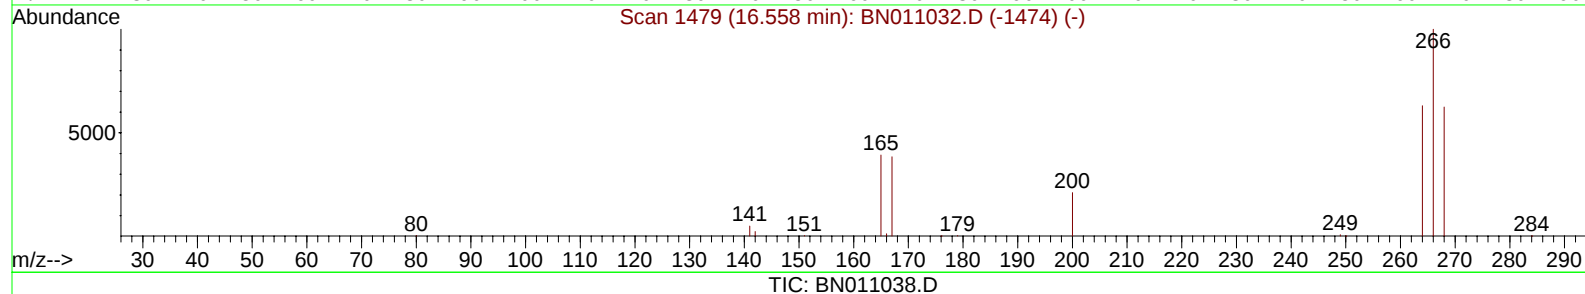
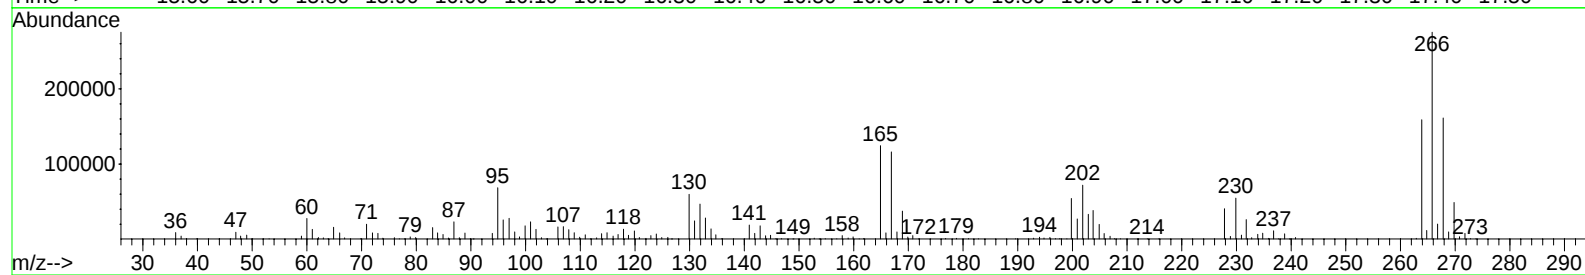


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN062420\
Data File : BN011038.D
Acq On : 24 Jun 2020 09:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 19:22:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN062320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 23 18:53:50 2020
Response via : Initial Calibration

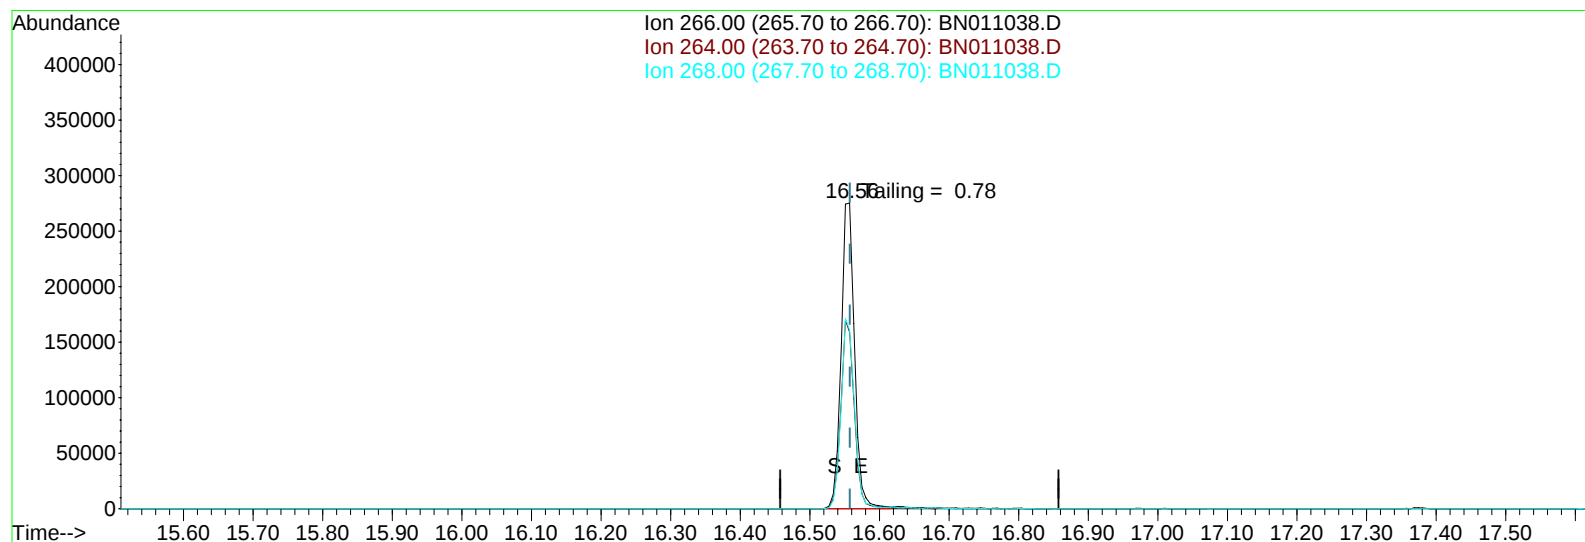

(24) Pentachlorophenol

16.557min (-0.000) 4931.80ng

response 368448

Ion	Exp%	Act%
266.00	100	100
264.00	64.20	62.22
268.00	68.60	61.83
0.00	0.00	0.00