


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062420\
 Data File : BN011038.D
 Acq On : 24 Jun 2020 09:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 23 18:53:50 2020

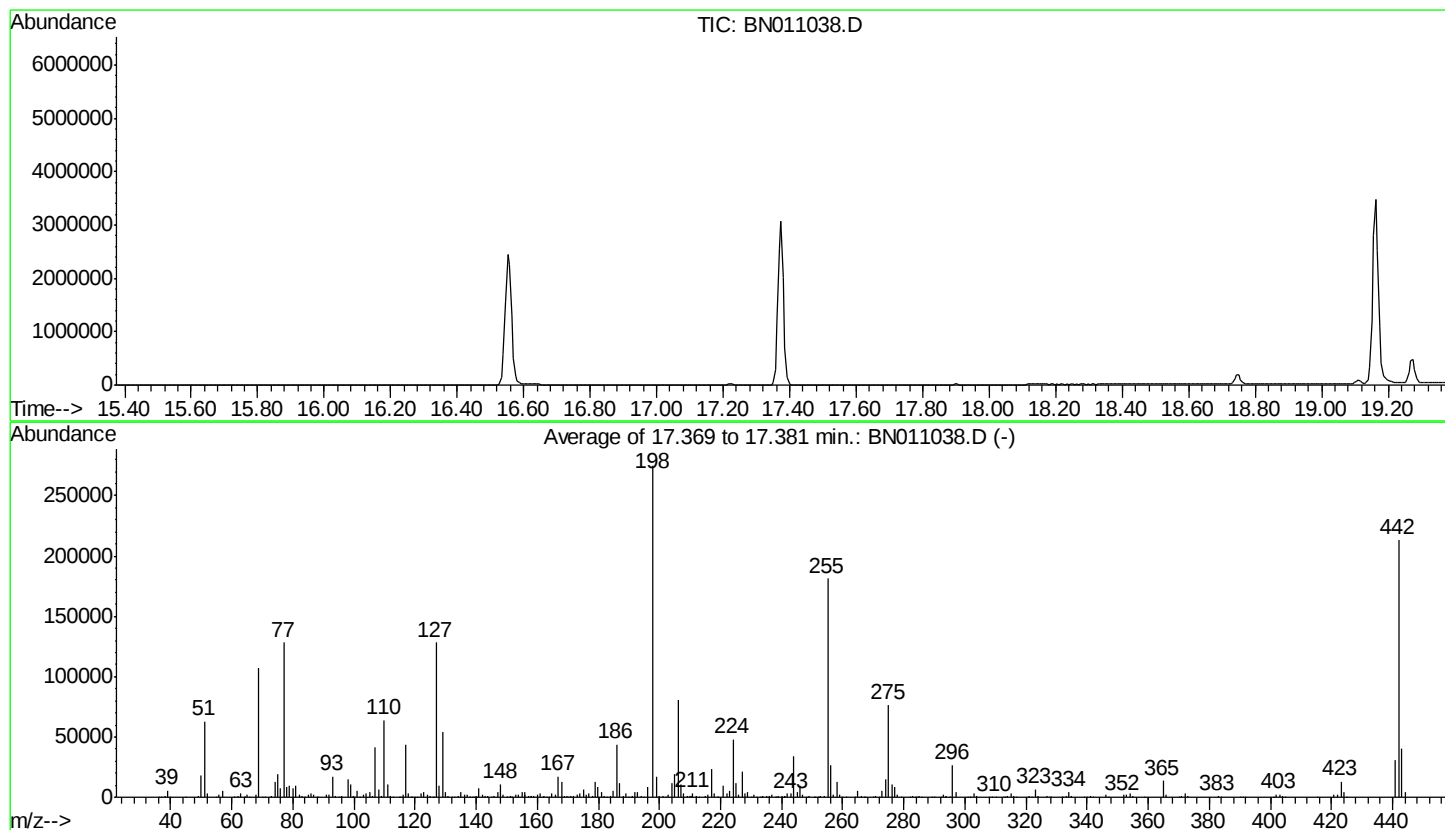

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.8	62776	PASS
68	69	0.00	2	1.9	2059	PASS
69	198	0.00	100	39.0	107186	PASS
70	69	0.00	2	0.4	439	PASS
127	198	10	80	46.5	127938	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	274965	PASS
199	198	5	9	6.3	17420	PASS
275	198	10	60	27.9	76640	PASS
365	198	1	100	4.9	13481	PASS
441	198	0.01	100	11.1	30458	PASS
442	198	50	100	77.7	213610	PASS
443	442	15	24	18.9	40450	PASS