

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062421\
 Data File : BN015009.D
 Acq On : 23 Jun 2021 15:18
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Jun 23 16:25:24 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN061621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 23 16:24:59 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.750	152	20368	0.400	ng	# 0.00
7) Naphthalene-d8	10.505	136	88422	0.400	ng	# 0.00
13) Acenaphthene-d10	14.359	164	45517	0.400	ng	0.00
19) Phenanthrene-d10	17.104	188	85204	0.400	ng	# 0.00
29) Chrysene-d12	21.303	240	77301	0.400	ng	# 0.00
35) Perylene-d12	23.554	264	67959	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.371	112	21682	0.344	ng	0.00
5) Phenol-d6	6.911	99	26107	0.327	ng	0.00
8) Nitrobenzene-d5	8.883	82	21262	0.318	ng	0.00
11) 2-Methylnaphthalene-d10	12.097	152	53357	0.352	ng	0.00
14) 2,4,6-Tribromophenol	15.843	330	5926	0.277	ng	0.00
15) 2-Fluorobiphenyl	12.976	172	69128	0.400	ng	0.00
27) Fluoranthene-d10	19.138	212	89872	0.335	ng	0.00
31) Terphenyl-d14	19.744	244	69278	0.362	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.352	88	3576	0.419	ng	# 72
3) n-Nitrosodimethylamine	3.702	42	6500	0.343	ng	# 72
6) bis(2-Chloroethyl)ether	7.179	93	24488	0.390	ng	# 84
9) Naphthalene	10.556	128	95463	0.385	ng	97
10) Hexachlorobutadiene	10.847	225	18527	0.377	ng	# 99
12) 2-Methylnaphthalene	12.173	142	61709	0.370	ng	# 90
16) Acenaphthylene	14.079	152	74009	0.322	ng	98
17) Acenaphthene	14.422	154	52533	0.373	ng	98
18) Fluorene	15.412	166	63418	0.365	ng	99
20) 4,6-Dinitro-2-methylph...	15.475	198	1144	0.323	ng	# 57
21) 4-Bromophenyl-phenylether	16.301	248	19612	0.356	ng	# 87
22) Hexachlorobenzene	16.410	284	23017	0.396	ng	# 92
23) Atrazine	16.568	200	11854	0.241	ng	94
24) Pentachlorophenol	16.751	266	5407	0.253	ng	100
25) Phenanthrene	17.140	178	101600	0.391	ng	99
26) Anthracene	17.238	178	83823	0.330	ng	99
28) Fluoranthene	19.168	202	111268	0.378	ng	# 97
30) Pyrene	19.536	202	110384	0.361	ng	99
32) Benzo(a)anthracene	21.282	228	94235	0.323	ng	98
33) Chrysene	21.335	228	105453	0.378	ng	98
34) Bis(2-ethylhexyl)phtha...	21.228	149	30522	0.150	ng	# 87
36) Indeno(1,2,3-cd)pyrene	25.813	276	81708	0.360	ng	# 86
37) Benzo(b)fluoranthene	22.876	252	96096	0.377	ng	# 96
38) Benzo(k)fluoranthene	22.921	252	104544	0.425	ng	# 94
39) Benzo(a)pyrene	23.455	252	79125	0.353	ng	# 95
40) Dibenzo(a,h)anthracene	25.830	278	63938	0.348	ng	# 90
41) Benzo(g,h,i)perylene	26.504	276	66480	0.337	ng	# 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062421\
Data File : BN015009.D
Acq On : 23 Jun 2021 15:18
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Jun 23 16:25:24 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN061621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 16:24:59 2021
Response via : Initial Calibration




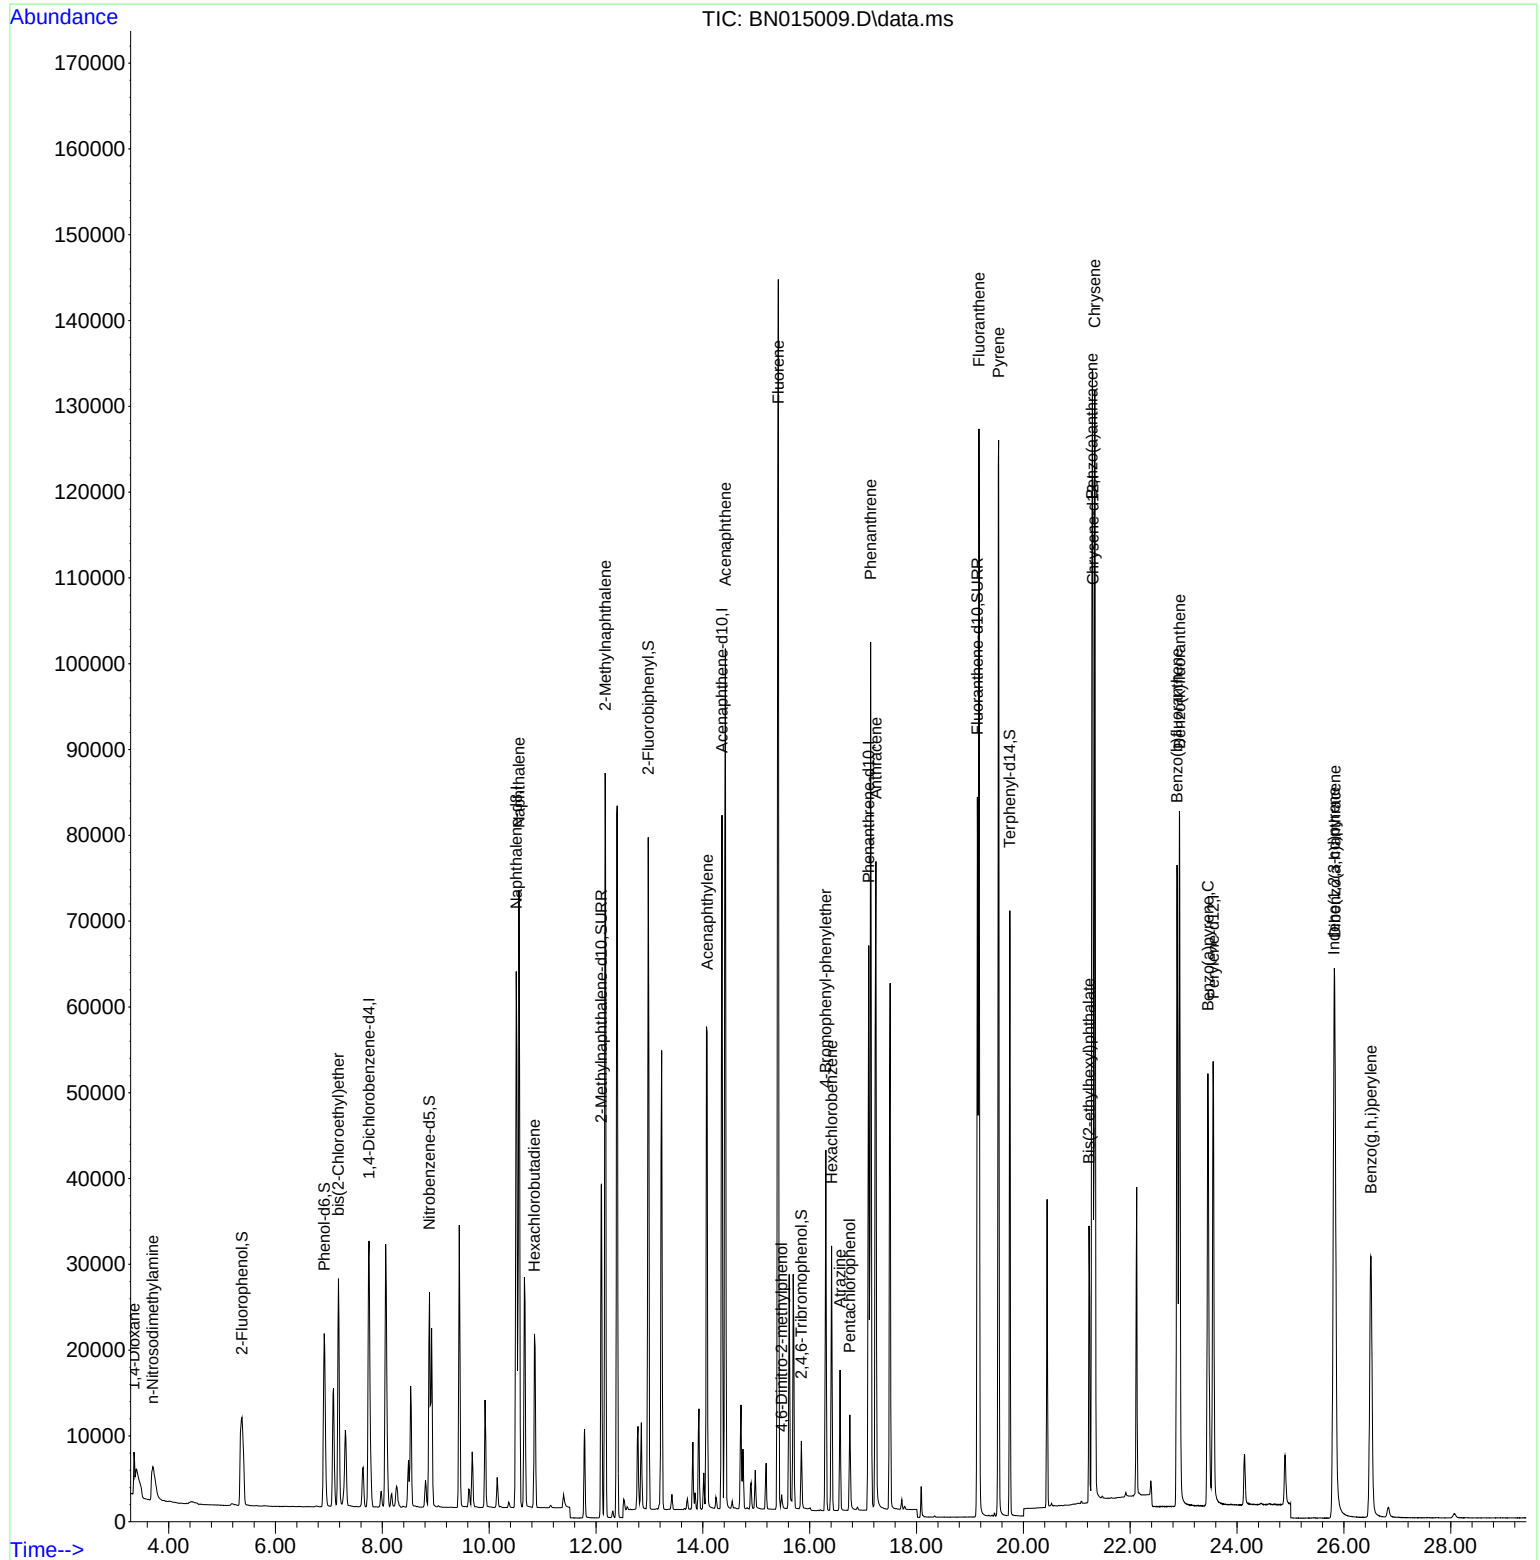




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.750 min Scan# 485
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 20368
Ion Ratio Lower Upper
152 100
150 154.3 119.0 178.6
115 59.6 62.2 93.4#

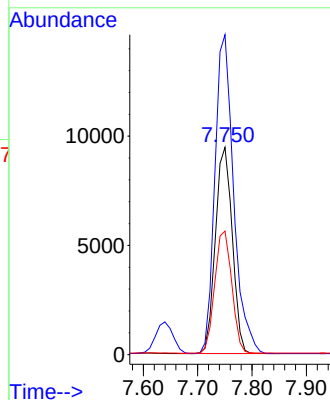

#2
1,4-Dioxane
Concen: 0.419 ng
RT: 3.352 min Scan# 8
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18

Tgt Ion: 88 Resp: 3576
Ion Ratio Lower Upper
88 100
43 24.0 12.9 19.3#
58 69.0 38.1 57.1#



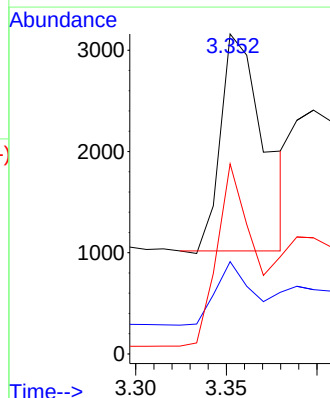





#3
n-Nitrosodimethylamine
Concen: 0.343 ng
RT: 3.702 min Scan# 46
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion: 42 Resp: 6500
Ion Ratio Lower Upper
42 100
74 145.3 149.5 224.3#
44 7.3 4.2 6.2#



#4
2-Fluorophenol
Concen: 0.344 ng
RT: 5.371 min Scan# 227
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18

Tgt Ion: 112 Resp: 21682
Ion Ratio Lower Upper
112 100
64 57.0 39.0 58.6
63 28.8 20.6 30.8







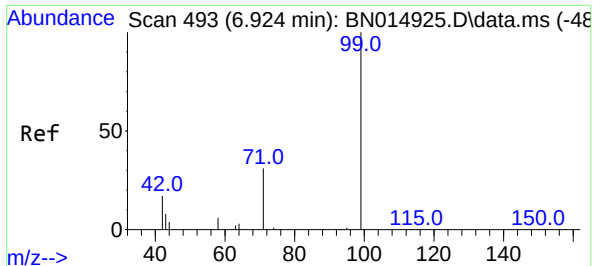

#5
Phenol-d6
Concen: 0.327 ng
RT: 6.911 min Scan# 394
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion: 99 Resp: 26107
Ion Ratio Lower Upper
99 100
42 17.8 8.9 13.3#
71 31.0 35.6 53.4#

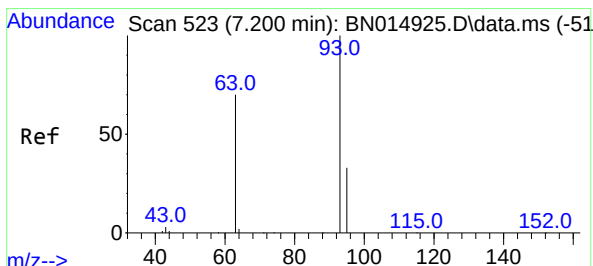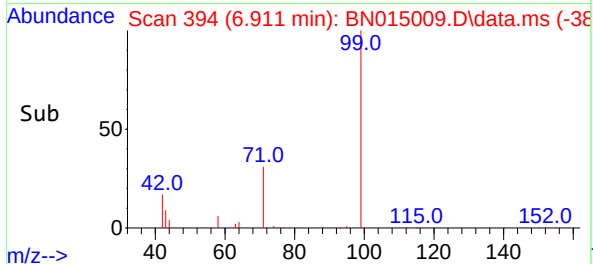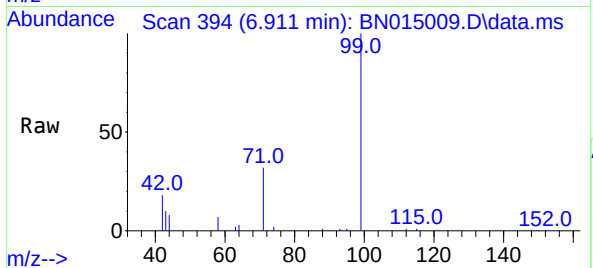

#6
bis(2-Chloroethyl)ether
Concen: 0.390 ng
RT: 7.179 min Scan# 423
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18

Tgt Ion: 93 Resp: 24488
Ion Ratio Lower Upper
93 100
63 76.0 46.6 70.0#
95 33.0 28.6 42.8


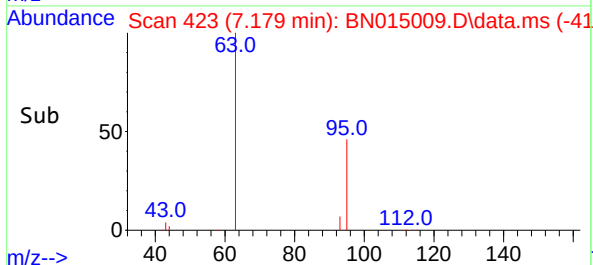

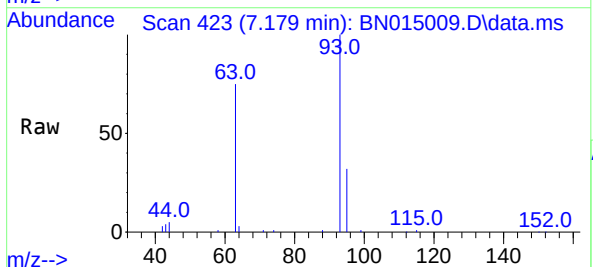




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.505 min Scan# 719
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	136	Resp:	88422
Ion Ratio	Lower	Upper	
136	100		
137	10.9	9.8	14.8
54	9.3	5.4	8.2#
68	7.4	4.9	7.3#

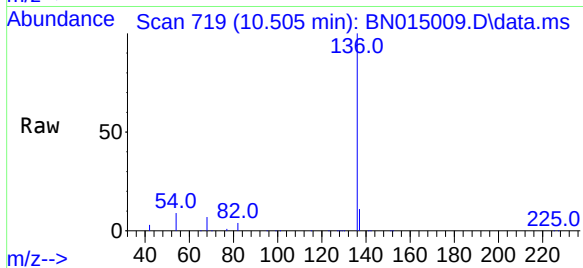

#8
Nitrobenzene-d5
Concen: 0.318 ng
RT: 8.883 min Scan# 591
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18

Tgt Ion:	82	Resp:	21262
Ion Ratio	Lower	Upper	
82	100		
128	42.2	31.6	47.4
54	47.3	29.0	43.4#


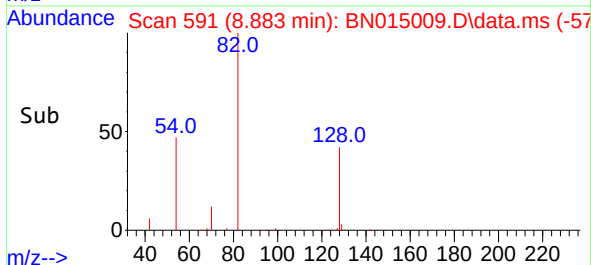
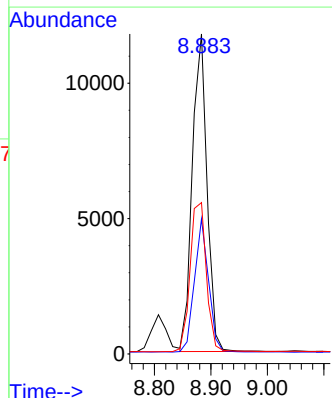
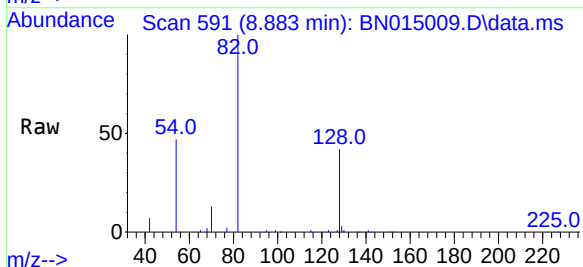




#9
Naphthalene
Concen: 0.385 ng
RT: 10.556 min Scan# 723
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	128	Resp:	95463
Ion	Ratio	Lower	Upper
128	100		
129	11.0	9.1	13.7
127	13.1	11.8	17.6

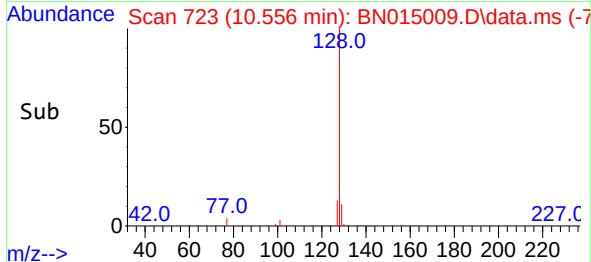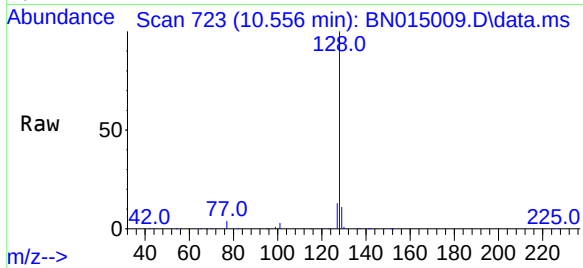

#10
Hexachlorobutadiene
Concen: 0.377 ng
RT: 10.847 min Scan# 746
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18

Tgt Ion:	225	Resp:	18527
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.5	50.2	75.2


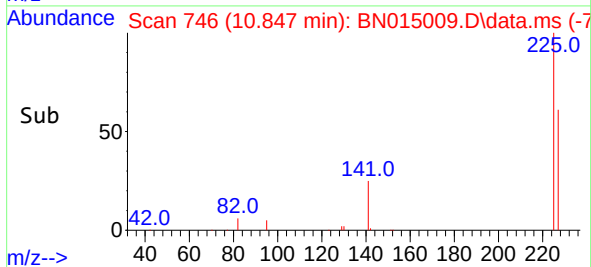

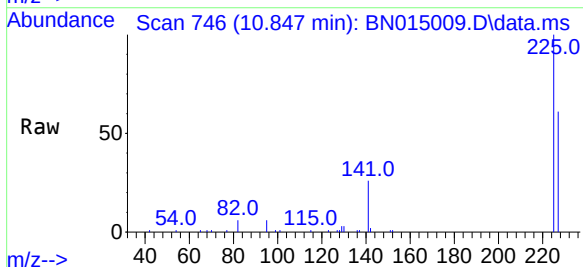




#11
2-Methylnaphthalene-d10
Concen: 0.352 ng
RT: 12.097 min Scan# 929
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 53357
Ion Ratio Lower Upper
152 100
151 20.5 16.7 25.1



#12
2-Methylnaphthalene
Concen: 0.370 ng
RT: 12.173 min Scan# 946
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18

Tgt Ion:142 Resp: 61709
Ion Ratio Lower Upper
142 100
141 88.5 72.3 108.5
115 33.8 40.7 61.1#


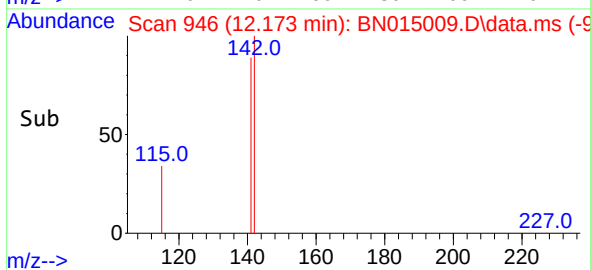




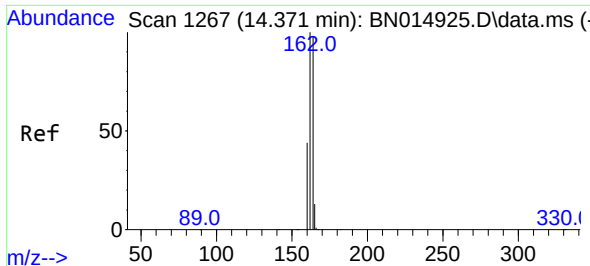

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.359 min Scan# 1167
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:164 Resp: 45517
Ion Ratio Lower Upper
164 100
162 99.5 83.8 125.6
160 43.8 37.4 56.0

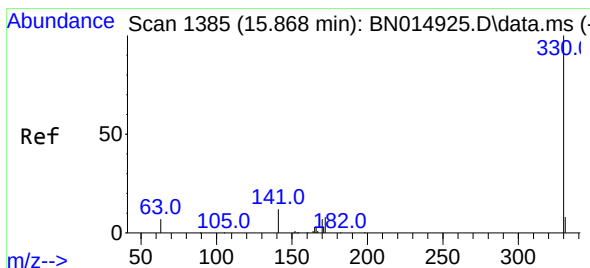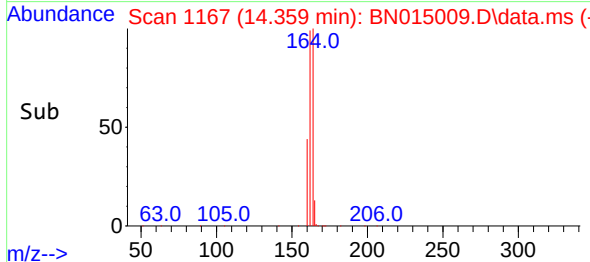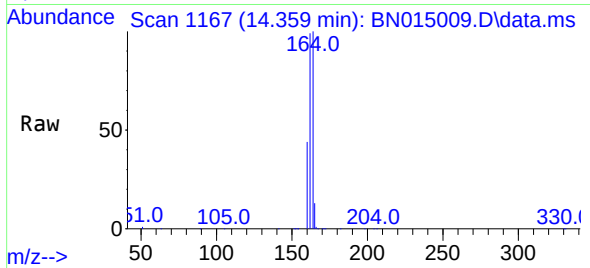

#14
2,4,6-Tribromophenol
Concen: 0.277 ng
RT: 15.843 min Scan# 1284
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18

Tgt Ion:330 Resp: 5926
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 35.2 22.4 33.6#

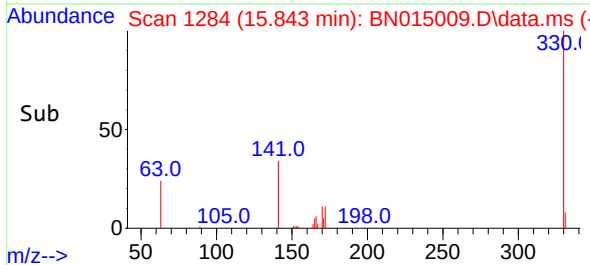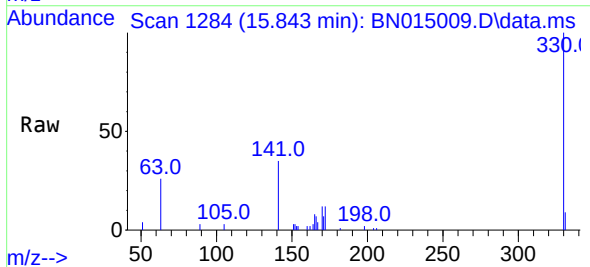







#15
2-Fluorobiphenyl
Concen: 0.400 ng
RT: 12.976 min Scan# 1058
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:172 Resp: 69128




Ion	Ratio	Lower	Upper
172	100		
171	35.2	30.6	45.8
170	23.9	20.2	30.4

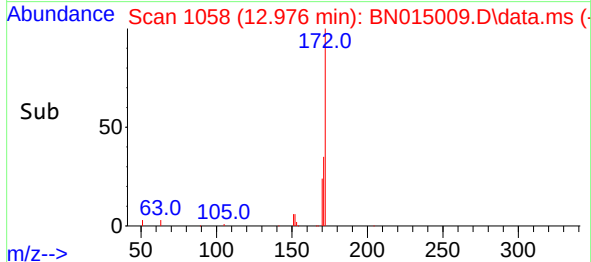


#16
Acenaphthylene
Concen: 0.322 ng
RT: 14.079 min Scan# 1145
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18

Tgt Ion:152 Resp: 74009

Ion	Ratio	Lower	Upper
152	100		
151	19.2	16.7	25.1
153	12.9	10.5	15.7


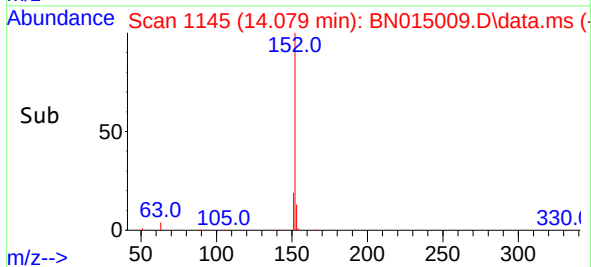

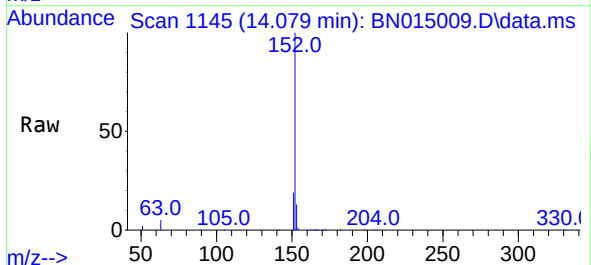




#17
Acenaphthene
Concen: 0.373 ng
RT: 14.422 min Scan# 1172
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:154 Resp: 52533
Ion Ratio Lower Upper
154 100
153 112.0 90.9 136.3
152 54.9 45.8 68.8

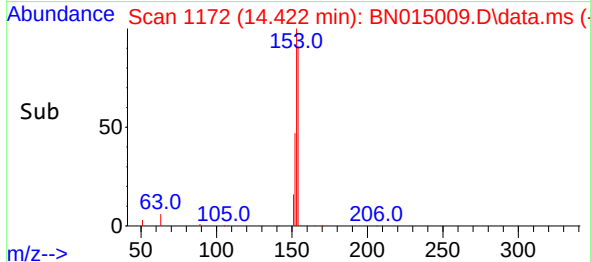

#18
Fluorene
Concen: 0.365 ng
RT: 15.412 min Scan# 1250
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18

Tgt Ion:166 Resp: 63418
Ion Ratio Lower Upper
166 100
165 97.3 79.2 118.8
167 13.4 10.7 16.1


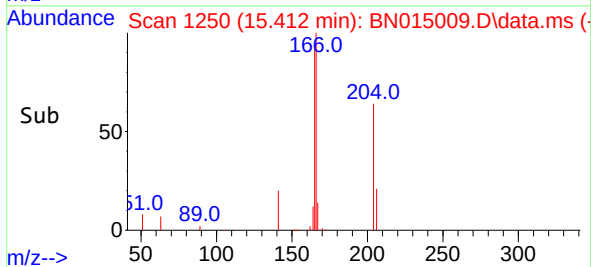

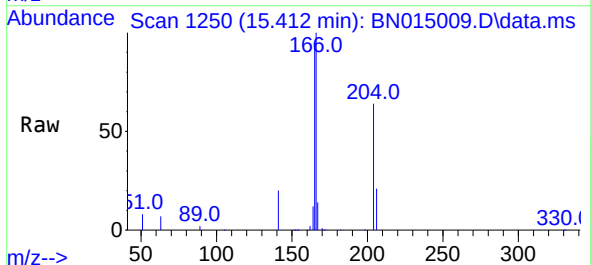


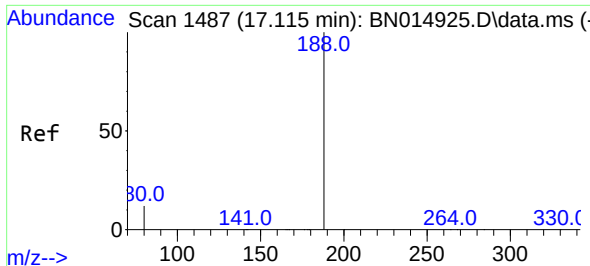

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.104 min Scan# 1387
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:188 Resp: 85204
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.5 9.0 13.4#

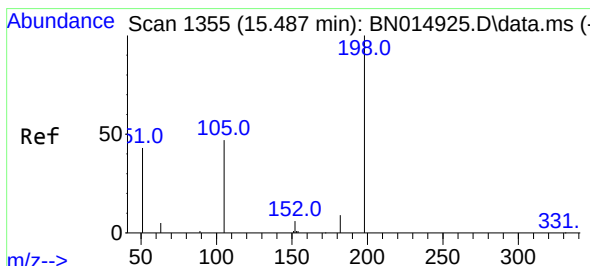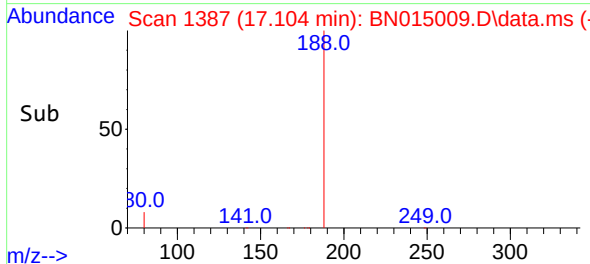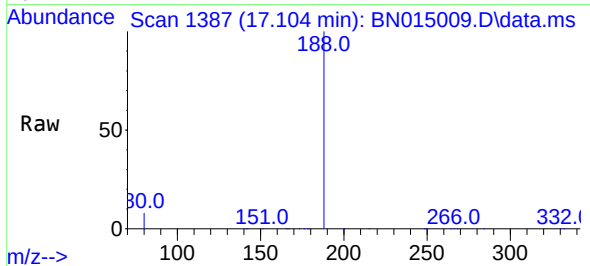

#20
4,6-Dinitro-2-methylphenol
Concen: 0.323 ng
RT: 15.475 min Scan# 1255
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18

Tgt Ion:198 Resp: 1144
Ion Ratio Lower Upper
198 100
182 15.8 34.5 51.7#
77 0.0 0.0 0.0


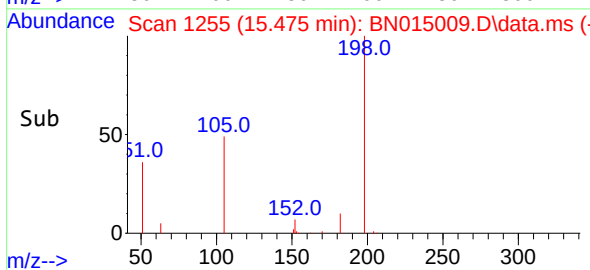

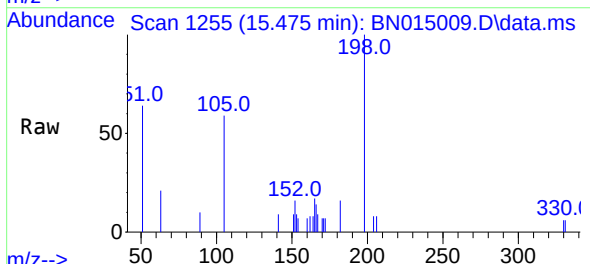




#21
4-Bromophenyl-phenylether
Concen: 0.356 ng
RT: 16.301 min Scan# 1321
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:248 Resp: 19612
Ion Ratio Lower Upper
248 100
250 96.1 86.2 129.4
141 56.8 36.2 54.2#



#22
Hexachlorobenzene
Concen: 0.396 ng
RT: 16.410 min Scan# 1330
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18

Tgt Ion:284 Resp: 23017
Ion Ratio Lower Upper
284 100
142 33.7 22.2 33.2#
249 30.7 26.6 39.8


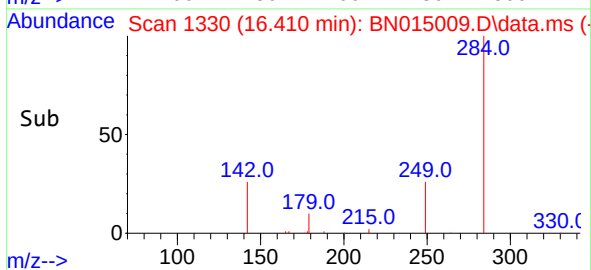




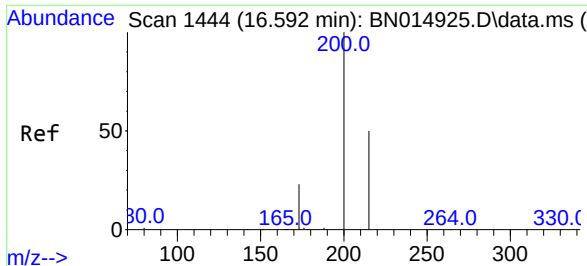

#23
Atrazine
Concen: 0.241 ng
RT: 16.568 min Scan# 1343
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:200 Resp: 11854
Ion Ratio Lower Upper
200 100
173 26.9 21.7 32.5
215 47.8 43.1 64.7

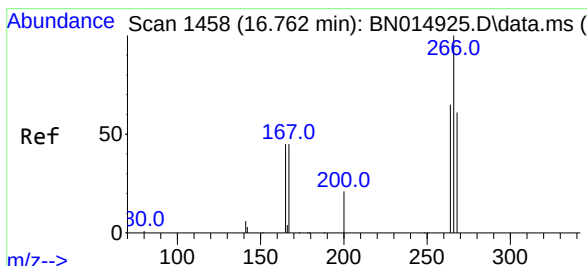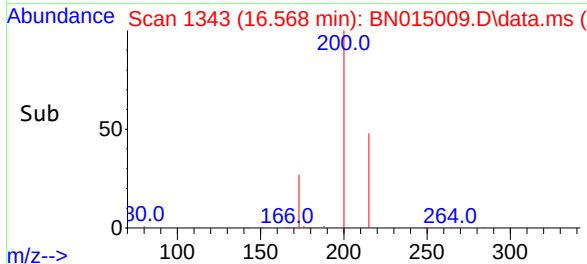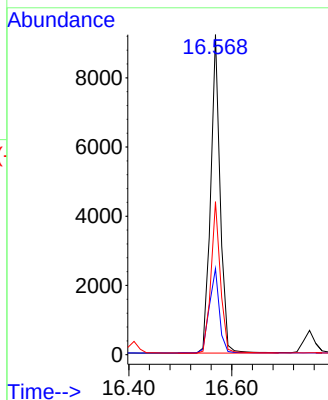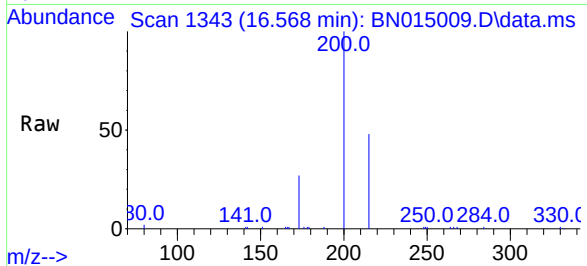

#24
Pentachlorophenol
Concen: 0.253 ng
RT: 16.751 min Scan# 1358
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18

Tgt Ion:266 Resp: 5407
Ion Ratio Lower Upper
266 100
264 63.6 51.0 76.4
268 63.9 50.6 76.0


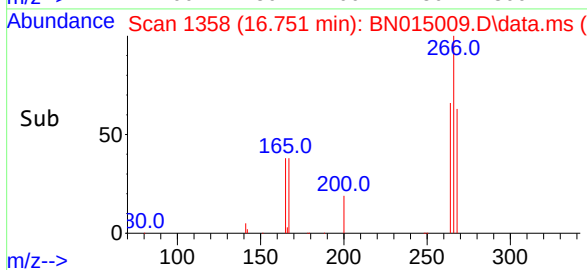
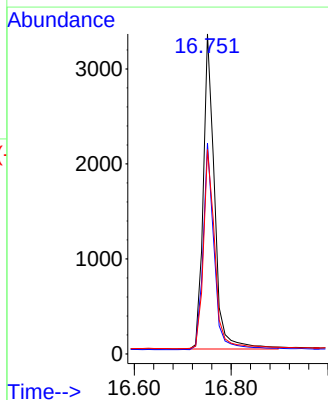
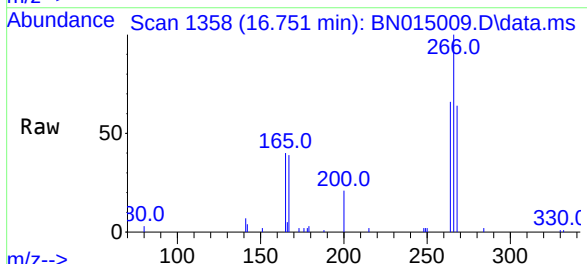




#25
Phenanthrene
Concen: 0.391 ng
RT: 17.140 min Scan# 1390
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:178 Resp: 101600
Ion Ratio Lower Upper
178 100
176 18.8 15.6 23.4
179 15.6 12.1 18.1



#26
Anthracene
Concen: 0.330 ng
RT: 17.238 min Scan# 1398
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18

Tgt Ion:178 Resp: 83823
Ion Ratio Lower Upper
178 100
176 18.2 15.1 22.7
179 15.3 12.2 18.2


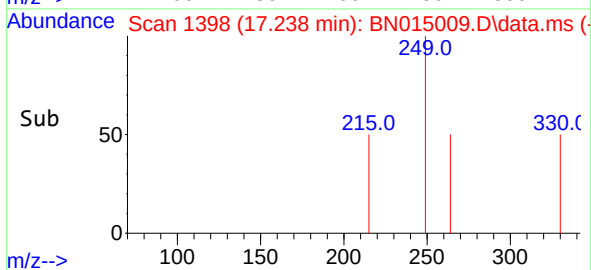






#27
Fluoranthene-d10
Concen: 0.335 ng
RT: 19.138 min Scan# 1688
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:212 Resp: 89872
Ion Ratio Lower Upper
212 100
106 14.1 7.0 10.6#
104 7.7 4.1 6.1#



#28
Fluoranthene
Concen: 0.378 ng
RT: 19.168 min Scan# 1694
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18

Tgt Ion:202 Resp: 111268
Ion Ratio Lower Upper
202 100
101 11.7 6.6 10.0#
203 17.3 13.9 20.9



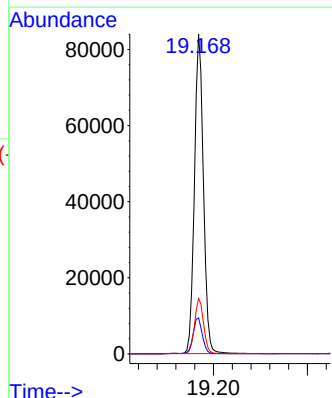



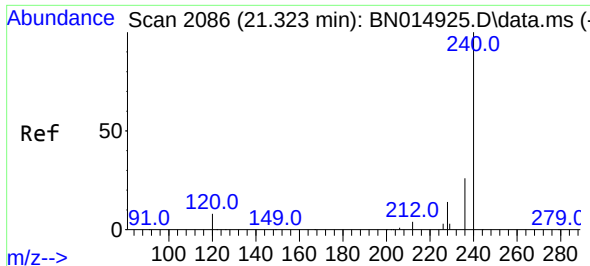

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.303 min Scan# 1985
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:240 Resp: 77301
Ion Ratio Lower Upper
240 100
120 8.0 4.2 6.4#
236 25.9 21.4 32.2

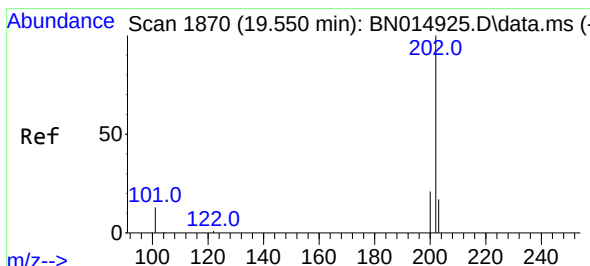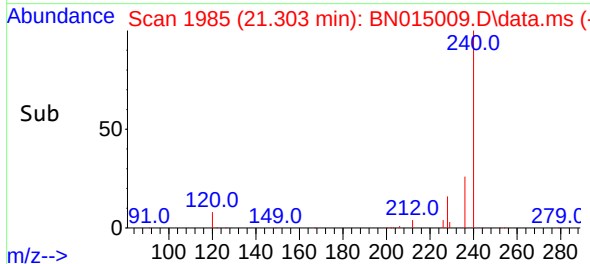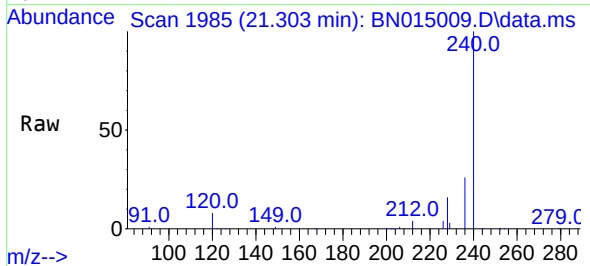

#30
Pyrene
Concen: 0.361 ng
RT: 19.536 min Scan# 1768
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18

Tgt Ion:202 Resp: 110384
Ion Ratio Lower Upper
202 100
200 20.5 16.9 25.3
203 17.4 13.9 20.9


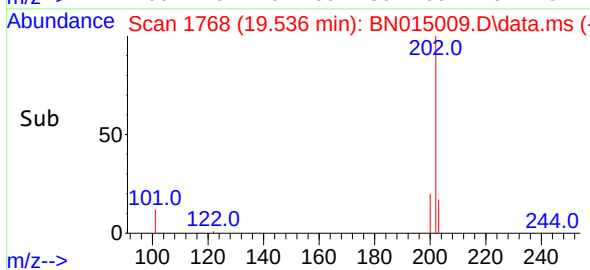

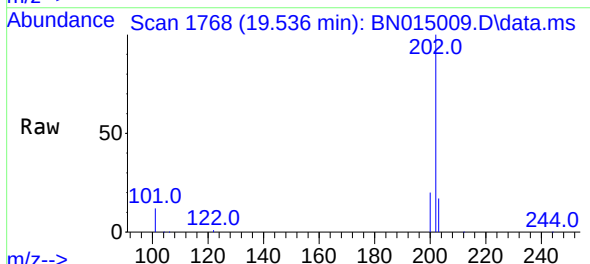




#31
Terphenyl-d14
Concen: 0.362 ng
RT: 19.744 min Scan# 1810
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:244 Resp: 69278
Ion Ratio Lower Upper
244 100
212 7.8 6.3 9.5
122 14.0 6.2 9.2#



#32
Benzo(a)anthracene
Concen: 0.323 ng
RT: 21.282 min Scan# 1983
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18

Tgt Ion:228 Resp: 94235
Ion Ratio Lower Upper
228 100
226 27.7 23.0 34.6
229 19.2 15.7 23.5


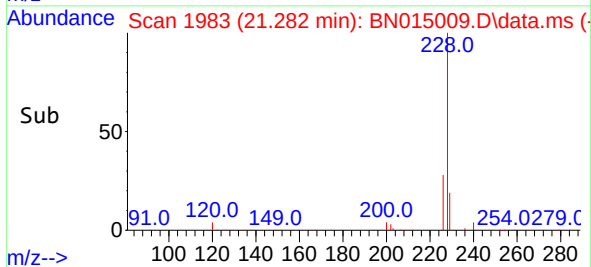

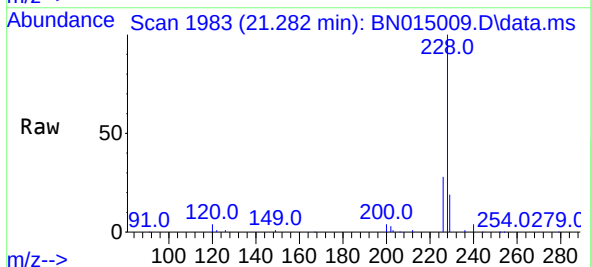


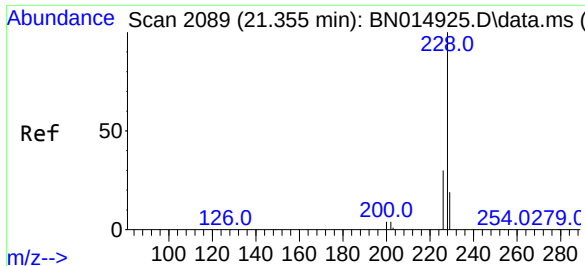

#33
Chrysene
Concen: 0.378 ng
RT: 21.335 min Scan# 1988
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:228 Resp: 105453
Ion Ratio Lower Upper
228 100
226 30.0 25.0 37.6
229 19.2 15.9 23.9

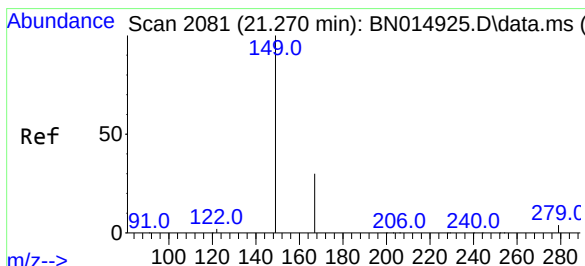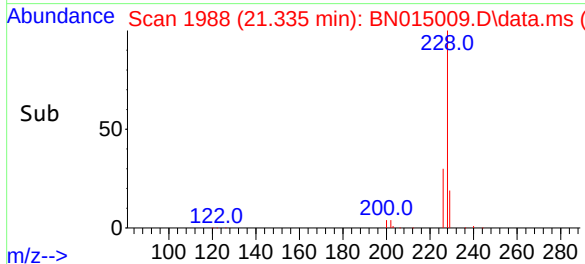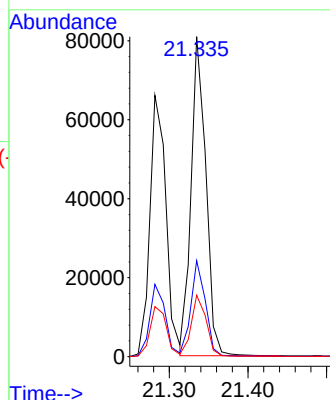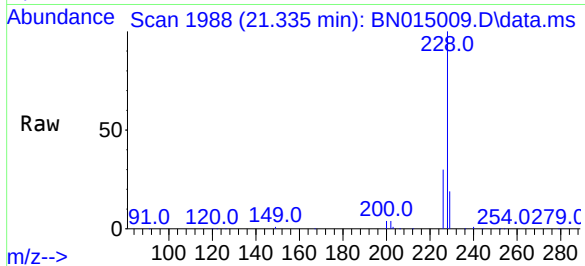

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.150 ng
RT: 21.228 min Scan# 1978
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18


Tgt Ion:149 Resp: 30522
Ion Ratio Lower Upper
149 100
167 27.7 28.9 43.3#
279 3.6 4.9 7.3#

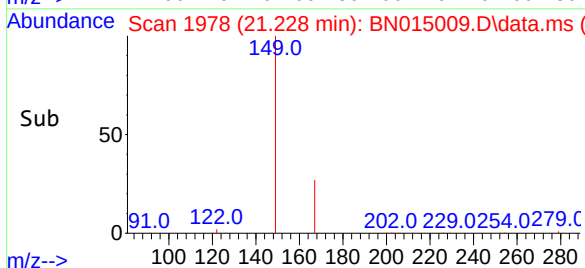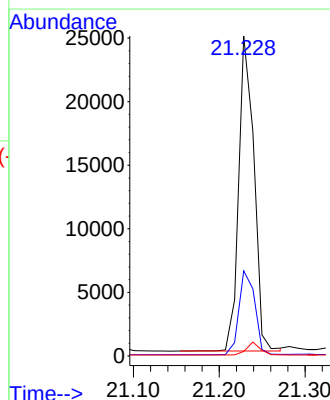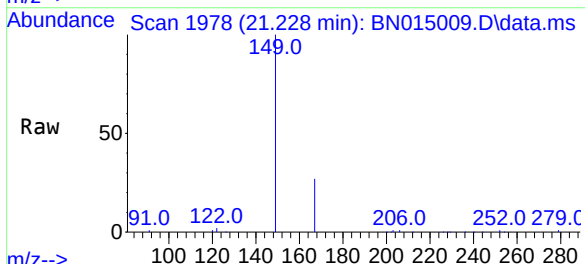






#35
Perylene-d12
Concen: 0.400 ng
RT: 23.554 min Scan# 2424
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4







Tgt Ion:264 Resp: 67959
Ion Ratio Lower Upper
264 100
260 24.9 20.6 31.0
265 24.1 21.4 32.2

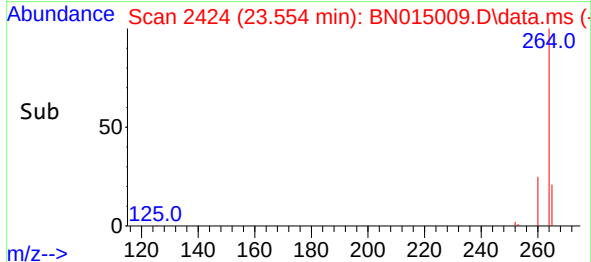

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.360 ng
RT: 25.813 min Scan# 3084
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18

Tgt Ion:276 Resp: 81708
Ion Ratio Lower Upper
276 100
138 28.1 10.0 15.0#
277 25.0 20.4 30.6

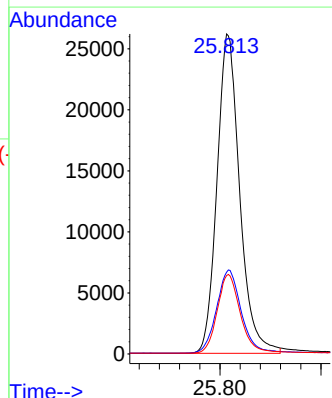



#37

Benzo(b)fluoranthene

Concen: 0.377 ng

RT: 22.876 min Scan# 2226

Delta R.T. 0.000 min

Lab File: BN015009.D

Acq: 23 Jun 2021 15:18

Tgt Ion:252 Resp: 96096





Ion	Ratio	Lower	Upper
252	100		
253	22.0	18.5	27.7
125	11.0	5.8	8.6#

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4



#38

Benzo(k)fluoranthene

Concen: 0.425 ng

RT: 22.921 min Scan# 2239




Delta R.T. 0.000 min


Lab File: BN015009.D

Acq: 23 Jun 2021 15:18

Tgt Ion:252 Resp: 104544

Ion	Ratio	Lower	Upper
252	100		
253	22.1	19.1	28.7
125	11.9	5.4	8.0#


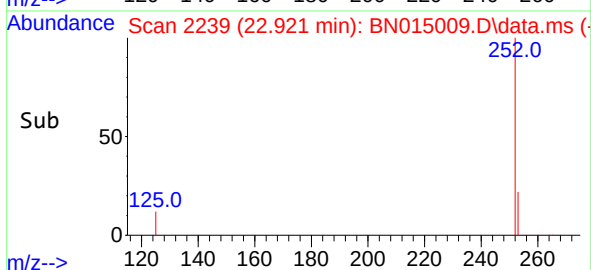






#39
Benzo(a)pyrene
Concen: 0.353 ng
RT: 23.455 min Scan# 2395
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:252 Resp: 79125
Ion Ratio Lower Upper
252 100
253 22.3 19.4 29.2
125 12.5 7.4 11.2#

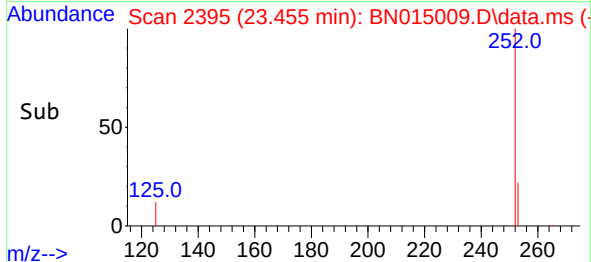

#40
Dibenzo(a,h)anthracene
Concen: 0.348 ng
RT: 25.830 min Scan# 3089
Delta R.T. 0.000 min
Lab File: BN015009.D
Acq: 23 Jun 2021 15:18

Tgt Ion:278 Resp: 63938
Ion Ratio Lower Upper
278 100
139 18.8 9.0 13.4#
279 23.6 21.0 31.4

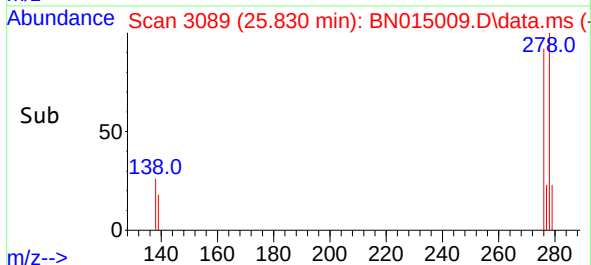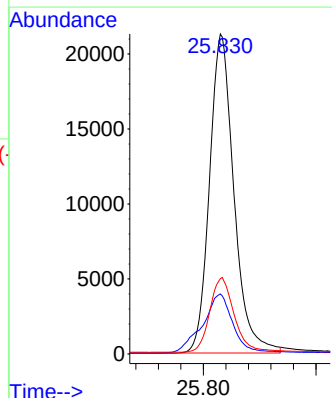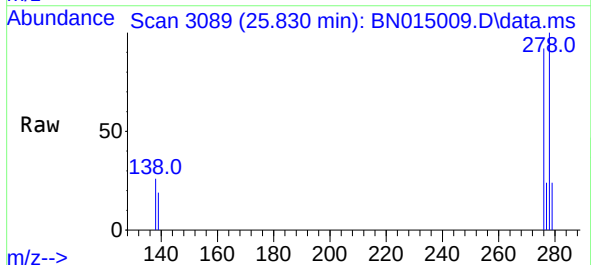

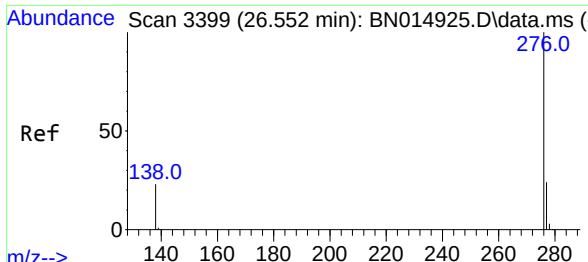

#41
 Benzo(g,h,i)perylene
 Concen: 0.337 ng
 RT: 26.504 min Scan# 3286
 Delta R.T. 0.000 min
 Lab File: BN015009.D
 Acq: 23 Jun 2021 15:18

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Tgt Ion:	276	Resp:	66480
Ion Ratio	Lower	Upper	
276	100		
277	24.1	19.7	29.5
138	23.9	9.8	14.6#

