

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062421\
 Data File : BN015026.D
 Acq On : 24 Jun 2021 01:28
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Manual Integrations
 APPROVED

mohammad
 6/24/2021 9:53:20 AM

Quant Time: Jun 24 03:21:56 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN061621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 23 16:24:59 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.750	152	22221	0.400	ng	# 0.00
7) Naphthalene-d8	10.505	136	97769	0.400	ng	# 0.00
13) Acenaphthene-d10	14.358	164	51891	0.400	ng	0.00
19) Phenanthrene-d10	17.103	188	98479	0.400	ng	# 0.00
29) Chrysene-d12	21.292	240	91415	0.400	ng	#-0.01
35) Perylene-d12	23.543	264	84499	0.400	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.371	112	25503	0.371	ng	0.00
5) Phenol-d6	6.911	99	31097	0.357	ng	0.00
8) Nitrobenzene-d5	8.883	82	27054	0.366	ng	0.00
11) 2-Methylnaphthalene-d10	12.097	152	59923	0.357	ng	0.00
14) 2,4,6-Tribromophenol	15.843	330	8577	0.352	ng	0.00
15) 2-Fluorobiphenyl	12.975	172	77201	0.392	ng	0.00
27) Fluoranthene-d10	19.138	212	108637	0.350	ng	0.00
31) Terphenyl-d14	19.739	244	81531	0.360	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.352	88	3443m	0.369	ng	
3) n-Nitrosodimethylamine	3.702	42	7309	0.354	ng	75
6) bis(2-Chloroethyl)ether	7.178	93	26873	0.393	ng	# 84
9) Naphthalene	10.556	128	104804	0.382	ng	97
10) Hexachlorobutadiene	10.847	225	20351	0.374	ng	# 99
12) 2-Methylnaphthalene	12.172	142	68809	0.373	ng	# 89
16) Acenaphthylene	14.066	152	89530	0.342	ng	98
17) Acenaphthene	14.422	154	59699	0.372	ng	98
18) Fluorene	15.411	166	72867	0.368	ng	99
20) 4,6-Dinitro-2-methylph...	15.475	198	633	0.212	ng	# 67
21) 4-Bromophenyl-phenylether	16.300	248	22970	0.361	ng	93
22) Hexachlorobenzene	16.410	284	25713	0.383	ng	# 93
23) Atrazine	16.568	200	16716	0.294	ng	93
24) Pentachlorophenol	16.751	266	8209	0.333	ng	99
25) Phenanthrene	17.140	178	115762	0.385	ng	99
26) Anthracene	17.237	178	101718	0.346	ng	99
28) Fluoranthene	19.168	202	131574	0.387	ng	# 97
30) Pyrene	19.530	202	133153	0.368	ng	99
32) Benzo(a)anthracene	21.281	228	121134	0.351	ng	97
33) Chrysene	21.334	228	126776	0.384	ng	97
34) Bis(2-ethylhexyl)phtha...	21.228	149	60451	0.252	ng	# 87
36) Indeno(1,2,3-cd)pyrene	25.799	276	104155	0.369	ng	# 85
37) Benzo(b)fluoranthene	22.869	252	123188	0.389	ng	# 95
38) Benzo(k)fluoranthene	22.910	252	127193	0.416	ng	# 94
39) Benzo(a)pyrene	23.444	252	106127	0.380	ng	# 92
40) Dibenzo(a,h)anthracene	25.816	278	82444	0.361	ng	# 91
41) Benzo(g,h,i)perylene	26.487	276	84234	0.344	ng	# 89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062421\
Data File : BN015026.D
Acq On : 24 Jun 2021 01:28
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

mohammad
6/24/2021 9:53:20 AM

Quant Time: Jun 24 03:21:56 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN061621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 16:24:59 2021
Response via : Initial Calibration



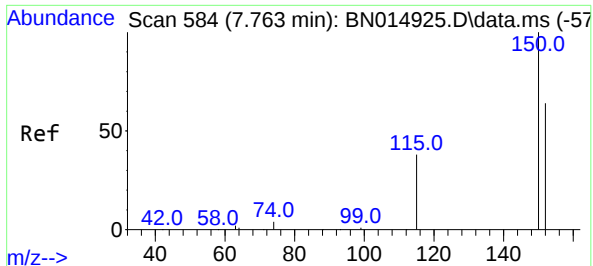





#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.750 min Scan# 485
 Delta R.T. -0.000 min
 Lab File: BN015026.D
 Acq: 24 Jun 2021 01:28

Tgt Ion: 152 Resp: 22221
 Ion Ratio Lower Upper
 152 100
 150 154.1 119.0 178.6
 115 58.7 62.2 93.4#

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC




Manual Integrations
 APPROVED


mohammad
 6/24/2021 9:53:20 AM



#2
 1,4-Dioxane
 Concen: 0.369 ng m
 RT: 3.352 min Scan# 8
 Delta R.T. -0.000 min
 Lab File: BN015026.D
 Acq: 24 Jun 2021 01:28


Tgt Ion: 88 Resp: 3443
 Ion Ratio Lower Upper
 88 100
 43 27.8 12.9 19.3#
 58 78.2 38.1 57.1#





#3
n-Nitrosodimethylamine
Concen: 0.354 ng
RT: 3.702 min Scan# 46
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC






Tgt Ion: 42 Resp: 7309


Ion	Ratio	Lower	Upper
42	100		
74	150.0	149.5	224.3
44	6.0	4.2	6.2

Manual Integrations
APPROVED

mohammad
6/24/2021 9:53:20 AM






#4
2-Fluorophenol
Concen: 0.371 ng
RT: 5.371 min Scan# 227
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28



Tgt Ion: 112 Resp: 25503


Ion	Ratio	Lower	Upper
112	100		
64	57.2	39.0	58.6
63	28.5	20.6	30.8





#5
Phenol-d6
Concen: 0.357 ng
RT: 6.911 min Scan# 394
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Tgt Ion: 99 Resp: 31097
Ion Ratio Lower Upper
99 100
42 17.2 8.9 13.3#
71 30.9 35.6 53.4#

Manual Integrations
APPROVED



mohammad
6/24/2021 9:53:20 AM




#6
bis(2-Chloroethyl)ether
Concen: 0.393 ng
RT: 7.178 min Scan# 423
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28




Tgt Ion: 93 Resp: 26873
Ion Ratio Lower Upper
93 100
63 75.5 46.6 70.0#
95 32.9 28.6 42.8





#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.505 min Scan# 719
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC



Tgt Ion: 136 Resp: 97769
Ion Ratio Lower Upper
136 100
137 11.0 9.8 14.8
54 8.7 5.4 8.2#
68 7.1 4.9 7.3




Manual Integrations
APPROVED


mohammad
6/24/2021 9:53:20 AM



#8
Nitrobenzene-d5
Concen: 0.366 ng
RT: 8.883 min Scan# 591
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28


Tgt Ion: 82 Resp: 27054
Ion Ratio Lower Upper
82 100
128 44.8 31.6 47.4
54 46.4 29.0 43.4#





#9
Naphthalene
Concen: 0.382 ng
RT: 10.556 min Scan# 723
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC



Tgt Ion:128 Resp: 104804
Ion Ratio Lower Upper
128 100
129 11.0 9.1 13.7
127 13.0 11.8 17.6




Manual Integrations
APPROVED


mohammad
6/24/2021 9:53:20 AM



#10
Hexachlorobutadiene
Concen: 0.374 ng
RT: 10.847 min Scan# 746
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28

Tgt Ion:225 Resp: 20351
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.7 50.2 75.2









#11
2-Methylnaphthalene-d10
Concen: 0.357 ng
RT: 12.097 min Scan# 929
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28

Tgt Ion:152 Resp: 59923
Ion Ratio Lower Upper
152 100
151 20.3 16.7 25.1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED


mohammad
6/24/2021 9:53:20 AM



#12
2-Methylnaphthalene
Concen: 0.373 ng
RT: 12.172 min Scan# 946
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28


Tgt Ion:142 Resp: 68809
Ion Ratio Lower Upper
142 100
141 87.7 72.3 108.5
115 32.6 40.7 61.1#





#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.358 min Scan# 1167
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC



Tgt Ion:164 Resp: 51891
Ion Ratio Lower Upper
164 100
162 99.0 83.8 125.6
160 43.5 37.4 56.0




Manual Integrations
APPROVED


mohammad
6/24/2021 9:53:20 AM



#14
2,4,6-Tribromophenol
Concen: 0.352 ng
RT: 15.843 min Scan# 1284
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28

Tgt Ion:330 Resp: 8577
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 34.8 22.4 33.6#









#15
2-Fluorobiphenyl
Concen: 0.392 ng
RT: 12.975 min Scan# 1058
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28

Tgt Ion:	172	Resp:	77201
Ion	Ratio	Lower	Upper
172	100		
171	35.1	30.6	45.8
170	23.5	20.2	30.4

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED


mohammad
6/24/2021 9:53:20 AM



#16
Acenaphthylene
Concen: 0.342 ng
RT: 14.066 min Scan# 1144
Delta R.T. -0.013 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28


Tgt Ion:	152	Resp:	89530
Ion	Ratio	Lower	Upper
152	100		
151	19.3	16.7	25.1
153	13.0	10.5	15.7





#17
Acenaphthene
Concen: 0.372 ng
RT: 14.422 min Scan# 1172
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC



Tgt Ion:154 Resp: 59699
Ion Ratio Lower Upper
154 100
153 112.4 90.9 136.3
152 54.2 45.8 68.8




Manual Integrations
APPROVED


mohammad
6/24/2021 9:53:20 AM



#18
Fluorene
Concen: 0.368 ng
RT: 15.411 min Scan# 1250
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28


Tgt Ion:166 Resp: 72867
Ion Ratio Lower Upper
166 100
165 97.5 79.2 118.8
167 13.5 10.7 16.1





#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.103 min Scan# 1387
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC



Tgt Ion:188 Resp: 98479
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 7.3 9.0 13.4#




Manual Integrations
APPROVED


mohammad
6/24/2021 9:53:20 AM




#20
4,6-Dinitro-2-methylphenol
Concen: 0.212 ng
RT: 15.475 min Scan# 1255
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28

Tgt Ion:198 Resp: 633
Ion Ratio Lower Upper
198 100
182 22.2 34.5 51.7#
77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 0.361 ng
RT: 16.300 min Scan# 1321
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28





Tgt Ion:248 Resp: 22970
Ion Ratio Lower Upper
248 100
250 98.9 86.2 129.4
141 47.3 36.2 54.2



#22
Hexachlorobenzene
Concen: 0.383 ng
RT: 16.410 min Scan# 1330
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28




Tgt Ion:284 Resp: 25713
Ion Ratio Lower Upper
284 100
142 33.5 22.2 33.2#
249 30.8 26.6 39.8



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

mohammad
6/24/2021 9:53:20 AM







#23
Atrazine
Concen: 0.294 ng
RT: 16.568 min Scan# 1343
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:200 Resp: 16716
Ion Ratio Lower Upper
200 100
173 24.8 21.7 32.5
215 48.4 43.1 64.7




Manual Integrations
APPROVED


mohammad
6/24/2021 9:53:20 AM



#24
Pentachlorophenol
Concen: 0.333 ng
RT: 16.751 min Scan# 1358
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28

Tgt Ion:266 Resp: 8209
Ion Ratio Lower Upper
266 100
264 62.7 51.0 76.4
268 64.2 50.6 76.0









#25
Phenanthrene
Concen: 0.385 ng
RT: 17.140 min Scan# 1390
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28

Tgt Ion:178 Resp: 115762
Ion Ratio Lower Upper
178 100
176 18.8 15.6 23.4
179 15.5 12.1 18.1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED


mohammad
6/24/2021 9:53:20 AM



#26
Anthracene
Concen: 0.346 ng
RT: 17.237 min Scan# 1398
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28

Tgt Ion:178 Resp: 101718
Ion Ratio Lower Upper
178 100
176 18.2 15.1 22.7
179 15.3 12.2 18.2









#27
Fluoranthene-d10
Concen: 0.350 ng
RT: 19.138 min Scan# 1688
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28

Tgt Ion:212 Resp: 108637
Ion Ratio Lower Upper
212 100
106 14.2 7.0 10.6#
104 7.8 4.1 6.1#

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED


mohammad
6/24/2021 9:53:20 AM




#28
Fluoranthene
Concen: 0.387 ng
RT: 19.168 min Scan# 1694
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28

Tgt Ion:202 Resp: 131574
Ion Ratio Lower Upper
202 100
101 11.7 6.6 10.0#
203 17.3 13.9 20.9









#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.292 min Scan# 1984
Delta R.T. -0.011 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28





Tgt Ion:240 Resp: 91415
Ion Ratio Lower Upper
240 100
120 12.6 4.2 6.4#
236 27.2 21.4 32.2



#30
Pyrene
Concen: 0.368 ng
RT: 19.530 min Scan# 1767
Delta R.T. -0.005 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28




Tgt Ion:202 Resp: 133153
Ion Ratio Lower Upper
202 100
200 20.5 16.9 25.3
203 17.4 13.9 20.9



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Manual Integrations
APPROVED

mohammad
6/24/2021 9:53:20 AM



#31
Terphenyl-d14
Concen: 0.360 ng
RT: 19.739 min Scan# 1809
Delta R.T. -0.005 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Tgt Ion:244 Resp: 81531
Ion Ratio Lower Upper
244 100
212 7.8 6.3 9.5
122 14.3 6.2 9.2#

Manual Integrations
APPROVED



mohammad
6/24/2021 9:53:20 AM




#32
Benzo(a)anthracene
Concen: 0.351 ng
RT: 21.281 min Scan# 1983
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28




Tgt Ion:228 Resp: 121134
Ion Ratio Lower Upper
228 100
226 25.8 23.0 34.6
229 19.7 15.7 23.5





#33
Chrysene
Concen: 0.384 ng
RT: 21.334 min Scan# 1988
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Tgt Ion:228 Resp: 126776
Ion Ratio Lower Upper
228 100
226 28.4 25.0 37.6
229 20.0 15.9 23.9

Manual Integrations
APPROVED



mohammad
6/24/2021 9:53:20 AM




#34
Bis(2-ethylhexyl)phthalate
Concen: 0.252 ng
RT: 21.228 min Scan# 1978
Delta R.T. -0.000 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28




Tgt Ion:149 Resp: 60451
Ion Ratio Lower Upper
149 100
167 28.2 28.9 43.3#
279 3.7 4.9 7.3#





#35
Perylene-d12
Concen: 0.400 ng
RT: 23.543 min Scan# 2421
Delta R.T. -0.011 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC



Tgt Ion:264 Resp: 84499
Ion Ratio Lower Upper
264 100
260 24.7 20.6 31.0
265 23.6 21.4 32.2




Manual Integrations
APPROVED


mohammad
6/24/2021 9:53:20 AM



#36
Indeno(1,2,3-cd)pyrene
Concen: 0.369 ng
RT: 25.799 min Scan# 3080
Delta R.T. -0.014 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28

Tgt Ion:276 Resp: 104155
Ion Ratio Lower Upper
276 100
138 30.3 10.0 15.0#
277 25.0 20.4 30.6









#37
Benzo(b)fluoranthene
Concen: 0.389 ng
RT: 22.869 min Scan# 2224
Delta R.T. -0.007 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28

Tgt Ion:252 Resp: 123188
Ion Ratio Lower Upper
252 100
253 22.0 18.5 27.7
125 12.0 5.8 8.6#

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC




Manual Integrations
APPROVED


mohammad
6/24/2021 9:53:20 AM




#38
Benzo(k)fluoranthene
Concen: 0.416 ng
RT: 22.910 min Scan# 2236
Delta R.T. -0.011 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28

Tgt Ion:252 Resp: 127193
Ion Ratio Lower Upper
252 100
253 22.2 19.1 28.7
125 12.1 5.4 8.0#









#39
Benzo(a)pyrene
Concen: 0.380 ng
RT: 23.444 min Scan# 2392
Delta R.T. -0.011 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28





Tgt Ion:252 Resp: 106127
Ion Ratio Lower Upper
252 100
253 22.6 19.4 29.2
125 17.1 7.4 11.2#



#40
Dibenzo(a,h)anthracene
Concen: 0.361 ng
RT: 25.816 min Scan# 3085
Delta R.T. -0.014 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28




Tgt Ion:278 Resp: 82444
Ion Ratio Lower Upper
278 100
139 18.6 9.0 13.4#
279 23.9 21.0 31.4




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED



mohammad
6/24/2021 9:53:20 AM



#41
Benzo(g,h,i)perylene
Concen: 0.344 ng
RT: 26.487 min Scan# 3281
Delta R.T. -0.017 min
Lab File: BN015026.D
Acq: 24 Jun 2021 01:28



Tgt Ion: 276 Resp: 84234
Ion Ratio Lower Upper
276 100
277 23.5 19.7 29.5
138 23.8 9.8 14.6#



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

mohammad
6/24/2021 9:53:20 AM