

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062421\  
 Data File : BN015033.D  
 Acq On : 24 Jun 2021 07:22  
 Operator : CG/JU  
 Sample : M2784-01  
 Misc :  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 RE132D7-20210618

Manual Integrations  
 APPROVED

mohammad  
 6/24/2021 9:53:39 AM

Quant Time: Jun 24 08:35:59 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-SIM-BN061621.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Jun 23 16:24:59 2021  
 Response via : Initial Calibration

| Compound                      | R.T.   | QIon | Response | Conc  | Units | Dev(Min) |
|-------------------------------|--------|------|----------|-------|-------|----------|
| -----                         |        |      |          |       |       |          |
| Internal Standards            |        |      |          |       |       |          |
| 1) 1,4-Dichlorobenzene-d4     | 7.741  | 152  | 21798    | 0.400 | ng    | # 0.00   |
| 7) Naphthalene-d8             | 10.505 | 136  | 98160    | 0.400 | ng    | 0.00     |
| 13) Acenaphthene-d10          | 14.346 | 164  | 51993    | 0.400 | ng    | -0.01    |
| 19) Phenanthrene-d10          | 17.104 | 188  | 99213    | 0.400 | ng    | # 0.00   |
| 29) Chrysene-d12              | 21.292 | 240  | 88685    | 0.400 | ng    | #-0.01   |
| 35) Perylene-d12              | 23.540 | 264  | 76297    | 0.400 | ng    | -0.01    |
| System Monitoring Compounds   |        |      |          |       |       |          |
| 4) 2-Fluorophenol             | 5.381  | 112  | 10003    | 0.148 | ng    | 0.00     |
| 5) Phenol-d6                  | 6.920  | 99   | 6974     | 0.082 | ng    | 0.00     |
| 8) Nitrobenzene-d5            | 8.870  | 82   | 27208    | 0.367 | ng    | -0.01    |
| 11) 2-Methylnaphthalene-d10   | 12.097 | 152  | 57770    | 0.343 | ng    | 0.00     |
| 14) 2,4,6-Tribromophenol      | 15.843 | 330  | 7484     | 0.307 | ng    | 0.00     |
| 15) 2-Fluorobiphenyl          | 12.976 | 172  | 84730    | 0.429 | ng    | 0.00     |
| 27) Fluoranthene-d10          | 19.133 | 212  | 112172   | 0.359 | ng    | 0.00     |
| 31) Terphenyl-d14             | 19.739 | 244  | 105768   | 0.481 | ng    | 0.00     |
| Target Compounds              |        |      |          |       |       |          |
| 2) 1,4-Dioxane                | 3.361  | 88   | 28881m   | 3.159 | ng    | Qvalue   |
| 6) bis(2-Chloroethyl)ether    | 7.179  | 93   | 2677     | 0.040 | ng    | # 86     |
| 34) Bis(2-ethylhexyl)phtha... | 21.218 | 149  | 45378    | 0.195 | ng    | # 87     |
| -----                         |        |      |          |       |       |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062421\  
Data File : BN015033.D  
Acq On : 24 Jun 2021 07:22  
Operator : CG/JU  
Sample : M2784-01  
Misc :  
ALS Vial : 24 Sample Multiplier: 1


Instrument :  
BNA\_N  
ClientSampleId :  
RE132D7-20210618

Manual Integrations  
APPROVED


mohammad  
6/24/2021 9:53:39 AM

Quant Time: Jun 24 08:35:59 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-SIM-BN061621.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jun 23 16:24:59 2021  
Response via : Initial Calibration



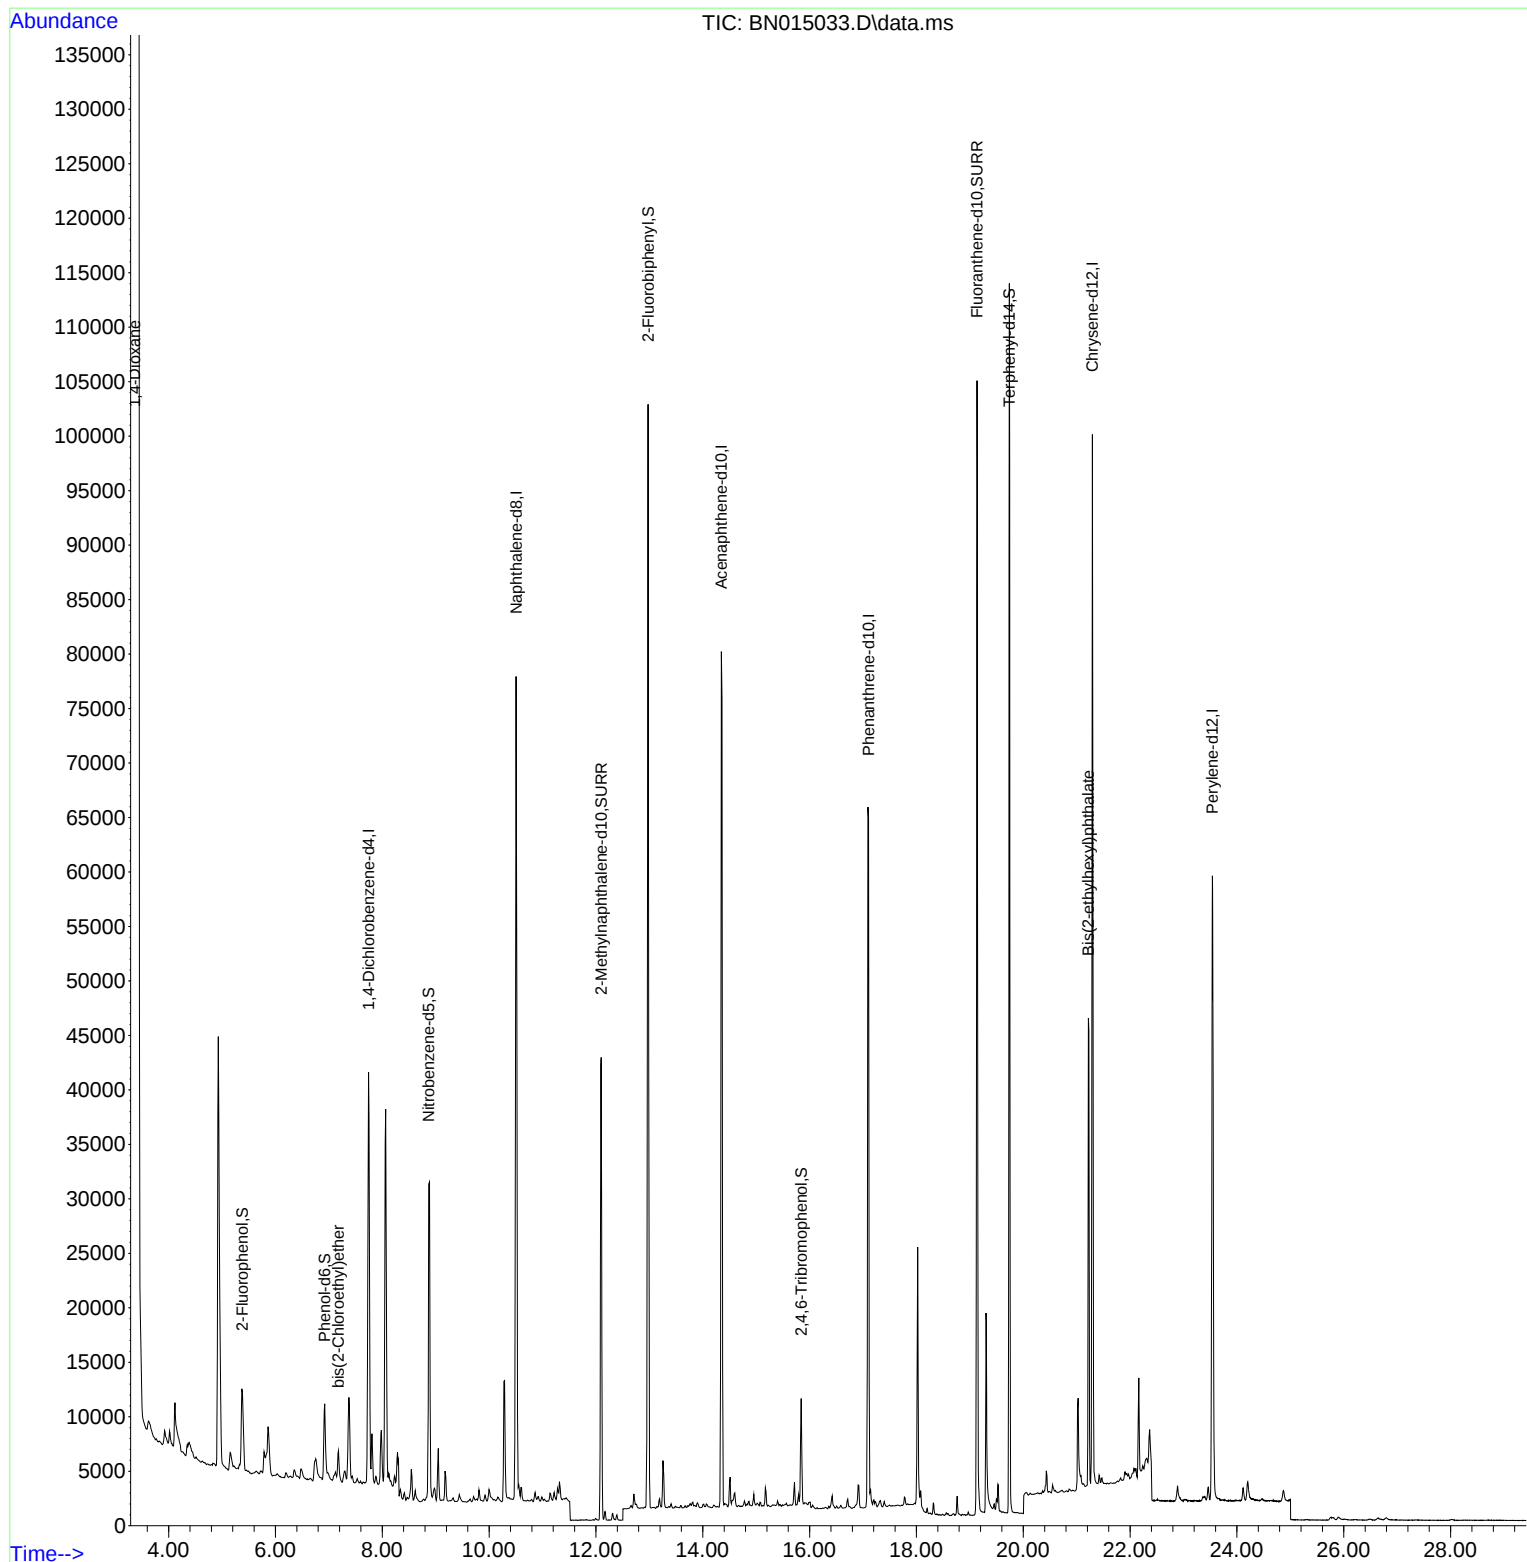


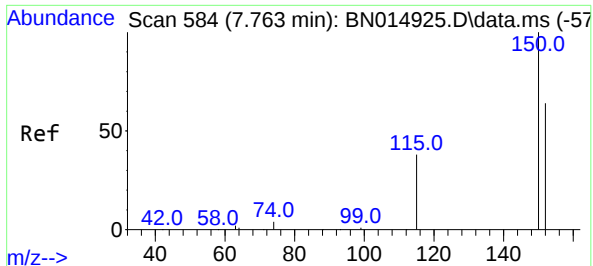


#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.741 min Scan# 484  
Delta R.T. -0.009 min  
Lab File: BN015033.D  
Acq: 24 Jun 2021 07:22

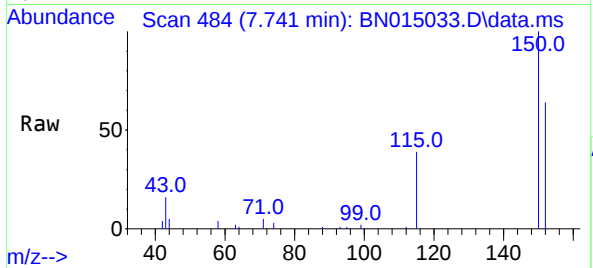



Tgt Ion: 152 Resp: 21798  
Ion Ratio Lower Upper  
152 100  
150 157.3 119.0 178.6  
115 61.1 62.2 93.4#

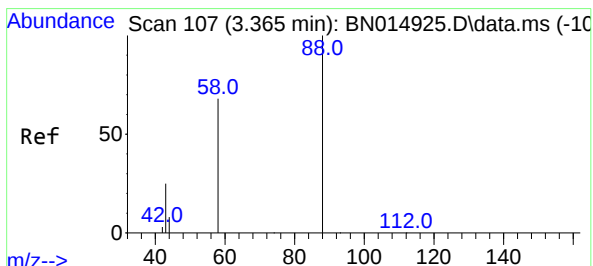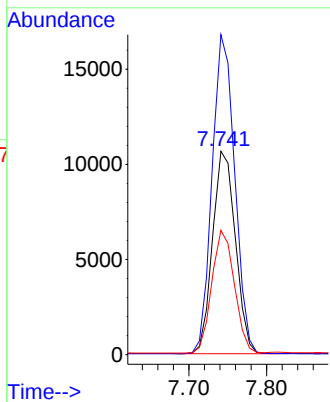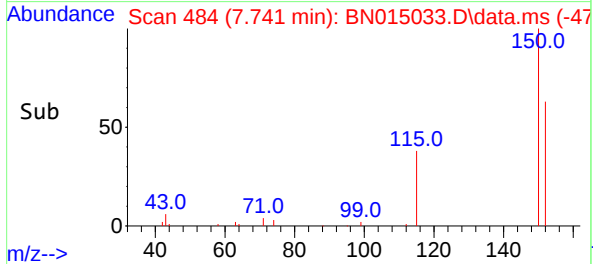

#2  
1,4-Dioxane  
Concen: 3.159 ng m  
RT: 3.361 min Scan# 9  
Delta R.T. 0.009 min  
Lab File: BN015033.D  
Acq: 24 Jun 2021 07:22

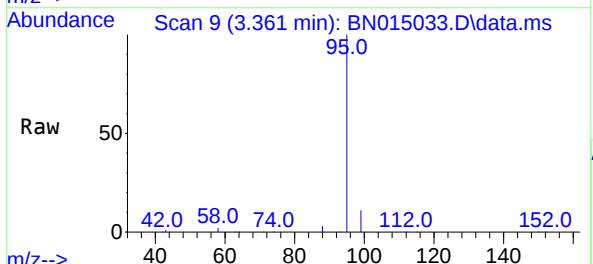


Tgt Ion: 88 Resp: 28881  
Ion Ratio Lower Upper  
88 100  
43 38.6 12.9 19.3#  
58 141.1 38.1 57.1#

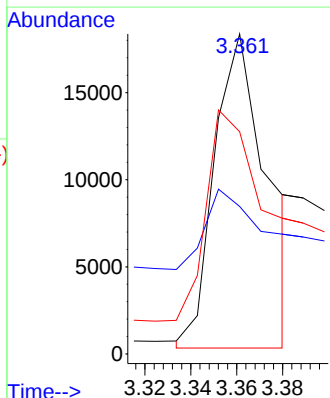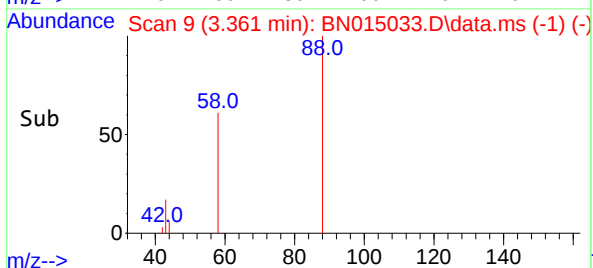

Instrument :  
BNA\_N  
ClientSampleId :  
RE132D7-20210618

Manual Integrations  
APPROVED

mohammad  
6/24/2021 9:53:39 AM

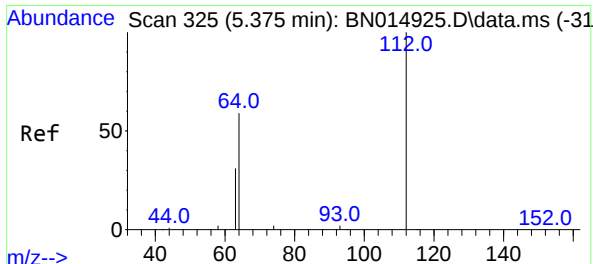





#4  
2-Fluorophenol  
Concen: 0.148 ng  
RT: 5.381 min Scan# 228  
Delta R.T. 0.009 min  
Lab File: BN015033.D  
Acq: 24 Jun 2021 07:22

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 112   | Resp: | 10003 |
| Ion      | Ratio | Lower | Upper |
| 112      | 100   |       |       |
| 64       | 57.9  | 39.0  | 58.6  |
| 63       | 30.1  | 20.6  | 30.8  |

Instrument :  
BNA\_N  
ClientSampleId :  
RE132D7-20210618




Manual Integrations  
APPROVED


mohammad  
6/24/2021 9:53:39 AM

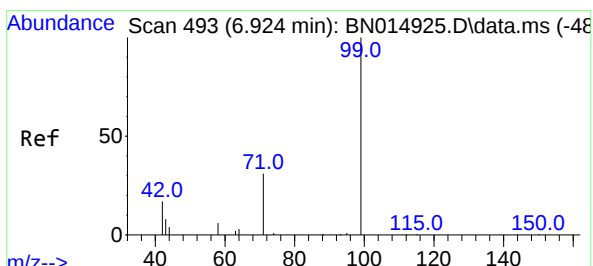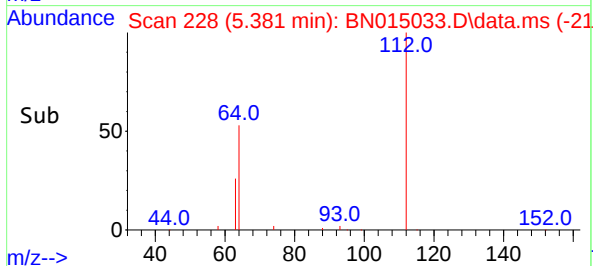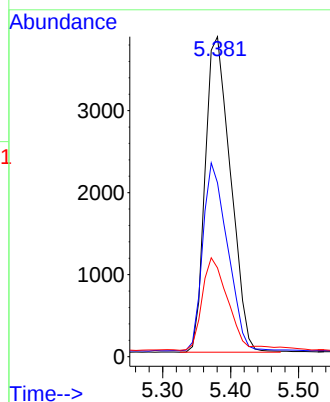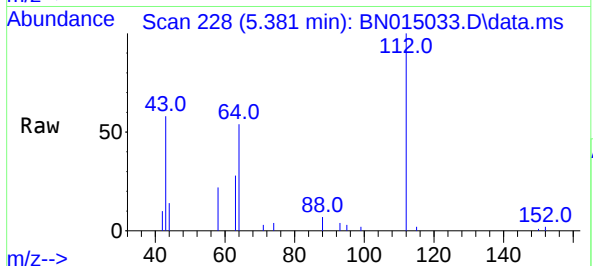

#5  
Phenol-d6  
Concen: 0.082 ng  
RT: 6.920 min Scan# 395  
Delta R.T. 0.009 min  
Lab File: BN015033.D  
Acq: 24 Jun 2021 07:22

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 99    | Resp: | 6974  |
| Ion      | Ratio | Lower | Upper |
| 99       | 100   |       |       |
| 42       | 17.3  | 8.9   | 13.3# |
| 71       | 36.5  | 35.6  | 53.4  |

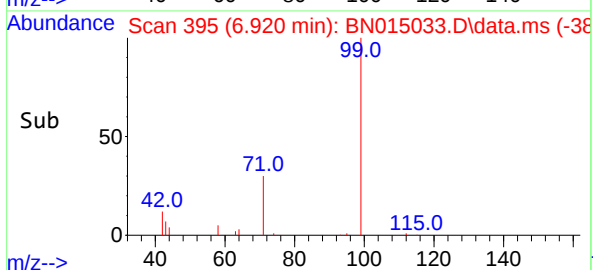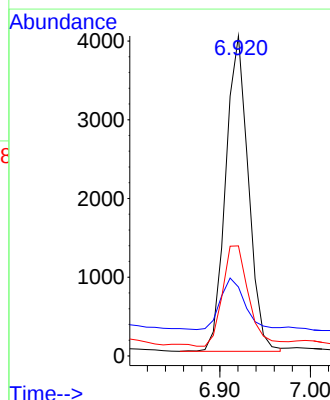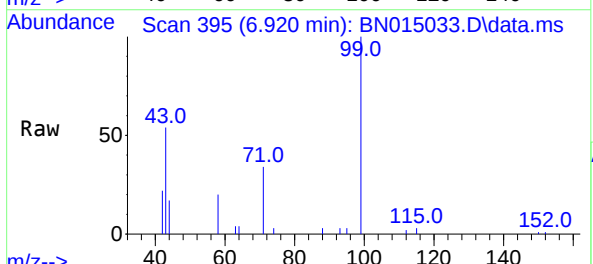

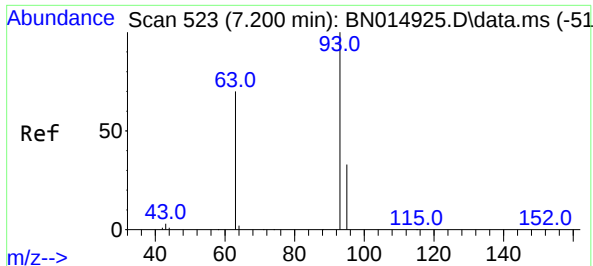





#6  
bis(2-Chloroethyl)ether  
Concen: 0.040 ng  
RT: 7.179 min Scan# 423  
Delta R.T. 0.000 min  
Lab File: BN015033.D  
Acq: 24 Jun 2021 07:22

Tgt Ion: 93 Resp: 2677  
Ion Ratio Lower Upper  
93 100  
63 72.5 46.6 70.0#  
95 31.7 28.6 42.8

Instrument :  
BNA\_N  
ClientSampleId :  
RE132D7-20210618




Manual Integrations  
APPROVED


mohammad  
6/24/2021 9:53:39 AM

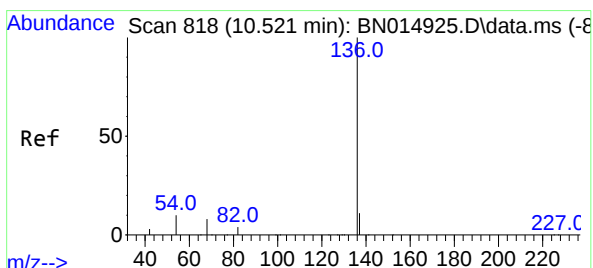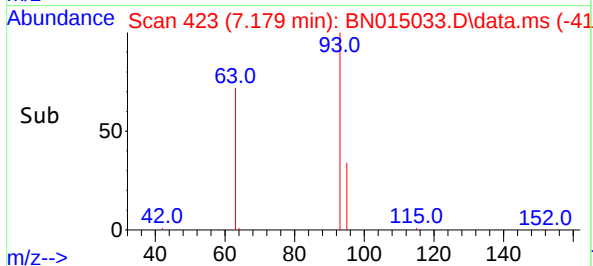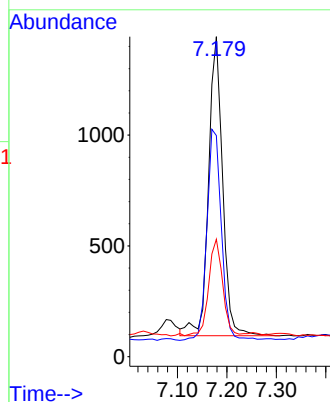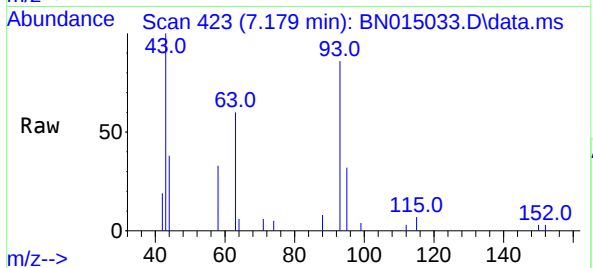

#7  
Naphthalene-d8  
Concen: 0.400 ng  
RT: 10.505 min Scan# 719  
Delta R.T. 0.000 min  
Lab File: BN015033.D  
Acq: 24 Jun 2021 07:22


Tgt Ion: 136 Resp: 98160  
Ion Ratio Lower Upper  
136 100  
137 11.0 9.8 14.8  
54 7.5 5.4 8.2  
68 6.2 4.9 7.3

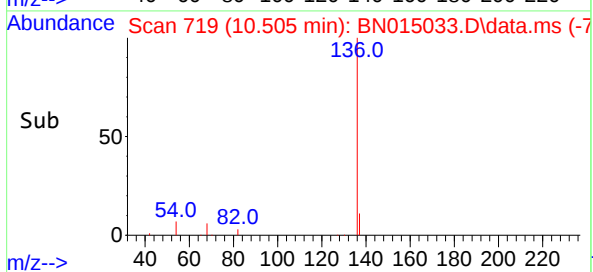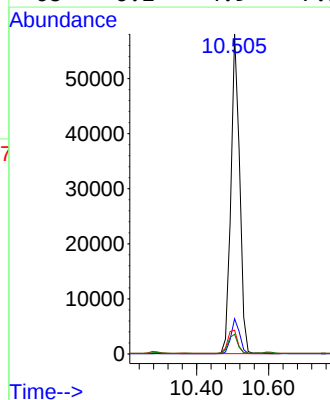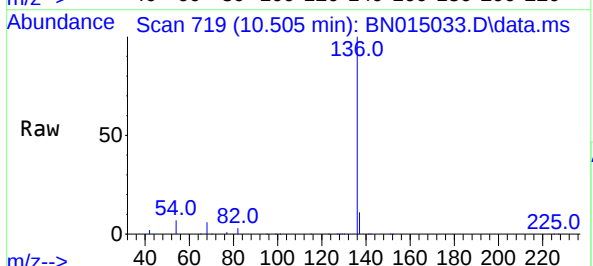

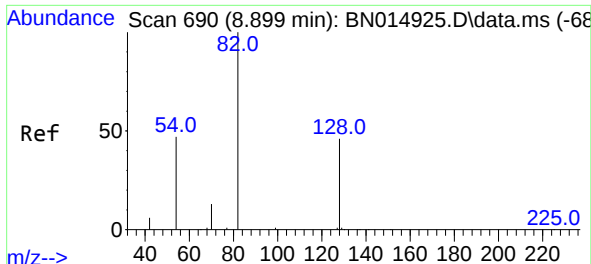

#8  
Nitrobenzene-d5  
Concen: 0.367 ng  
RT: 8.870 min Scan# 590  
Delta R.T. -0.013 min  
Lab File: BN015033.D  
Acq: 24 Jun 2021 07:22




Instrument :  
BNA\_N  
ClientSampleId :  
RE132D7-20210618

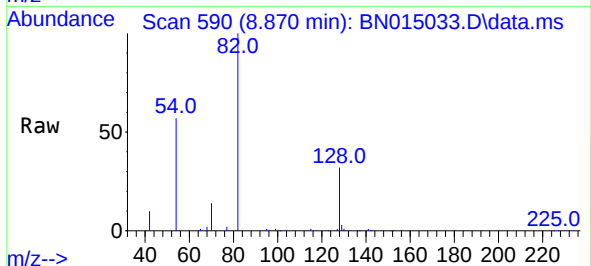

Tgt Ion: 82 Resp: 27208  
Ion Ratio Lower Upper  
82 100  
128 32.0 31.6 47.4  
54 56.7 29.0 43.4#




Manual Integrations  
APPROVED


mohammad  
6/24/2021 9:53:39 AM

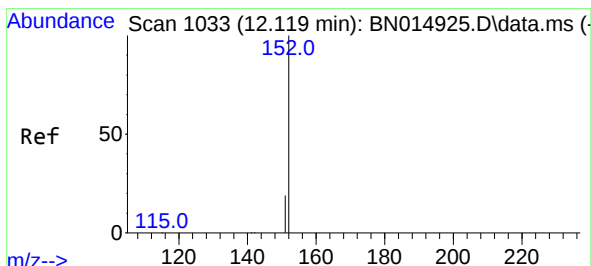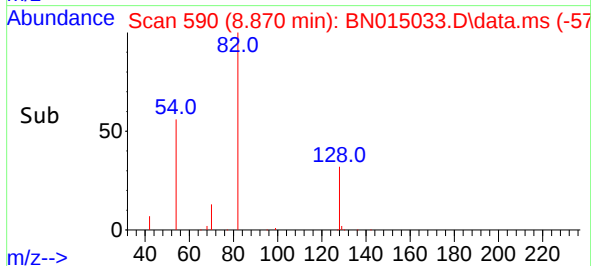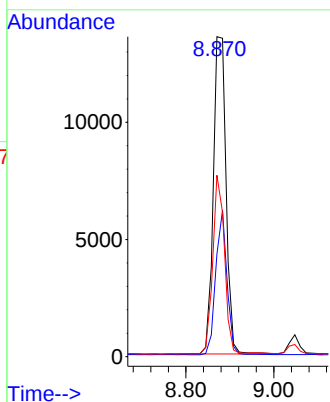

#11  
2-Methylnaphthalene-d10  
Concen: 0.343 ng  
RT: 12.097 min Scan# 929  
Delta R.T. 0.000 min  
Lab File: BN015033.D  
Acq: 24 Jun 2021 07:22


Tgt Ion: 152 Resp: 57770  
Ion Ratio Lower Upper  
152 100  
151 20.4 16.7 25.1

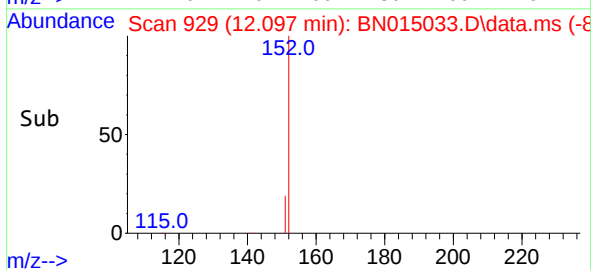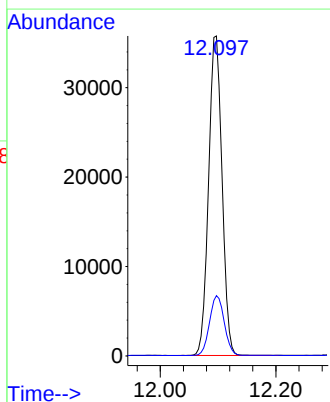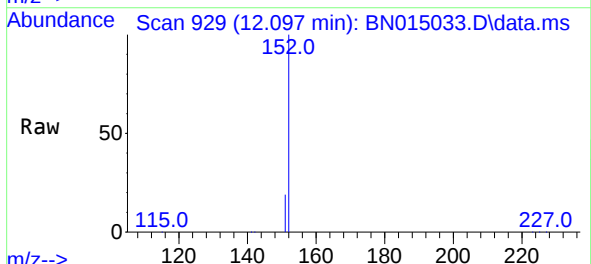

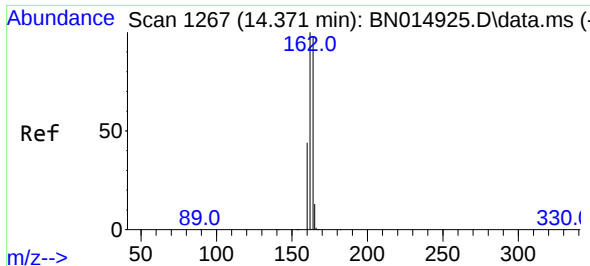

#13  
Acenaphthene-d10  
Concen: 0.400 ng  
RT: 14.346 min Scan# 1166  
Delta R.T. -0.013 min  
Lab File: BN015033.D  
Acq: 24 Jun 2021 07:22




Instrument :  
BNA\_N  
ClientSampleId :  
RE132D7-20210618

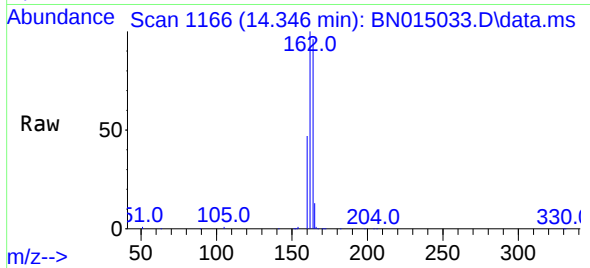

Tgt Ion:164 Resp: 51993  
Ion Ratio Lower Upper  
164 100  
162 104.4 83.8 125.6  
160 48.6 37.4 56.0




Manual Integrations  
APPROVED


mohammad  
6/24/2021 9:53:39 AM

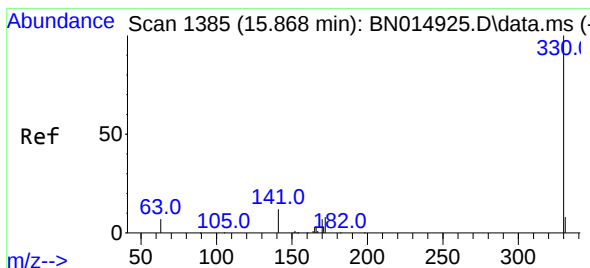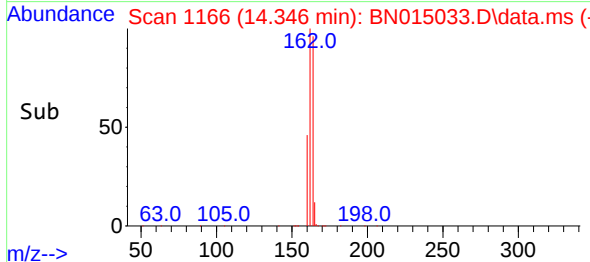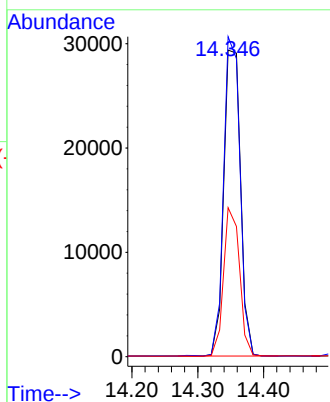

#14  
2,4,6-Tribromophenol  
Concen: 0.307 ng  
RT: 15.843 min Scan# 1284  
Delta R.T. 0.000 min  
Lab File: BN015033.D  
Acq: 24 Jun 2021 07:22

Tgt Ion:330 Resp: 7484  
Ion Ratio Lower Upper  
330 100  
332 0.0 0.0 0.0  
141 35.7 22.4 33.6#

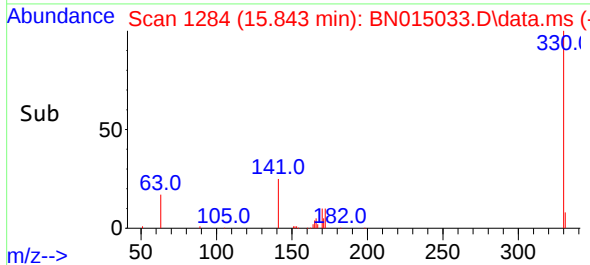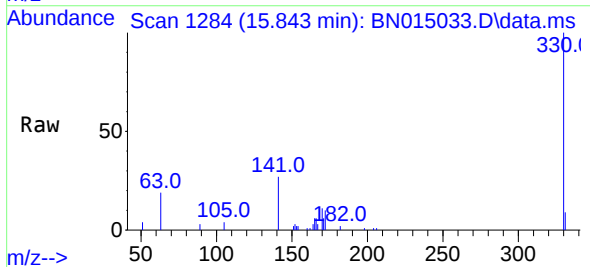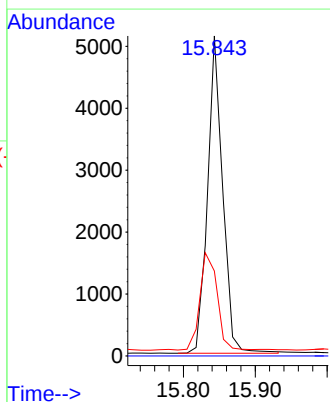

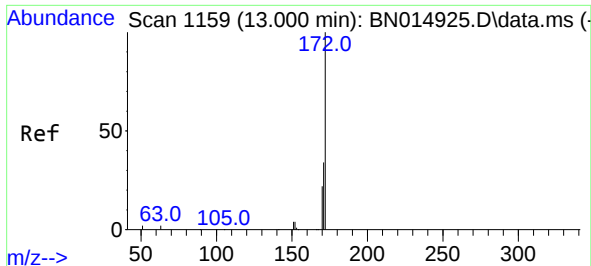





#15  
2-Fluorobiphenyl  
Concen: 0.429 ng  
RT: 12.976 min Scan# 1058  
Delta R.T. 0.000 min  
Lab File: BN015033.D  
Acq: 24 Jun 2021 07:22

|           |       |       |       |
|-----------|-------|-------|-------|
| Tgt Ion:  | 172   | Resp: | 84730 |
| Ion Ratio | Lower | Upper |       |
| 172       | 100   |       |       |
| 171       | 34.4  | 30.6  | 45.8  |
| 170       | 22.8  | 20.2  | 30.4  |

Instrument :  
BNA\_N  
ClientSampleId :  
RE132D7-20210618




Manual Integrations  
APPROVED


mohammad  
6/24/2021 9:53:39 AM

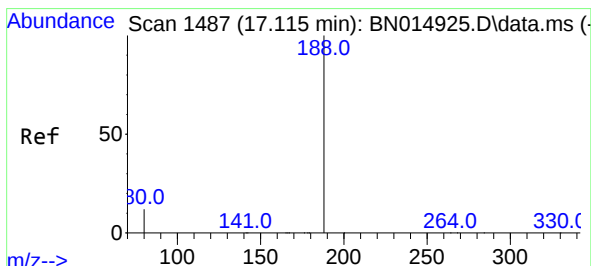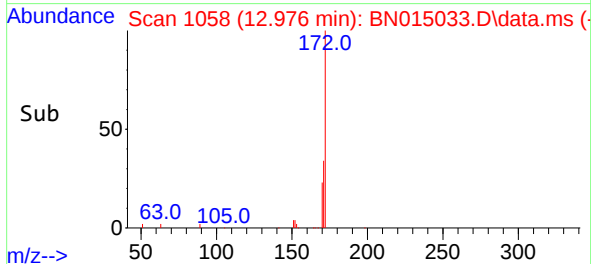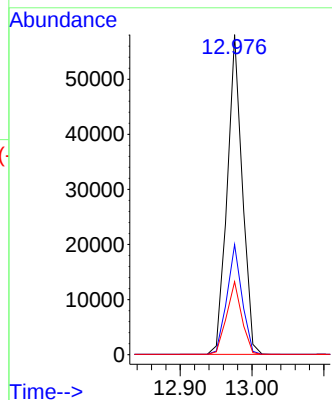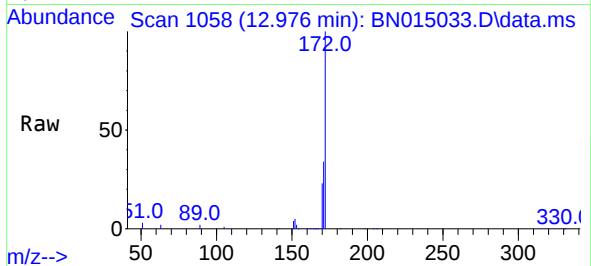

#19  
Phenanthrene-d10  
Concen: 0.400 ng  
RT: 17.104 min Scan# 1387  
Delta R.T. 0.000 min  
Lab File: BN015033.D  
Acq: 24 Jun 2021 07:22


|           |       |       |       |
|-----------|-------|-------|-------|
| Tgt Ion:  | 188   | Resp: | 99213 |
| Ion Ratio | Lower | Upper |       |
| 188       | 100   |       |       |
| 94        | 0.0   | 0.0   | 0.0   |
| 80        | 6.8   | 9.0   | 13.4  |

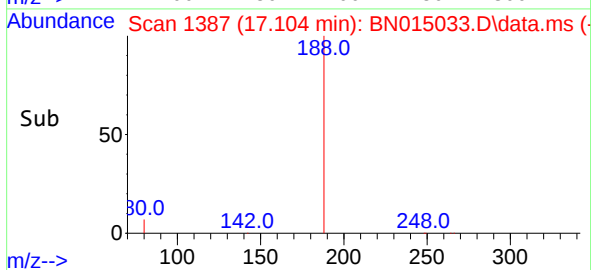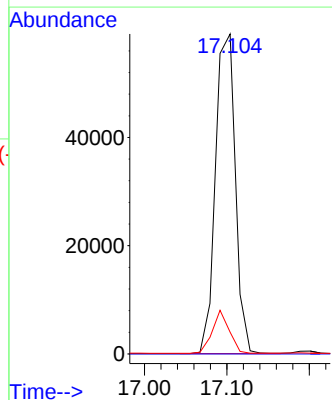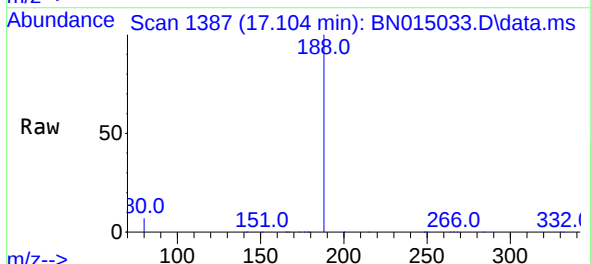

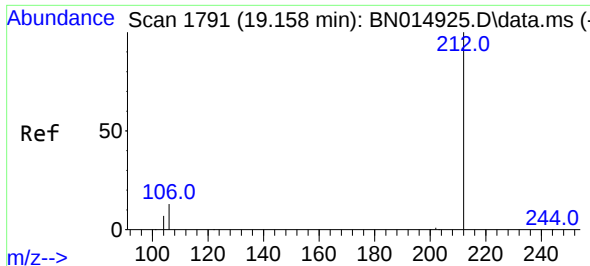

#27  
Fluoranthene-d10  
Concen: 0.359 ng  
RT: 19.133 min Scan# 1687  
Delta R.T. -0.005 min  
Lab File: BN015033.D  
Acq: 24 Jun 2021 07:22




Instrument :  
BNA\_N  
ClientSampleId :  
RE132D7-20210618

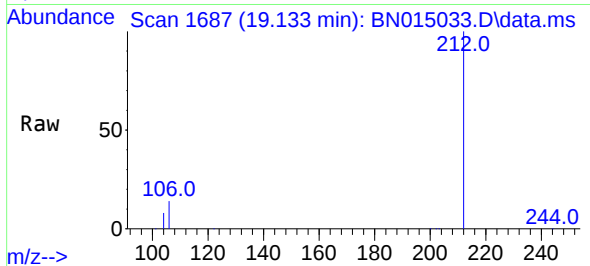


Tgt Ion:212 Resp: 112172  
Ion Ratio Lower Upper  
212 100  
106 14.4 7.0 10.6#  
104 7.7 4.1 6.1#

Manual Integrations  
APPROVED



mohammad  
6/24/2021 9:53:39 AM

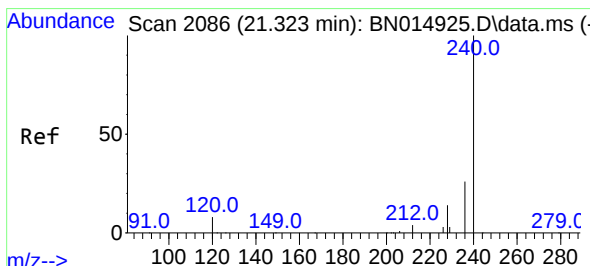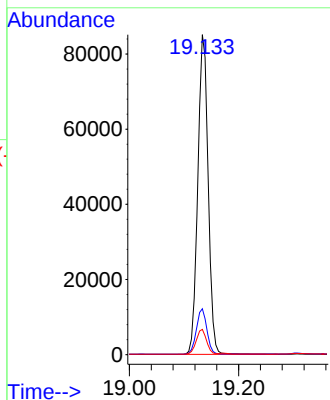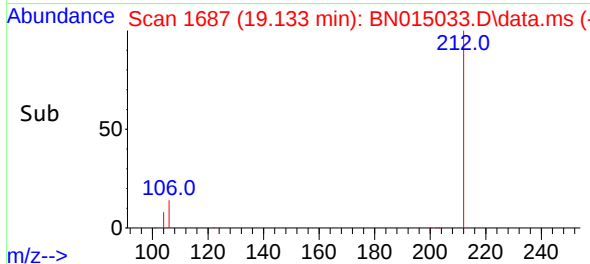


#29  
Chrysene-d12  
Concen: 0.400 ng  
RT: 21.292 min Scan# 1984  
Delta R.T. -0.011 min  
Lab File: BN015033.D  
Acq: 24 Jun 2021 07:22

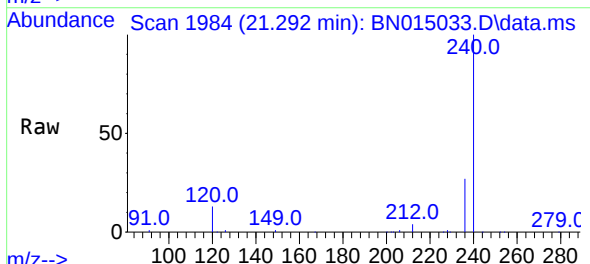


Tgt Ion:240 Resp: 88685  
Ion Ratio Lower Upper  
240 100  
120 12.7 4.2 6.4#  
236 26.7 21.4 32.2


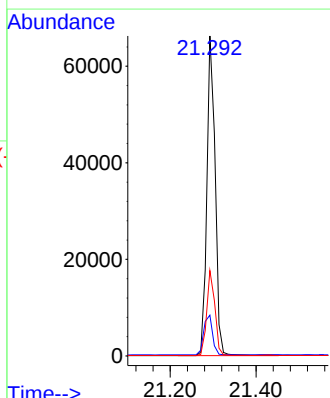
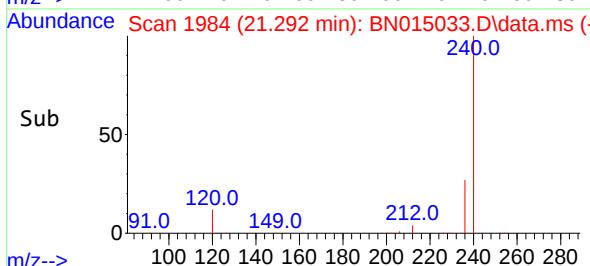


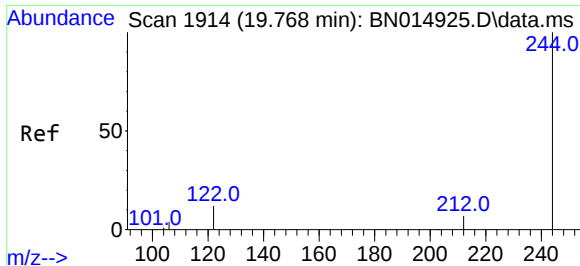


#31  
Terphenyl-d14  
Concen: 0.481 ng  
RT: 19.739 min Scan# 1809  
Delta R.T. -0.005 min  
Lab File: BN015033.D  
Acq: 24 Jun 2021 07:22

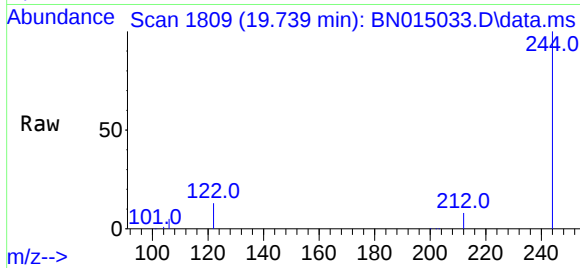



Tgt Ion:244 Resp: 105768  
Ion Ratio Lower Upper  
244 100  
212 7.6 6.3 9.5  
122 13.4 6.2 9.2#

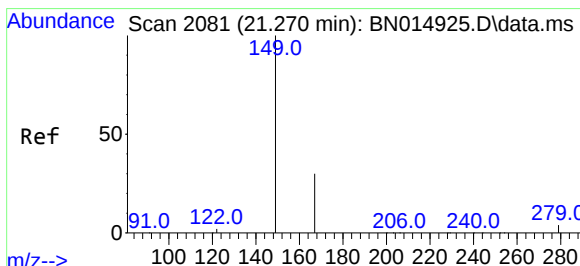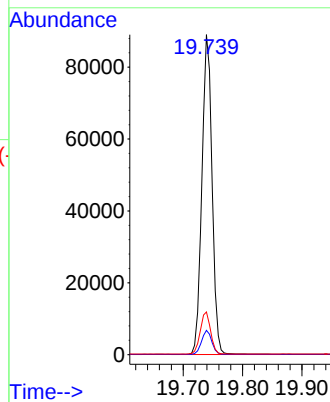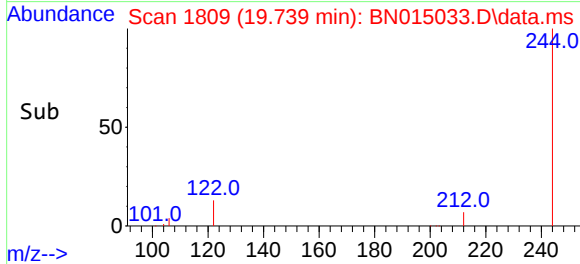

#34  
Bis(2-ethylhexyl)phthalate  
Concen: 0.195 ng  
RT: 21.218 min Scan# 1977  
Delta R.T. -0.011 min  
Lab File: BN015033.D  
Acq: 24 Jun 2021 07:22

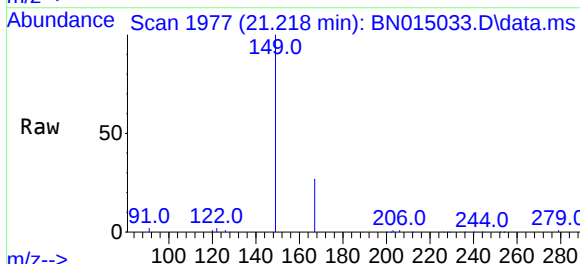


Tgt Ion:149 Resp: 45378  
Ion Ratio Lower Upper  
149 100  
167 28.1 28.9 43.3#  
279 3.7 4.9 7.3#

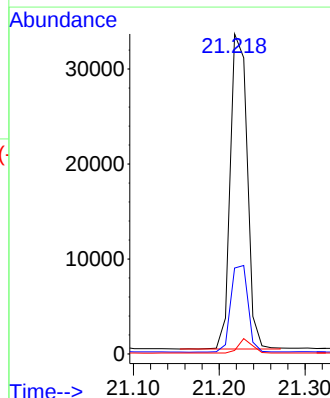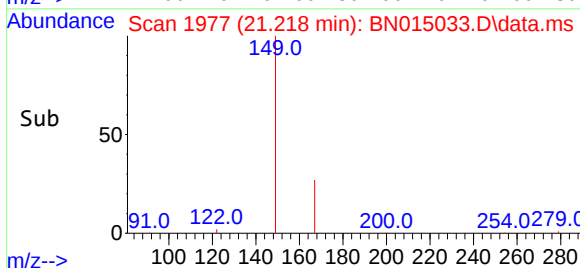

Instrument :  
BNA\_N  
ClientSampleId :  
RE132D7-20210618


Manual Integrations  
APPROVED

mohammad  
6/24/2021 9:53:39 AM

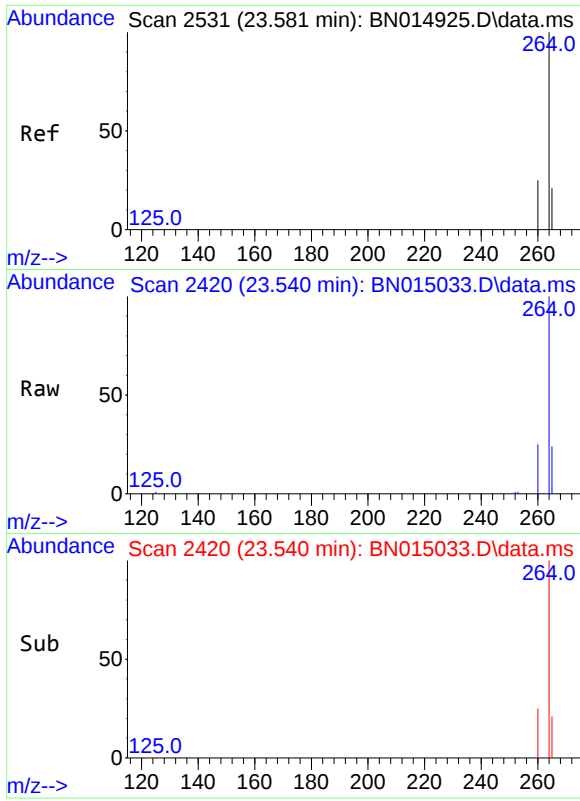

#35  
Perylene-d12  
Concen: 0.400 ng  
RT: 23.540 min Scan# 2420  
Delta R.T. -0.014 min  
Lab File: BN015033.D  
Acq: 24 Jun 2021 07:22

|             |       |             |
|-------------|-------|-------------|
| Tgt Ion:264 | Resp: | 76297       |
| Ion         | Ratio | Lower Upper |
| 264         | 100   |             |
| 260         | 24.8  | 20.6 31.0   |
| 265         | 24.1  | 21.4 32.2   |

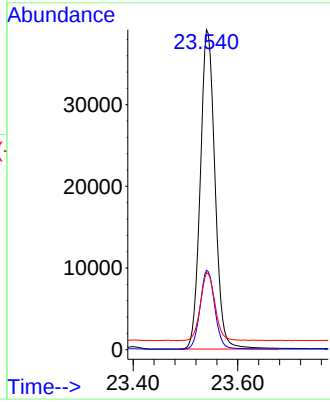

Instrument :  
BNA\_N  
ClientSampleId :  
RE132D7-20210618

Manual Integrations  
APPROVED  
mohammad  
6/24/2021 9:53:39 AM