
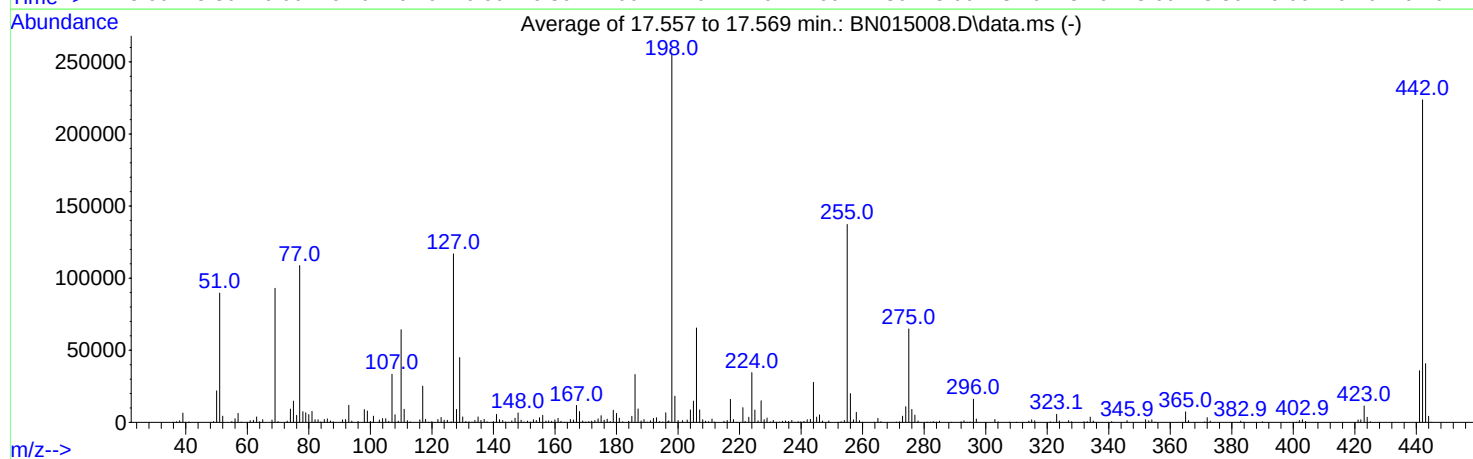


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062421\
 Data File : BN015008.D
 Acq On : 23 Jun 2021 14:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN061621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 23 16:24:59 2021

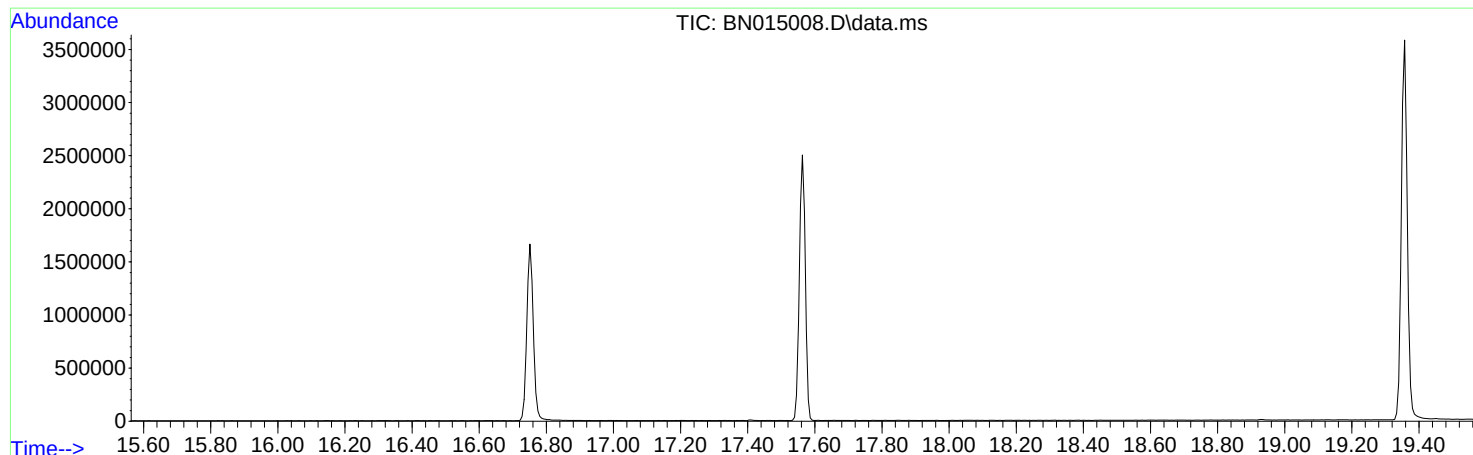




AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	89672	PASS
68	69	0.00	2	1.8	1660	PASS
69	198	0.00	100	36.5	93008	PASS
70	69	0.00	2	0.6	518	PASS
127	198	10	80	45.8	116880	PASS
197	198	0.00	2	0.4	1109	PASS
198	198	100	100	100.0	255147	PASS
199	198	5	9	7.2	18251	PASS
275	198	10	60	25.4	64795	PASS
365	198	1	100	2.9	7321	PASS
441	198	0.01	100	14.0	35835	PASS
442	442	50	100	100.0	223744	PASS
443	442	15	24	18.2	40736	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062421\
Data File : BN015008.D
Acq On : 23 Jun 2021 14:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 23 16:21:57 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

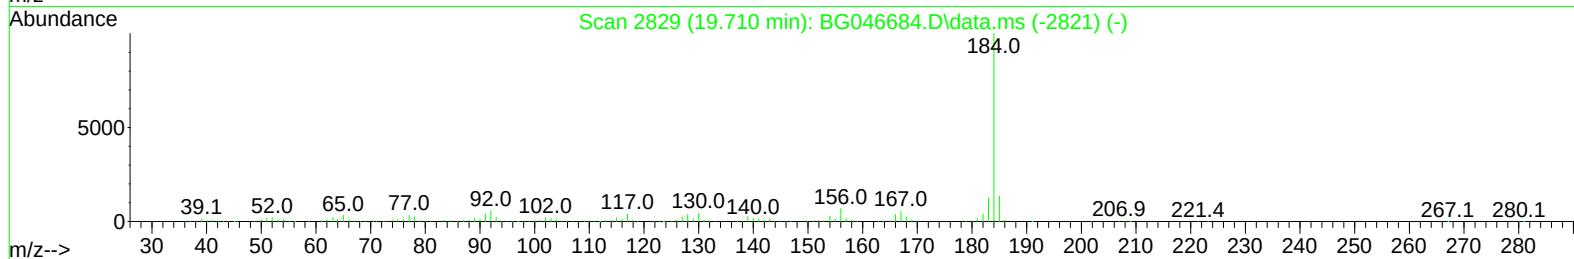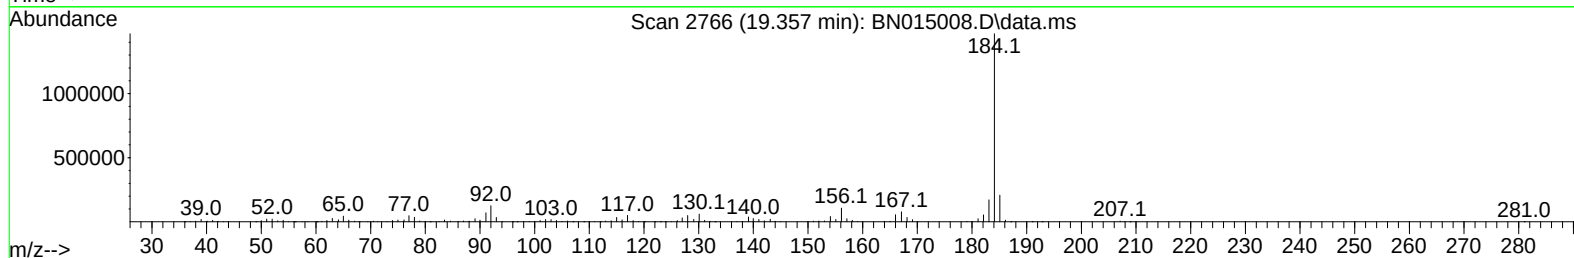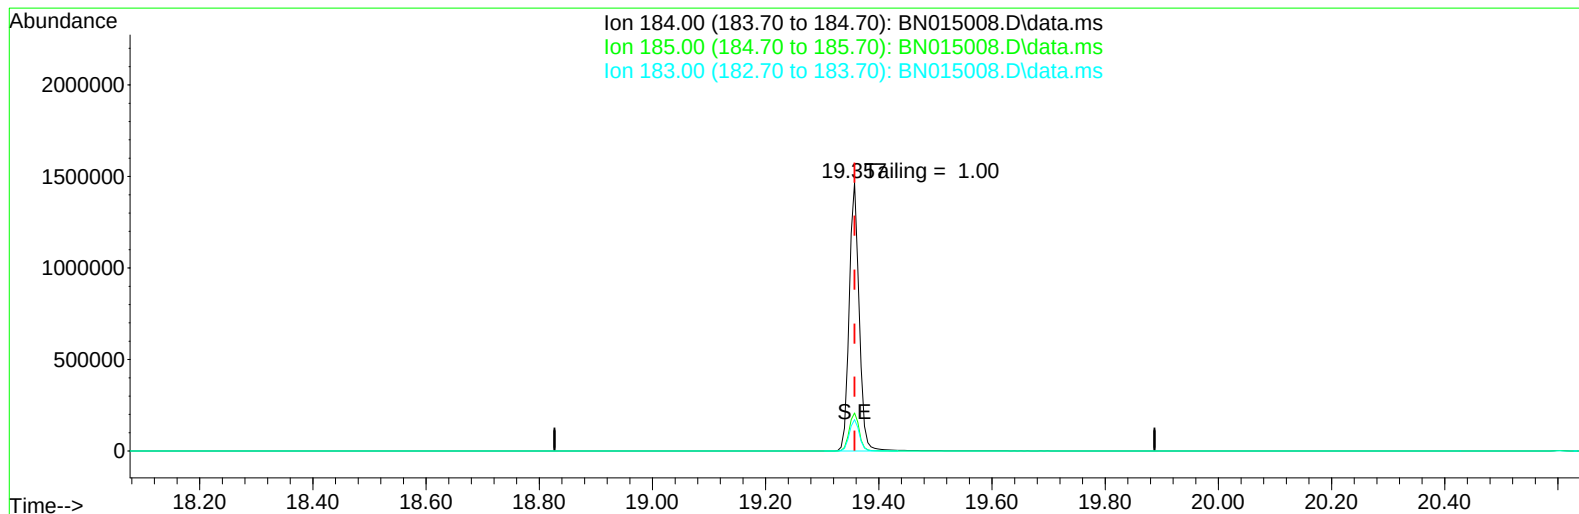

TIC: BN015008.D\data.ms

(77) Benzidine

19.357min (+ 0.000) 0.00 ng




response 1807830

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.19
183.00	13.20	11.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062421\
Data File : BN015008.D
Acq On : 23 Jun 2021 14:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 23 16:21:57 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

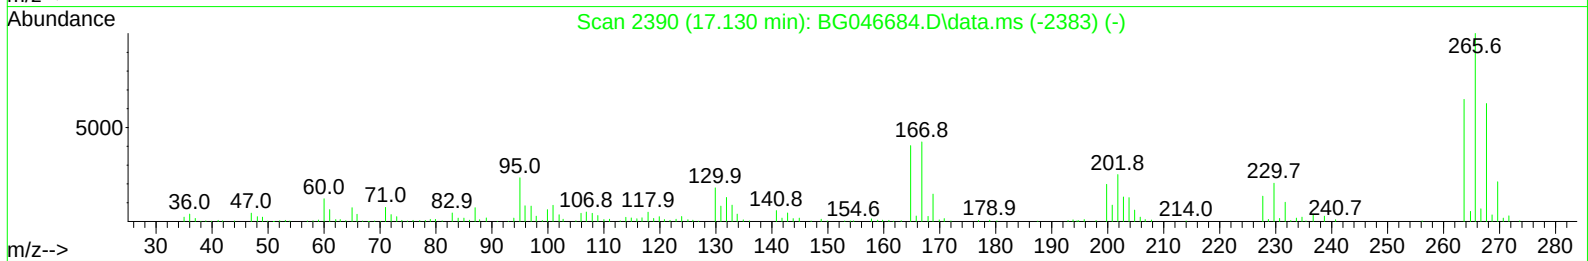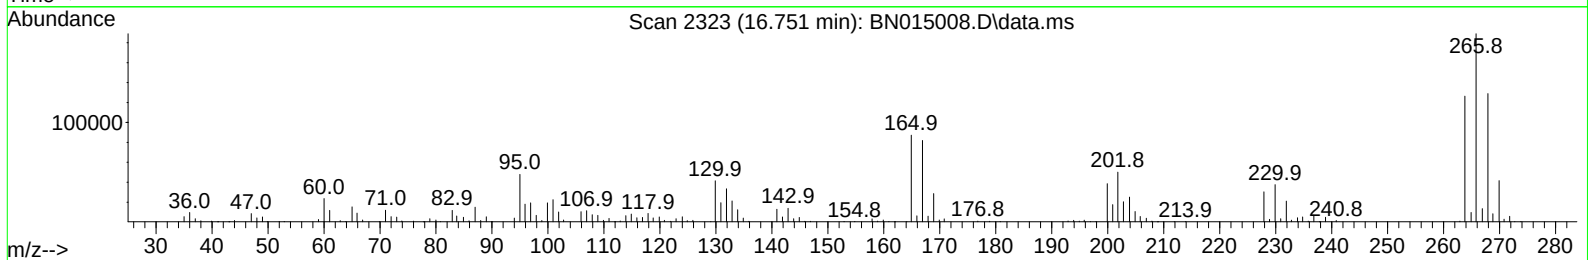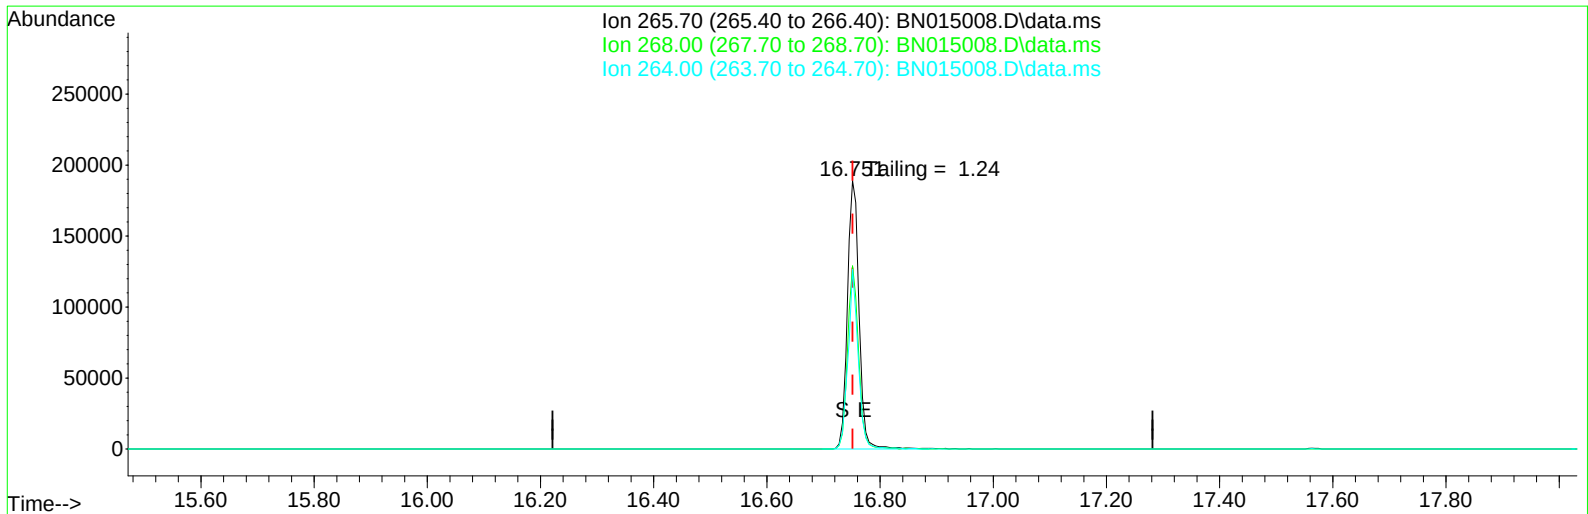

TIC: BN015008.D\data.ms

(70) Pentachlorophenol (C)

16.751min (+ 0.000) 22643.48 ng

response 269216

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.25
264.00	61.60	66.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/24/2021	BNA_N	<u>BN015008.D</u>
Compound Name	Response	Retention Time
DDT	810581	20.6
DDD	16106	20.15
DDE	1382	19.65
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17488	828069	2.11