
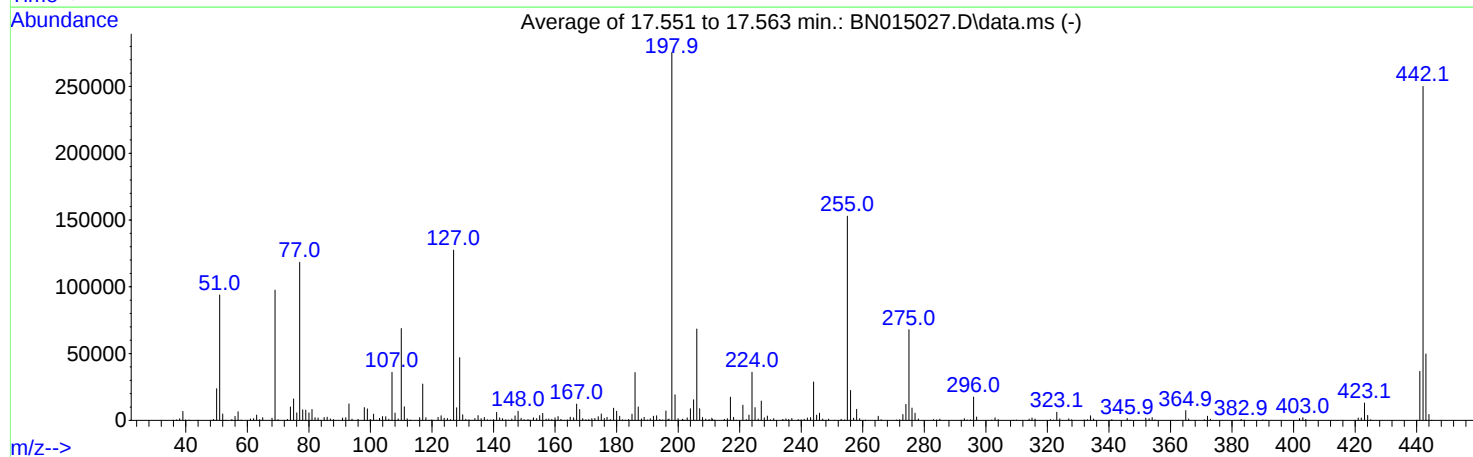


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062421\
 Data File : BN015027.D
 Acq On : 24 Jun 2021 03:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN061621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 23 16:24:59 2021

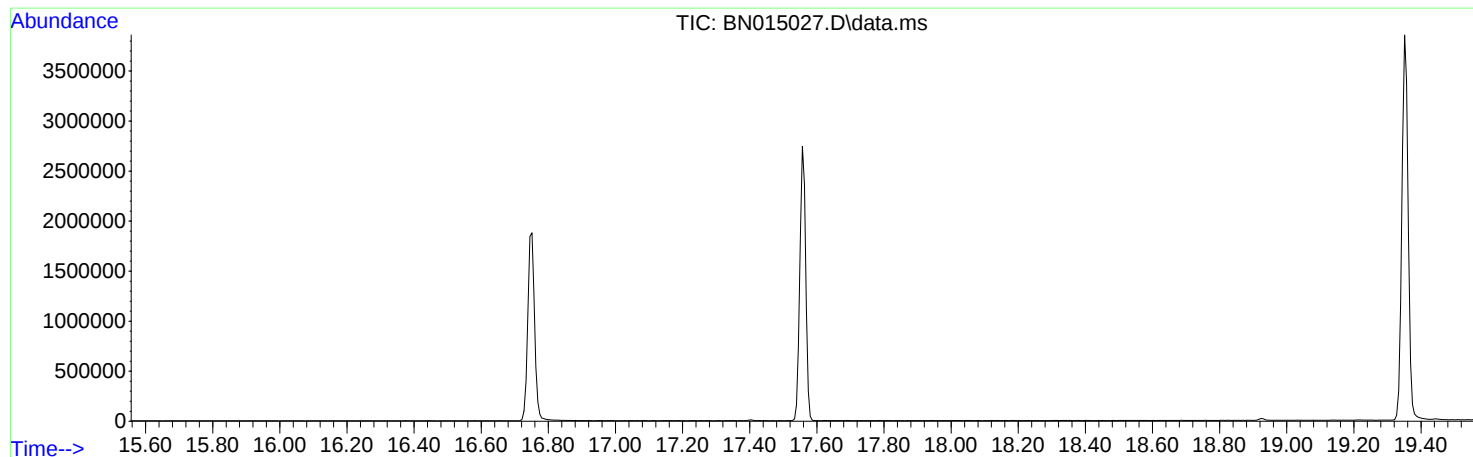




AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	93955	PASS
68	69	0.00	2	1.8	1735	PASS
69	198	0.00	100	35.4	97536	PASS
70	69	0.00	2	0.6	566	PASS
127	198	10	80	46.3	127435	PASS
197	198	0.00	2	0.4	1033	PASS
198	198	100	100	100.0	275435	PASS
199	198	5	9	7.0	19192	PASS
275	198	10	60	24.7	67931	PASS
365	198	1	100	2.7	7318	PASS
441	198	0.01	100	13.3	36712	PASS
442	442	50	100	100.0	250069	PASS
443	442	15	24	19.9	49728	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062421\
Data File : BN015027.D
Acq On : 24 Jun 2021 03:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 24 04:49:25 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

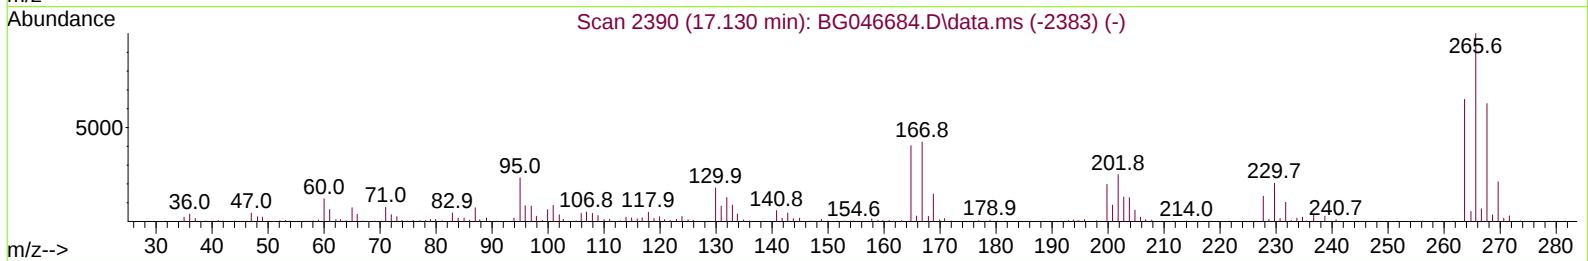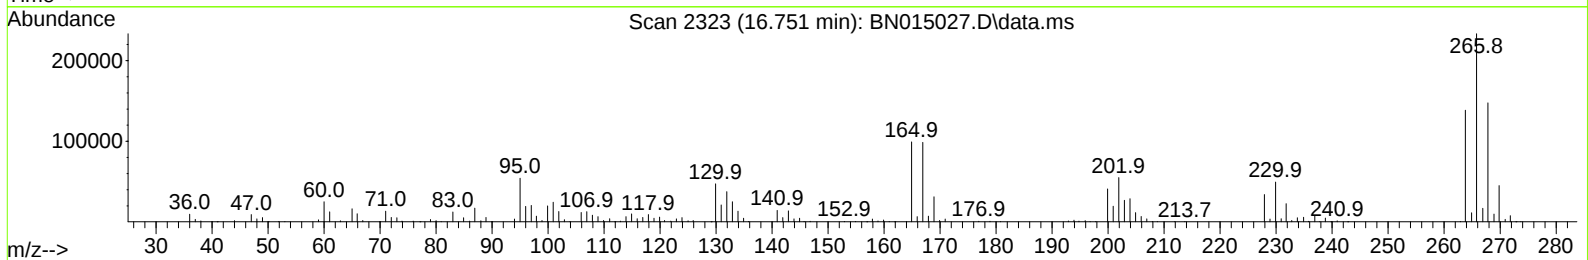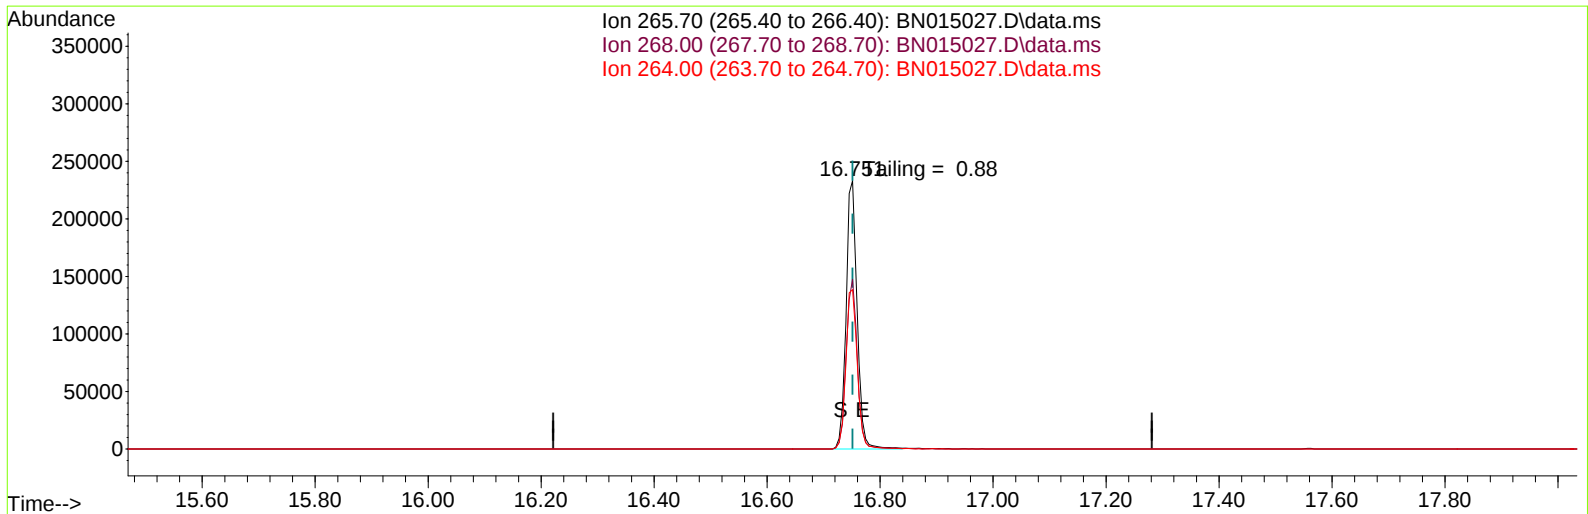

TIC: BN015027.D\data.ms

(70) Pentachlorophenol (C)

16.751min (-0.000) 26905.43 ng




response 317354

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.26
264.00	61.60	59.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062421\
Data File : BN015027.D
Acq On : 24 Jun 2021 03:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 24 04:49:25 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

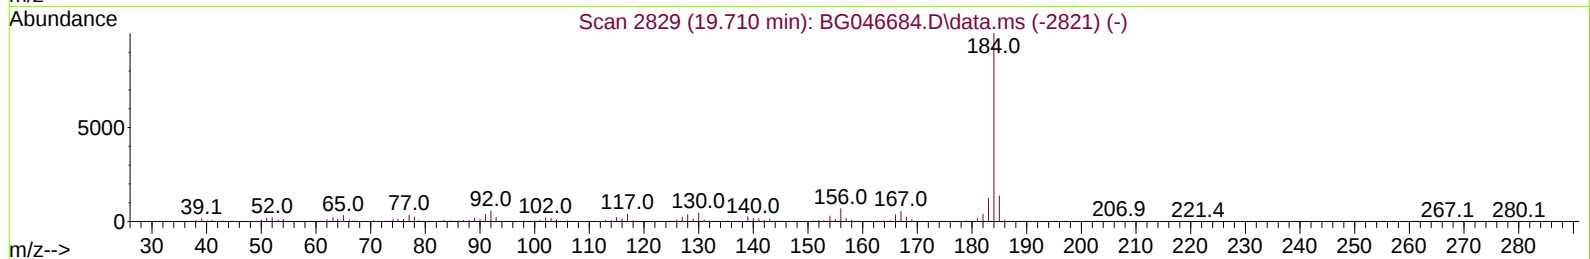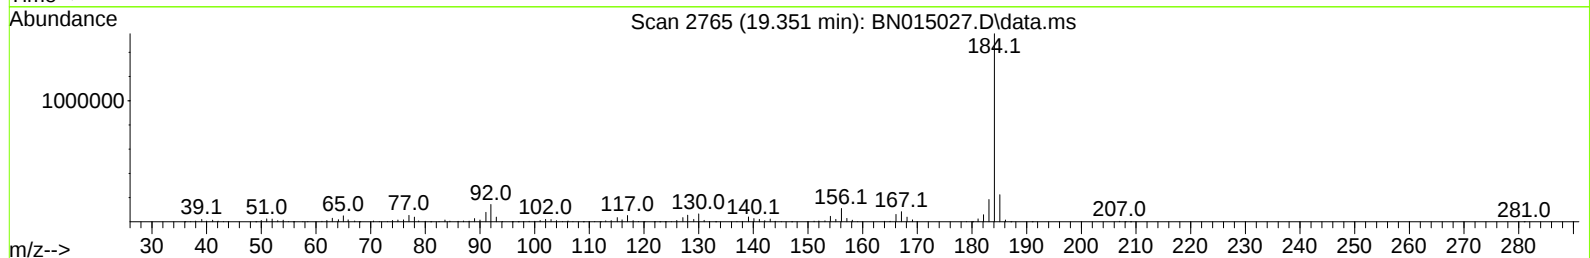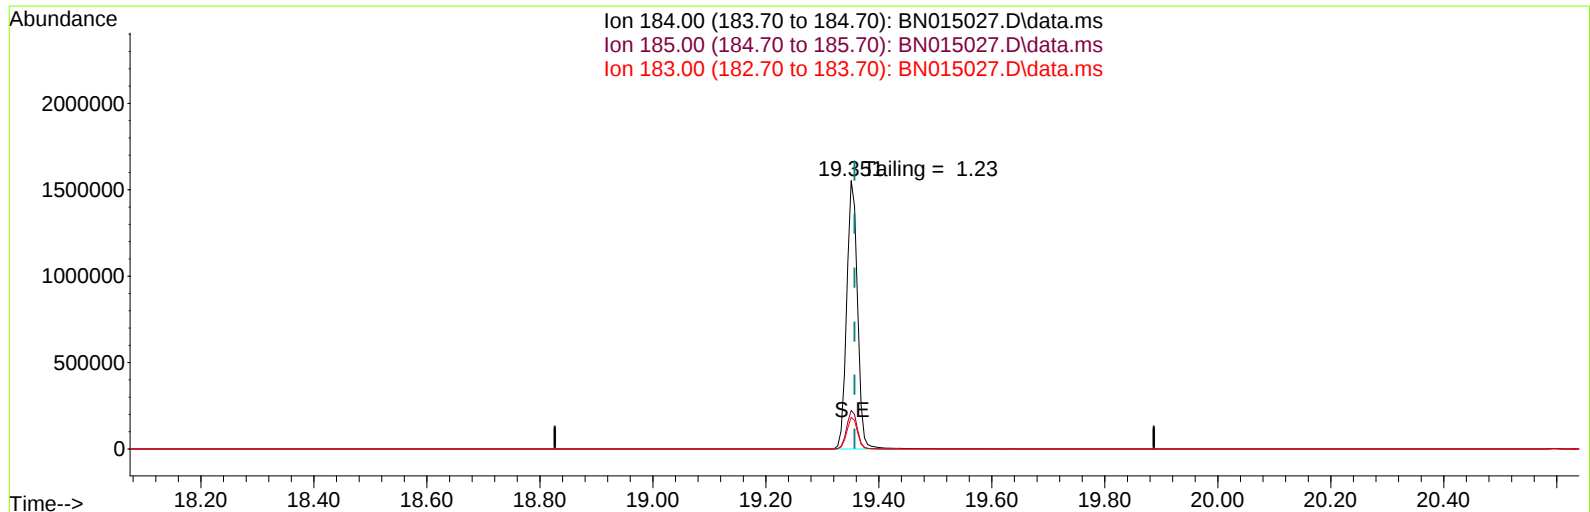

TIC: BN015027.D\data.ms

(77) Benzidine

19.351min (-0.006) 0.00 ng

response 2067116

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.37
183.00	13.20	11.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/24/2021	BNA_N	<u>BN015027.D</u>
Compound Name	Response	Retention Time
DDT	861397	20.598
DDD	37028	20.157
DDE	1667	19.645
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
38695	900092	4.30