
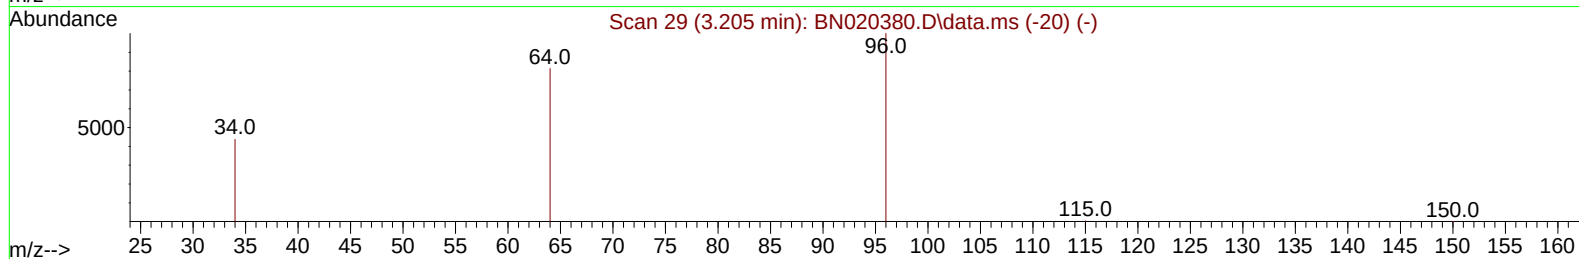
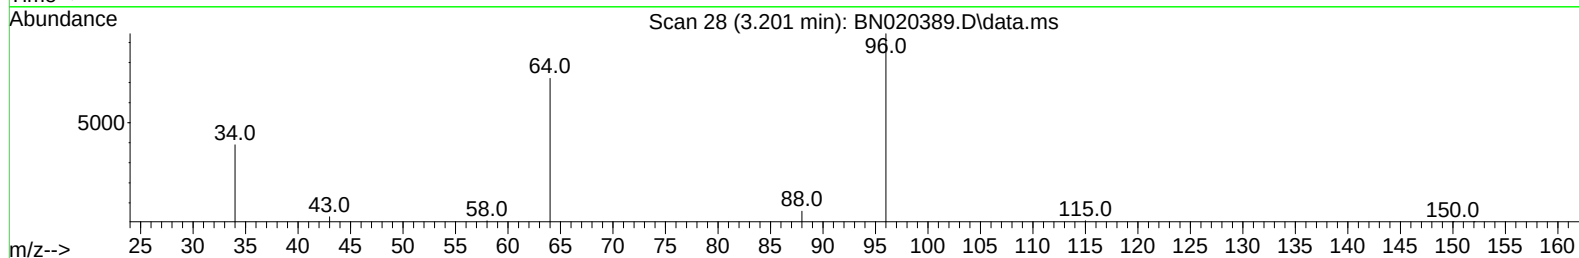


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
Data File : BN020389.D
Acq On : 24 Jun 2022 09:59
Operator : CG/JU
Sample : N3355-20
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 25 00:54:30 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:17:34 2022
Response via : Initial Calibration

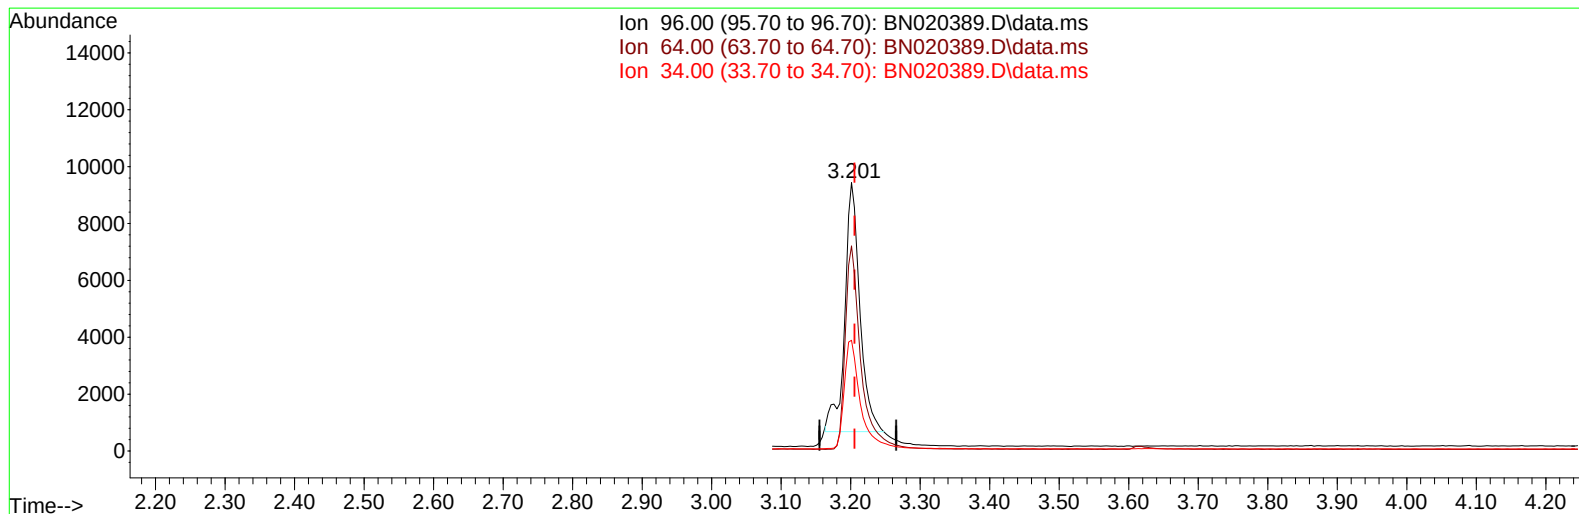

TIC: BN020389.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.201min (-0.004) 4.15 ng/ul

response 13238

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	72.10	76.43
34.00	43.00	41.29
0.00	0.00	0.00