

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020387.D
 Acq On : 24 Jun 2022 08:47
 Operator : CG/JU
 Sample : PB145674BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 25 00:54:24 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.745	152	3575	0.400	ng/ul	0.00
4) Naphthalene-d8	10.528	136	12036	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.376	164	7925	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.119	188	17788	0.400	ng/ul	0.00
17) Chrysene-d12	21.312	240	15069	0.400	ng/ul	0.00
23) Perylene-d12	23.592	264	15362	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	22982	5.549	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.128	152	5987	0.303	ng/ul	0.00
18) Fluoranthene-d10	19.149	212	15119	0.304	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.370	166	1993	0.056	ng/ul#	14
20) Pyrene	19.511	202	2033	0.028	ng/ul#	1
26) Benzo(a)pyrene	23.446	252	4549	0.070	ng/ul#	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
Data File : BN020387.D
Acq On : 24 Jun 2022 08:47
Operator : CG/JU
Sample : PB145674BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Jun 25 00:54:24 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:17:34 2022
Response via : Initial Calibration

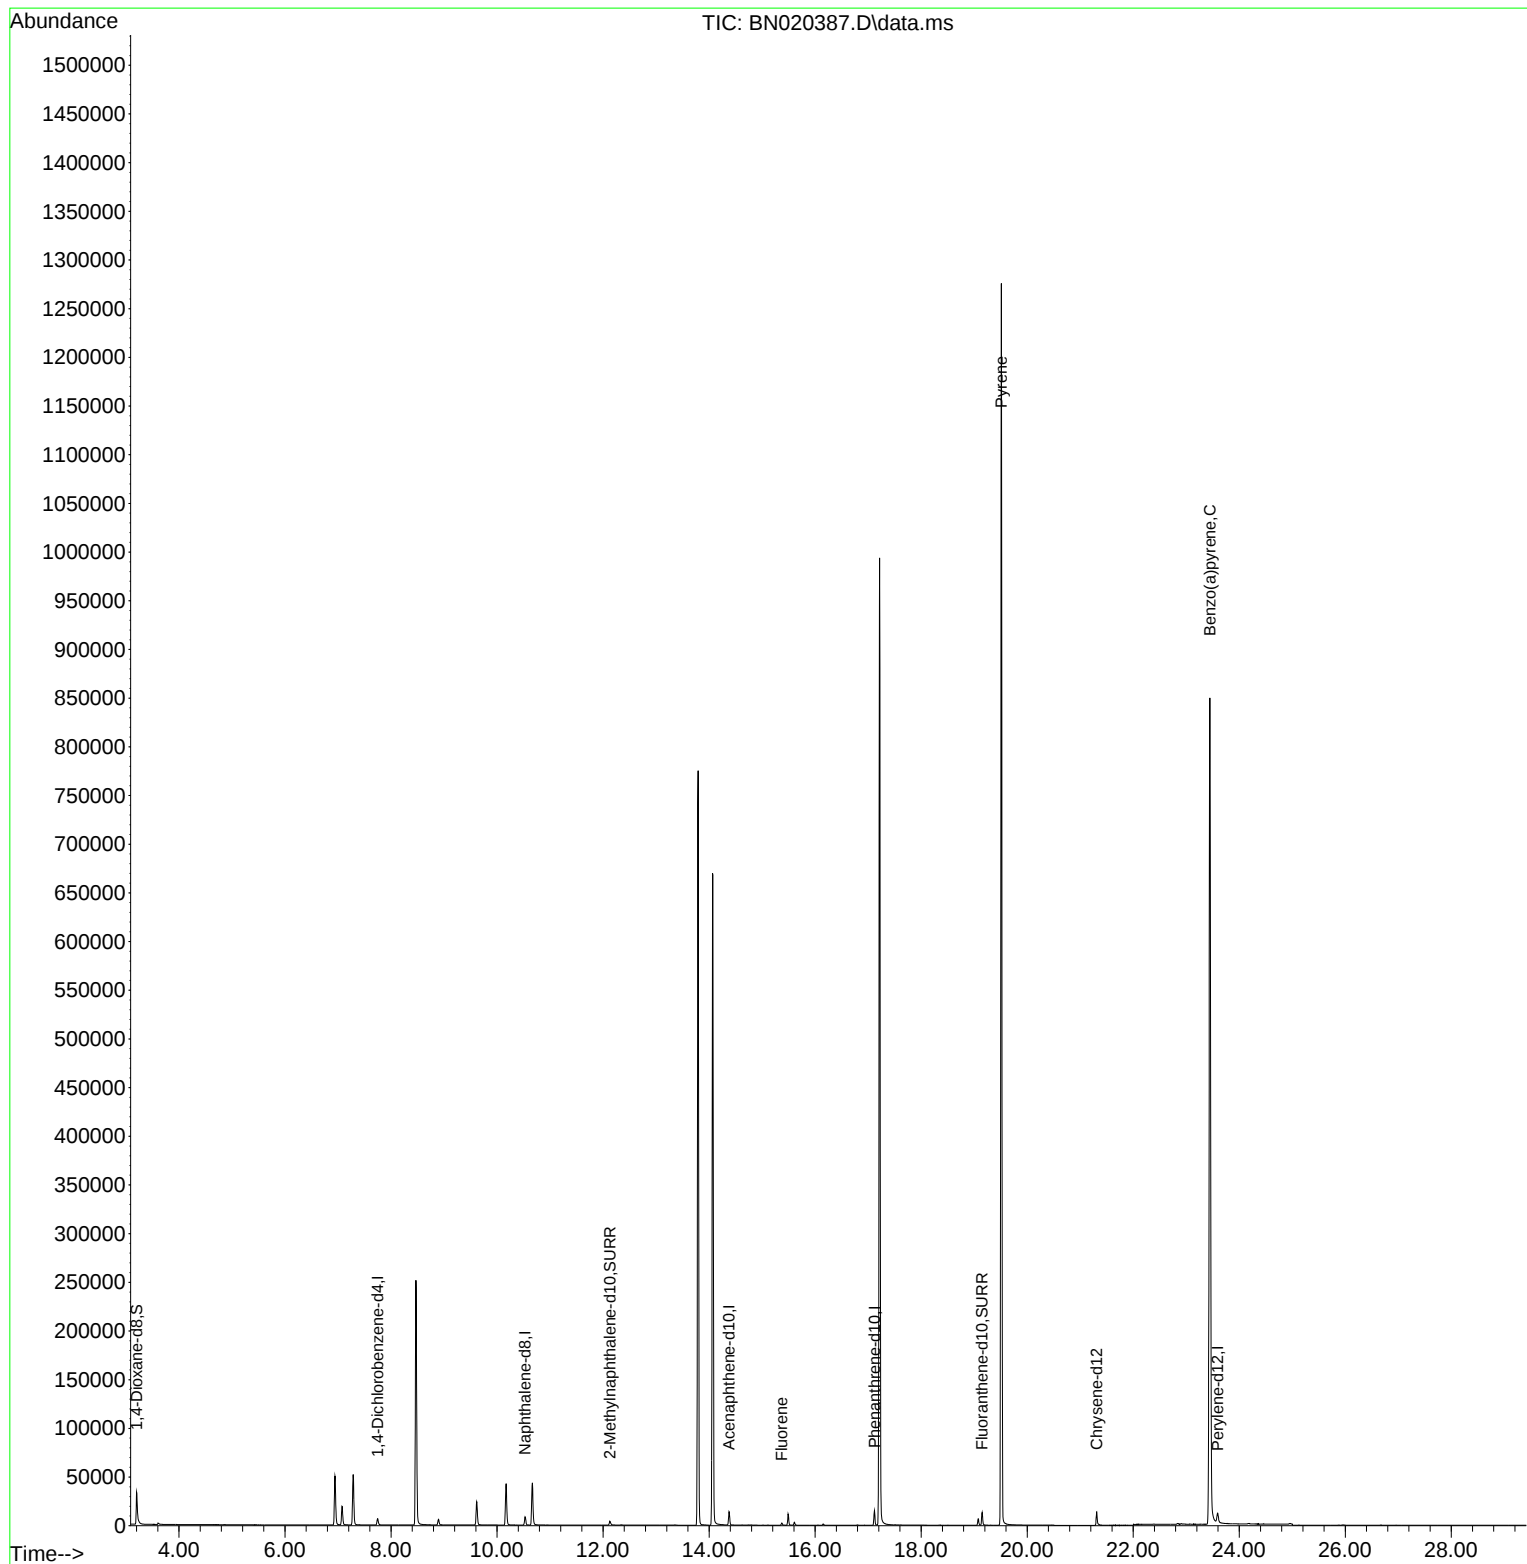


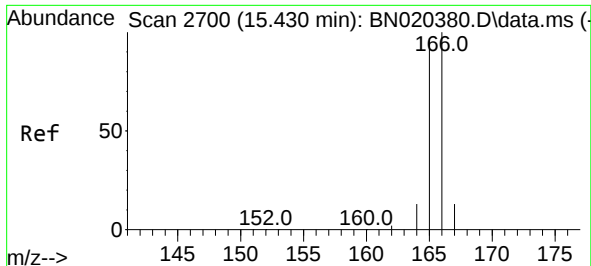


#12
Fluorene
Concen: 0.056 ng/ul
RT: 15.370 min Scan# 2687
Delta R.T. -0.060 min
Lab File: BN020387.D
Acq: 24 Jun 2022 08:47

Instrument :
BNA_N
ClientSampleId :



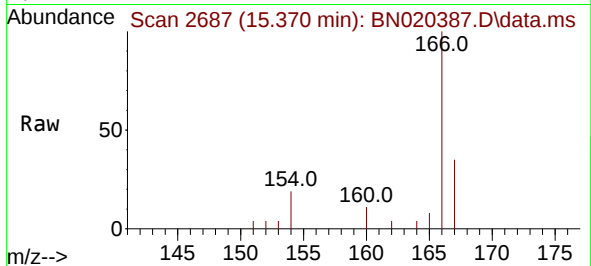



Tgt Ion:166 Resp: 1993
Ion Ratio Lower Upper
166 100
165 7.6 78.2 117.2#
167 34.6 11.3 16.9#

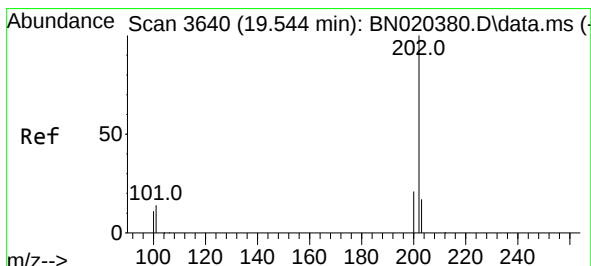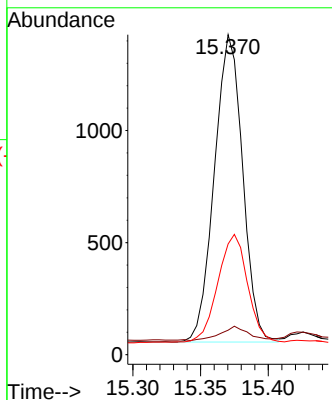

#20
Pyrene
Concen: 0.028 ng/ul
RT: 19.511 min Scan# 3633
Delta R.T. -0.032 min
Lab File: BN020387.D
Acq: 24 Jun 2022 08:47

Tgt Ion:202 Resp: 2033
Ion Ratio Lower Upper
202 100
101 182.8 11.6 17.4#
100 1328.7 9.2 13.8#

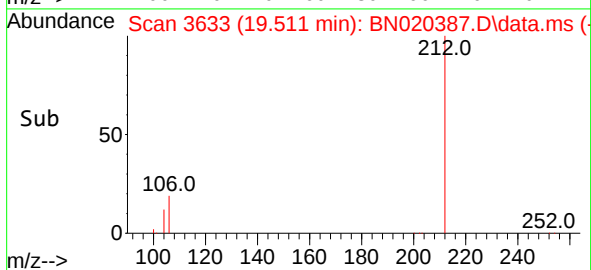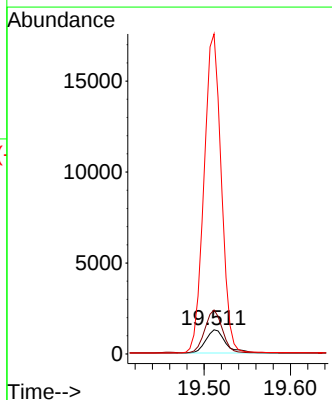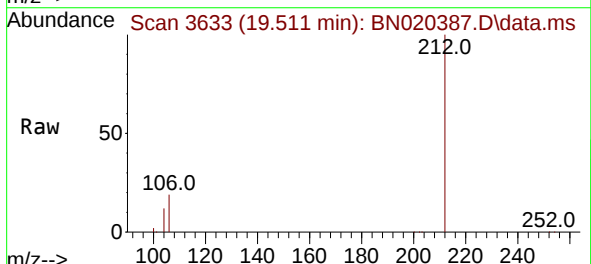

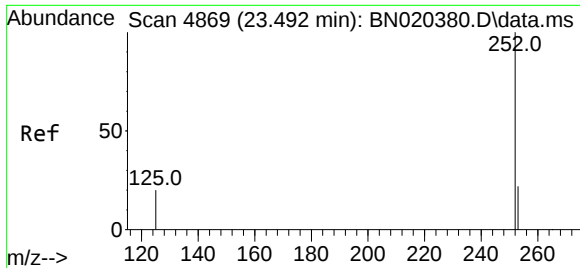

#26

Benzo(a)pyrene

Concen: 0.070 ng/ul

RT: 23.446 min Scan# 41

Delta R.T. -0.047 min


Lab File: BN020387.D

Acq: 24 Jun 2022 08:47

Instrument :

BNA_N

ClientSampleId :

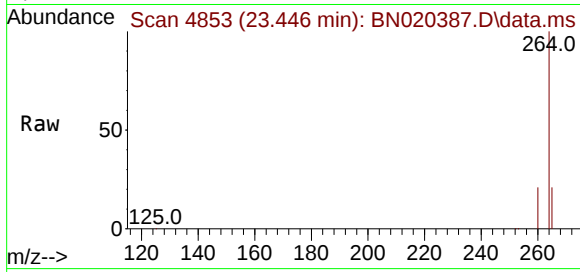

Tgt Ion:252 Resp: 4549

Ion Ratio Lower Upper

252 100

253 40.3 21.0 31.4#

125 33.2 18.8 28.2#

