

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020389.D
 Acq On : 24 Jun 2022 09:59
 Operator : CG/JU
 Sample : N3355-20
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 25 00:54:30 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.749	152	2755	0.400	ng/ul	0.00
4) Naphthalene-d8	10.535	136	9444	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.377	164	6251	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.120	188	14042	0.400	ng/ul	0.00
17) Chrysene-d12	21.312	240	12599	0.400	ng/ul	0.00
23) Perylene-d12	23.595	264	12805	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	13238	4.148	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.129	152	4840	0.312	ng/ul	0.00
18) Fluoranthene-d10	19.151	212	13941	0.336	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.371	166	1735	0.062	ng/ul#	14
20) Pyrene	19.513	202	1728	0.029	ng/ul#	1
26) Benzo(a)pyrene	23.446	252	3990	0.074	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
Data File : BN020389.D
Acq On : 24 Jun 2022 09:59
Operator : CG/JU
Sample : N3355-20
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Jun 25 00:54:30 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:17:34 2022
Response via : Initial Calibration

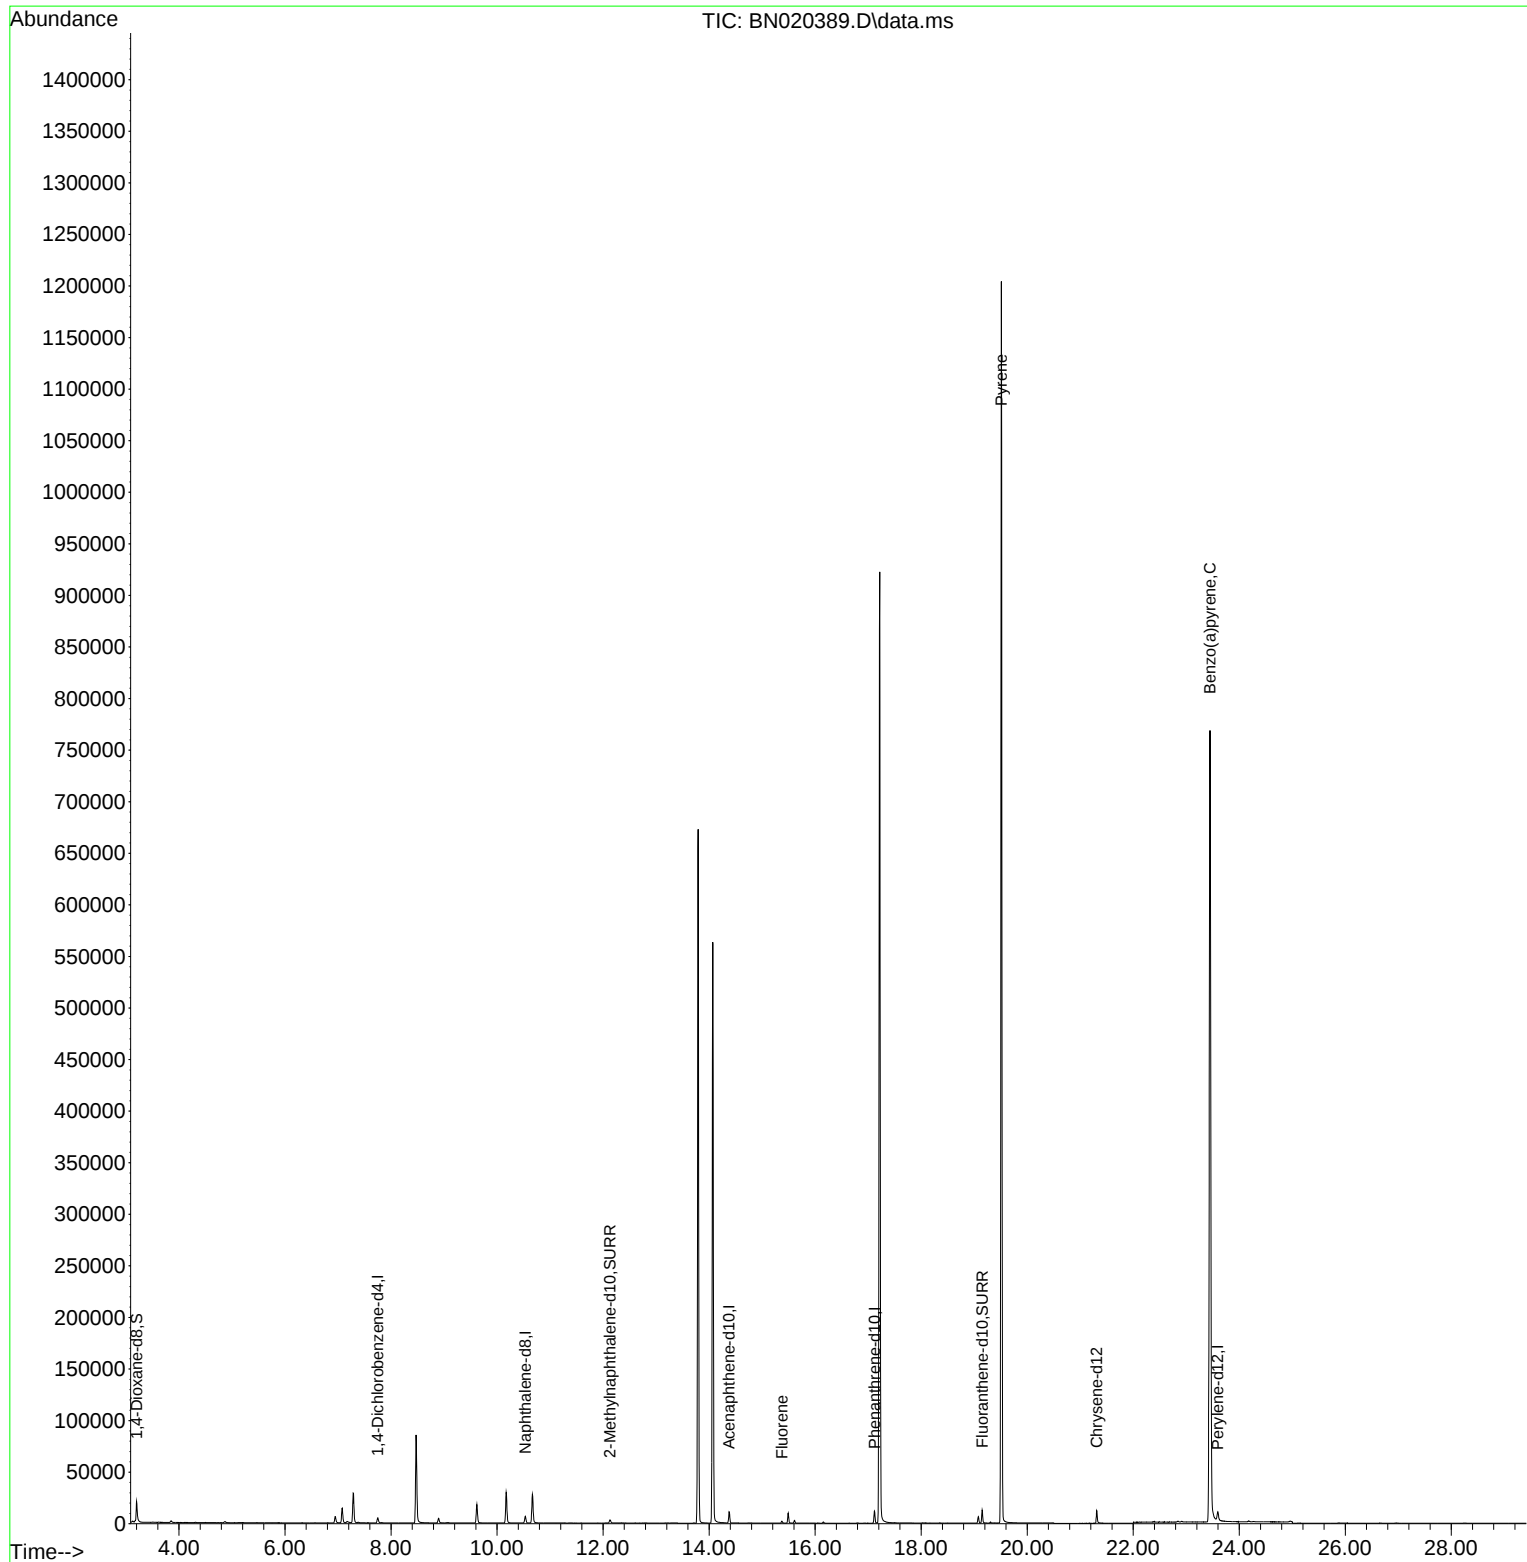



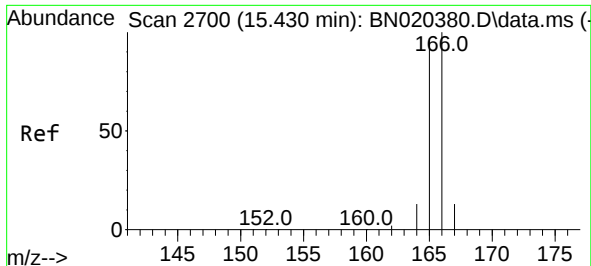


#12
Fluorene
Concen: 0.062 ng/ul
RT: 15.371 min Scan# 2687
Delta R.T. -0.059 min
Lab File: BN020389.D
Acq: 24 Jun 2022 09:59

Instrument :
BNA_N
ClientSampleId :



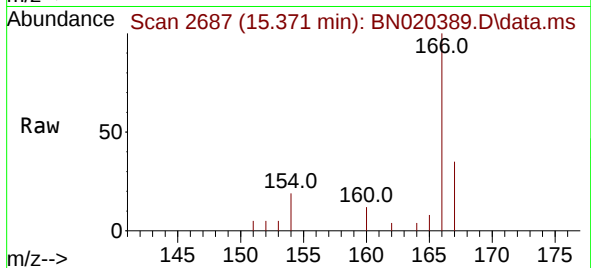



Tgt Ion:166 Resp: 1735
Ion Ratio Lower Upper
166 100
165 8.3 78.2 117.2#
167 35.0 11.3 16.9#

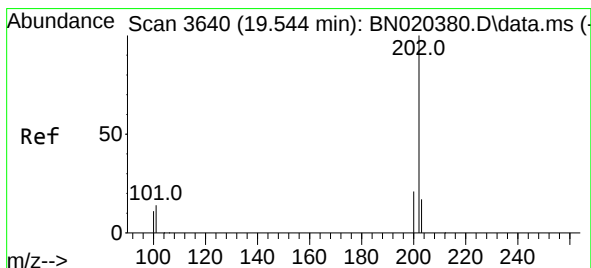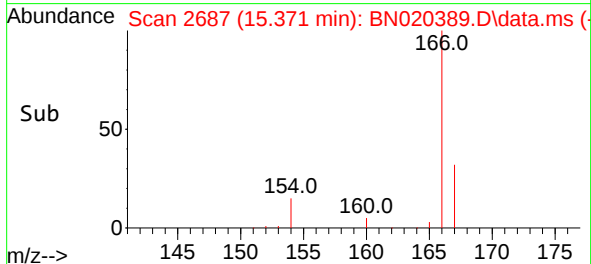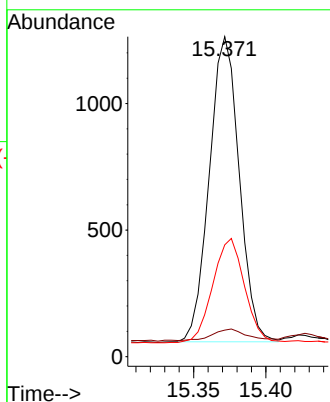

#20
Pyrene
Concen: 0.029 ng/ul
RT: 19.513 min Scan# 3633
Delta R.T. -0.031 min
Lab File: BN020389.D
Acq: 24 Jun 2022 09:59


Tgt Ion:202 Resp: 1728
Ion Ratio Lower Upper
202 100
101 171.8 11.6 17.4#
100 1251.3 9.2 13.8#

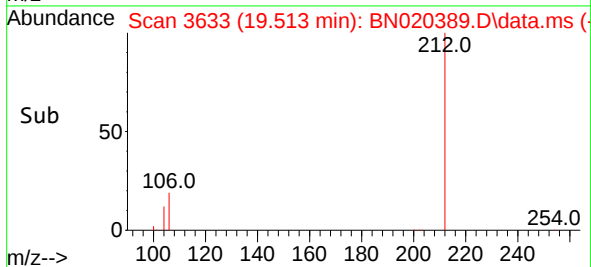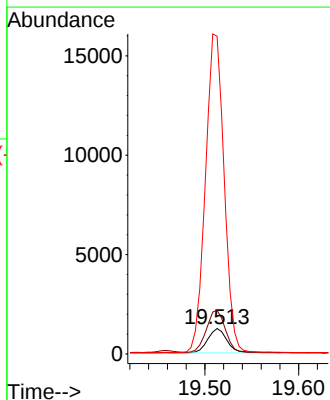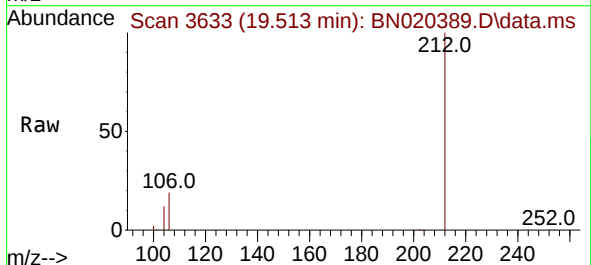

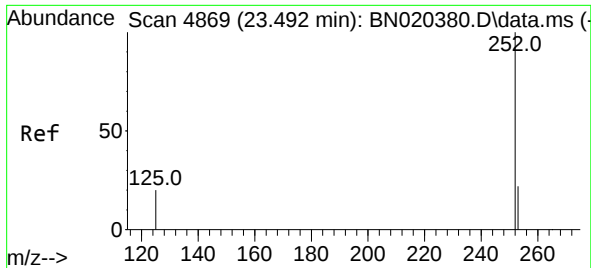

#26
Benzo(a)pyrene
Concen: 0.074 ng/ul
RT: 23.446 min Scan# 4853
Delta R.T. -0.047 min
Lab File: BN020389.D
Acq: 24 Jun 2022 09:59

Instrument :
BNA_N
ClientSampleId :

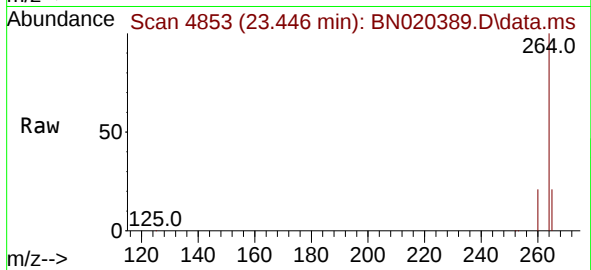

Tgt Ion:252 Resp: 3990
Ion Ratio Lower Upper
252 100
253 42.6 21.0 31.4#
125 35.3 18.8 28.2#

