

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020397.D
 Acq On : 24 Jun 2022 14:48
 Operator : CG/JU
 Sample : N3401-15
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 25 00:54:59 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.750	152	2640	0.400	ng/ul	0.00
4) Naphthalene-d8	10.535	136	9377	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.382	164	6404	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.120	188	14202	0.400	ng/ul	0.00
17) Chrysene-d12	21.312	240	13230	0.400	ng/ul	0.00
23) Perylene-d12	23.592	264	13356	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	14303	4.677	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.130	152	6157	0.400	ng/ul	0.00
18) Fluoranthene-d10	19.151	212	16533	0.379	ng/ul	0.00
Target Compounds						Qvalue
12) Fluorene	15.372	166	2082	0.072	ng/ul#	15
20) Pyrene	19.518	202	2121	0.034	ng/ul#	1
26) Benzo(a)pyrene	23.452	252	4628	0.082	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
Data File : BN020397.D
Acq On : 24 Jun 2022 14:48
Operator : CG/JU
Sample : N3401-15
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 25 00:54:59 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:17:34 2022
Response via : Initial Calibration




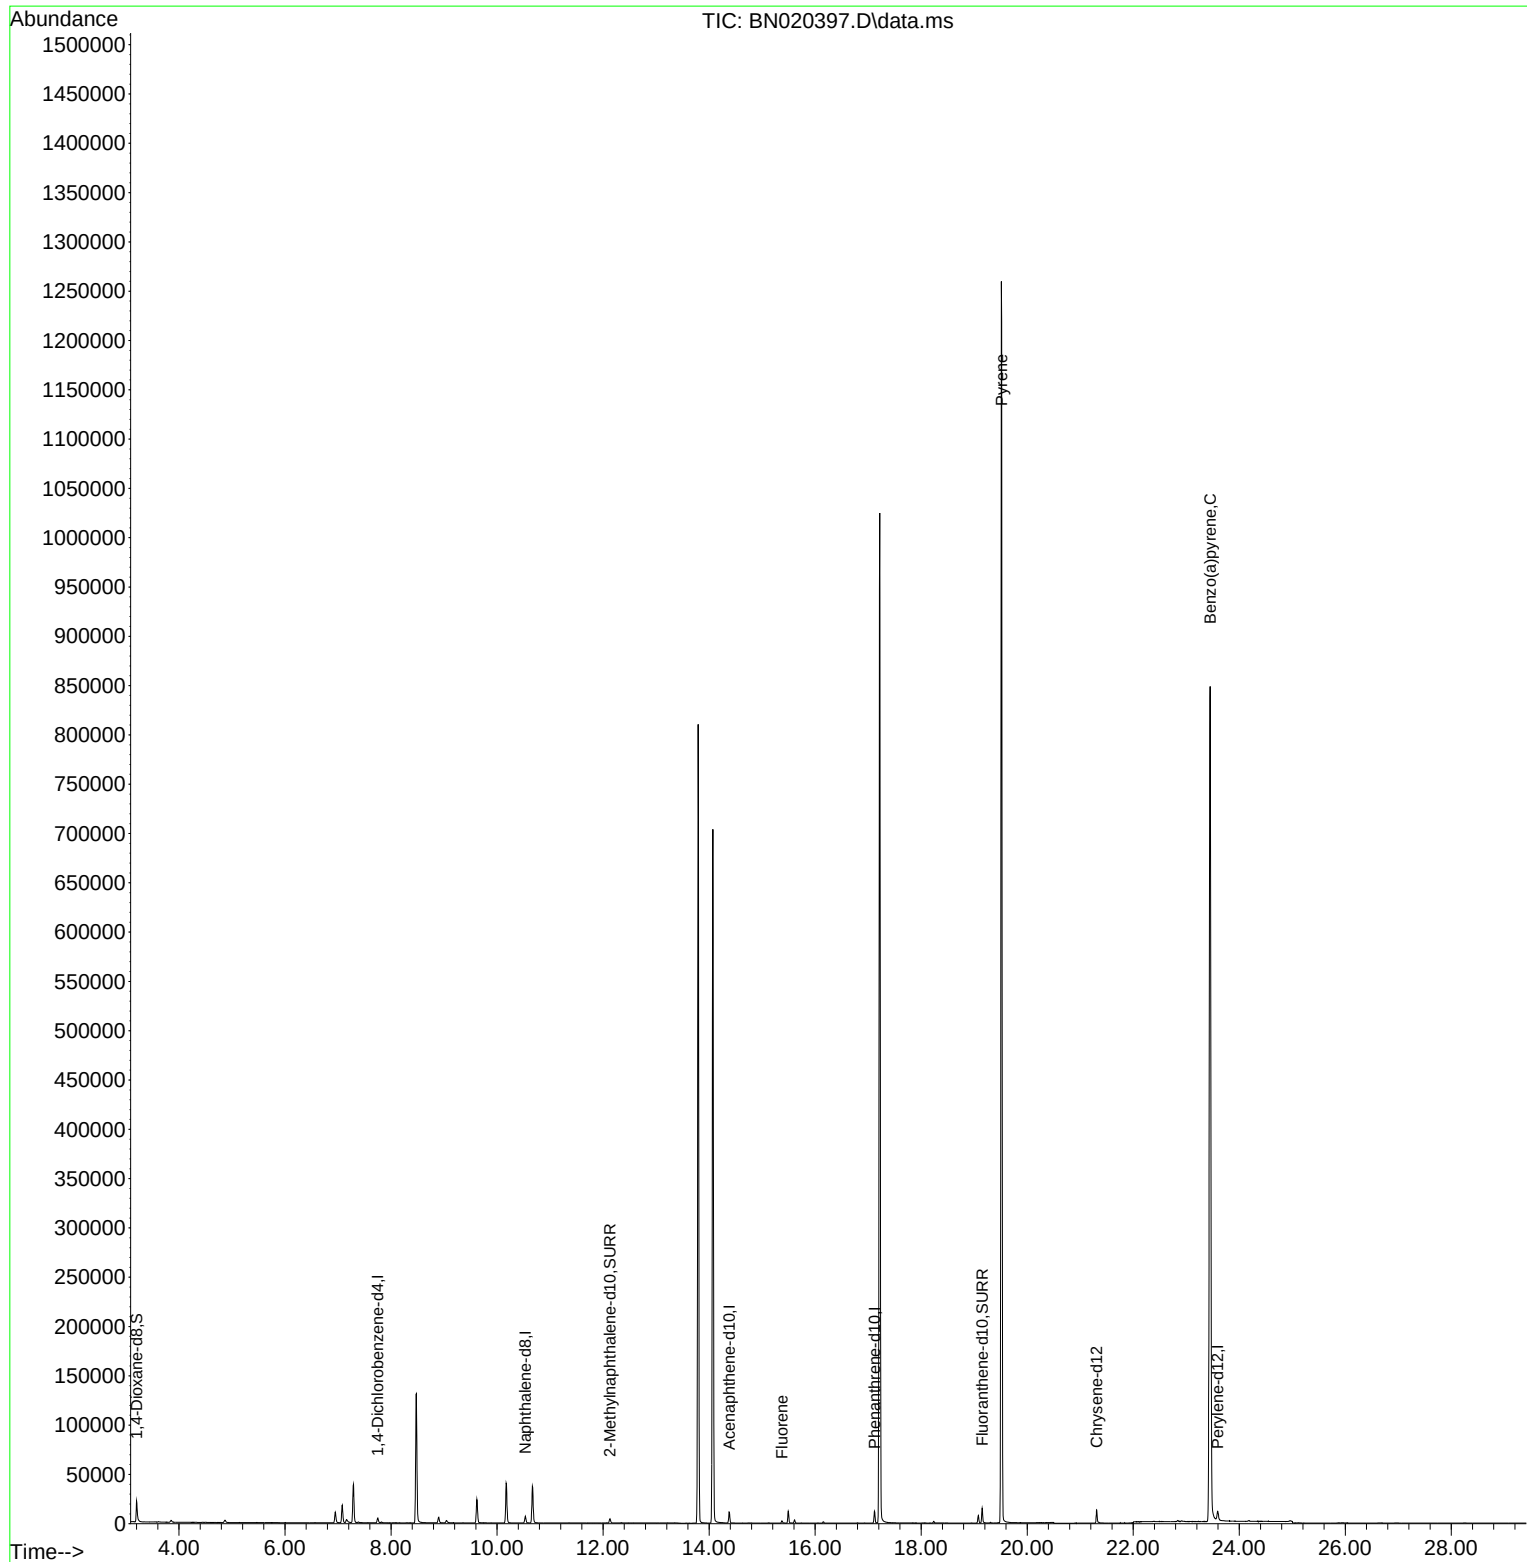


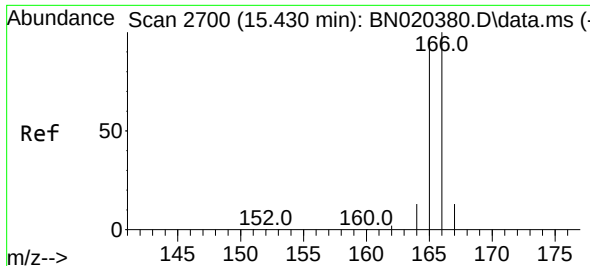

#12
Fluorene
Concen: 0.072 ng/ul
RT: 15.372 min Scan# 2082
Delta R.T. -0.059 min
Lab File: BN020397.D
Acq: 24 Jun 2022 14:48




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:166 Resp: 2082
Ion Ratio Lower Upper
166 100
165 8.2 78.2 117.2#
167 33.6 11.3 16.9#

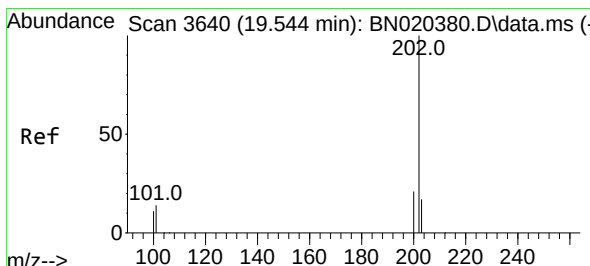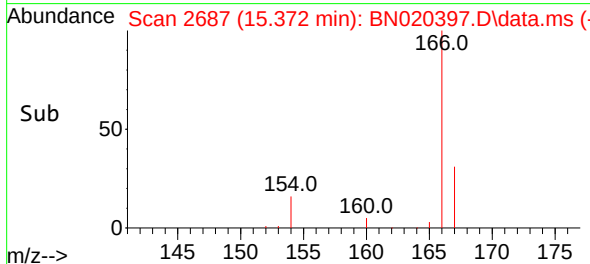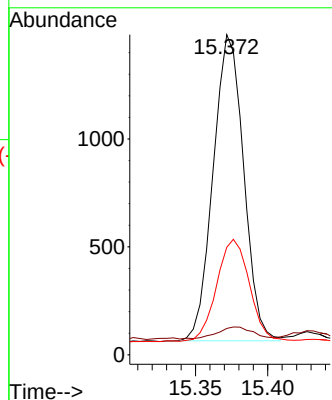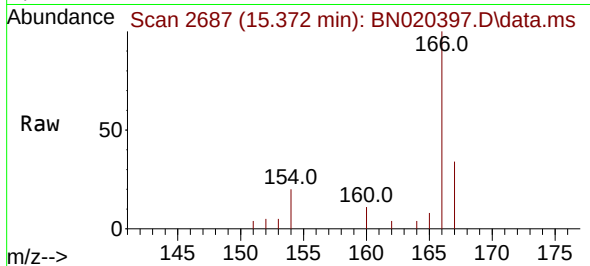

#20
Pyrene
Concen: 0.034 ng/ul
RT: 19.518 min Scan# 3634
Delta R.T. -0.026 min
Lab File: BN020397.D
Acq: 24 Jun 2022 14:48

Tgt Ion:202 Resp: 2121
Ion Ratio Lower Upper
202 100
101 162.6 11.6 17.4#
100 1105.7 9.2 13.8#

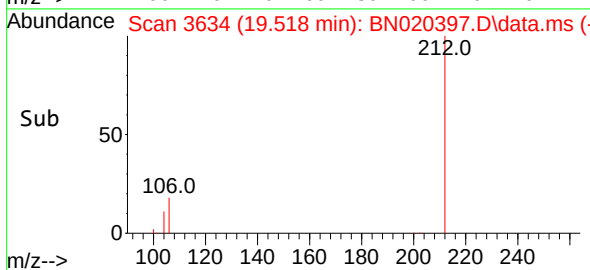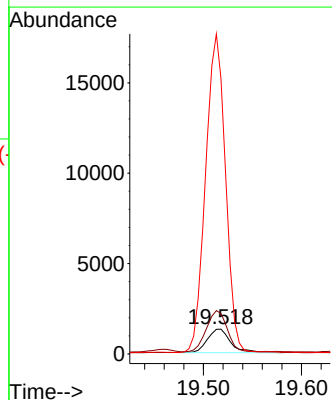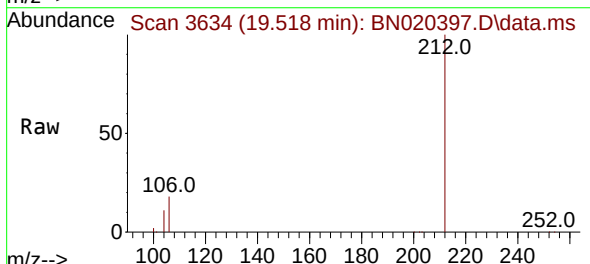

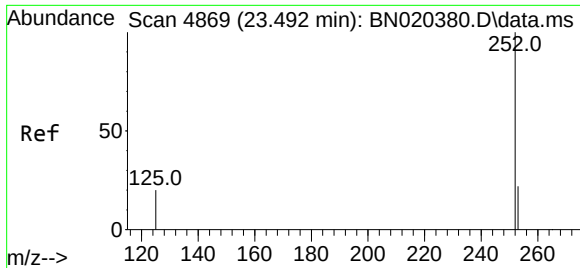

#26

Benzo(a)pyrene

Concen: 0.082 ng/ul

RT: 23.452 min Scan# 41

Delta R.T. -0.041 min


Lab File: BN020397.D

Acq: 24 Jun 2022 14:48

Instrument :

BNA_N

ClientSampleId :

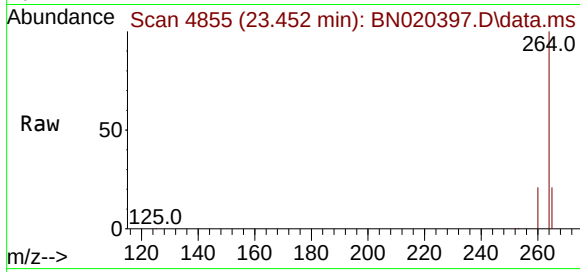

Tgt Ion:252 Resp: 4628

Ion Ratio Lower Upper

252 100

253 45.5 21.0 31.4#

125 38.8 18.8 28.2#

