

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020398.D
 Acq On : 24 Jun 2022 15:25
 Operator : CG/JU
 Sample : N3401-16
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 25 00:55:02 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.750	152	3193	0.400	ng/ul	0.00
4) Naphthalene-d8	10.535	136	11055	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.382	164	7882	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.120	188	16933	0.400	ng/ul	0.00
17) Chrysene-d12	21.308	240	14925	0.400	ng/ul	0.00
23) Perylene-d12	23.591	264	14717	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	16174	4.372	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.130	152	6279	0.346	ng/ul	0.00
18) Fluoranthene-d10	19.151	212	16645	0.338	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.513	202	2108	0.030	ng/ul#	1
26) Benzo(a)pyrene	23.444	252	4575	0.074	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
Data File : BN020398.D
Acq On : 24 Jun 2022 15:25
Operator : CG/JU
Sample : N3401-16
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 25 00:55:02 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:17:34 2022
Response via : Initial Calibration




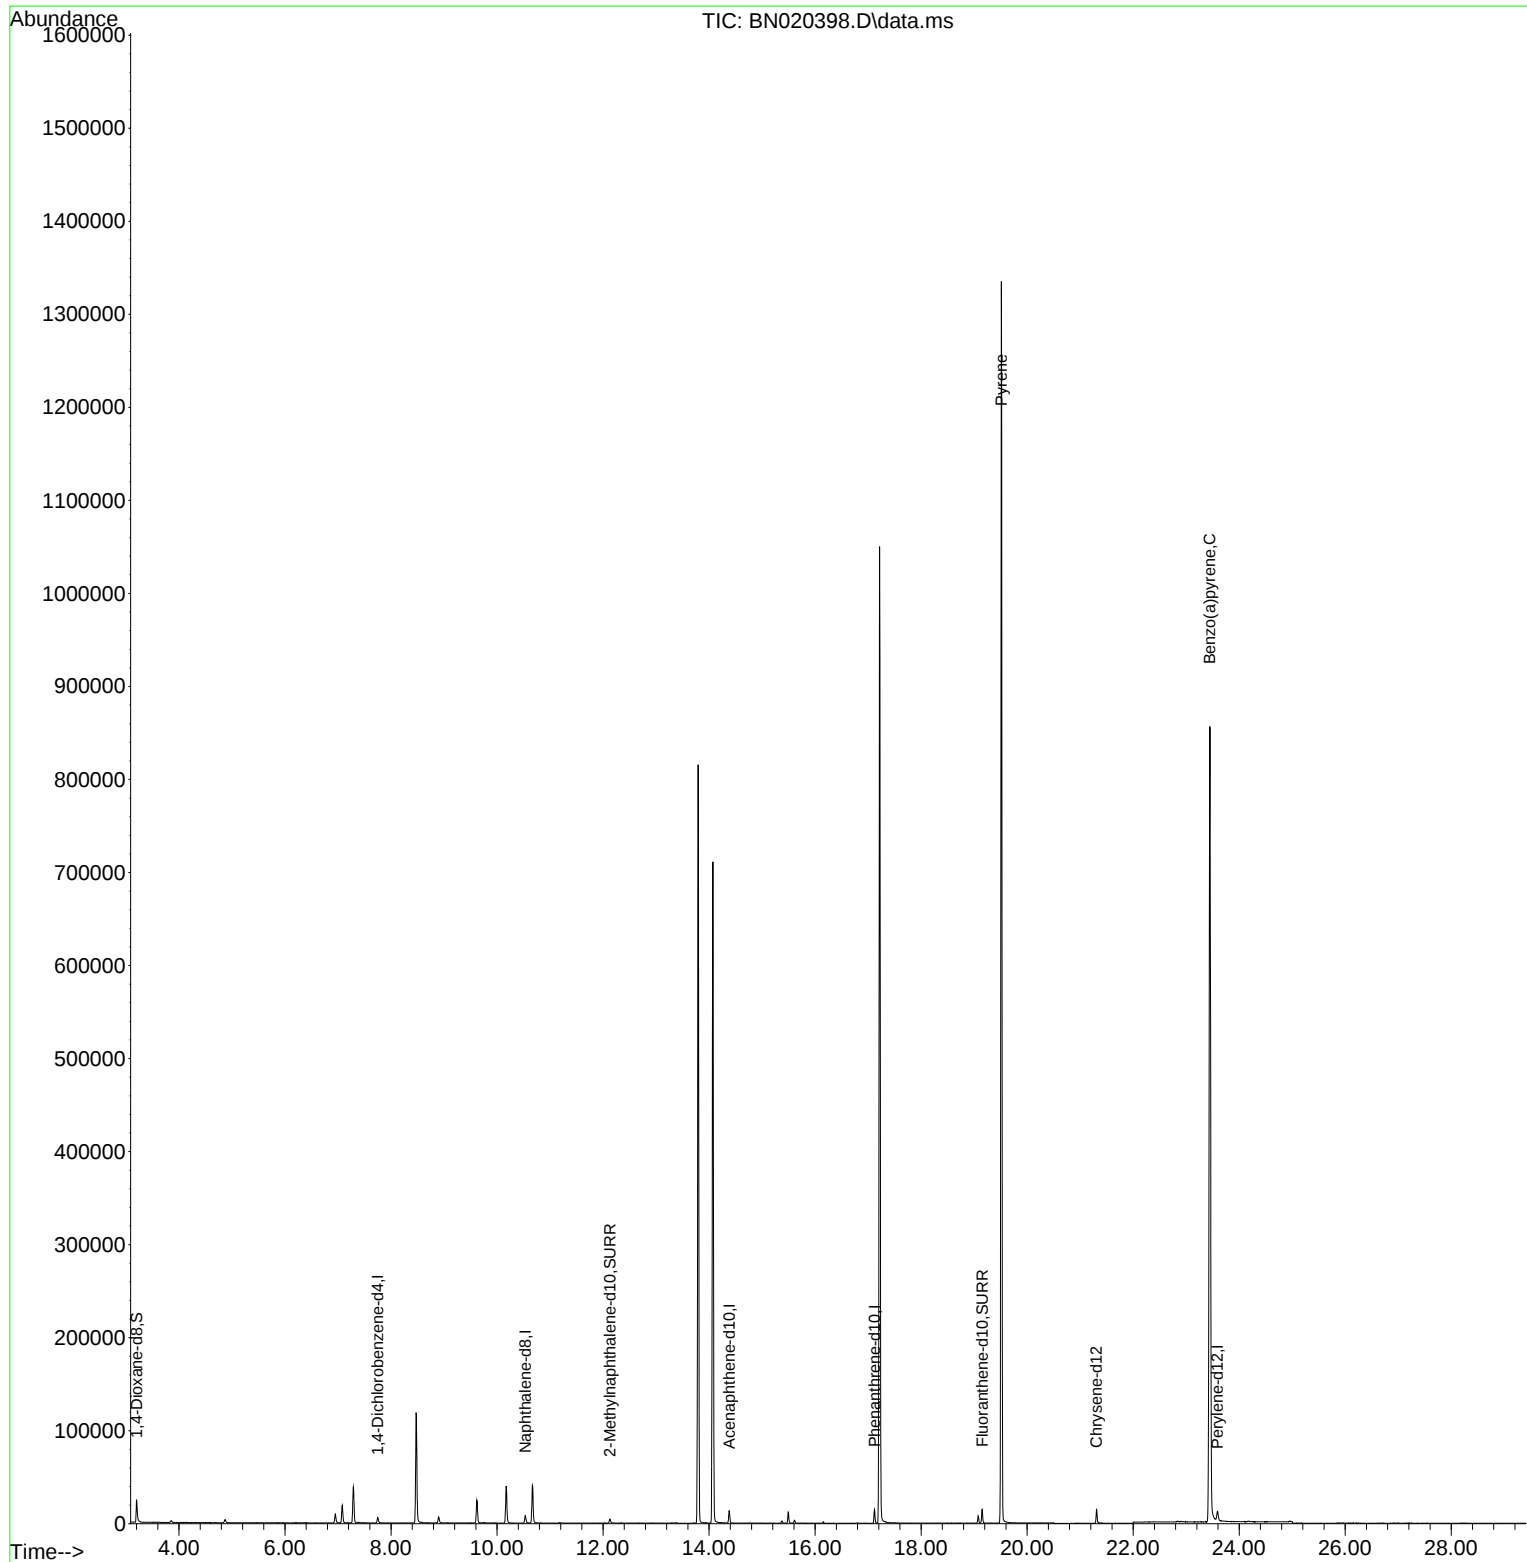


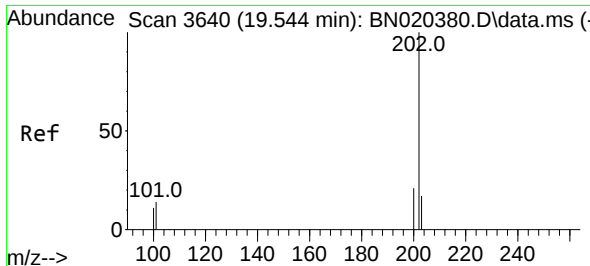

#20
Pyrene
Concen: 0.030 ng/ul
RT: 19.513 min Scan# 30
Delta R.T. -0.031 min
Lab File: BN020398.D
Acq: 24 Jun 2022 15:25

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:202 Resp: 2108
Ion Ratio Lower Upper
202 100
101 173.1 11.6 17.4#
100 1259.8 9.2 13.8#

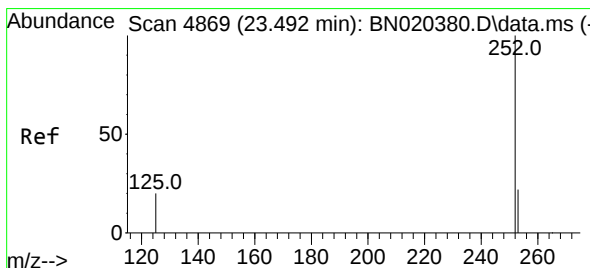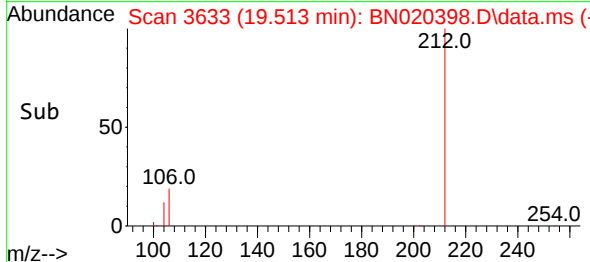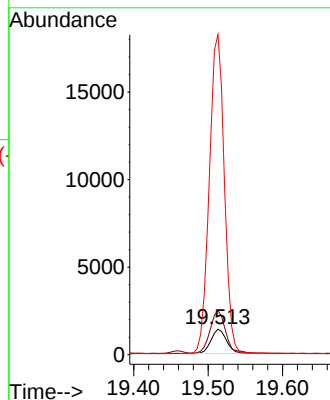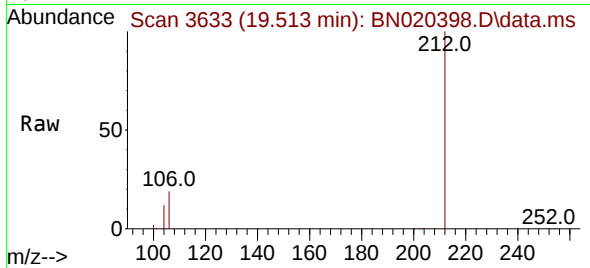

#26
Benzo(a)pyrene
Concen: 0.074 ng/ul
RT: 23.444 min Scan# 4852
Delta R.T. -0.048 min
Lab File: BN020398.D
Acq: 24 Jun 2022 15:25

Tgt Ion:252 Resp: 4575
Ion Ratio Lower Upper
252 100
253 42.8 21.0 31.4#
125 35.2 18.8 28.2#

