

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020405.D
 Acq On : 24 Jun 2022 20:18
 Operator : CG/JU
 Sample : PB145725BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 25 00:55:32 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.750	152	2973	0.400	ng/ul	0.00
4) Naphthalene-d8	10.535	136	10132	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.382	164	6730	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.120	188	15015	0.400	ng/ul	0.00
17) Chrysene-d12	21.311	240	12662	0.400	ng/ul	0.00
23) Perylene-d12	23.594	264	12459	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	20975	6.090	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.135	152	5569	0.335	ng/ul	0.00
18) Fluoranthene-d10	19.151	212	14406	0.345	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.513	202	1943	0.032	ng/ul#	1
26) Benzo(a)pyrene	23.445	252	4080	0.078	ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
Data File : BN020405.D
Acq On : 24 Jun 2022 20:18
Operator : CG/JU
Sample : PB145725BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 25 00:55:32 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:17:34 2022
Response via : Initial Calibration




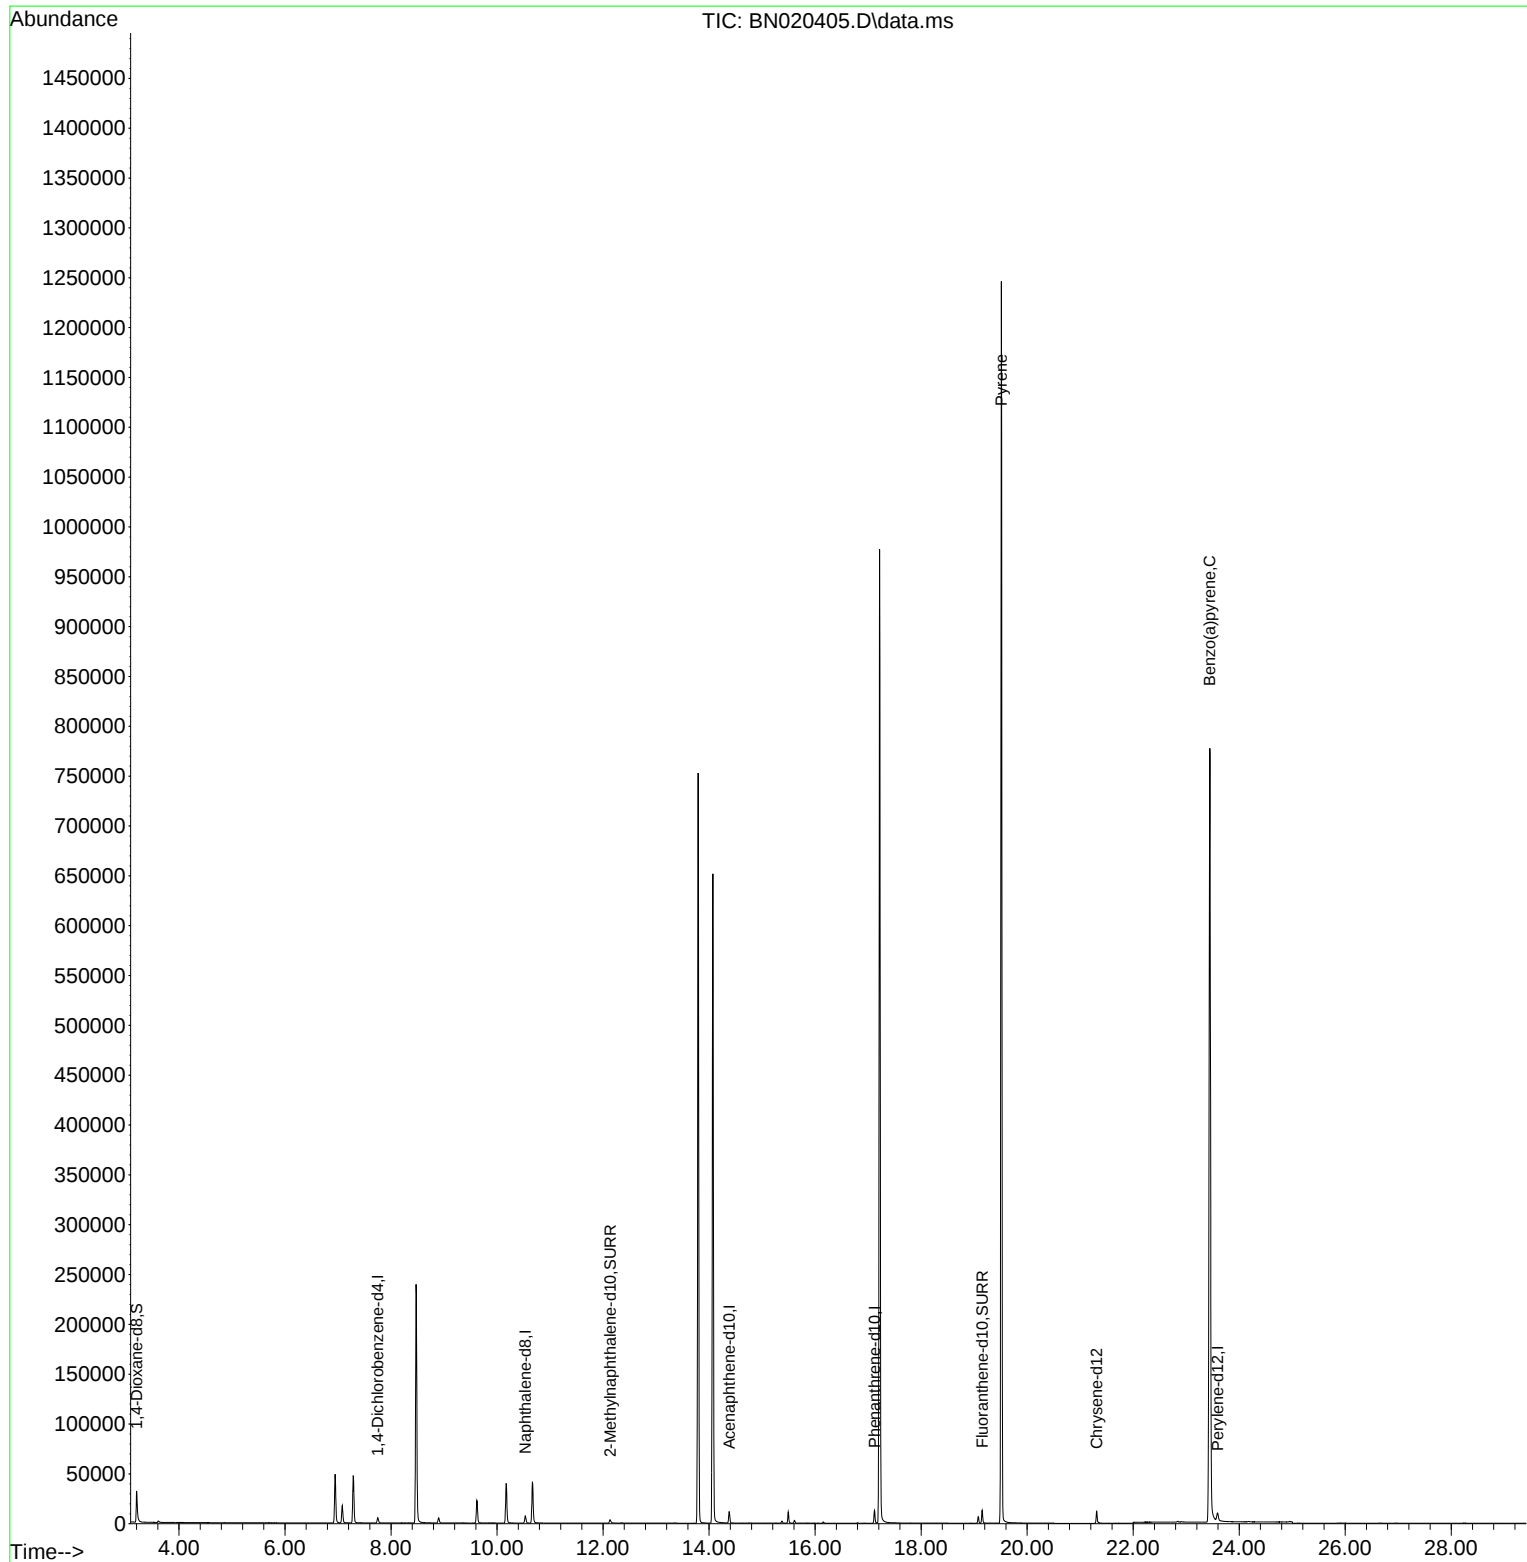


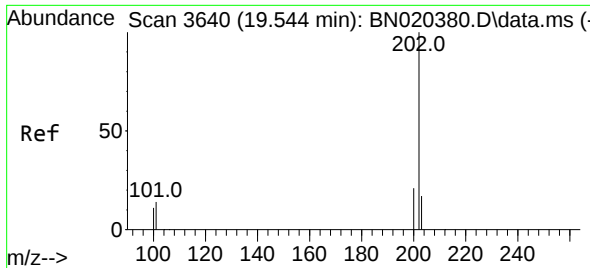

#20
Pyrene
Concen: 0.032 ng/ul
RT: 19.513 min Scan# 3633
Delta R.T. -0.031 min
Lab File: BN020405.D
Acq: 24 Jun 2022 20:18

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:202 Resp: 1943
Ion Ratio Lower Upper
202 100
101 173.1 11.6 17.4#
100 1270.9 9.2 13.8#

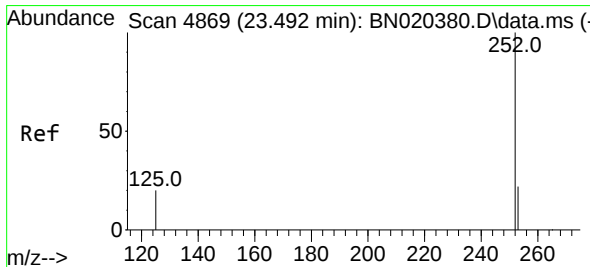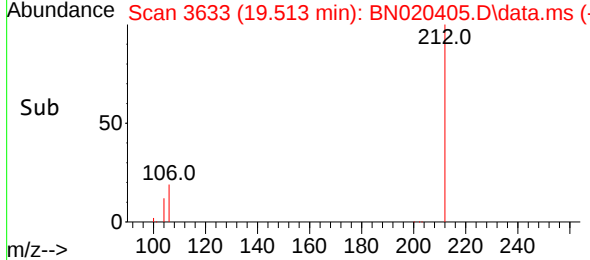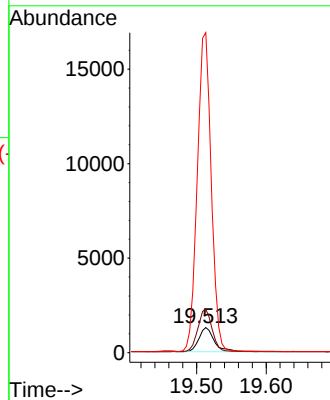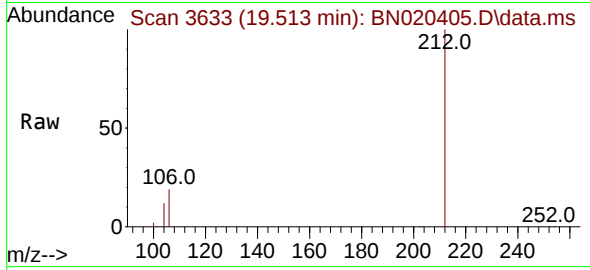

#26
Benzo(a)pyrene
Concen: 0.078 ng/ul
RT: 23.445 min Scan# 4852
Delta R.T. -0.048 min
Lab File: BN020405.D
Acq: 24 Jun 2022 20:18

Tgt Ion:252 Resp: 4080
Ion Ratio Lower Upper
252 100
253 42.0 21.0 31.4#
125 33.1 18.8 28.2#

