

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020422.D
 Acq On : 25 Jun 2022 07:11
 Operator : CG/JU
 Sample : PB145555BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 27 03:41:46 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.750	152	3232	0.400	ng/ul	0.00
4) Naphthalene-d8	10.529	136	11631	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.377	164	7514	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.120	188	16928	0.400	ng/ul	0.00
17) Chrysene-d12	21.309	240	15000	0.400	ng/ul	0.00
23) Perylene-d12	23.592	264	14405	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	21129	5.643	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.130	152	5670	0.297	ng/ul	0.00
18) Fluoranthene-d10	19.151	212	14066	0.284	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.372	166	1839	0.054	ng/ul#	15
20) Pyrene	19.513	202	1748	0.025	ng/ul#	1
26) Benzo(a)pyrene	23.449	252	3739	0.062	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
Data File : BN020422.D
Acq On : 25 Jun 2022 07:11
Operator : CG/JU
Sample : PB145555BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Jun 27 03:41:46 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:17:34 2022
Response via : Initial Calibration

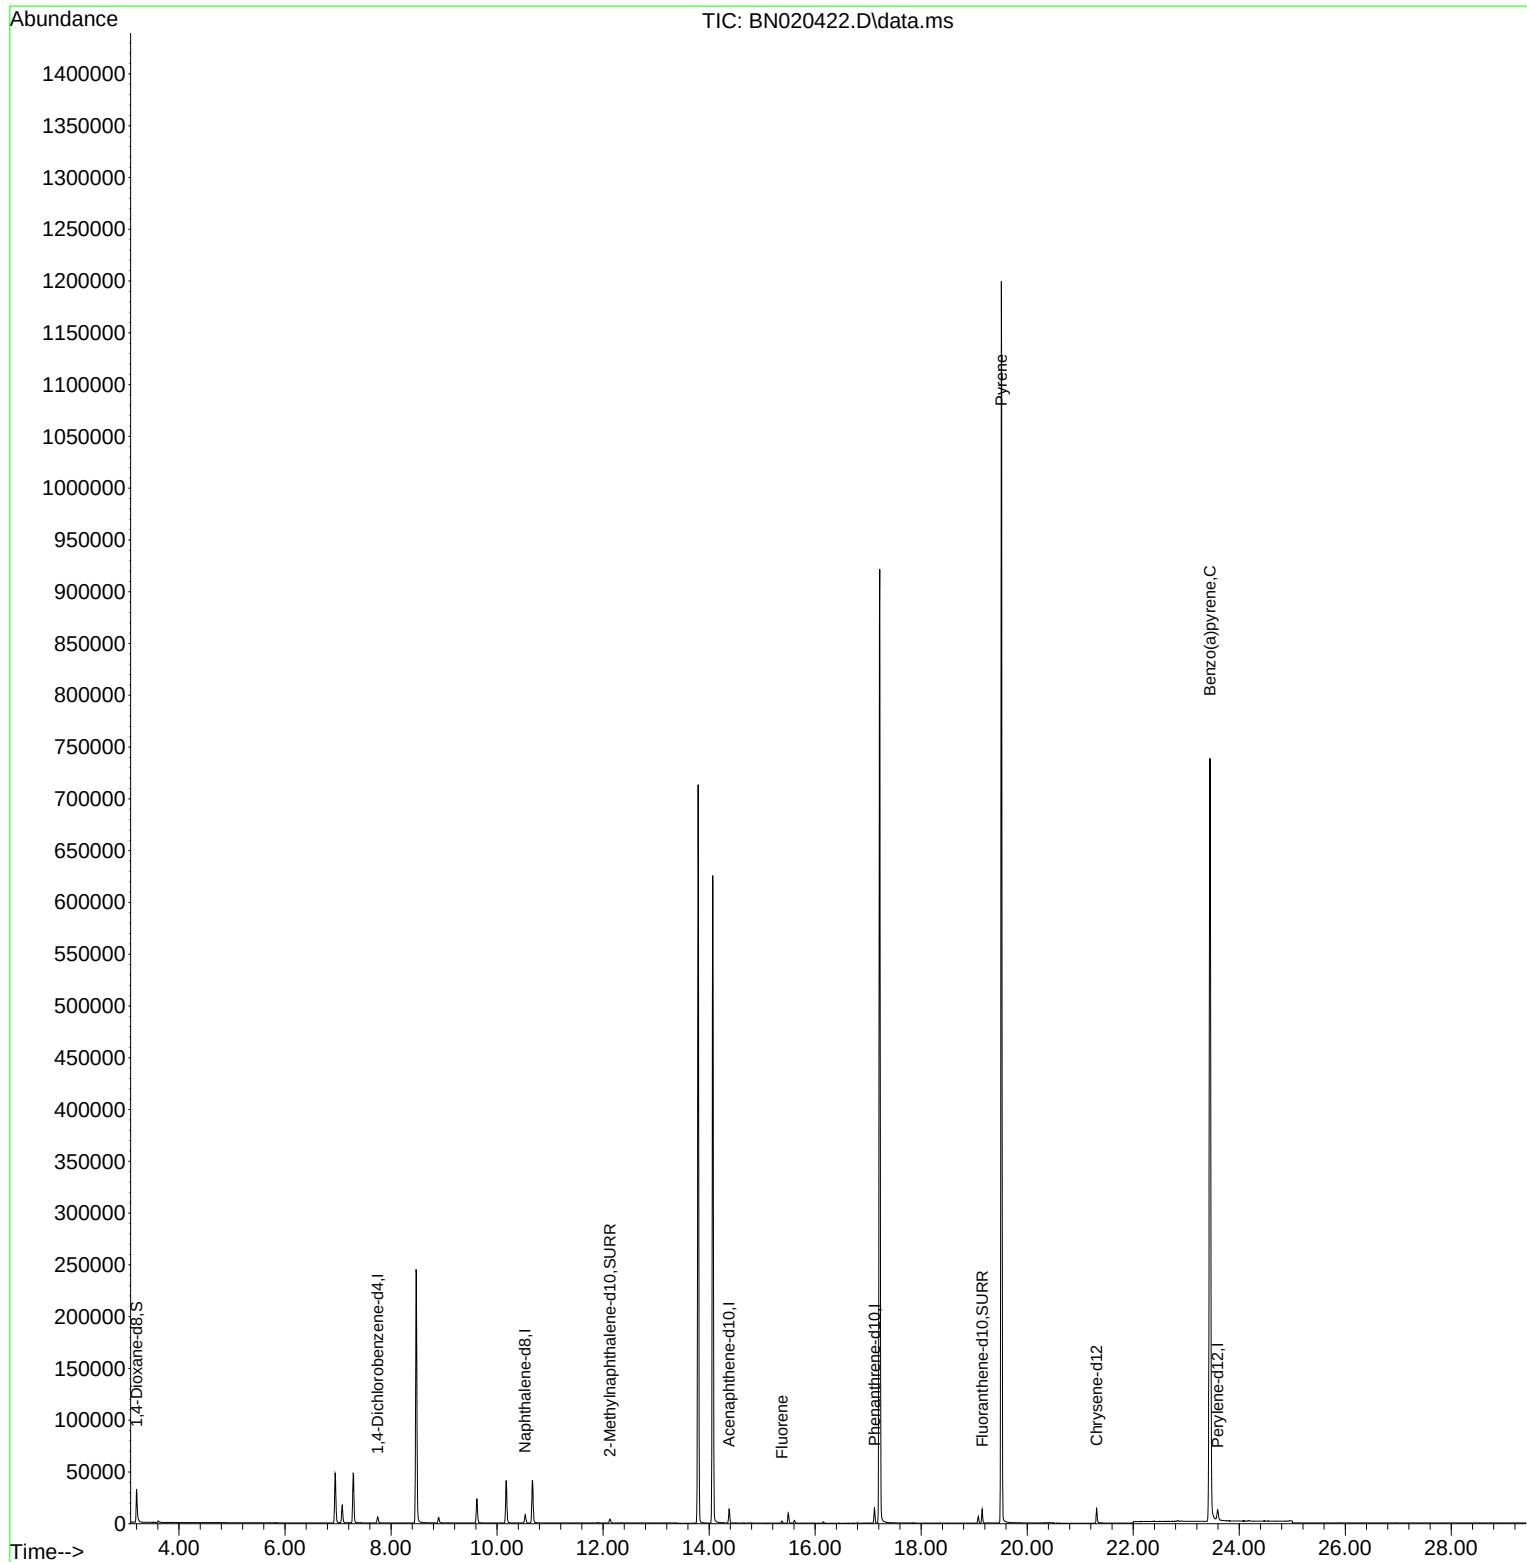



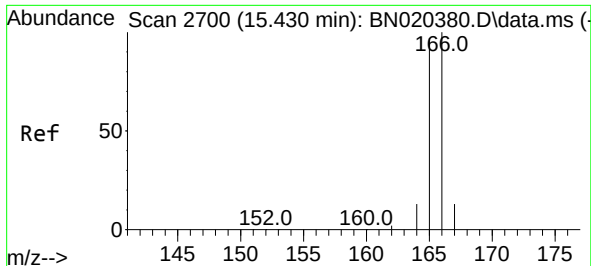


#12
Fluorene
Concen: 0.054 ng/ul
RT: 15.372 min Scan# 2687
Delta R.T. -0.059 min
Lab File: BN020422.D
Acq: 25 Jun 2022 07:11

Instrument :
BNA_N
ClientSampleId :



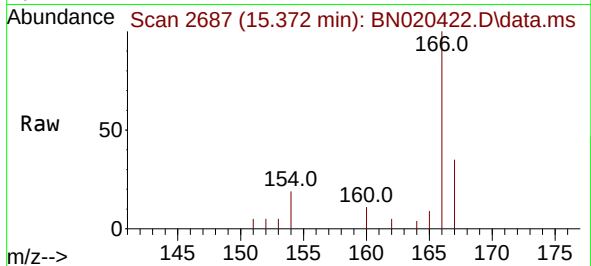



Tgt Ion:166 Resp: 1839
Ion Ratio Lower Upper
166 100
165 8.7 78.2 117.2#
167 35.5 11.3 16.9#

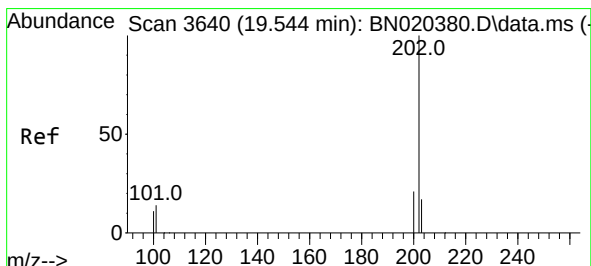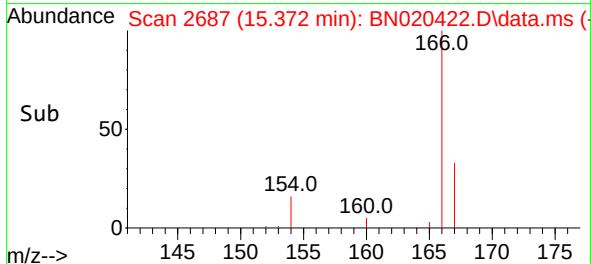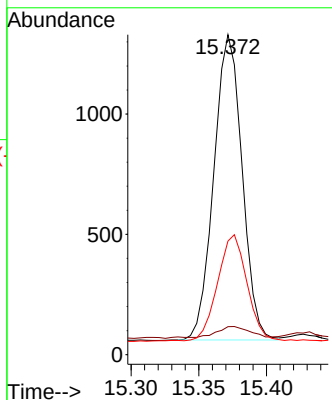

#20
Pyrene
Concen: 0.025 ng/ul
RT: 19.513 min Scan# 3633
Delta R.T. -0.031 min
Lab File: BN020422.D
Acq: 25 Jun 2022 07:11


Tgt Ion:202 Resp: 1748
Ion Ratio Lower Upper
202 100
101 173.2 11.6 17.4#
100 1272.6 9.2 13.8#

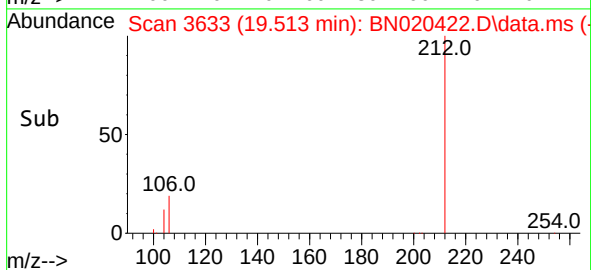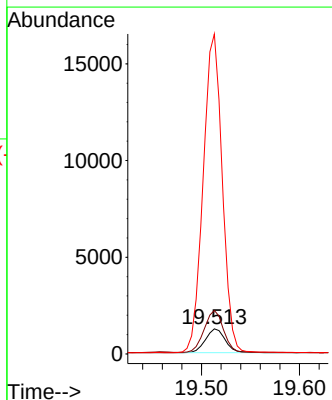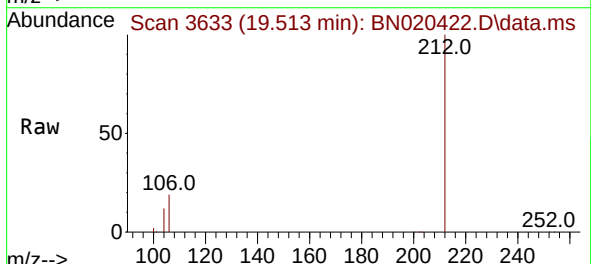

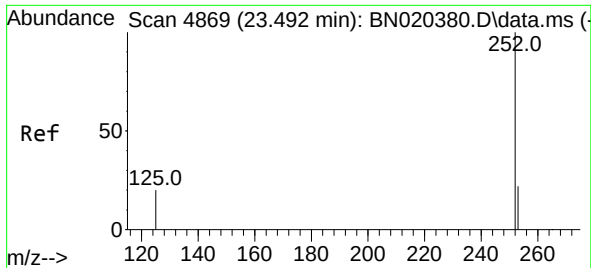

#26
 Benzo(a)pyrene
 Concen: 0.062 ng/ul
 RT: 23.449 min Scan# 4854
 Delta R.T. -0.044 min
 Lab File: BN020422.D
 Acq: 25 Jun 2022 07:11

Instrument :
 BNA_N
 ClientSampleId :

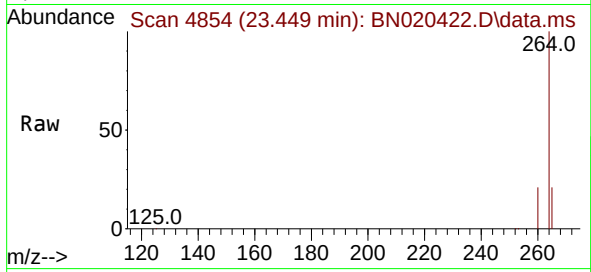

Tgt Ion:252	Resp:	3739
Ion	Ratio	Lower Upper
252	100	
253	46.5	21.0 31.4#
125	37.8	18.8 28.2#

