

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020426.D
 Acq On : 25 Jun 2022 09:36
 Operator : CG/JU
 Sample : PB145678BL
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 27 03:42:05 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.750	152	3079	0.400	ng/ul	0.00
4) Naphthalene-d8	10.533	136	10838	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.380	164	7257	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.119	188	16127	0.400	ng/ul	0.00
17) Chrysene-d12	21.309	240	13460	0.400	ng/ul	0.00
23) Perylene-d12	23.592	264	12398	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	18502	5.187	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.128	152	4989	0.281	ng/ul	0.00
18) Fluoranthene-d10	19.149	212	12502	0.282	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.516	202	1778	0.028	ng/ul#	1
26) Benzo(a)pyrene	23.446	252	3350	0.064	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
Data File : BN020426.D
Acq On : 25 Jun 2022 09:36
Operator : CG/JU
Sample : PB145678BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 27 03:42:05 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:17:34 2022
Response via : Initial Calibration




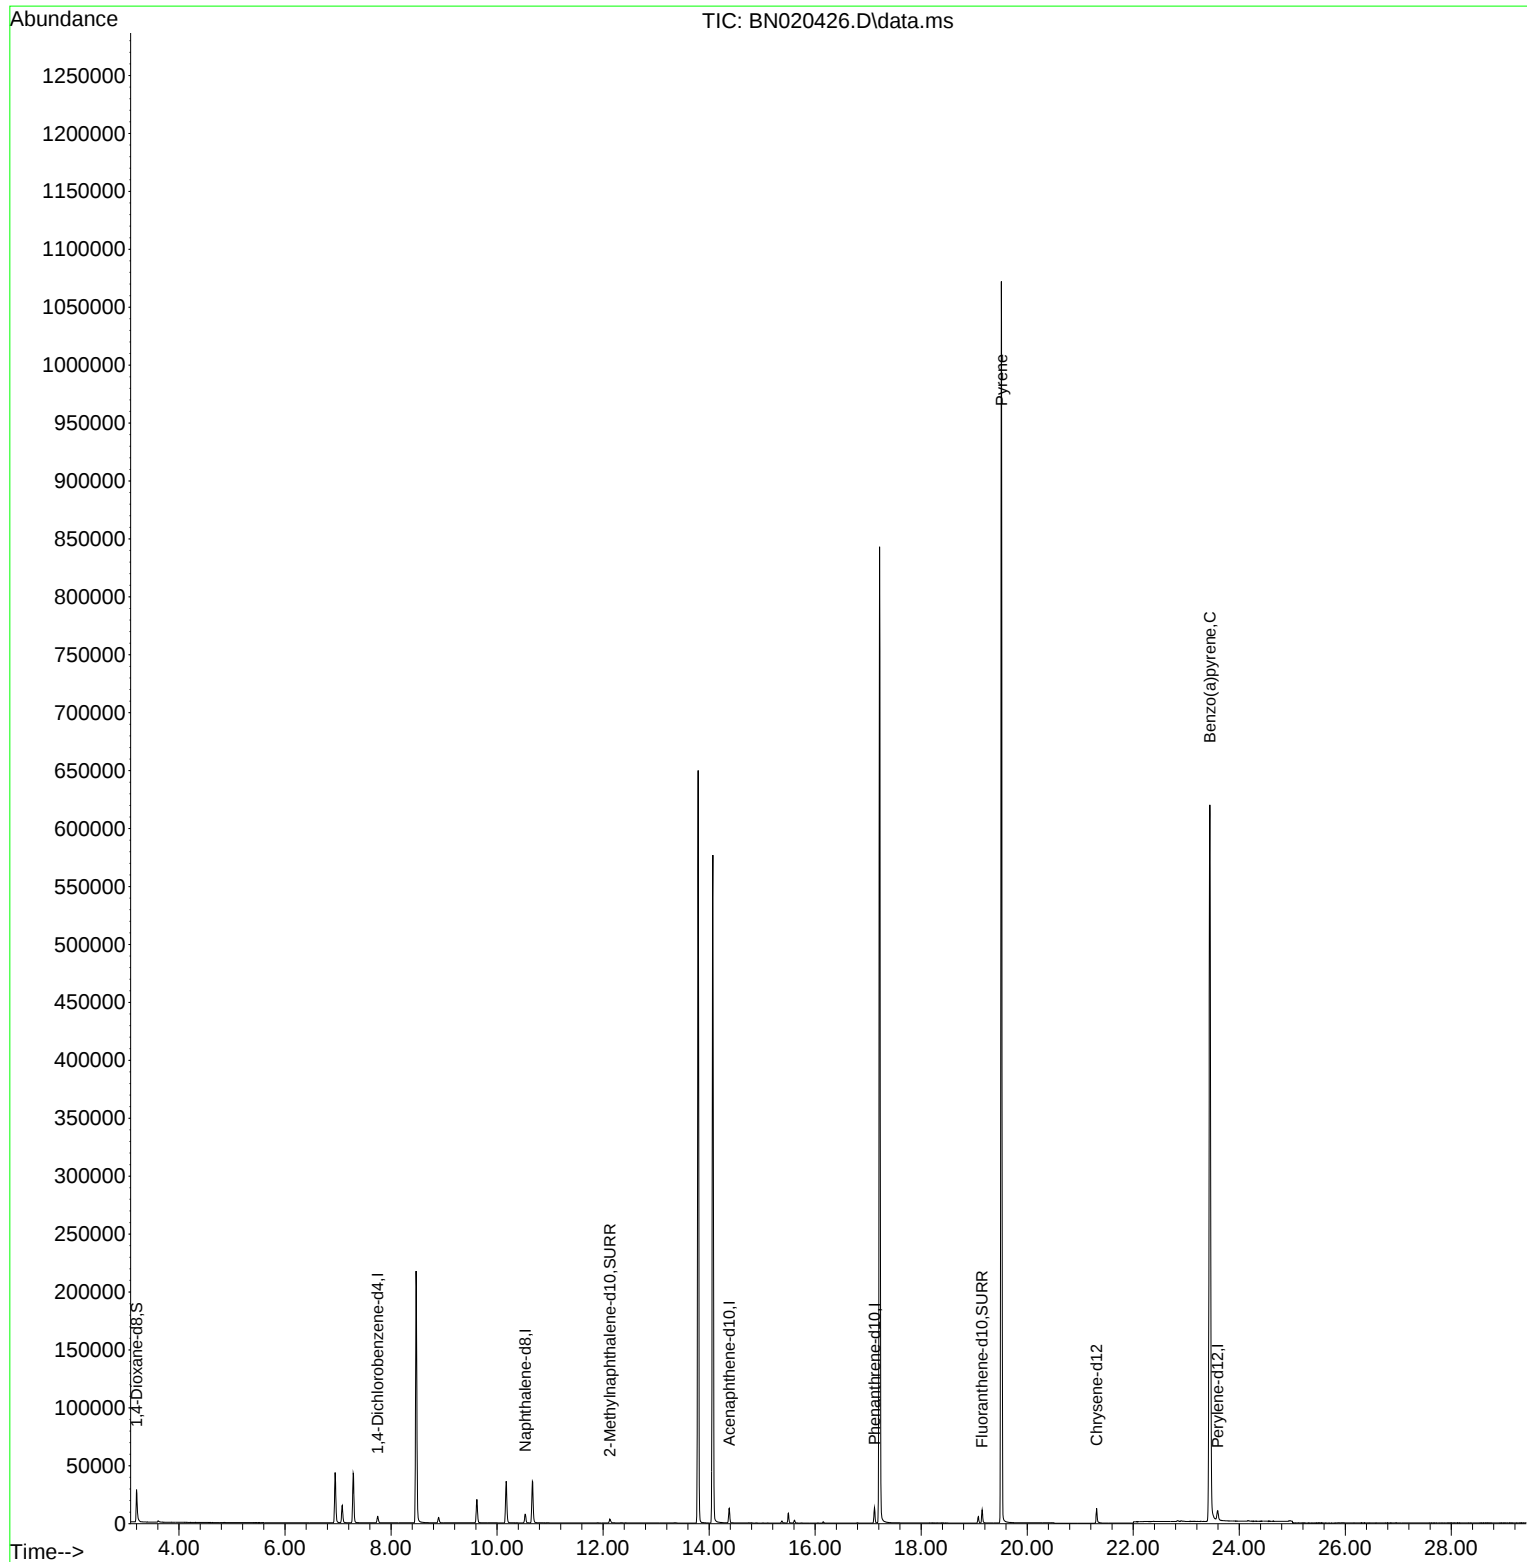


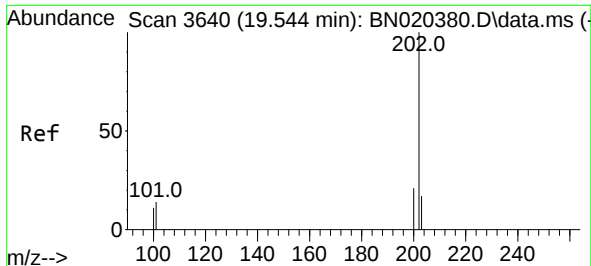

#20
Pyrene
Concen: 0.028 ng/ul
RT: 19.516 min Scan# 30
Delta R.T. -0.028 min
Lab File: BN020426.D
Acq: 25 Jun 2022 09:36

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:202 Resp: 1778
Ion Ratio Lower Upper
202 100
101 160.2 11.6 17.4#
100 1101.7 9.2 13.8#

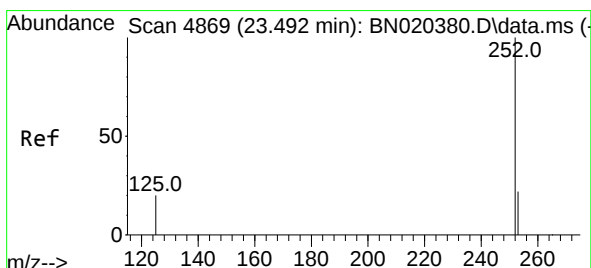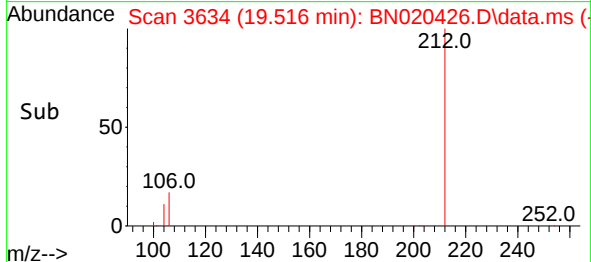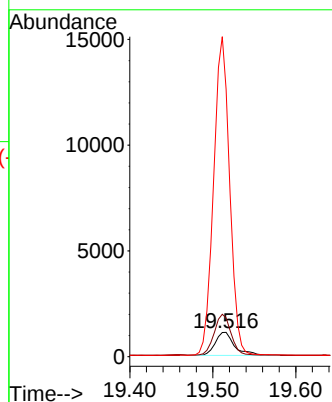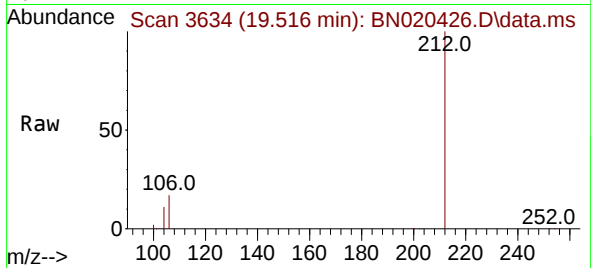

#26
Benzo(a)pyrene
Concen: 0.064 ng/ul
RT: 23.446 min Scan# 4853
Delta R.T. -0.047 min
Lab File: BN020426.D
Acq: 25 Jun 2022 09:36

Tgt Ion:252 Resp: 3350
Ion Ratio Lower Upper
252 100
253 47.7 21.0 31.4#
125 38.0 18.8 28.2#

