

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020427.D
 Acq On : 25 Jun 2022 10:12
 Operator : CG/JU
 Sample : PB145680BL
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 27 03:42:08 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.749	152	2625	0.400	ng/ul	0.00
4) Naphthalene-d8	10.529	136	8947	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.377	164	5991	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.120	188	13208	0.400	ng/ul	0.00
17) Chrysene-d12	21.313	240	11359	0.400	ng/ul	0.00
23) Perylene-d12	23.593	264	11397	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	17440	5.735	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.129	152	4540	0.309	ng/ul	0.00
18) Fluoranthene-d10	19.150	212	11293	0.302	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.512	202	1628	0.030	ng/ul#	1
26) Benzo(a)pyrene	23.444	252	3382	0.071	ng/ul#	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
Data File : BN020427.D
Acq On : 25 Jun 2022 10:12
Operator : CG/JU
Sample : PB145680BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 27 03:42:08 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:17:34 2022
Response via : Initial Calibration




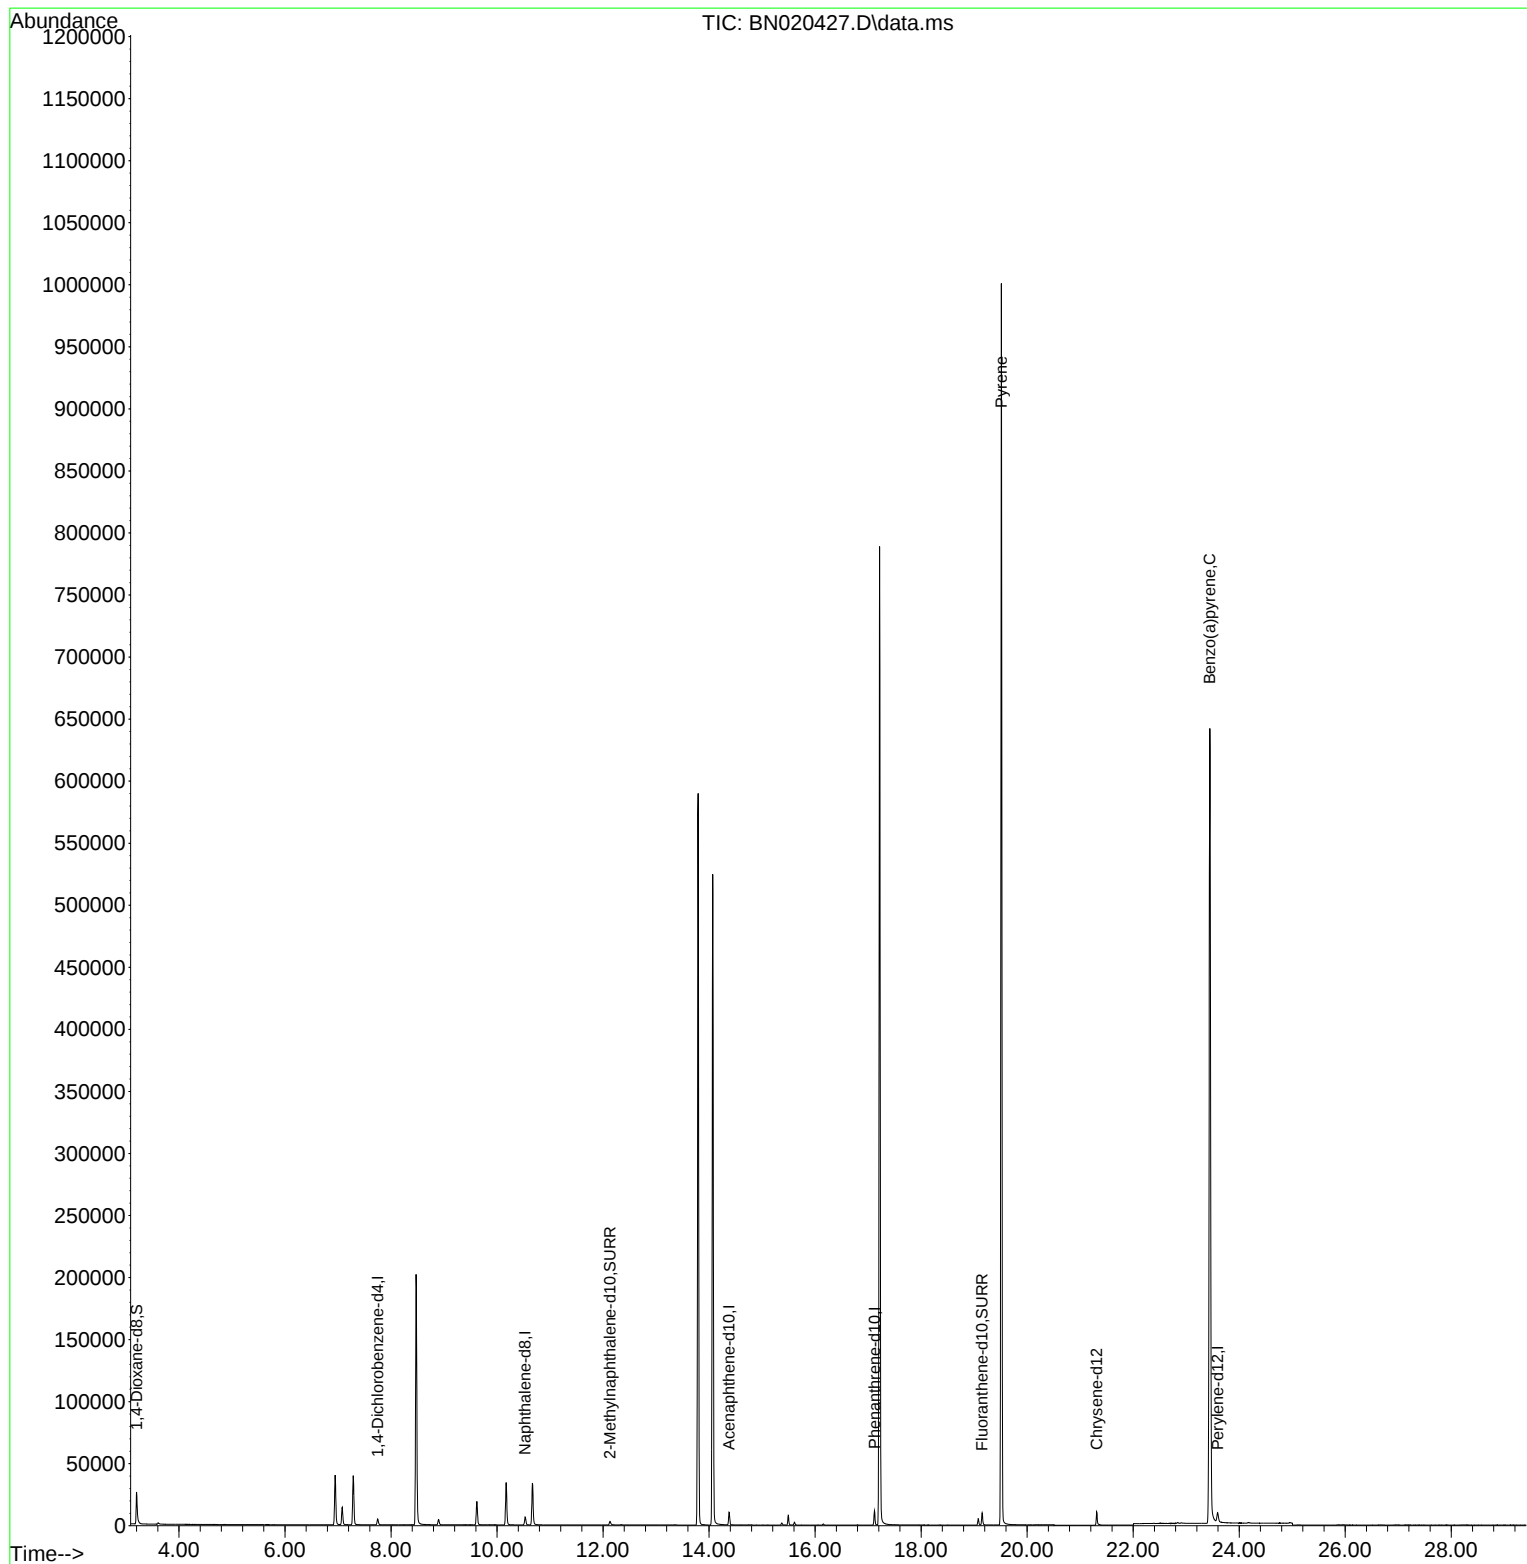


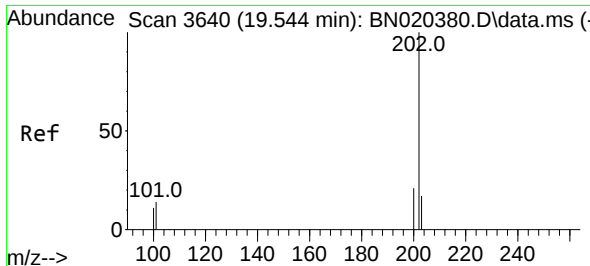

#20
Pyrene
Concen: 0.030 ng/ul
RT: 19.512 min Scan# 30
Delta R.T. -0.032 min
Lab File: BN020427.D
Acq: 25 Jun 2022 10:12

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:202 Resp: 1628
Ion Ratio Lower Upper
202 100
101 171.7 11.6 17.4#
100 1276.0 9.2 13.8#

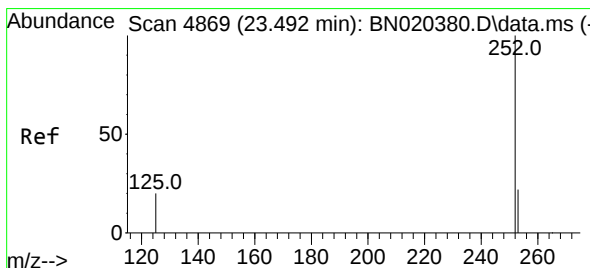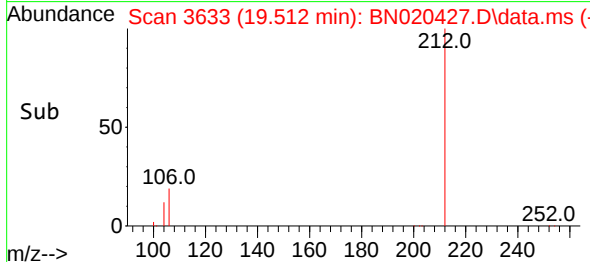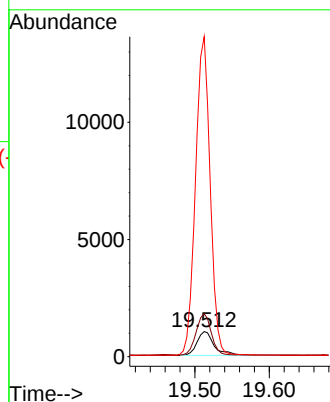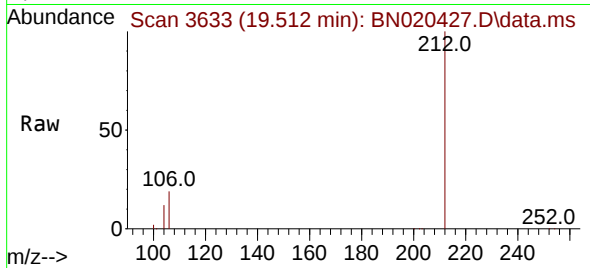

#26
Benzo(a)pyrene
Concen: 0.071 ng/ul
RT: 23.444 min Scan# 4852
Delta R.T. -0.049 min
Lab File: BN020427.D
Acq: 25 Jun 2022 10:12

Tgt Ion:252 Resp: 3382
Ion Ratio Lower Upper
252 100
253 45.8 21.0 31.4#
125 36.5 18.8 28.2#

