

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020436.D
 Acq On : 25 Jun 2022 15:39
 Operator : CG/JU
 Sample : N3395-11
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 27 03:42:36 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.749	152	2631	0.400	ng/ul	0.00
4) Naphthalene-d8	10.534	136	9203	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.376	164	6121	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.119	188	13577	0.400	ng/ul	0.00
17) Chrysene-d12	21.310	240	11976	0.400	ng/ul	0.00
23) Perylene-d12	23.593	264	11517	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	13098	4.297	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.129	152	4586	0.304	ng/ul	0.00
18) Fluoranthene-d10	19.150	212	14058	0.356	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.513	202	1819	0.032	ng/ul#	1
26) Benzo(a)pyrene	23.450	252	3783	0.078	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
Data File : BN020436.D
Acq On : 25 Jun 2022 15:39
Operator : CG/JU
Sample : N3395-11
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 27 03:42:36 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:17:34 2022
Response via : Initial Calibration




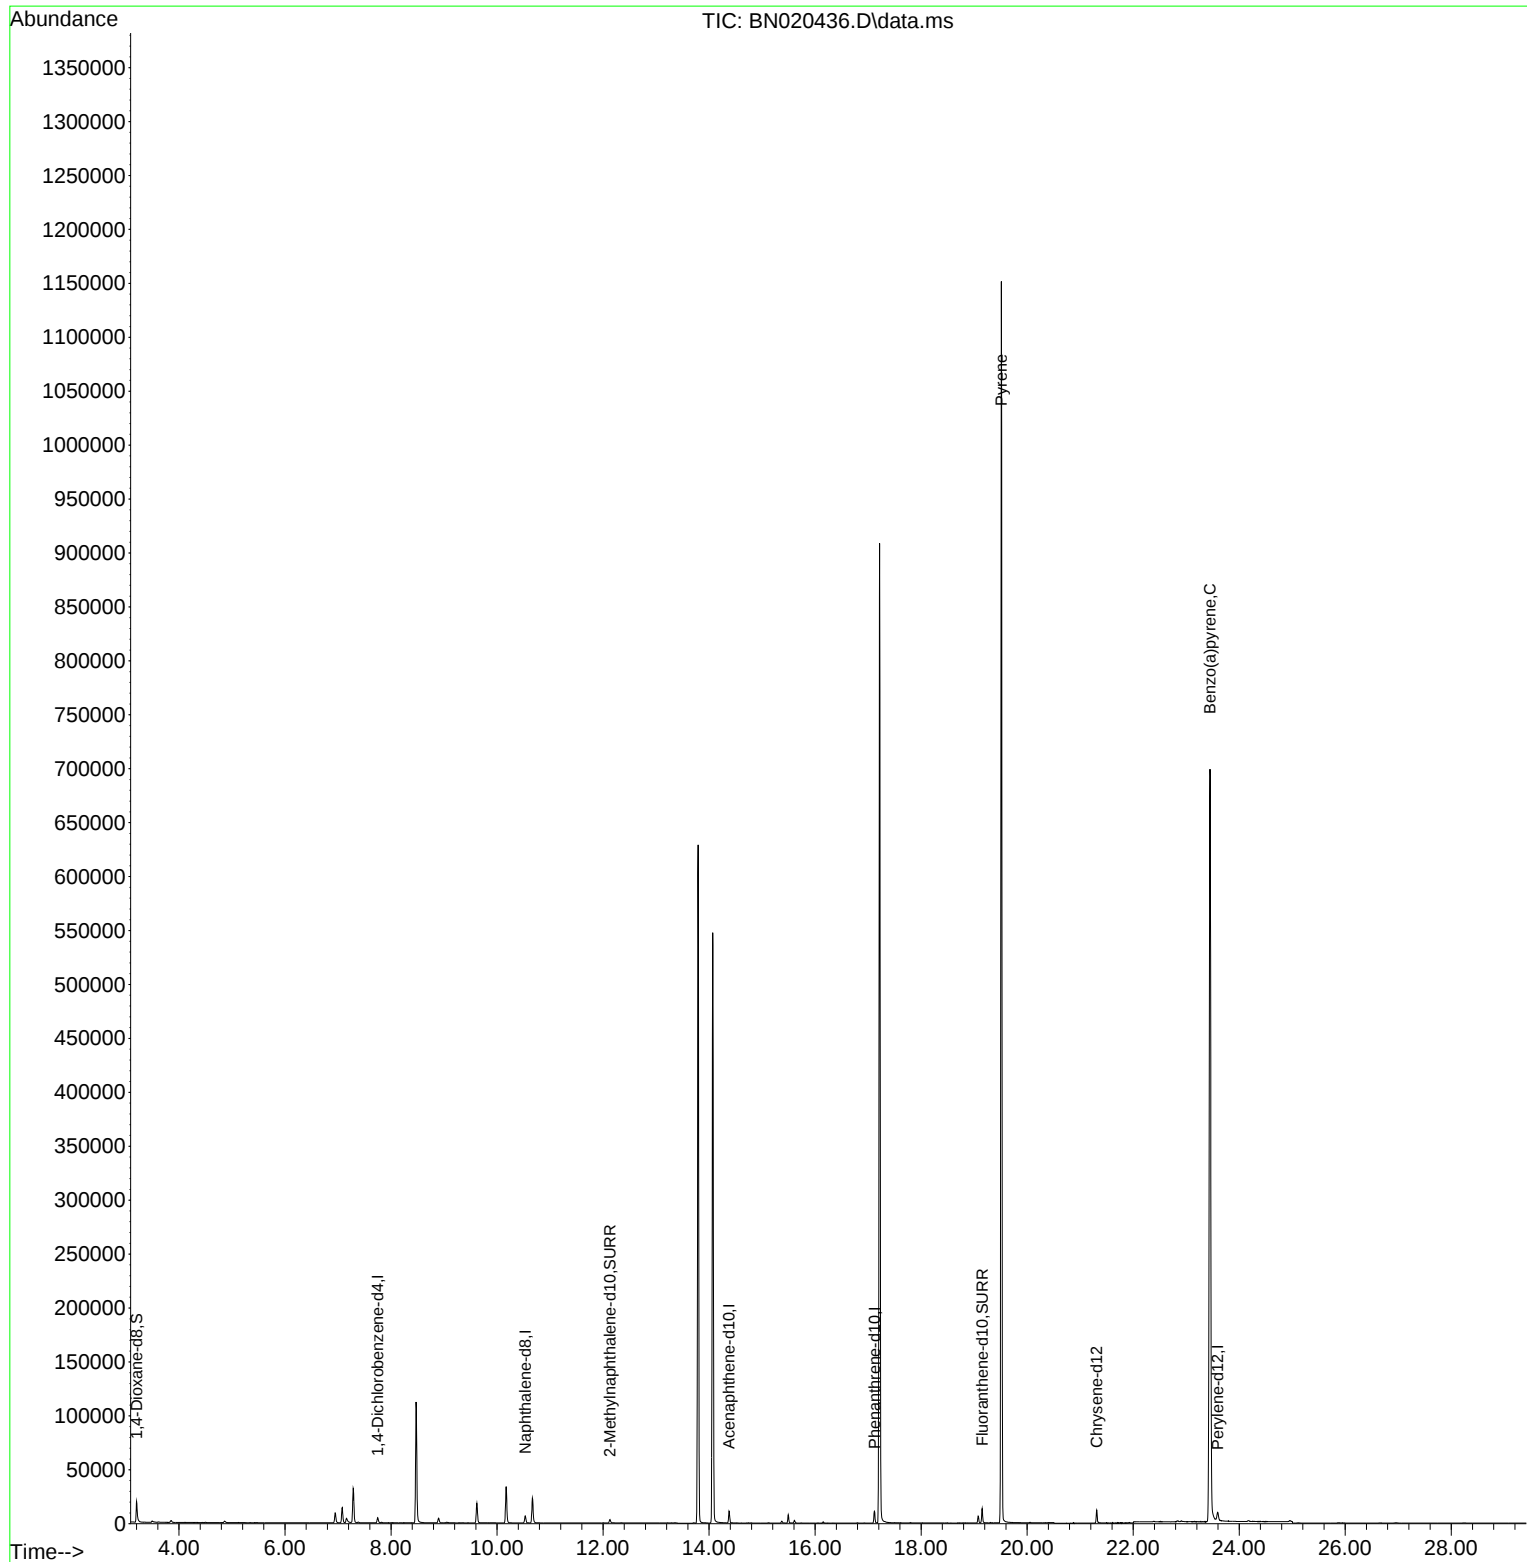


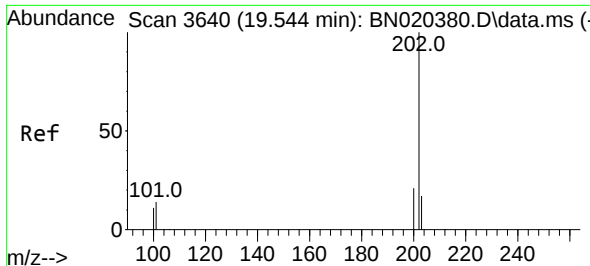

#20
Pyrene
Concen: 0.032 ng/ul
RT: 19.513 min Scan# 30
Delta R.T. -0.031 min
Lab File: BN020436.D
Acq: 25 Jun 2022 15:39

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:202 Resp: 1819
Ion Ratio Lower Upper
202 100
101 169.2 11.6 17.4#
100 1210.2 9.2 13.8#

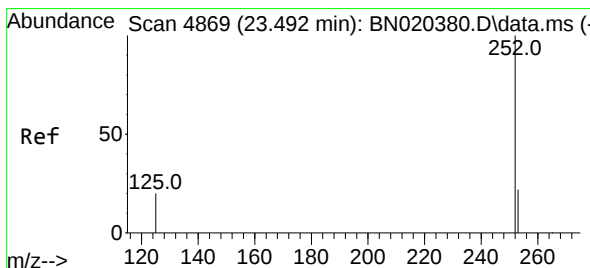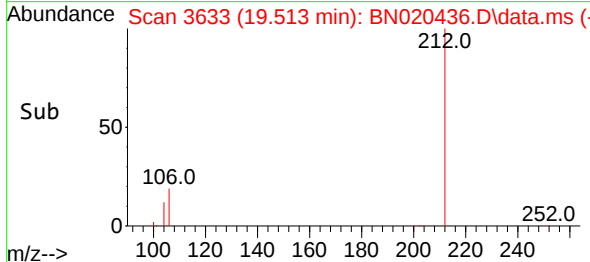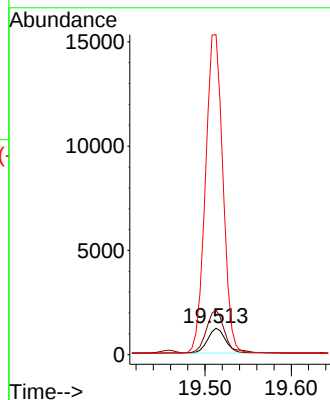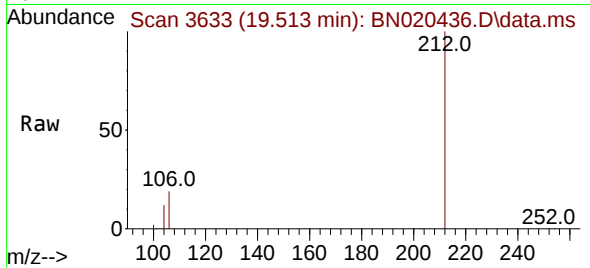

#26
Benzo(a)pyrene
Concen: 0.078 ng/ul
RT: 23.450 min Scan# 4854
Delta R.T. -0.042 min
Lab File: BN020436.D
Acq: 25 Jun 2022 15:39

Tgt Ion:252 Resp: 3783
Ion Ratio Lower Upper
252 100
253 46.9 21.0 31.4#
125 37.5 18.8 28.2#

