

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020439.D
 Acq On : 25 Jun 2022 17:28
 Operator : CG/JU
 Sample : N3395-19
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 27 03:42:49 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.750	152	2965	0.400	ng/ul	0.00
4) Naphthalene-d8	10.529	136	10530	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.377	164	6922	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.120	188	15311	0.400	ng/ul	0.00
17) Chrysene-d12	21.311	240	12870	0.400	ng/ul	0.00
23) Perylene-d12	23.591	264	12190	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	15483	4.507	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.130	152	5290	0.306	ng/ul	0.00
18) Fluoranthene-d10	19.151	212	14500	0.342	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.513	202	1887	0.031	ng/ul#	1
26) Benzo(a)pyrene	23.447	252	3720	0.073	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
Data File : BN020439.D
Acq On : 25 Jun 2022 17:28
Operator : CG/JU
Sample : N3395-19
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 27 03:42:49 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:17:34 2022
Response via : Initial Calibration




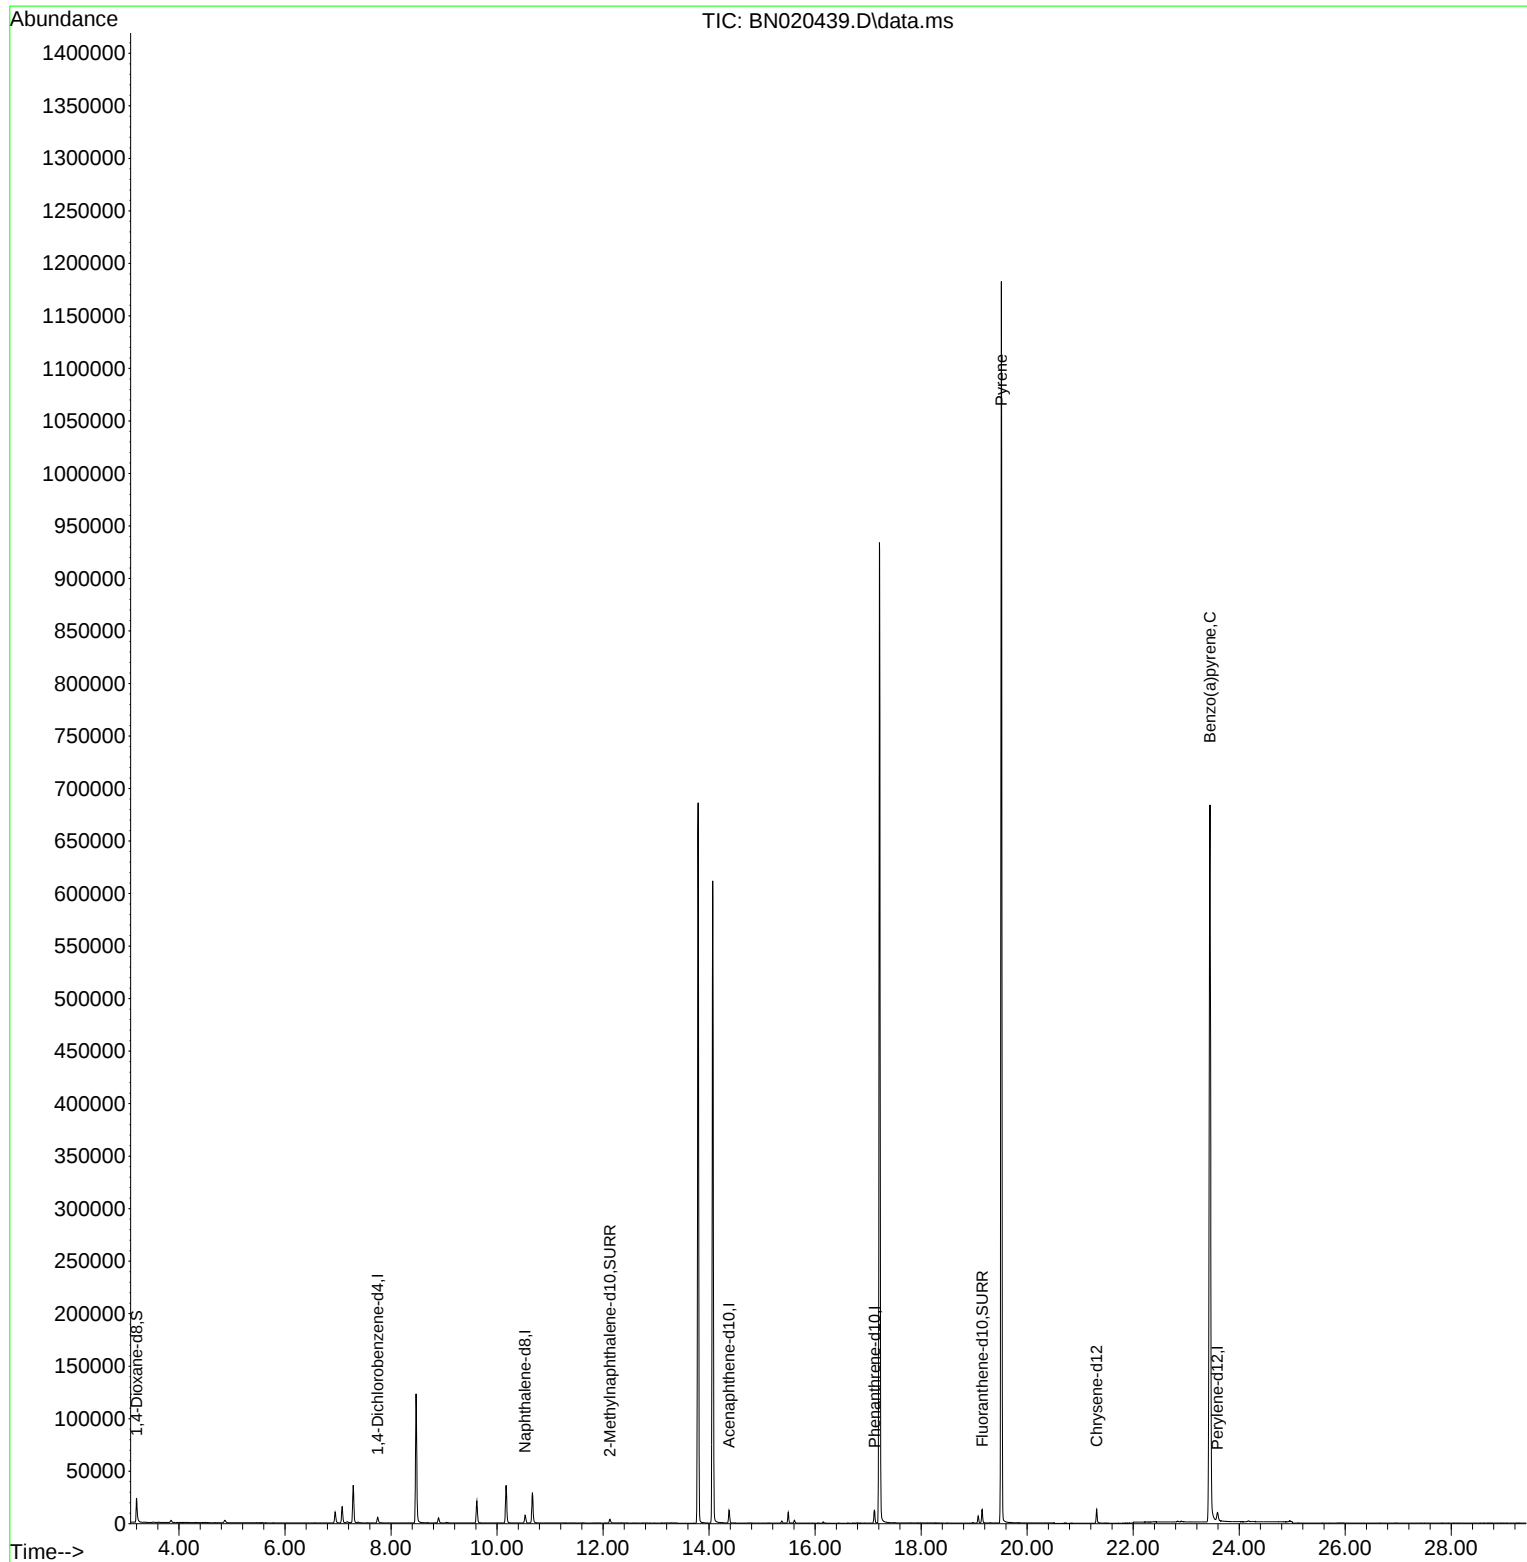


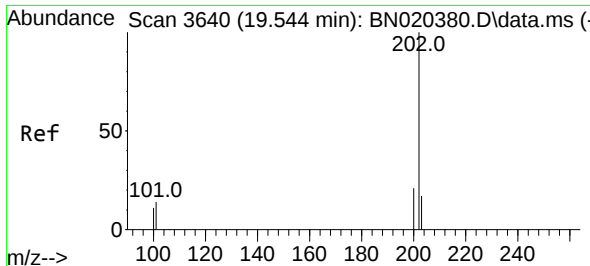

#20
Pyrene
Concen: 0.031 ng/u1
RT: 19.513 min Scan# 3633
Delta R.T. -0.031 min
Lab File: BN020439.D
Acq: 25 Jun 2022 17:28

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:202 Resp: 1887
Ion Ratio Lower Upper
202 100
101 170.2 11.6 17.4#
100 1212.7 9.2 13.8#

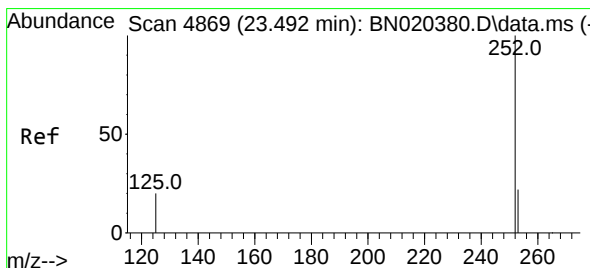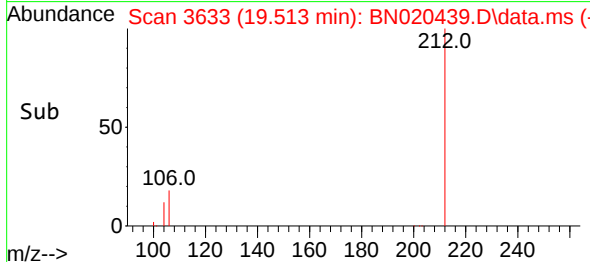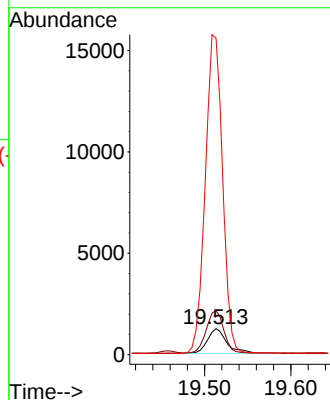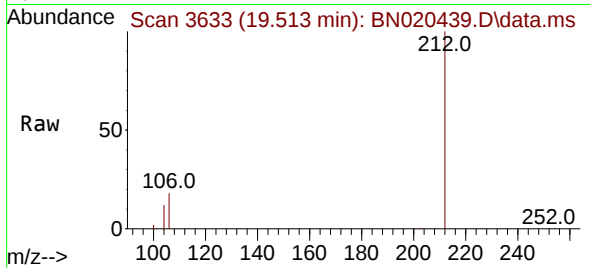

#26
Benzo(a)pyrene
Concen: 0.073 ng/u1
RT: 23.447 min Scan# 4853
Delta R.T. -0.045 min
Lab File: BN020439.D
Acq: 25 Jun 2022 17:28

Tgt Ion:252 Resp: 3720
Ion Ratio Lower Upper
252 100
253 45.1 21.0 31.4#
125 35.3 18.8 28.2#

