

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020443.D
 Acq On : 25 Jun 2022 20:30
 Operator : CG/JU
 Sample : PB145682BL
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 27 03:43:14 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.749	152	2014	0.400	ng/ul	0.00
4) Naphthalene-d8	10.533	136	7065	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.380	164	4672	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.118	188	10306	0.400	ng/ul	0.00
17) Chrysene-d12	21.312	240	9358	0.400	ng/ul	0.00
23) Perylene-d12	23.588	264	10194	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	14070	6.030	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.133	152	3667	0.316	ng/ul	0.00
18) Fluoranthene-d10	19.148	212	9362	0.303	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.511	202	1366	0.031	ng/ul#	1
26) Benzo(a)pyrene	23.442	252	3147	0.073	ng/ul#	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
Data File : BN020443.D
Acq On : 25 Jun 2022 20:30
Operator : CG/JU
Sample : PB145682BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 27 03:43:14 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:17:34 2022
Response via : Initial Calibration




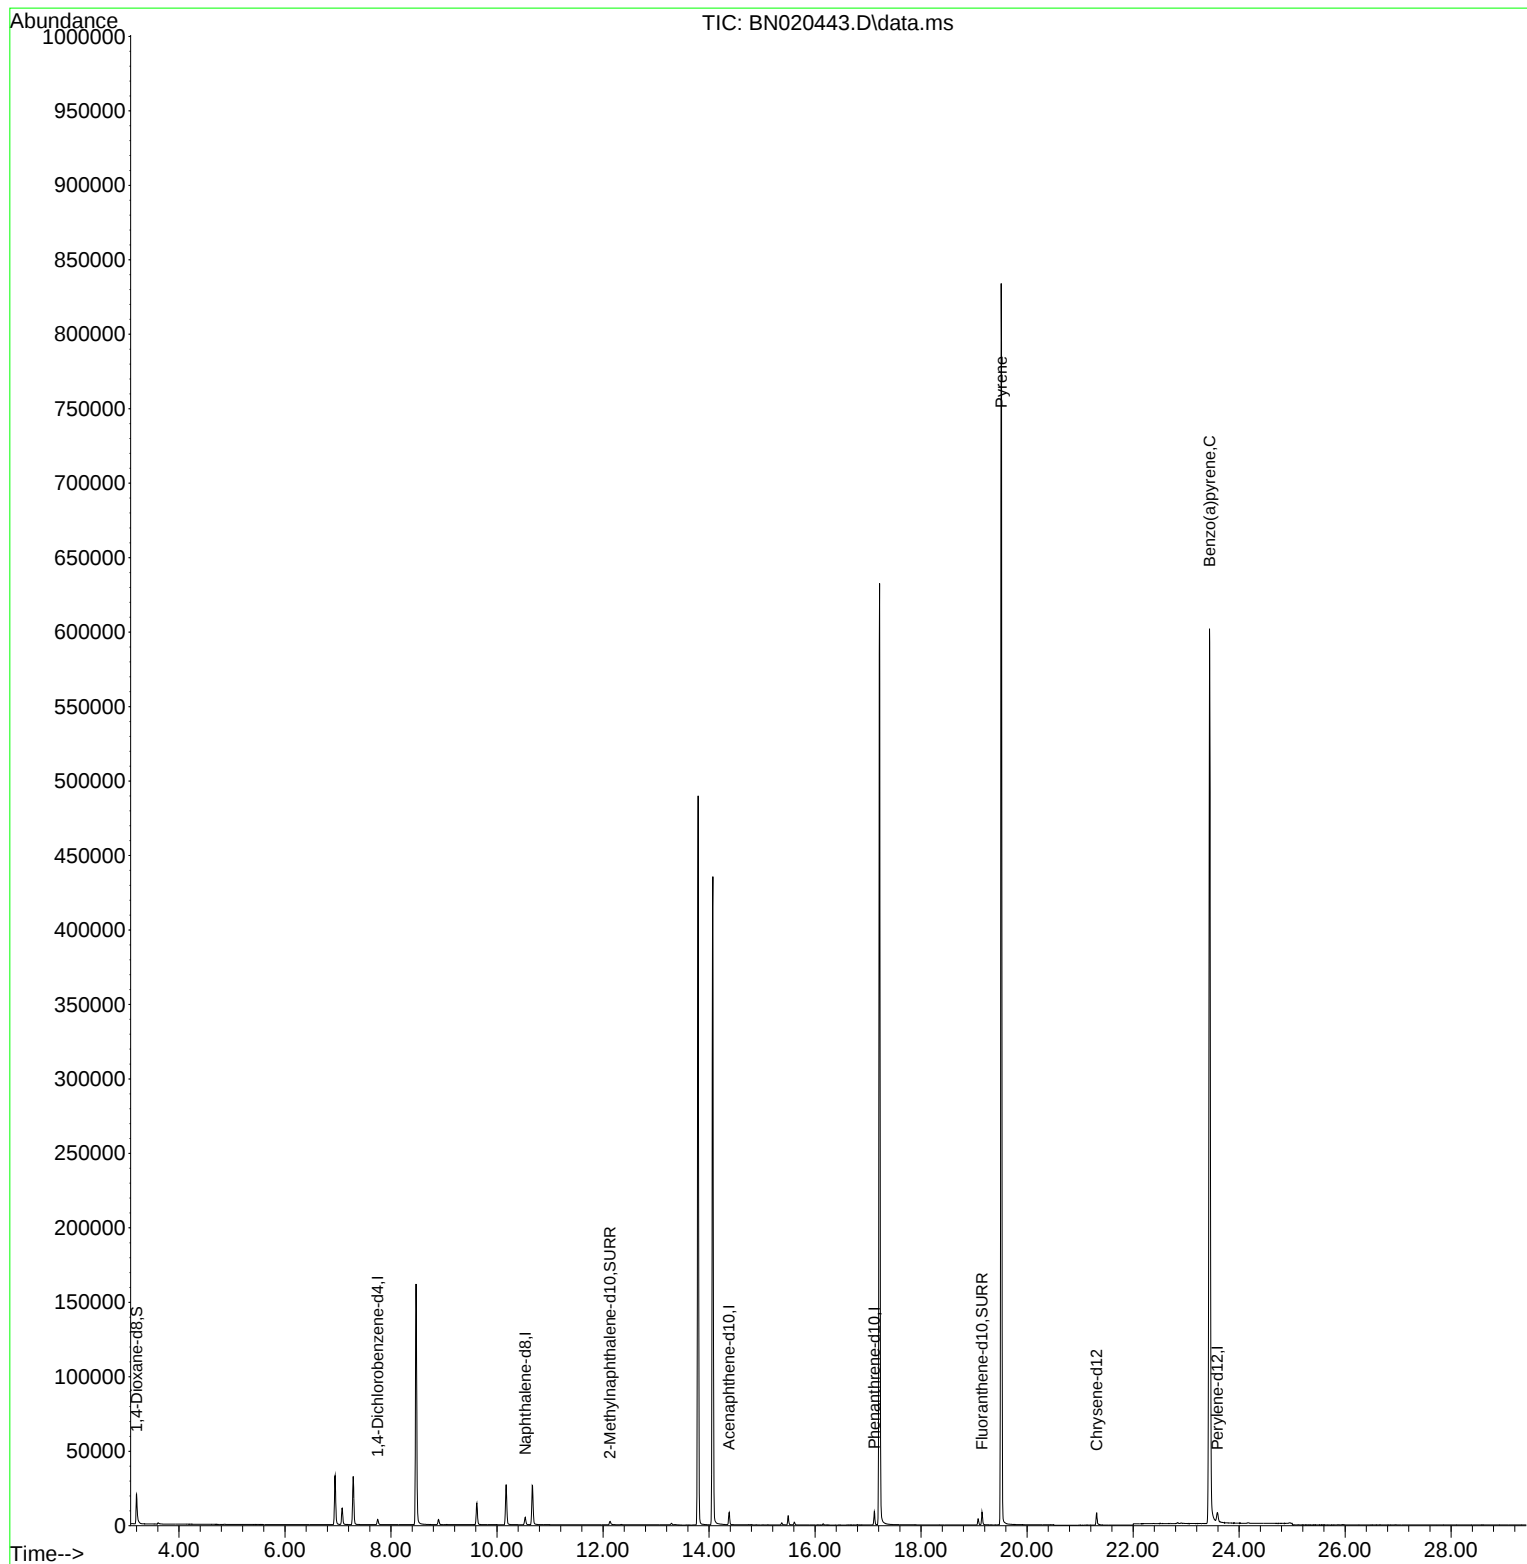


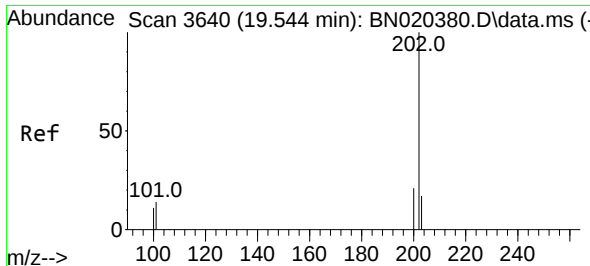

#20
Pyrene
Concen: 0.031 ng/ul
RT: 19.511 min Scan# 3633
Delta R.T. -0.033 min
Lab File: BN020443.D
Acq: 25 Jun 2022 20:30

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:202 Resp: 1366
Ion Ratio Lower Upper
202 100
101 178.3 11.6 17.4#
100 1297.7 9.2 13.8#

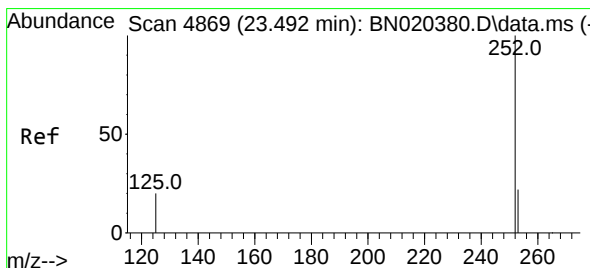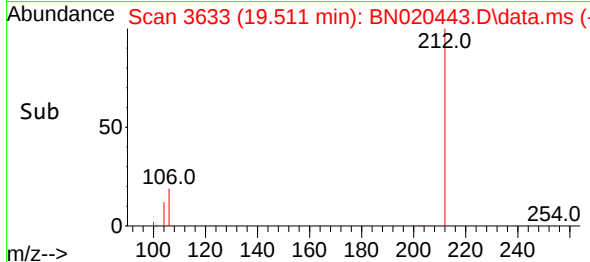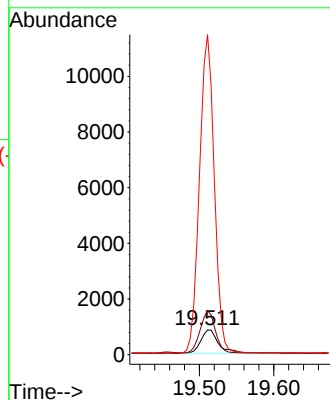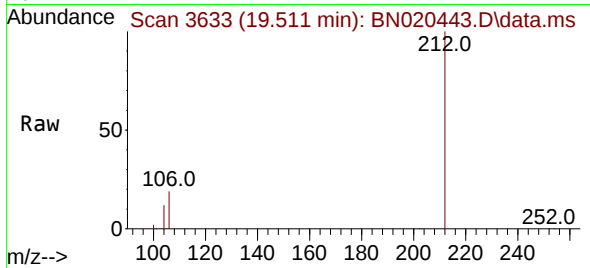

#26
Benzo(a)pyrene
Concen: 0.073 ng/ul
RT: 23.442 min Scan# 4852
Delta R.T. -0.050 min
Lab File: BN020443.D
Acq: 25 Jun 2022 20:30

Tgt Ion:252 Resp: 3147
Ion Ratio Lower Upper
252 100
253 45.3 21.0 31.4#
125 35.8 18.8 28.2#

