

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020444.D
 Acq On : 25 Jun 2022 21:07
 Operator : CG/JU
 Sample : PB145684BL
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 27 03:43:17 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.750	152	2868	0.400	ng/ul	0.00
4) Naphthalene-d8	10.529	136	10093	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.377	164	6665	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.120	188	14700	0.400	ng/ul	0.00
17) Chrysene-d12	21.306	240	12430	0.400	ng/ul	0.00
23) Perylene-d12	23.586	264	12328	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	18586	5.594	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.130	152	4941	0.298	ng/ul	0.00
18) Fluoranthene-d10	19.151	212	12228	0.298	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.513	202	1732	0.029	ng/ul#	1
26) Benzo(a)pyrene	23.437	252	3583	0.069	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
Data File : BN020444.D
Acq On : 25 Jun 2022 21:07
Operator : CG/JU
Sample : PB145684BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 27 03:43:17 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:17:34 2022
Response via : Initial Calibration




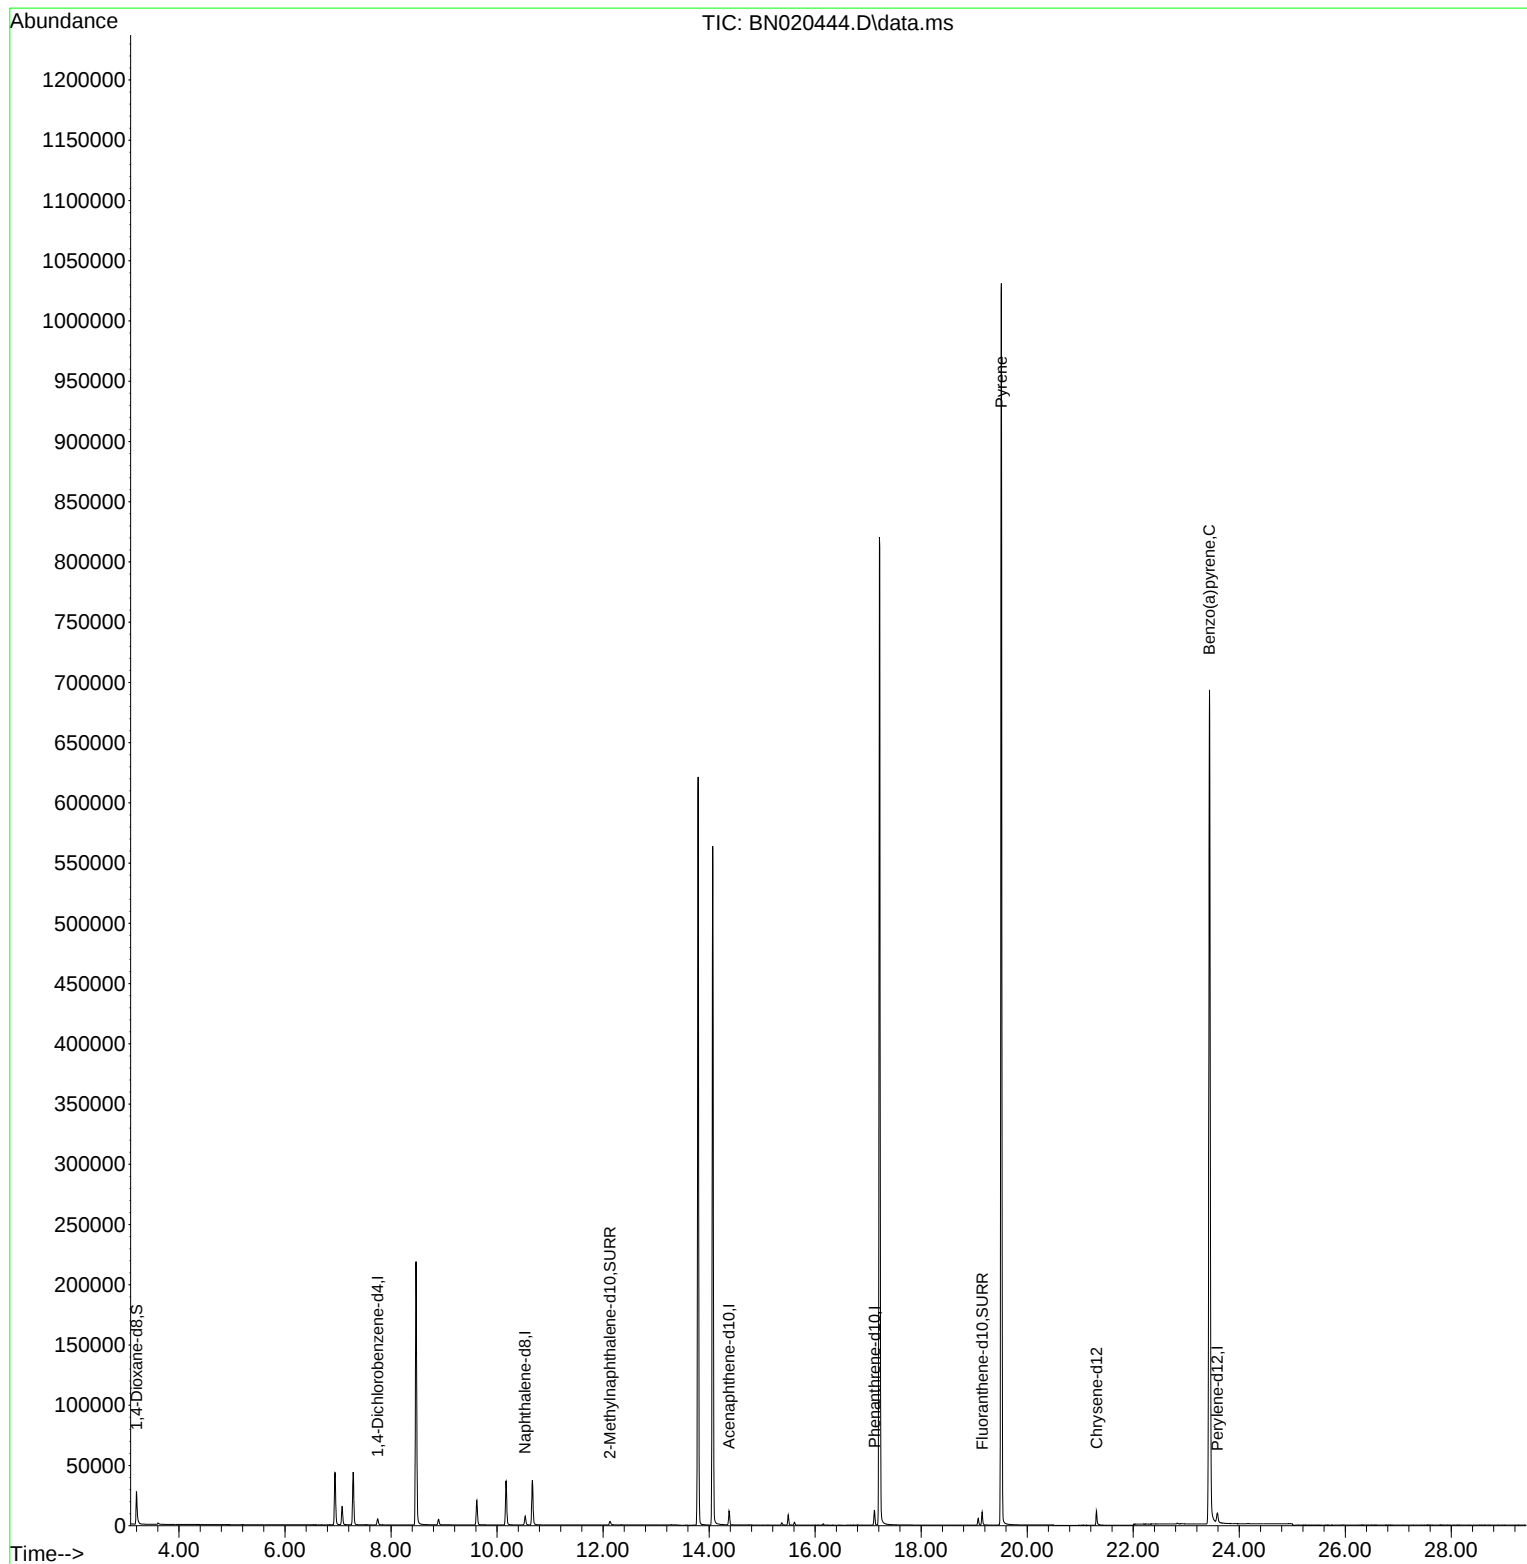


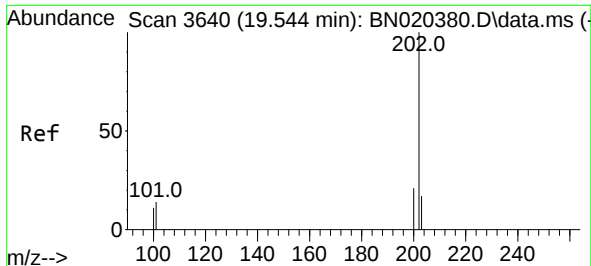

#20
Pyrene
Concen: 0.029 ng/ul
RT: 19.513 min Scan# 3633
Delta R.T. -0.031 min
Lab File: BN020444.D
Acq: 25 Jun 2022 21:07

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:202 Resp: 1732
Ion Ratio Lower Upper
202 100
101 169.1 11.6 17.4#
100 1177.1 9.2 13.8#

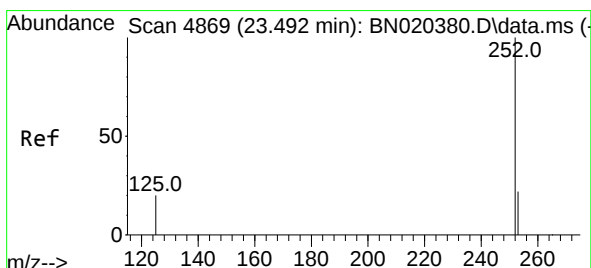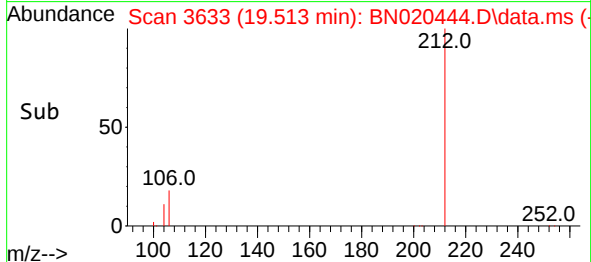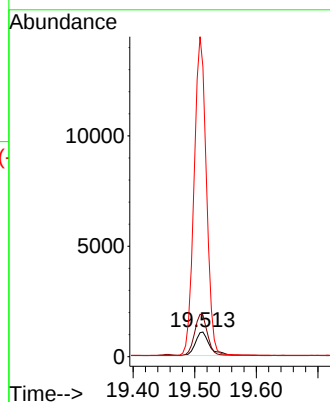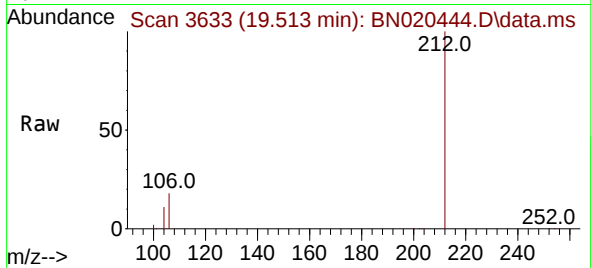

#26
Benzo(a)pyrene
Concen: 0.069 ng/ul
RT: 23.437 min Scan# 4850
Delta R.T. -0.055 min
Lab File: BN020444.D
Acq: 25 Jun 2022 21:07

Tgt Ion:252 Resp: 3583
Ion Ratio Lower Upper
252 100
253 42.7 21.0 31.4#
125 34.5 18.8 28.2#

