

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020445.D
 Acq On : 25 Jun 2022 21:43
 Operator : CG/JU
 Sample : PB145701BL
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 27 03:43:21 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.750	152	2062	0.400	ng/ul	0.00
4) Naphthalene-d8	10.529	136	7150	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.377	164	4747	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.120	188	10332	0.400	ng/ul	0.00
17) Chrysene-d12	21.306	240	9239	0.400	ng/ul	0.00
23) Perylene-d12	23.586	264	10108	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	17880	7.485	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.130	152	4761	0.406	ng/ul	0.00
18) Fluoranthene-d10	19.151	212	11890	0.390	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.372	166	1595	0.075	ng/ul#	14
20) Pyrene	19.513	202	1553	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.440	252	3792	0.089	ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
Data File : BN020445.D
Acq On : 25 Jun 2022 21:43
Operator : CG/JU
Sample : PB145701BL
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 27 03:43:21 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:17:34 2022
Response via : Initial Calibration




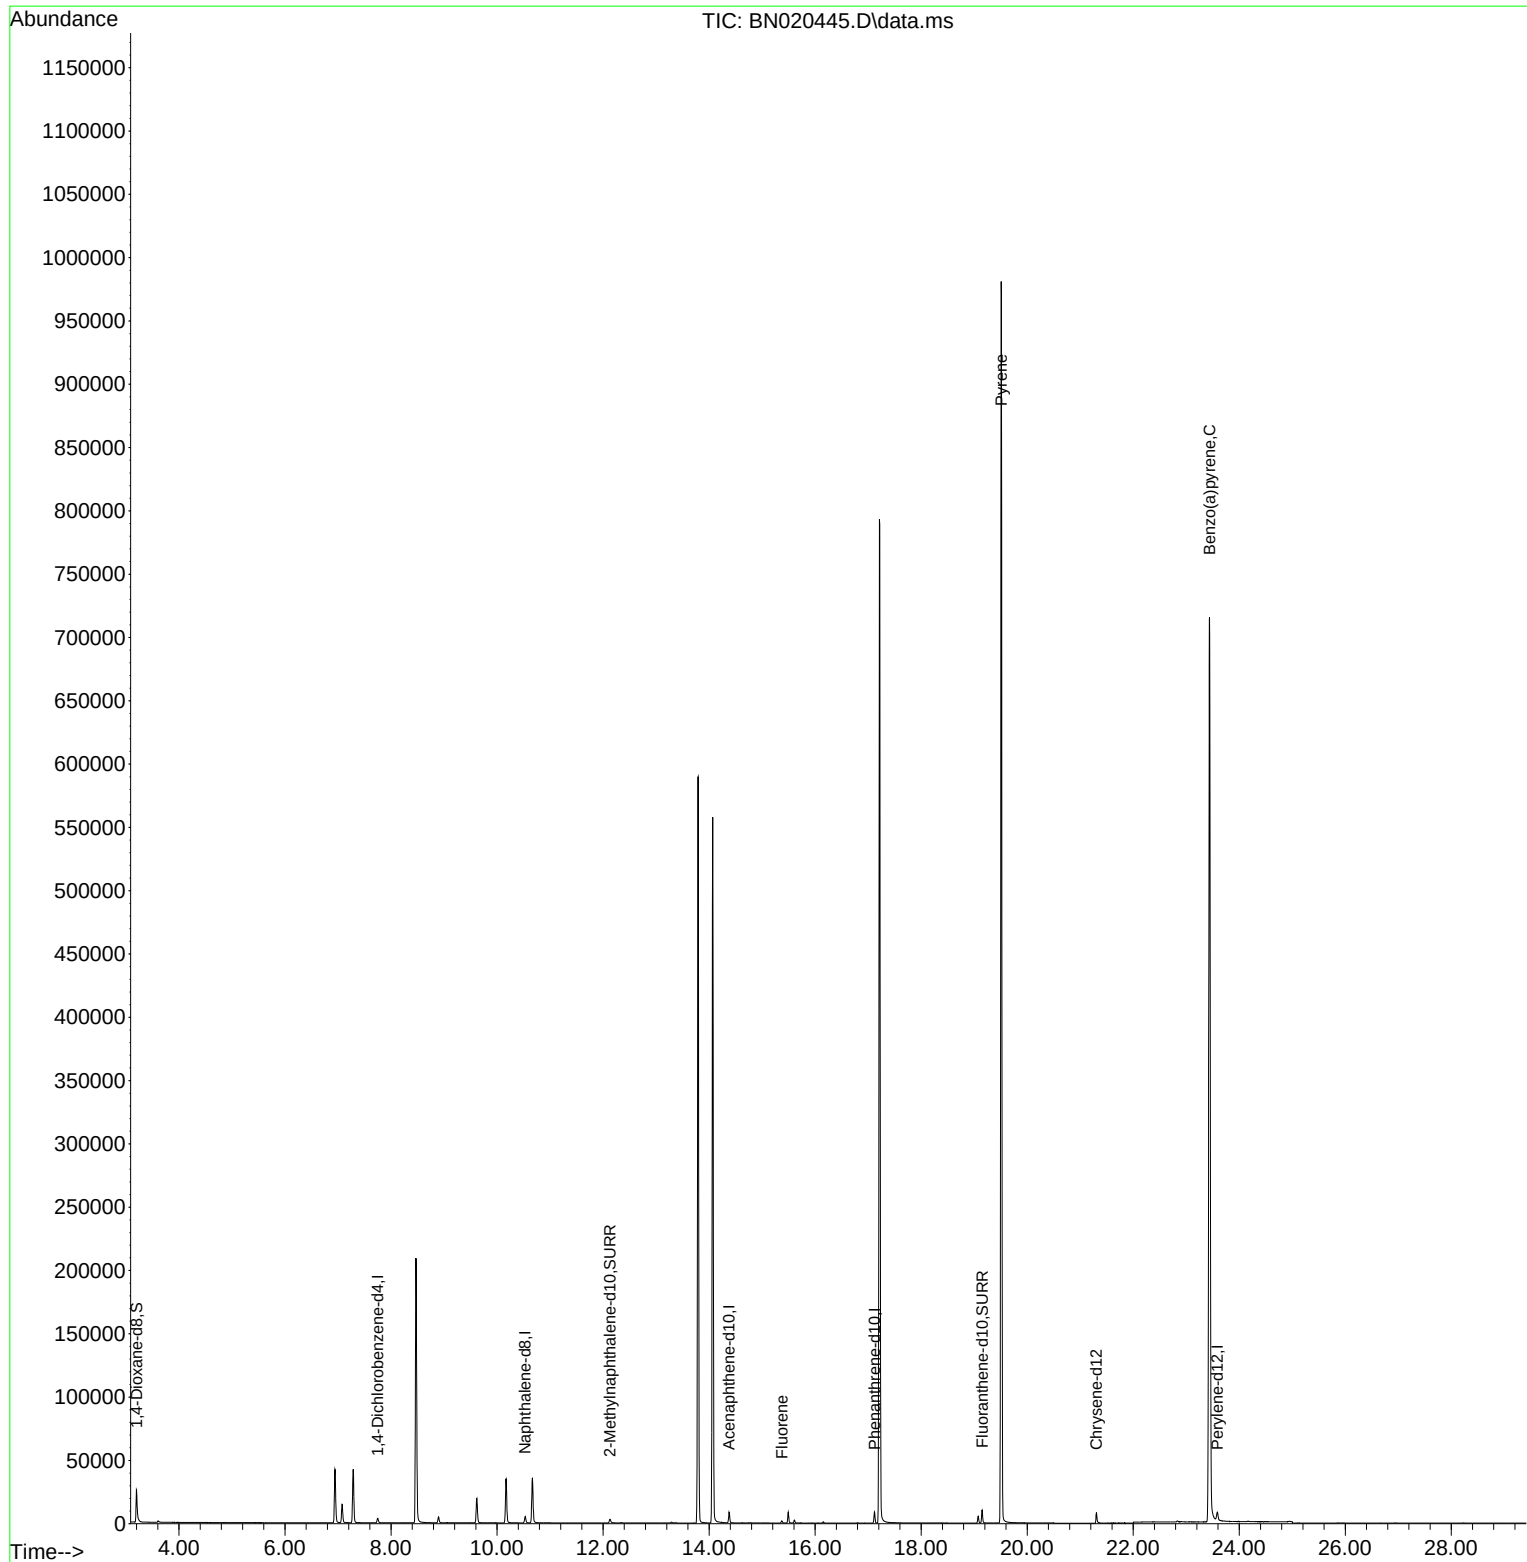


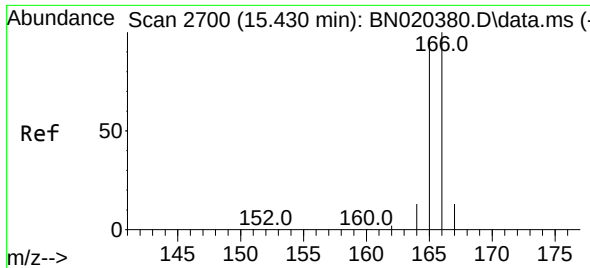

#12
Fluorene
Concen: 0.075 ng/ul
RT: 15.372 min Scan# 20445
Delta R.T. -0.059 min
Lab File: BN020445.D
Acq: 25 Jun 2022 21:43




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:166 Resp: 1595
Ion Ratio Lower Upper
166 100
165 8.9 78.2 117.2#
167 38.2 11.3 16.9#

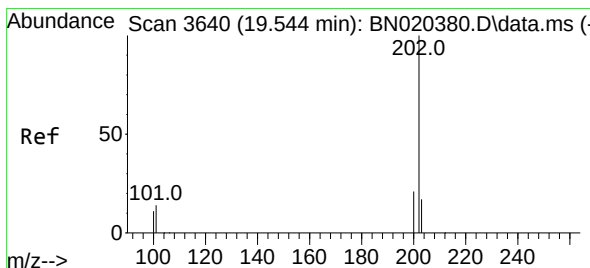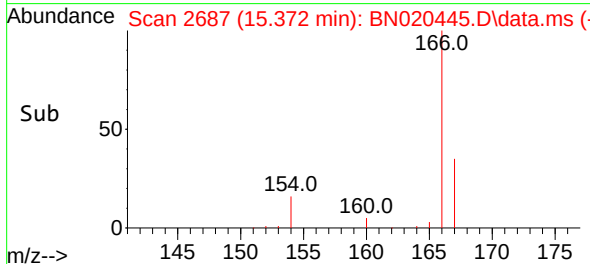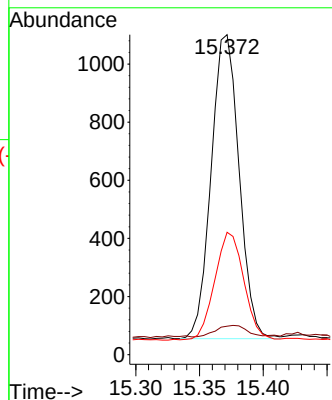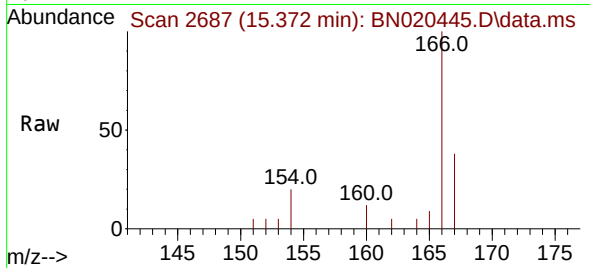

#20
Pyrene
Concen: 0.035 ng/ul
RT: 19.513 min Scan# 3633
Delta R.T. -0.031 min
Lab File: BN020445.D
Acq: 25 Jun 2022 21:43


Tgt Ion:202 Resp: 1553
Ion Ratio Lower Upper
202 100
101 169.0 11.6 17.4#
100 1188.8 9.2 13.8#

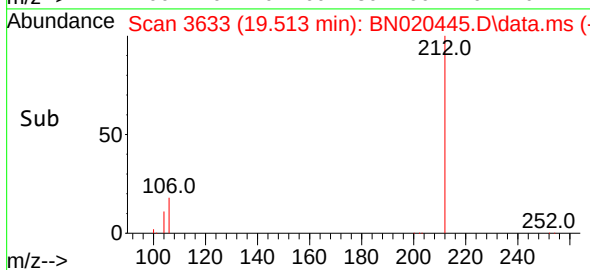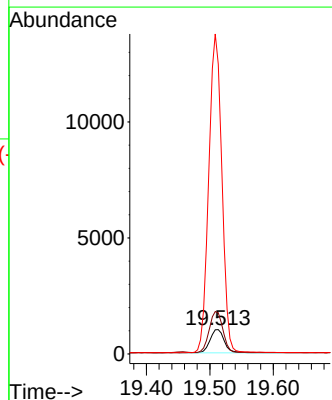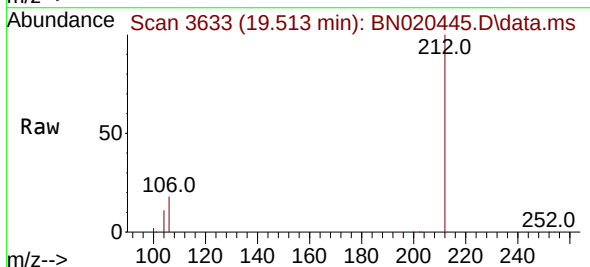

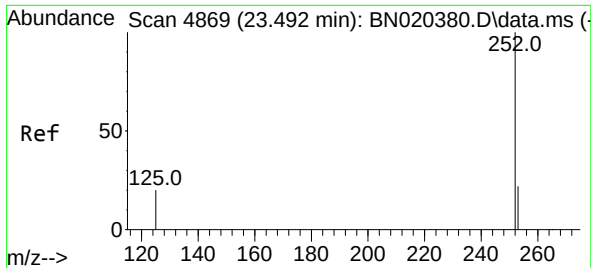

#26
Benzo(a)pyrene
Concen: 0.089 ng/ul
RT: 23.440 min Scan# 4851
Delta R.T. -0.052 min
Lab File: BN020445.D
Acq: 25 Jun 2022 21:43

Instrument :
BNA_N
ClientSampleId :

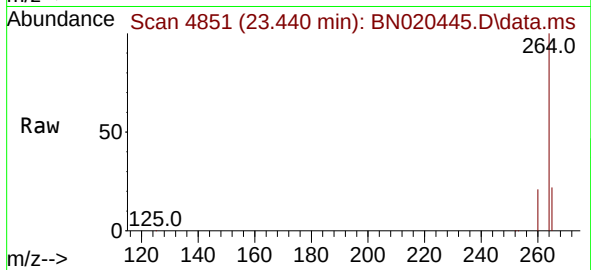

Tgt Ion:252 Resp: 3792
Ion Ratio Lower Upper
252 100
253 42.0 21.0 31.4#
125 33.8 18.8 28.2#

