

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020449.D
 Acq On : 26 Jun 2022 00:08
 Operator : CG/JU
 Sample : N3395-17
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 27 03:43:39 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.749	152	2747	0.400	ng/ul	0.00
4) Naphthalene-d8	10.529	136	9752	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.378	164	6494	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.116	188	14156	0.400	ng/ul	0.00
17) Chrysene-d12	21.307	240	11658	0.400	ng/ul	0.00
23) Perylene-d12	23.587	264	11090	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	14999	4.713	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.129	152	5468	0.342	ng/ul	0.00
18) Fluoranthene-d10	19.147	212	15765	0.410	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.231	88	69	0.021	ng/ul#	67
20) Pyrene	19.509	202	2287	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.441	252	4191	0.090	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
Data File : BN020449.D
Acq On : 26 Jun 2022 00:08
Operator : CG/JU
Sample : N3395-17
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Jun 27 03:43:39 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:17:34 2022
Response via : Initial Calibration

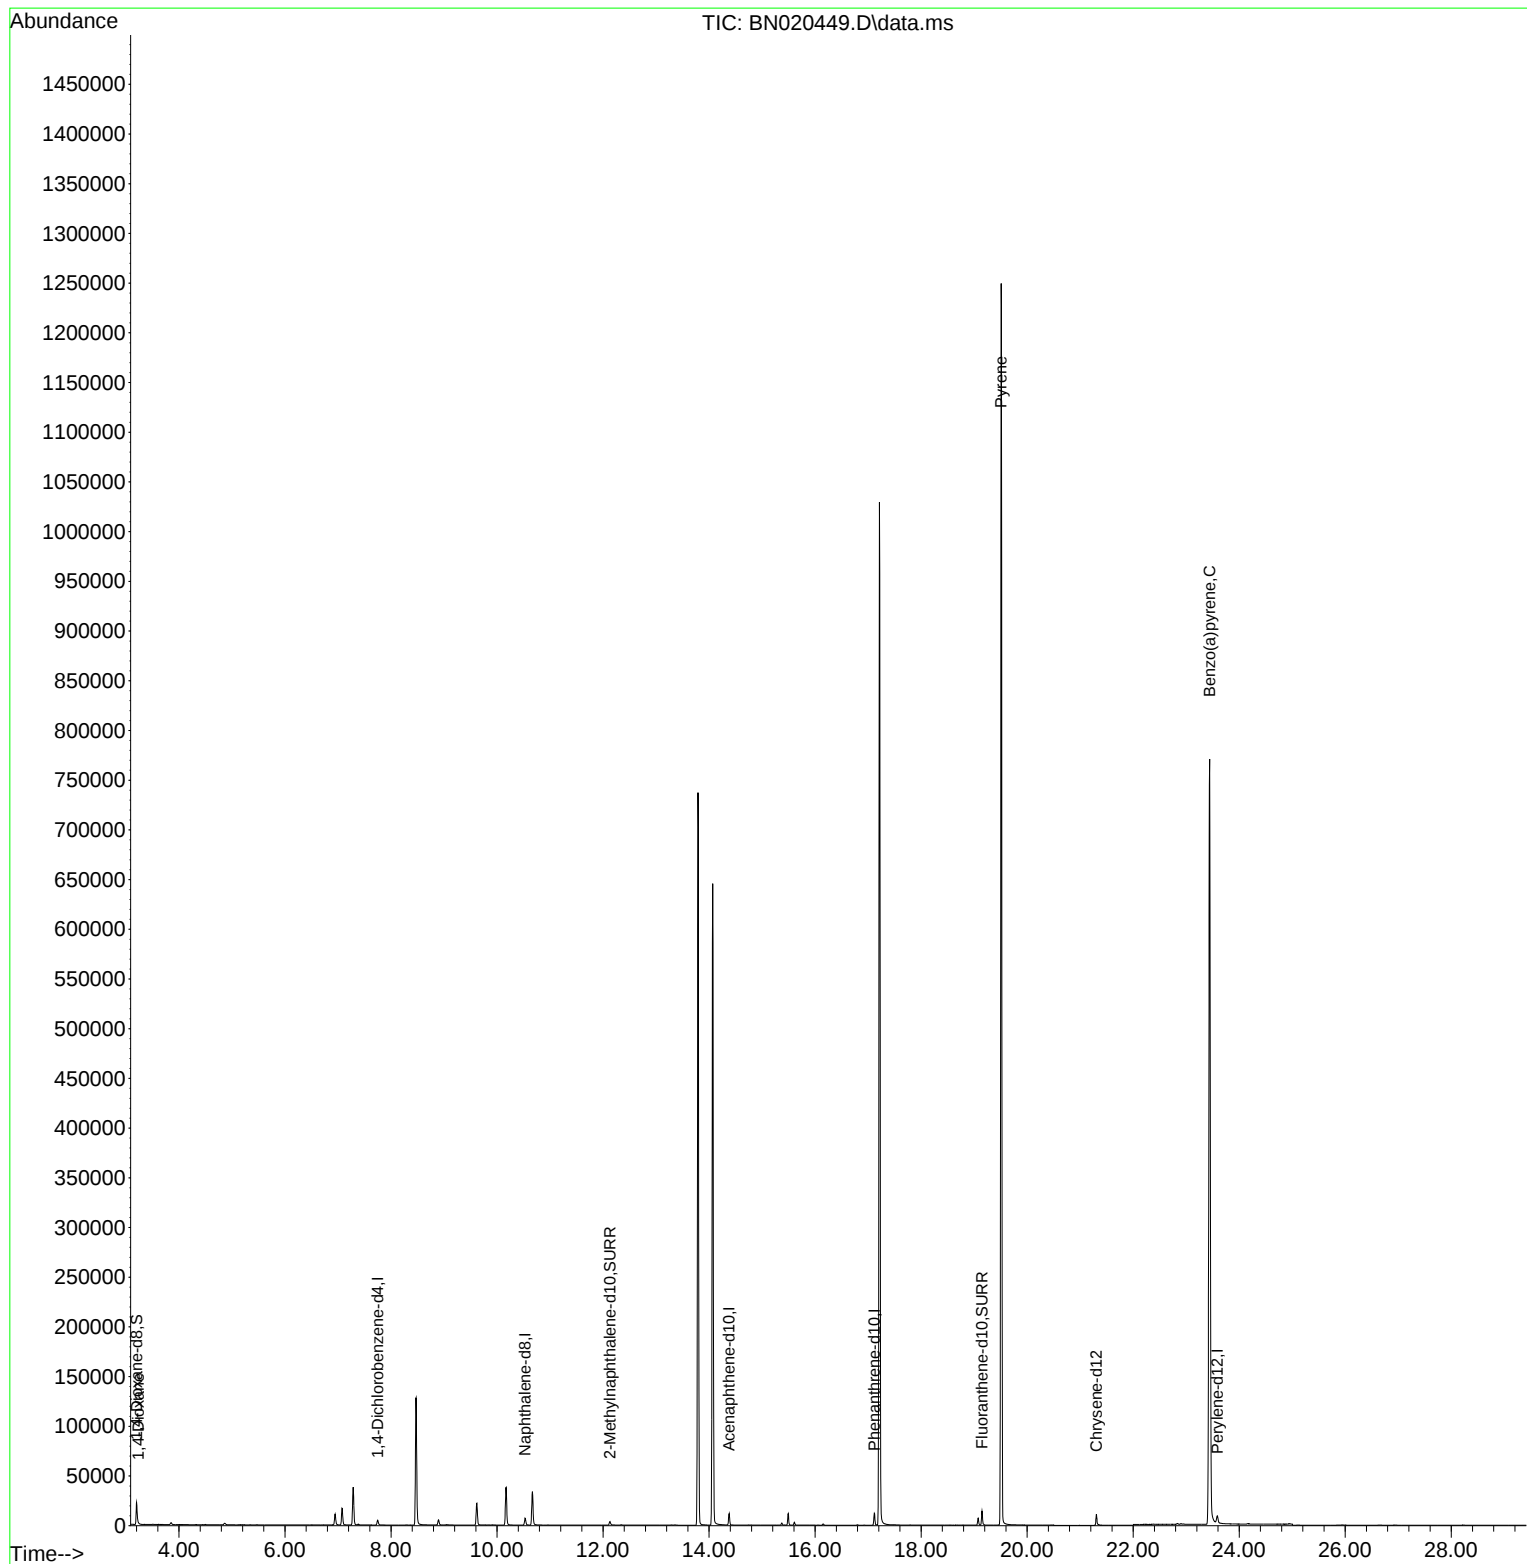



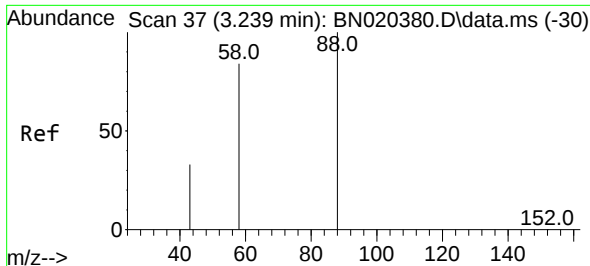


#2
1,4-Dioxane
Concen: 0.021 ng/ul
RT: 3.231 min Scan# 31
Delta R.T. -0.009 min
Lab File: BN020449.D
Acq: 26 Jun 2022 00:08

Instrument :
BNA_N
ClientSampleId :



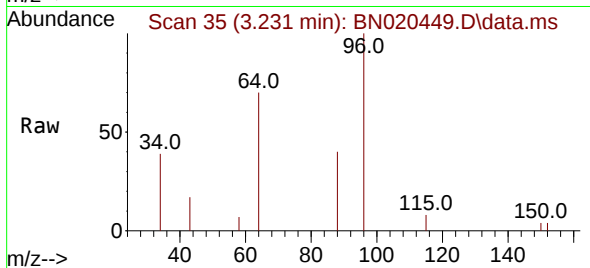



Tgt Ion: 88 Resp: 69
Ion Ratio Lower Upper
88 100
43 41.7 32.5 48.7
58 17.4 46.2 69.2#

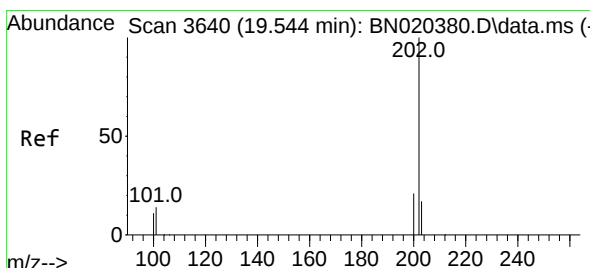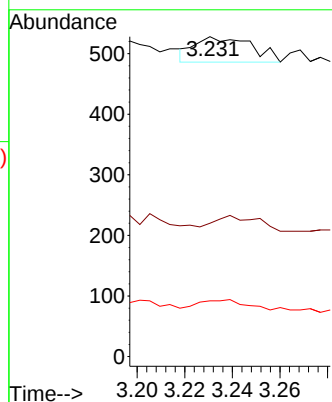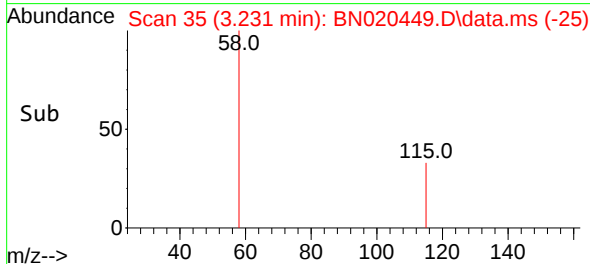

#20
Pyrene
Concen: 0.041 ng/ul
RT: 19.509 min Scan# 3632
Delta R.T. -0.035 min
Lab File: BN020449.D
Acq: 26 Jun 2022 00:08


Tgt Ion: 202 Resp: 2287
Ion Ratio Lower Upper
202 100
101 180.6 11.6 17.4#
100 1326.3 9.2 13.8#

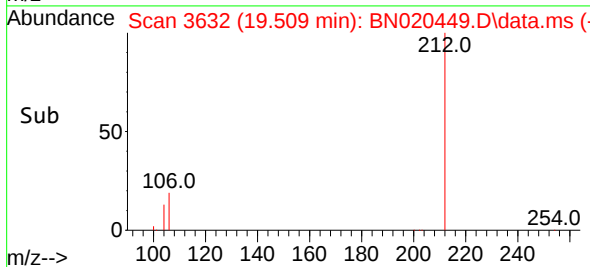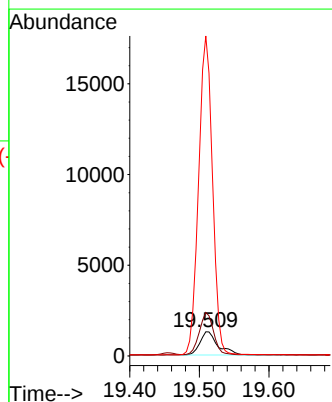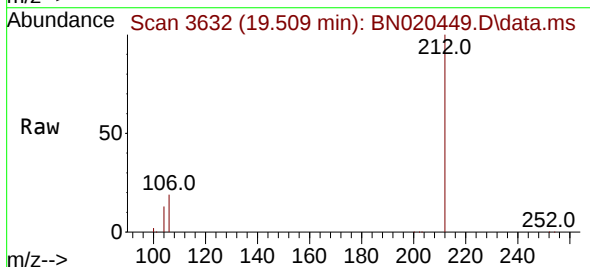

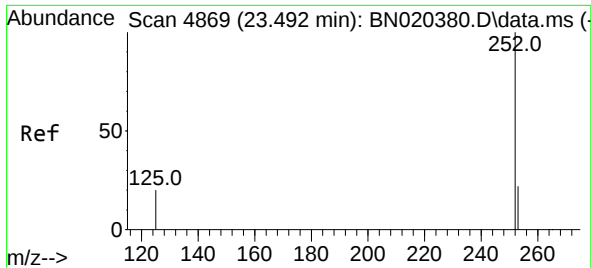

#26
 Benzo(a)pyrene
 Concen: 0.090 ng/ul
 RT: 23.441 min Scan# 41
 Delta R.T. -0.052 min
 Lab File: BN020449.D
 Acq: 26 Jun 2022 00:08

Instrument :
 BNA_N
 ClientSampleId :

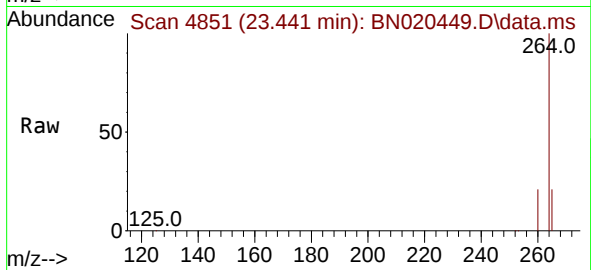

Tgt Ion:252 Resp: 4191
 Ion Ratio Lower Upper
 252 100
 253 41.0 21.0 31.4#
 125 34.0 18.8 28.2#

