

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020450.D
 Acq On : 26 Jun 2022 00:45
 Operator : CG/JU
 Sample : N3395-14
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 27 03:43:44 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.750	152	3042	0.400	ng/ul	0.00
4) Naphthalene-d8	10.529	136	10970	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.377	164	7275	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.116	188	16068	0.400	ng/ul	0.00
17) Chrysene-d12	21.305	240	14213	0.400	ng/ul	0.00
23) Perylene-d12	23.585	264	13591	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	18053	5.123	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.130	152	6485	0.360	ng/ul	0.00
18) Fluoranthene-d10	19.151	212	18096	0.386	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.513	202	2241	0.033	ng/ul#	1
26) Benzo(a)pyrene	23.442	252	4535	0.079	ng/ul#	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
Data File : BN020450.D
Acq On : 26 Jun 2022 00:45
Operator : CG/JU
Sample : N3395-14
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 27 03:43:44 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:17:34 2022
Response via : Initial Calibration




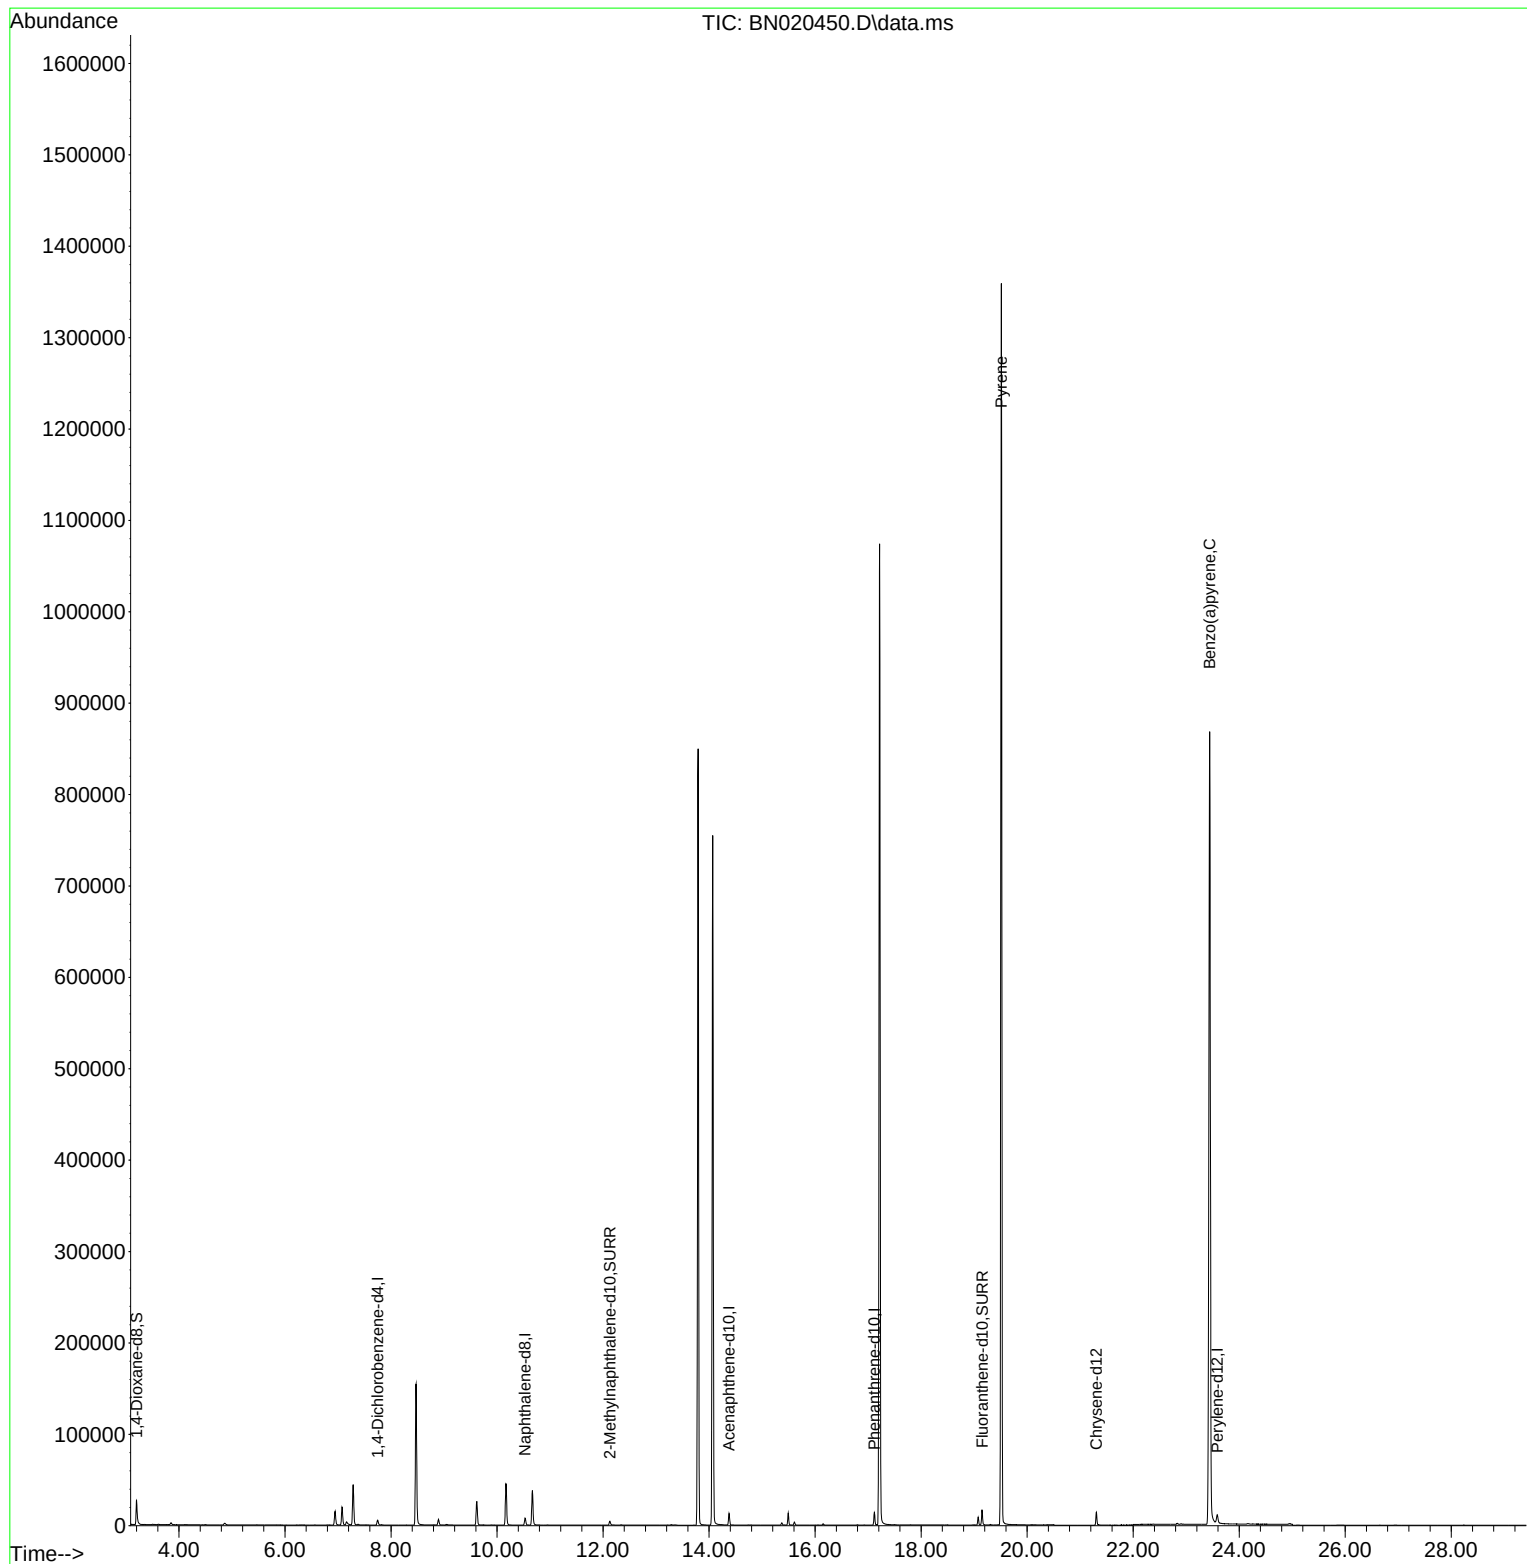


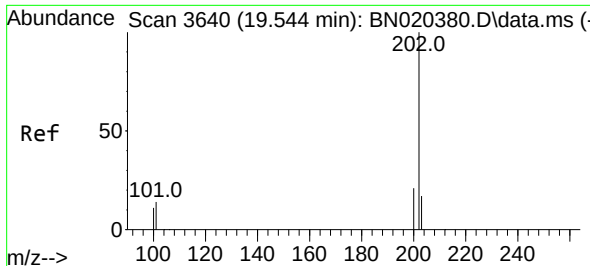

#20
Pyrene
Concen: 0.033 ng/ul
RT: 19.513 min Scan# 3633
Delta R.T. -0.031 min
Lab File: BN020450.D
Acq: 26 Jun 2022 00:45

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:202 Resp: 2241
Ion Ratio Lower Upper
202 100
101 170.1 11.6 17.4#
100 1211.7 9.2 13.8#

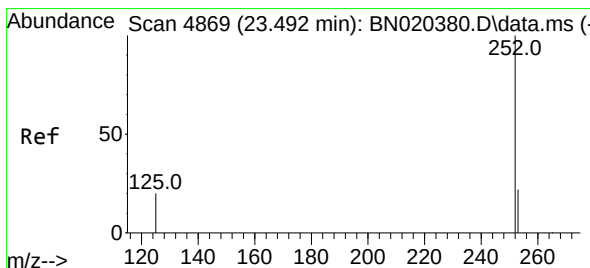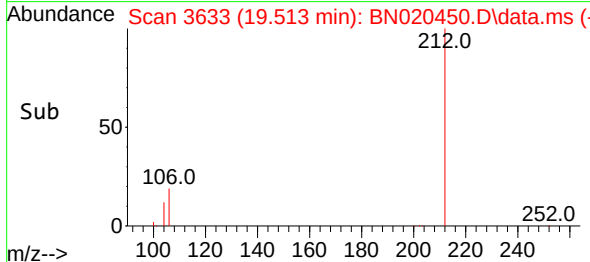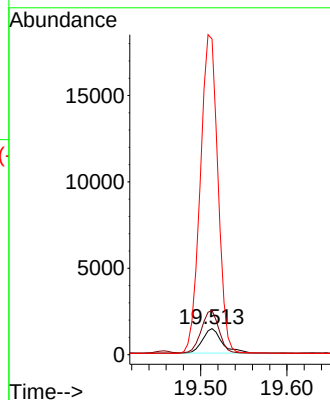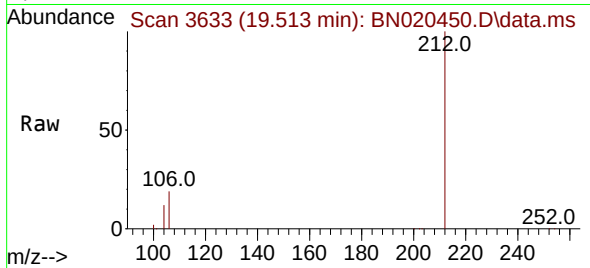

#26
Benzo(a)pyrene
Concen: 0.079 ng/ul
RT: 23.442 min Scan# 4851
Delta R.T. -0.051 min
Lab File: BN020450.D
Acq: 26 Jun 2022 00:45

Tgt Ion:252 Resp: 4535
Ion Ratio Lower Upper
252 100
253 42.6 21.0 31.4#
125 33.5 18.8 28.2#

