




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
Data File : BN020389.D
Acq On : 24 Jun 2022 09:59
Operator : CG/JU
Sample : N3355-20
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EY0D3

Manual IntegrationsAPPROVED

Quant Time: Jun 25 00:54:30 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:17:34 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/28/2022
Supervised By :mohammad ahmed 06/29/2022

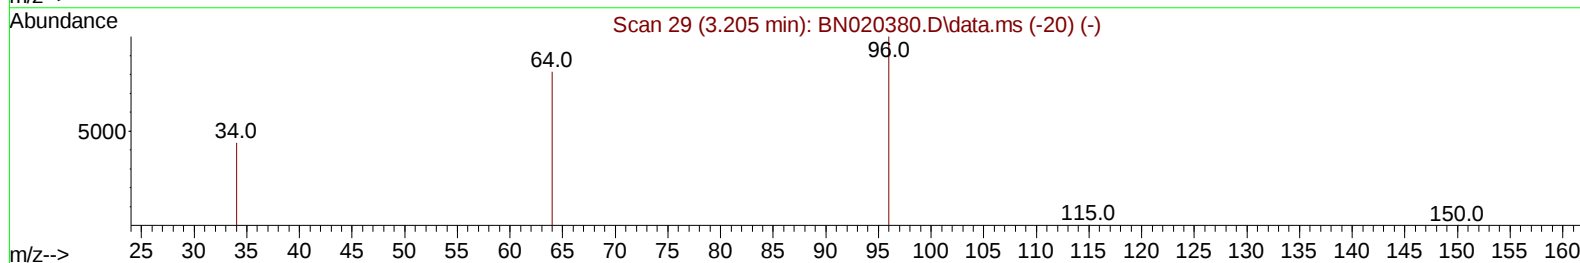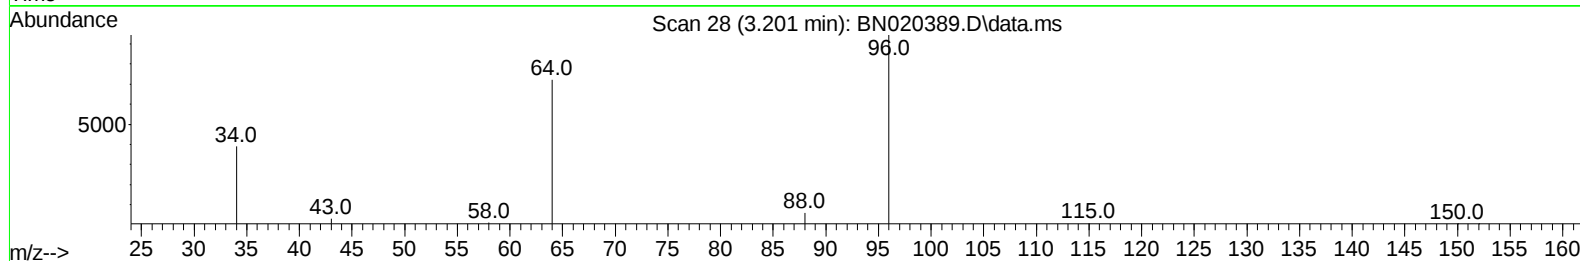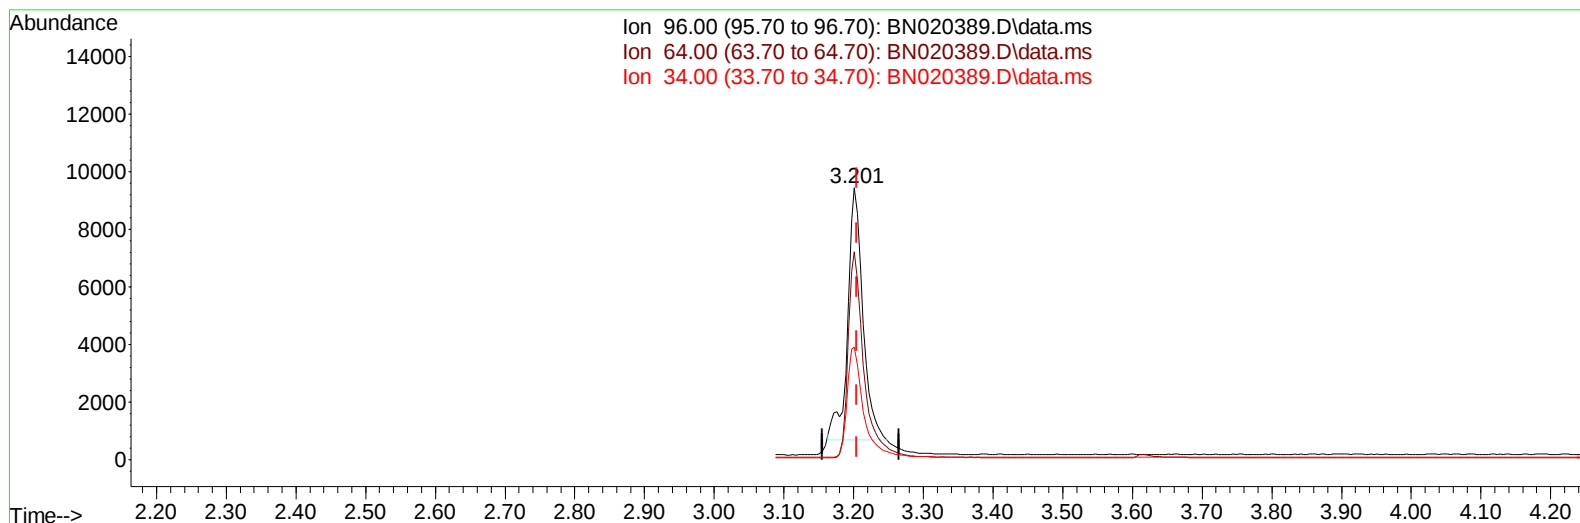

TIC: BN020389.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.201min (-0.004) 4.15 ng/u1

response 13238

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	72.10	76.43
34.00	43.00	41.29
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020389.D
 Acq On : 24 Jun 2022 09:59
 Operator : CG/JU
 Sample : N3355-20
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EY0D3

Manual IntegrationsAPPROVED

Quant Time: Jun 25 00:54:30 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/28/2022
 Supervised By :mohammad ahmed 06/29/2022

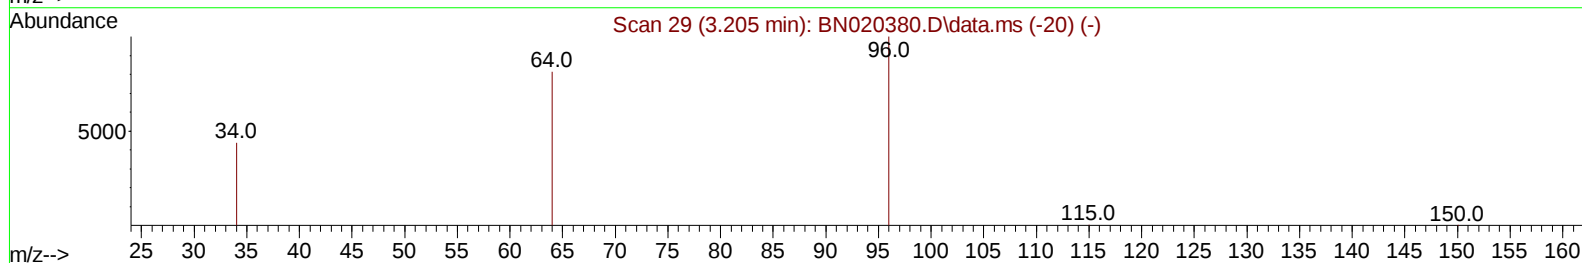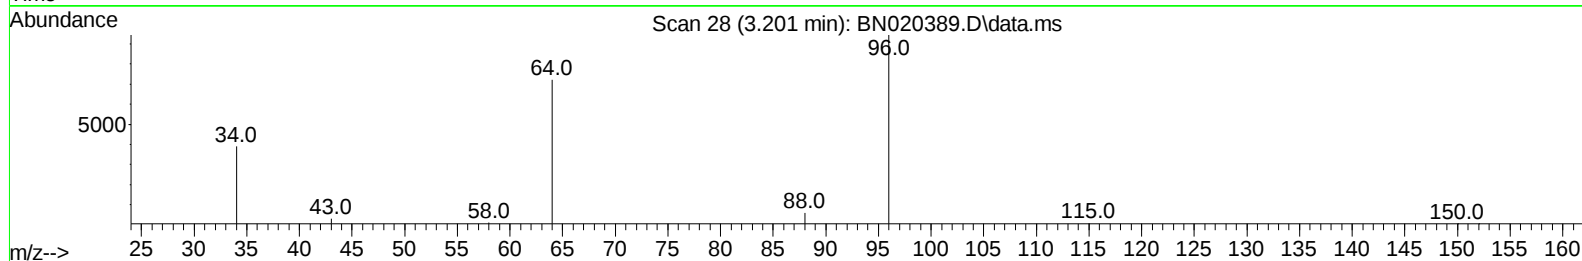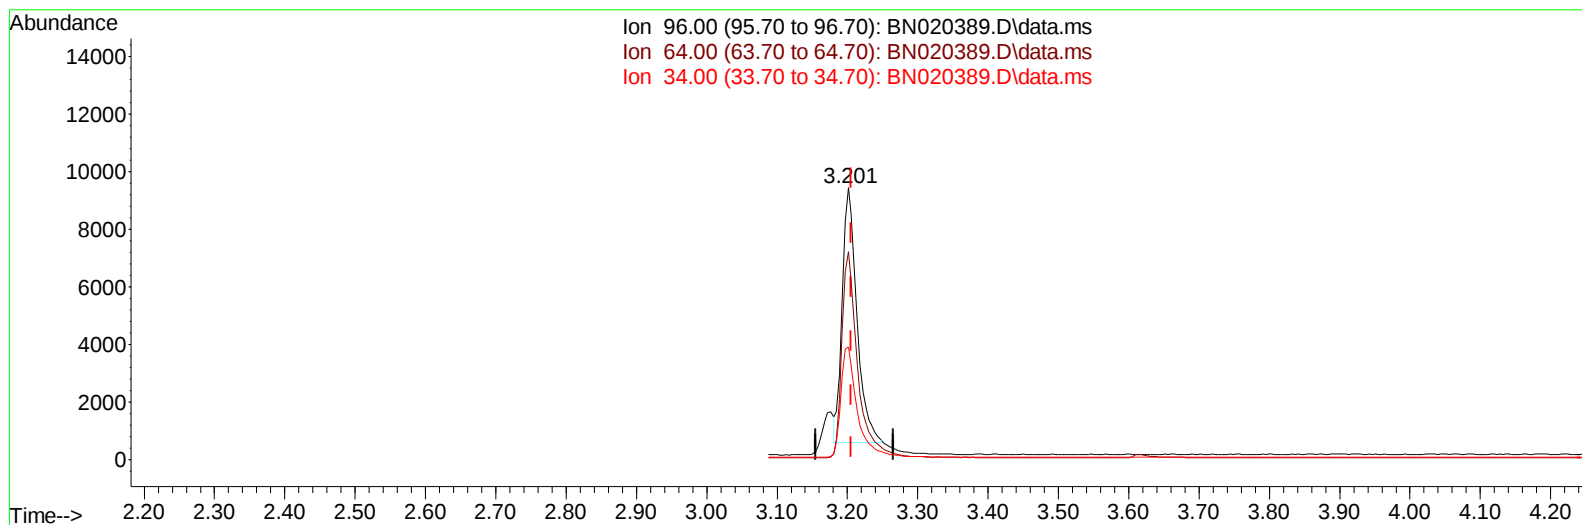

TIC: BN020389.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.201min (-0.004) 4.00 ng/ul m

response 12781

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	72.10	76.43
34.00	43.00	41.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020389.D
 Acq On : 24 Jun 2022 09:59
 Operator : CG/JU
 Sample : N3355-20
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EY0D3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/28/2022
 Supervised By :mohammad ahmed 06/29/2022

Quant Time: Jun 25 00:54:30 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.749	152		2755	0.400	ng/ul	0.00
4) Naphthalene-d8	10.535	136		9444	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.377	164		6251	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.120	188		14042	0.400	ng/ul	0.00
17) Chrysene-d12	21.312	240		12599	0.400	ng/ul	0.00
23) Perylene-d12	23.595	264		12805	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.201	96		12781m	4.004	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.129	152		4840	0.312	ng/ul	0.00
18) Fluoranthene-d10	19.151	212		13941	0.336	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
Data File : BN020389.D
Acq On : 24 Jun 2022 09:59
Operator : CG/JU
Sample : N3355-20
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EY0D3

Manual IntegrationsAPPROVED

Quant Time: Jun 25 00:54:30 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:17:34 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/28/2022
Supervised By :mohammad ahmed 06/29/2022

