




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020438.D
 Acq On : 25 Jun 2022 16:52
 Operator : CG/JU
 Sample : N3395-13
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0160

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:42:44 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :mohammad ahmed 06/29/2022

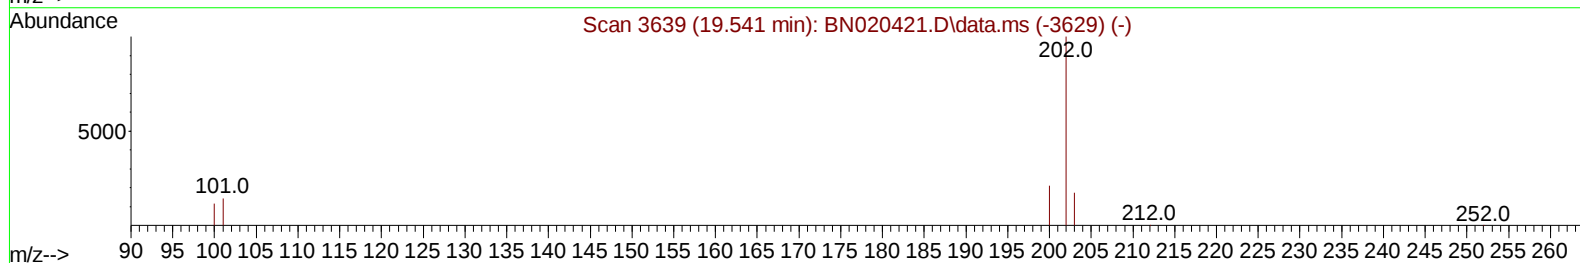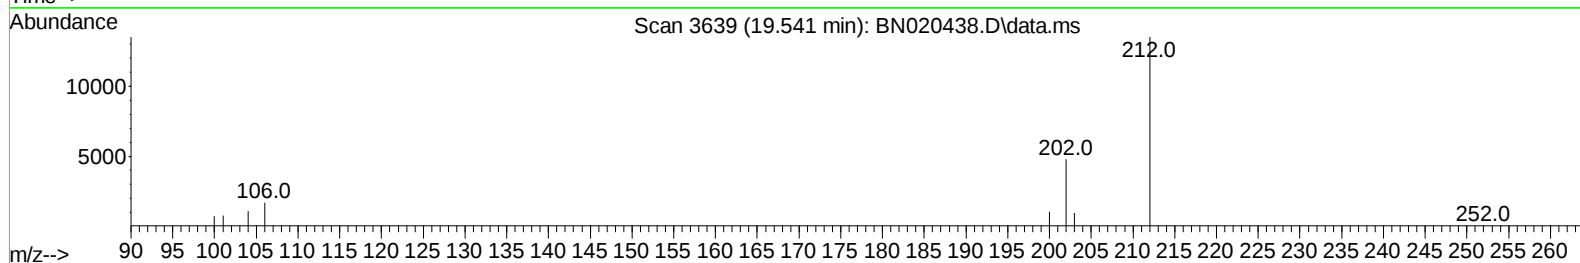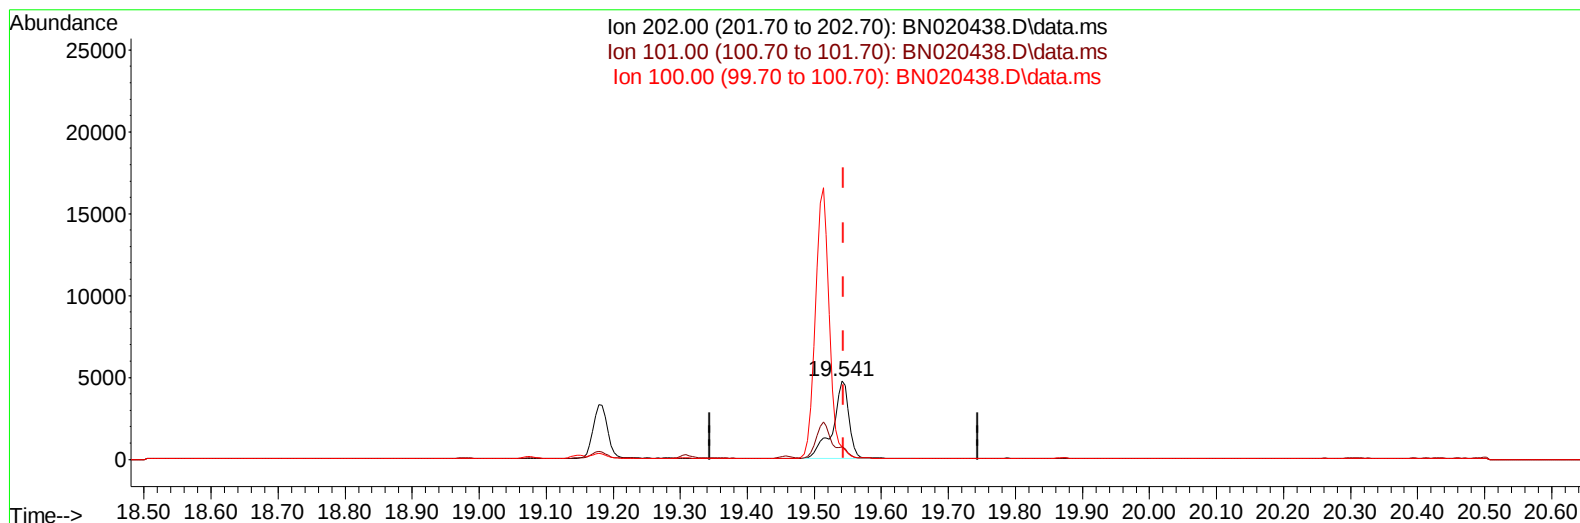

TIC: BN020438.D\data.ms

(20) Pyrene

19.541min (-0.003) 0.12 ng/u1

response 8011

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.50	16.17
100.00	11.50	15.89#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020438.D
 Acq On : 25 Jun 2022 16:52
 Operator : CG/JU
 Sample : N3395-13
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0160

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:42:44 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :mohammad ahmed 06/29/2022

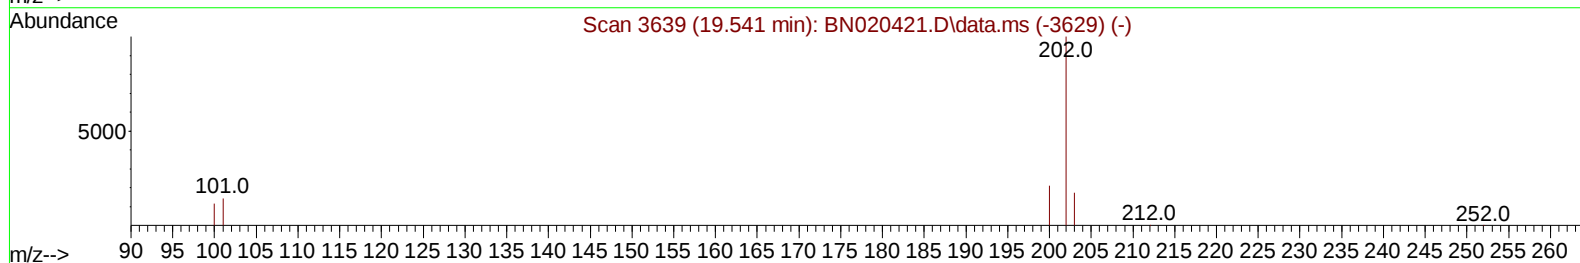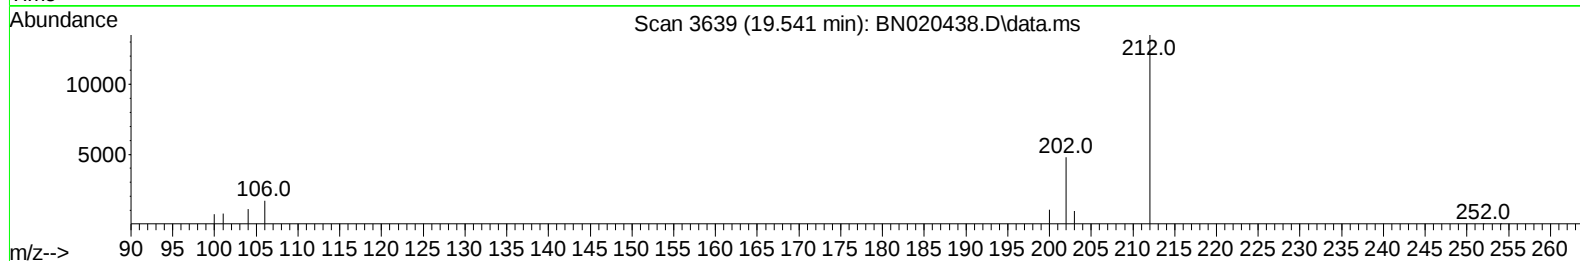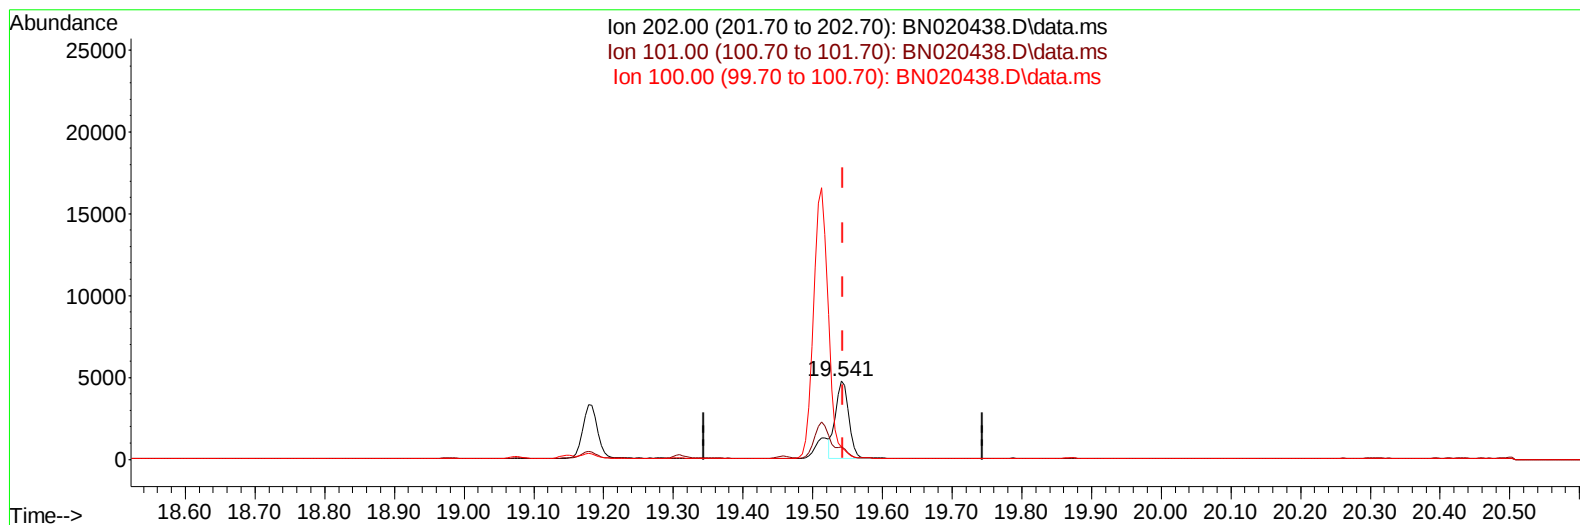

TIC: BN020438.D\data.ms

(20) Pyrene

19.541min (-0.003) 0.10 ng/ul m

response 6318

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.50	16.17
100.00	11.50	15.89#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020438.D
 Acq On : 25 Jun 2022 16:52
 Operator : CG/JU
 Sample : N3395-13
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0160

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/27/2022
 Supervised By :mohammad ahmed 06/29/2022

Quant Time: Jun 27 03:42:44 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.750	152		2933	0.400	ng/ul	0.00
4) Naphthalene-d8	10.529	136		10365	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.377	164		6985	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.120	188		15622	0.400	ng/ul	0.00
17) Chrysene-d12	21.311	240		13553	0.400	ng/ul	0.00
23) Perylene-d12	23.594	264		12540	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.201	96		17110	5.035	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.130	152		5772	0.339	ng/ul	0.00
18) Fluoranthene-d10	19.151	212		15327	0.343	ng/ul	0.00
Target Compounds							Qvalue
11) Acenaphthene	14.442	153		1584	0.060	ng/ul	99
12) Fluorene	15.427	166		1156	0.037	ng/ul#	96
19) Fluoranthene	19.179	202		4906	0.079	ng/ul#	94
20) Pyrene	19.541	202		6318m	0.098	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
Data File : BN020438.D
Acq On : 25 Jun 2022 16:52
Operator : CG/JU
Sample : N3395-13
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0160

Manual IntegrationsAPPROVED

Quant Time: Jun 27 03:42:44 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:17:34 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/27/2022
Supervised By :mohammad ahmed 06/29/2022

