

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020406.D
 Acq On : 24 Jun 2022 20:54
 Operator : CG/JU
 Sample : N3359-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4S2

Quant Time: Jun 25 00:55:36 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.750	152	3201	0.400	ng/ul	0.00
4) Naphthalene-d8	10.535	136	11028	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.382	164	7309	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.120	188	16582	0.400	ng/ul	0.00
17) Chrysene-d12	21.308	240	15532	0.400	ng/ul	0.00
23) Perylene-d12	23.588	264	15156	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	19341	5.215	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.130	152	6469	0.357	ng/ul	0.00
18) Fluoranthene-d10	19.146	212	19761	0.386	ng/ul	0.00
Target Compounds						
5) Naphthalene	10.584	128	1619	0.048	ng/ul#	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
Data File : BN020406.D
Acq On : 24 Jun 2022 20:54
Operator : CG/JU
Sample : N3359-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4S2


Quant Time: Jun 25 00:55:36 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:17:34 2022
Response via : Initial Calibration

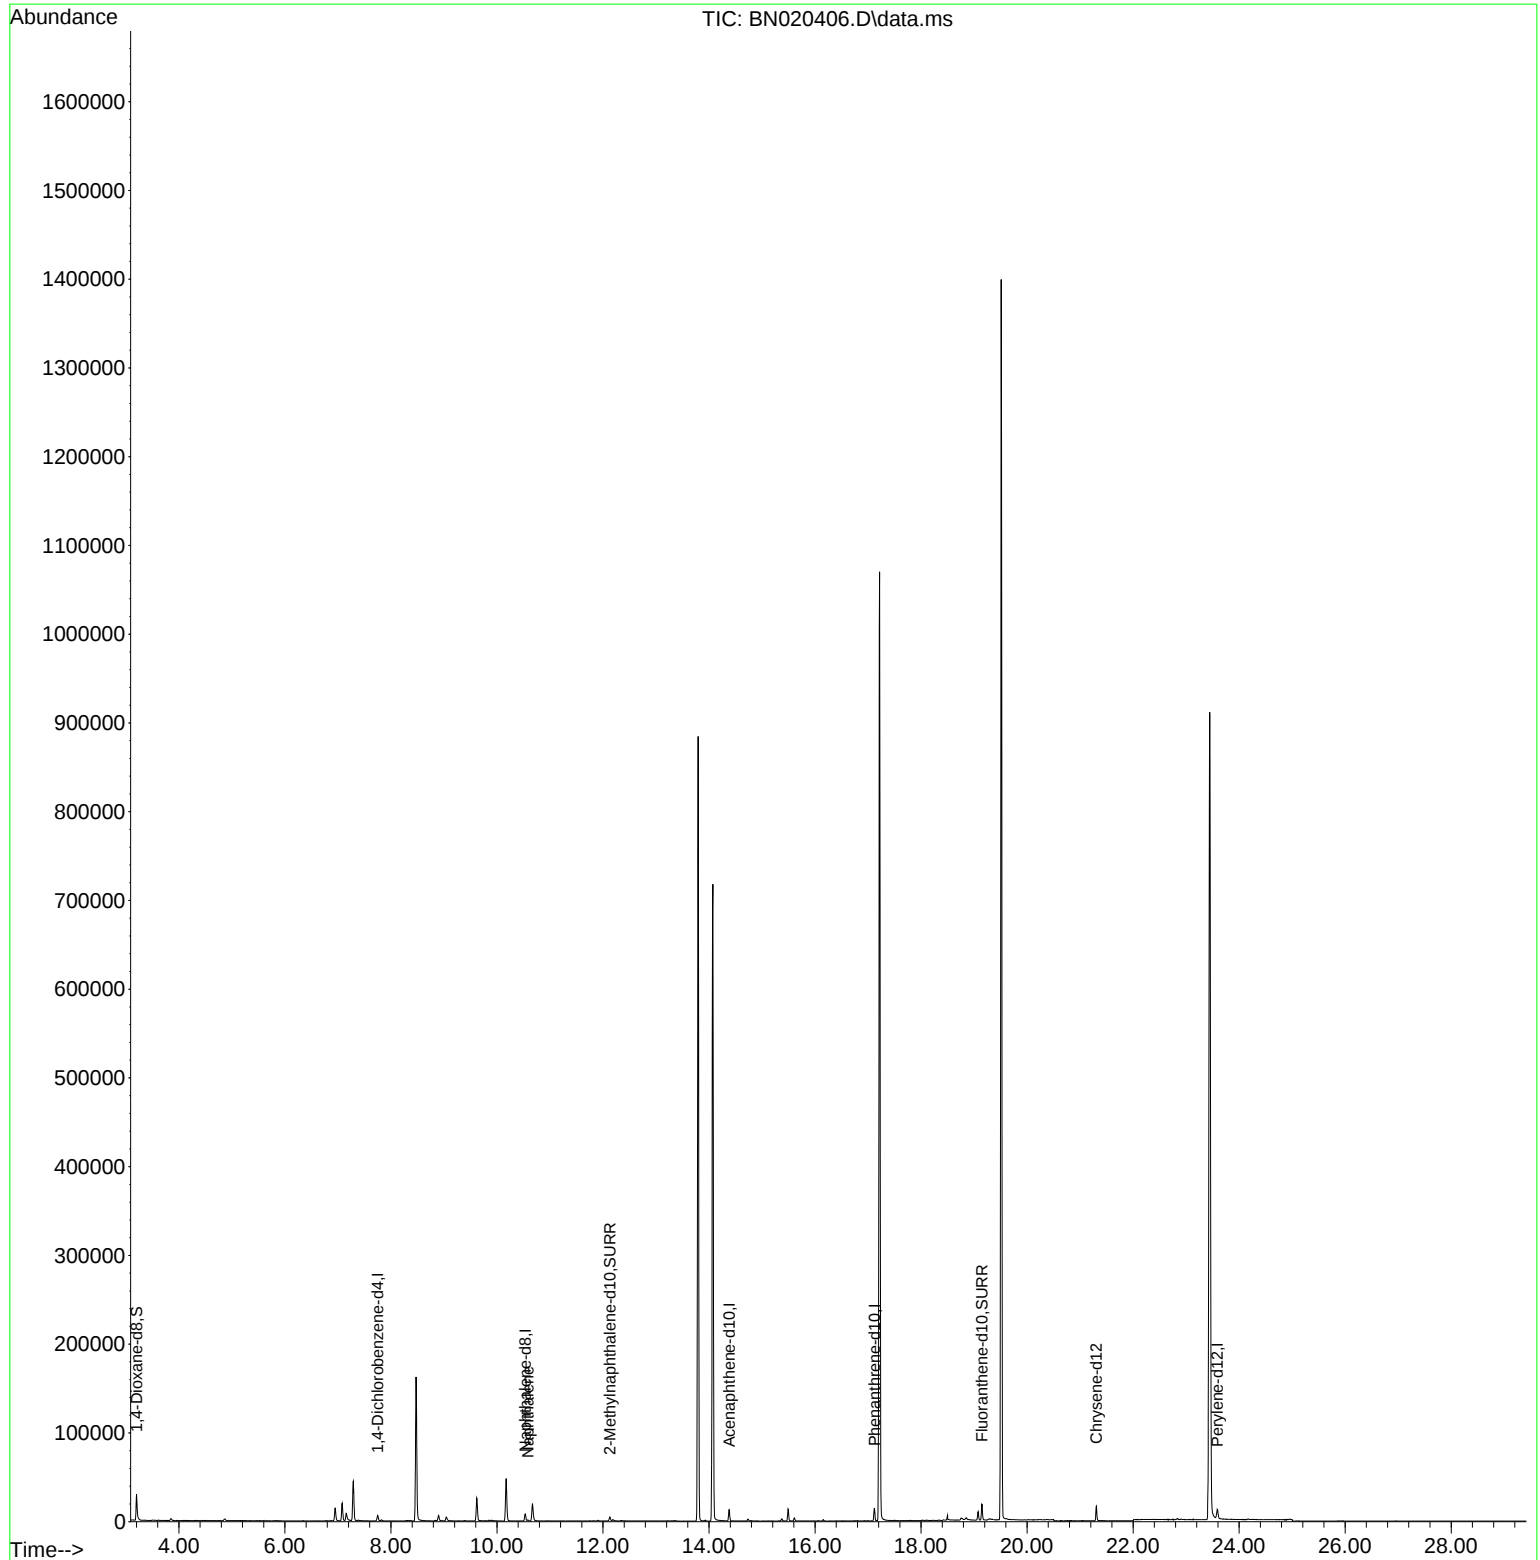

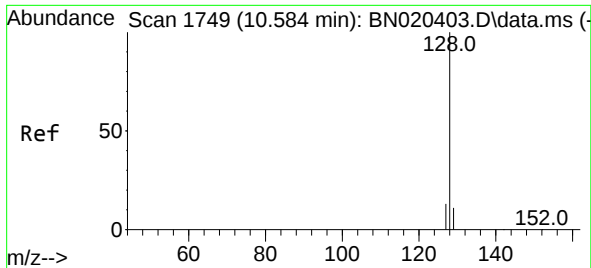

#5
Naphthalene
Concen: 0.048 ng/ul
RT: 10.584 min Scan# 11
Delta R.T. 0.001 min
Lab File: BN020406.D
Acq: 24 Jun 2022 20:54

Instrument :
BNA_N
ClientSampleId :
EW4S2

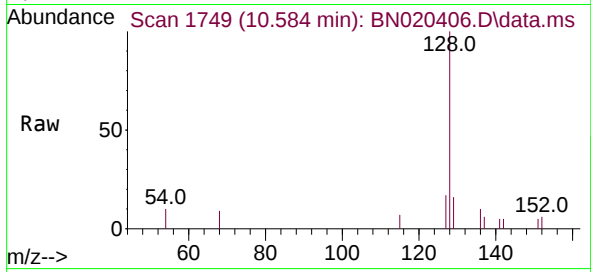

Tgt Ion:128 Resp: 1619
Ion Ratio Lower Upper
128 100
129 15.9 9.5 14.3#
127 17.1 11.3 16.9#

